

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082225\
 Data File : PL096944.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2025 09:31
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 25 04:09:30 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
 Quant Title : GC Extractables
 QLast Update : Thu Aug 21 06:34:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.530	2.826	71034403	108.5E6	18.011	19.248
28)	SA Decachlor...	9.005	7.987	54419488	105.4E6	18.381	21.977
Target Compounds							
14)	MA Endrin	0.000	5.714	0	7523498	N.D.	1.274 #
15)	B Endosulfa...	6.735	0.000	11777310	0	2.674	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082225\
Data File : PL096944.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2025 09:31
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 25 04:09:30 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL082025.M
Quant Title : GC Extractables
QLast Update : Thu Aug 21 06:34:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

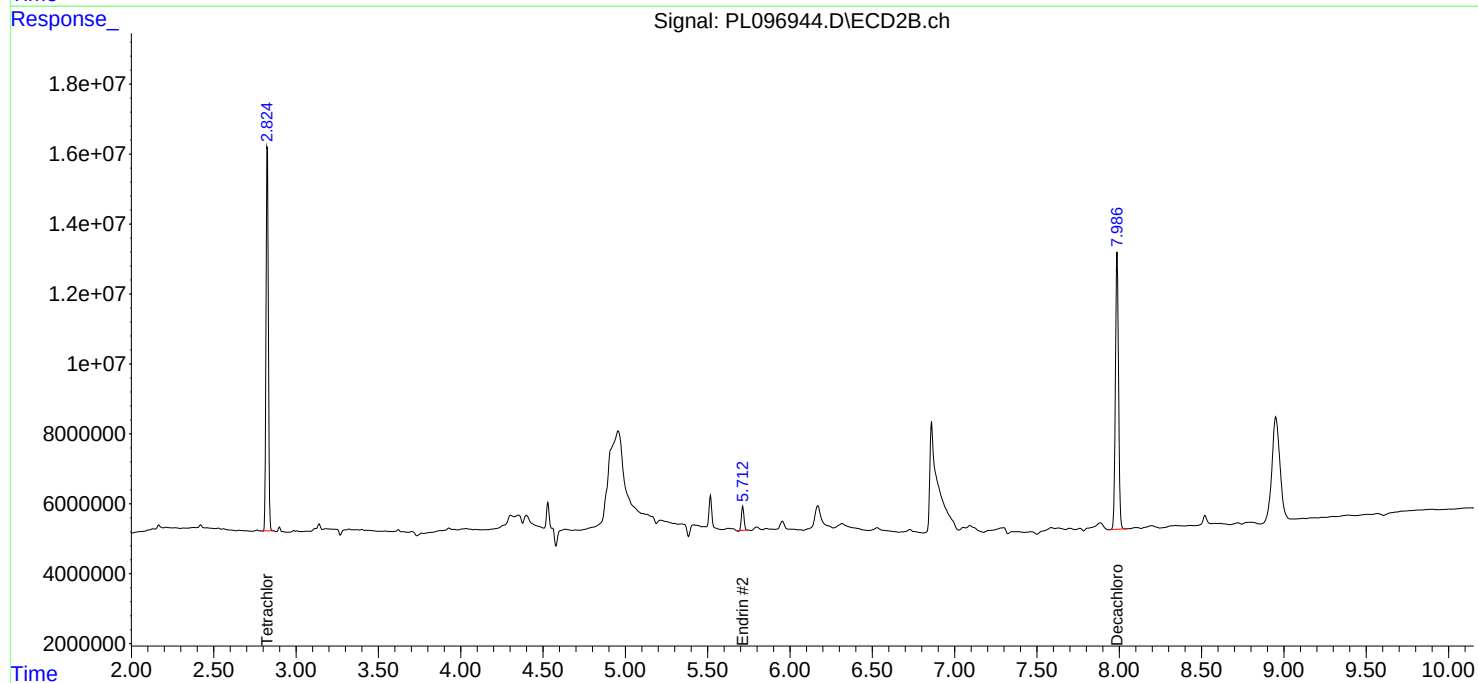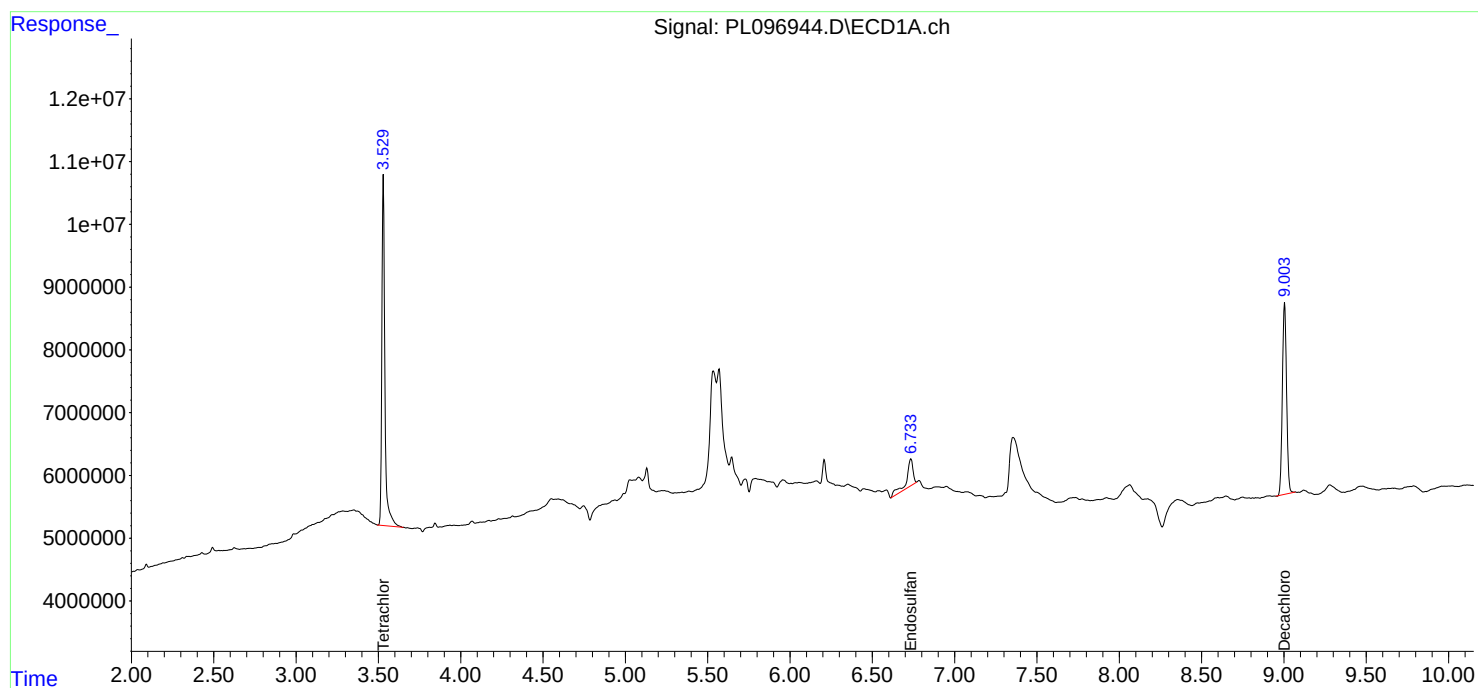


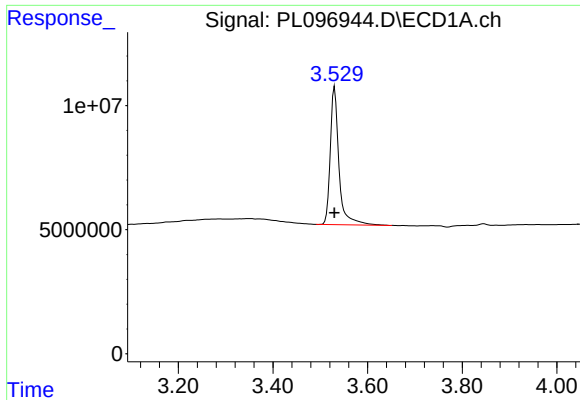

#1 Tetrachloro-m-xylene


R.T.: 3.530 min
Delta R.T.: 0.000 min
Response: 71034403
Conc: 18.01 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

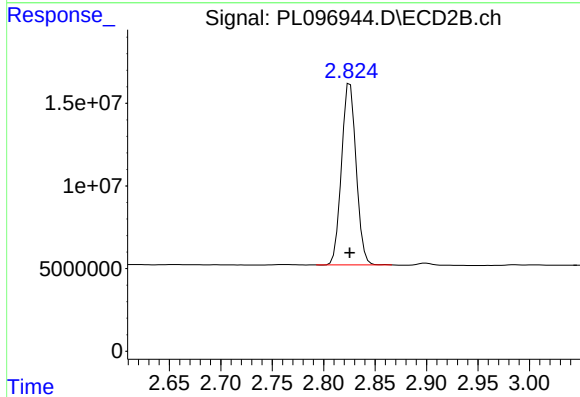


#1 Tetrachloro-m-xylene

R.T.: 2.826 min
Delta R.T.: 0.000 min
Response: 108495675
Conc: 19.25 ng/ml

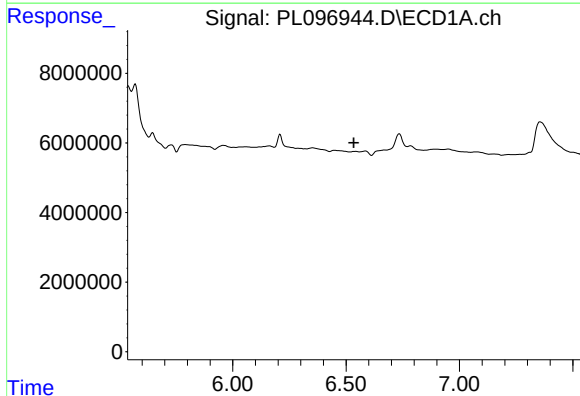


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.534 min
Response: 0
Conc: N.D.

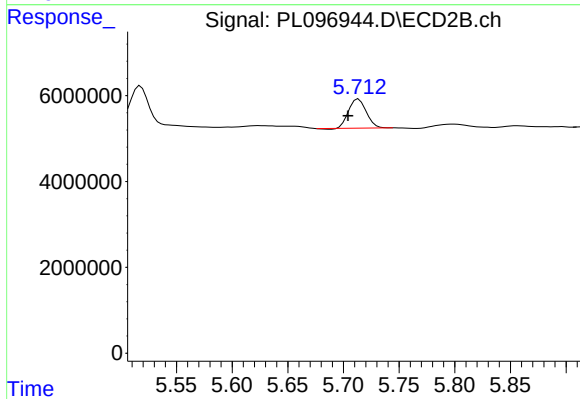

#14 Endrin


R.T.: 5.714 min
Delta R.T.: 0.010 min
Response: 7523498
Conc: 1.27 ng/ml

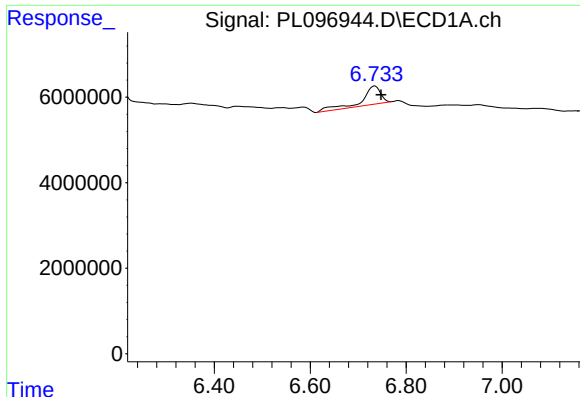

#15 Endosulfan II


R.T.: 6.735 min
Delta R.T.: -0.013 min
Response: 11777310
Conc: 2.67 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

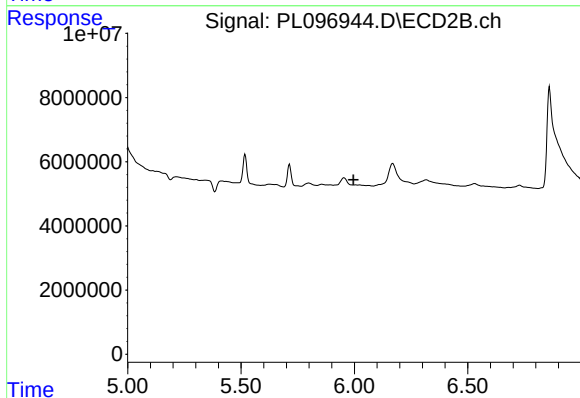


#15 Endosulfan II

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

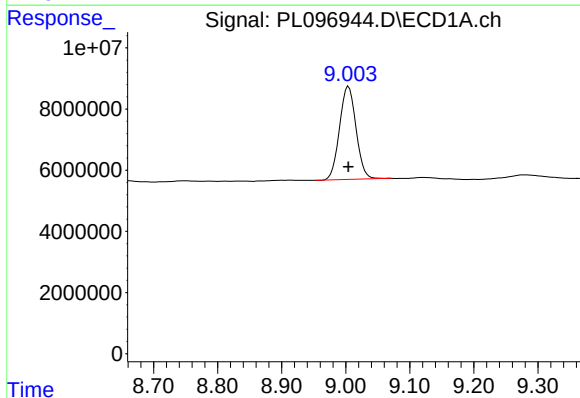

#28 Decachlorobiphenyl

R.T.: 9.005 min
Delta R.T.: 0.000 min
Response: 54419488
Conc: 18.38 ng/ml

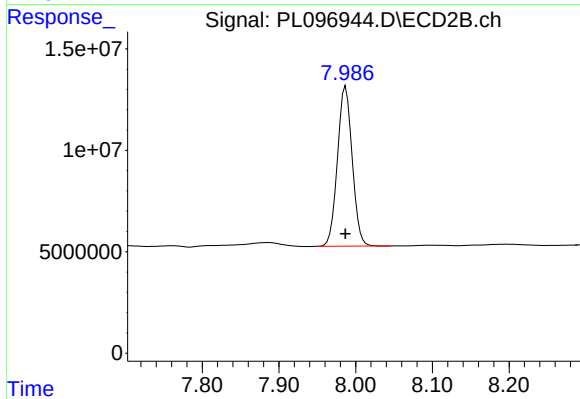

#28 Decachlorobiphenyl

R.T.: 7.987 min
Delta R.T.: 0.000 min
Response: 105398094
Conc: 21.98 ng/ml