

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091824\
 Data File : PL091813.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2024 16:08
 Operator : AR\AJ
 Sample : P4087-25
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NB-614-COMP-05

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/19/2024
 Supervised By :Ankita Jodhani 09/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 01:43:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 09 19:26:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.781	30167637	37560214	19.356m	20.082
28) SA Decachlor...	9.059	7.923	16892631	27663768	13.900	14.981

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091824\
Data File : PL091813.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2024 16:08
Operator : AR\AJ
Sample : P4087-25
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NB-614-COMP-05


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/19/2024
Supervised By : Ankita Jodhani 09/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 01:43:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
Quant Title : GC Extractables
QLast Update : Mon Sep 09 19:26:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

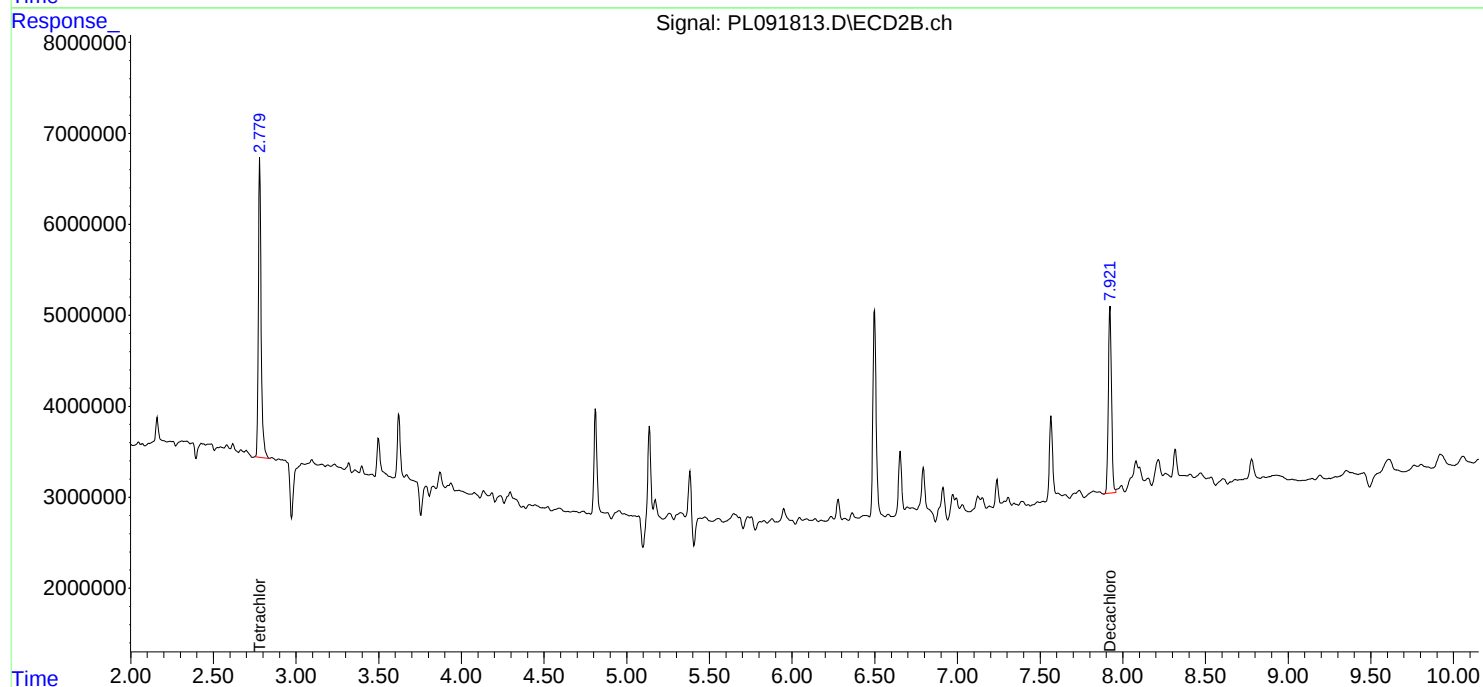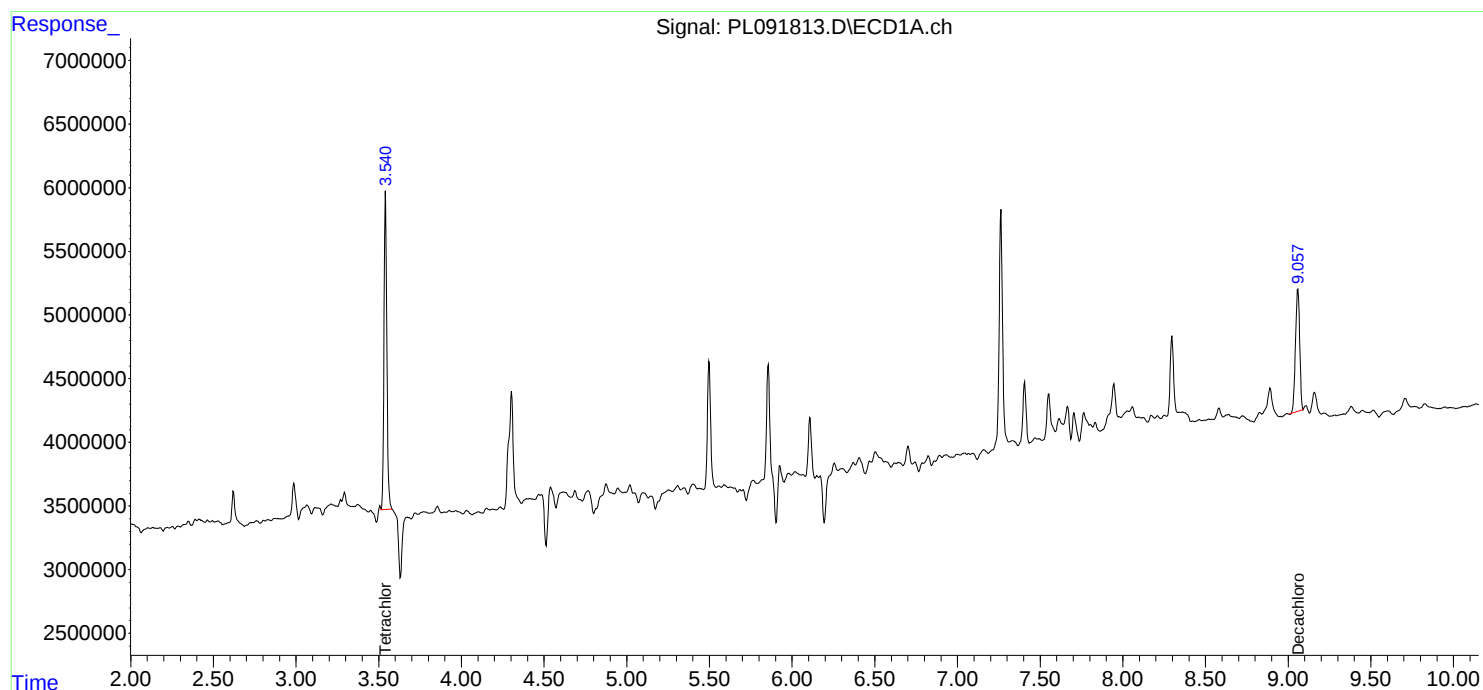

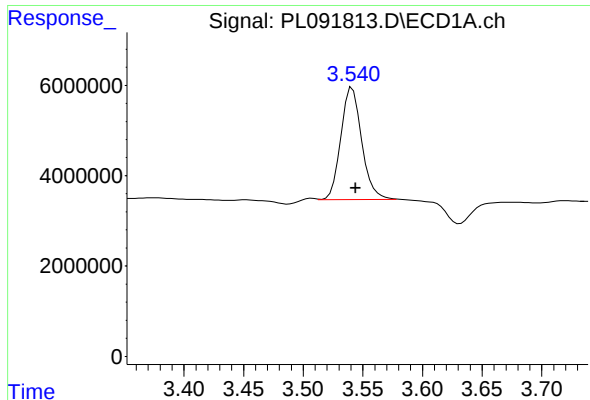


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 30167637
Conc: 19.36 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-614-COMP-05


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/19/2024
Supervised By :Ankita Jodhani 09/19/2024

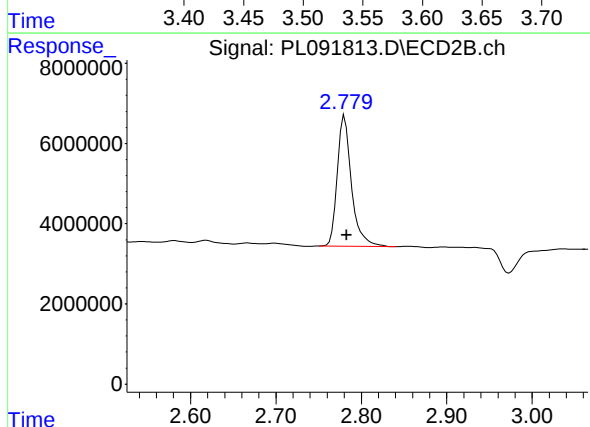


#1 Tetrachloro-m-xylene

R.T.: 2.781 min
Delta R.T.: -0.002 min
Response: 37560214
Conc: 20.08 ng/ml

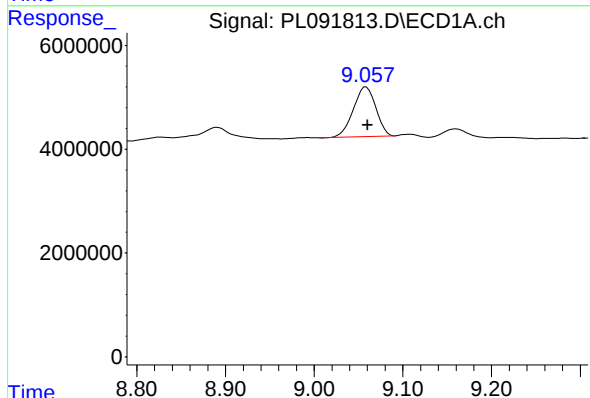

#28 Decachlorobiphenyl

R.T.: 9.059 min
Delta R.T.: -0.002 min
Response: 16892631
Conc: 13.90 ng/ml

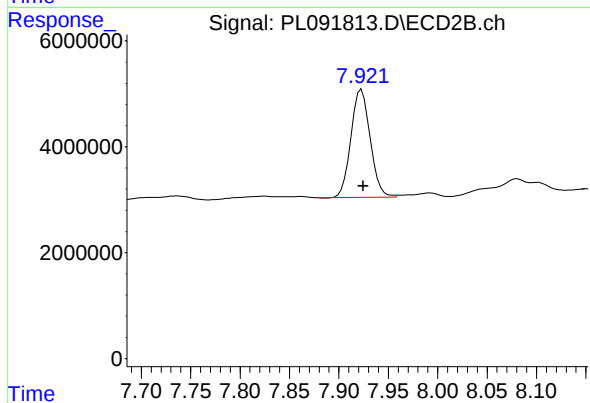

#28 Decachlorobiphenyl

R.T.: 7.923 min
Delta R.T.: -0.002 min
Response: 27663768
Conc: 14.98 ng/ml