

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091824\
 Data File : PL091818.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2024 17:46
 Operator : AR\AJ
 Sample : P4088-07
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 NB-614-COMP-08

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/19/2024
 Supervised By :Ankita Jodhani 09/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 01:46:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
 Quant Title : GC Extractables
 QLast Update : Mon Sep 09 19:26:36 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.540	2.780	32929810	39116788	21.128m	20.915
28) SA Decachlor...	9.059	7.920	20299446	33336544	16.703	18.053m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL091824\
Data File : PL091818.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2024 17:46
Operator : AR\AJ
Sample : P4088-07
Misc :
ALS Vial : 22 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
NB-614-COMP-08


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/19/2024
Supervised By : Ankita Jodhani 09/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 01:46:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL090924.M
Quant Title : GC Extractables
QLast Update : Mon Sep 09 19:26:36 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

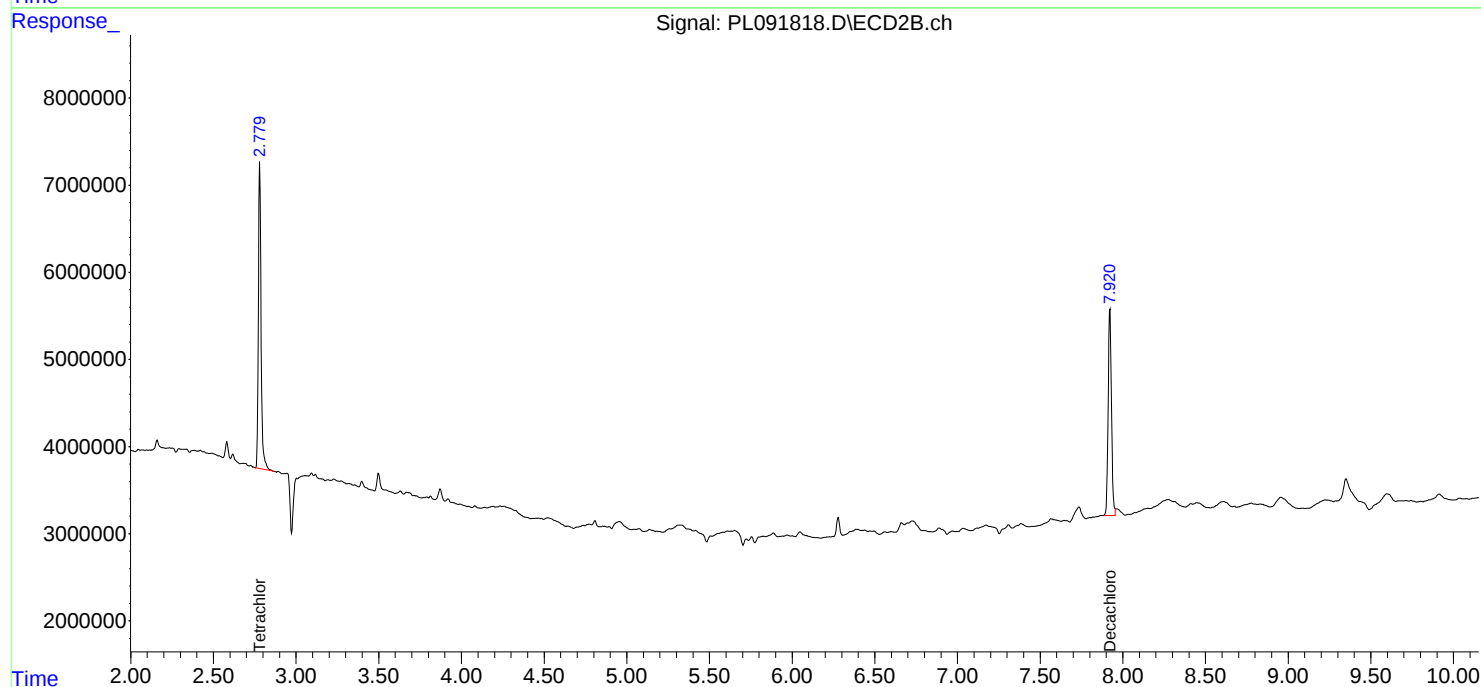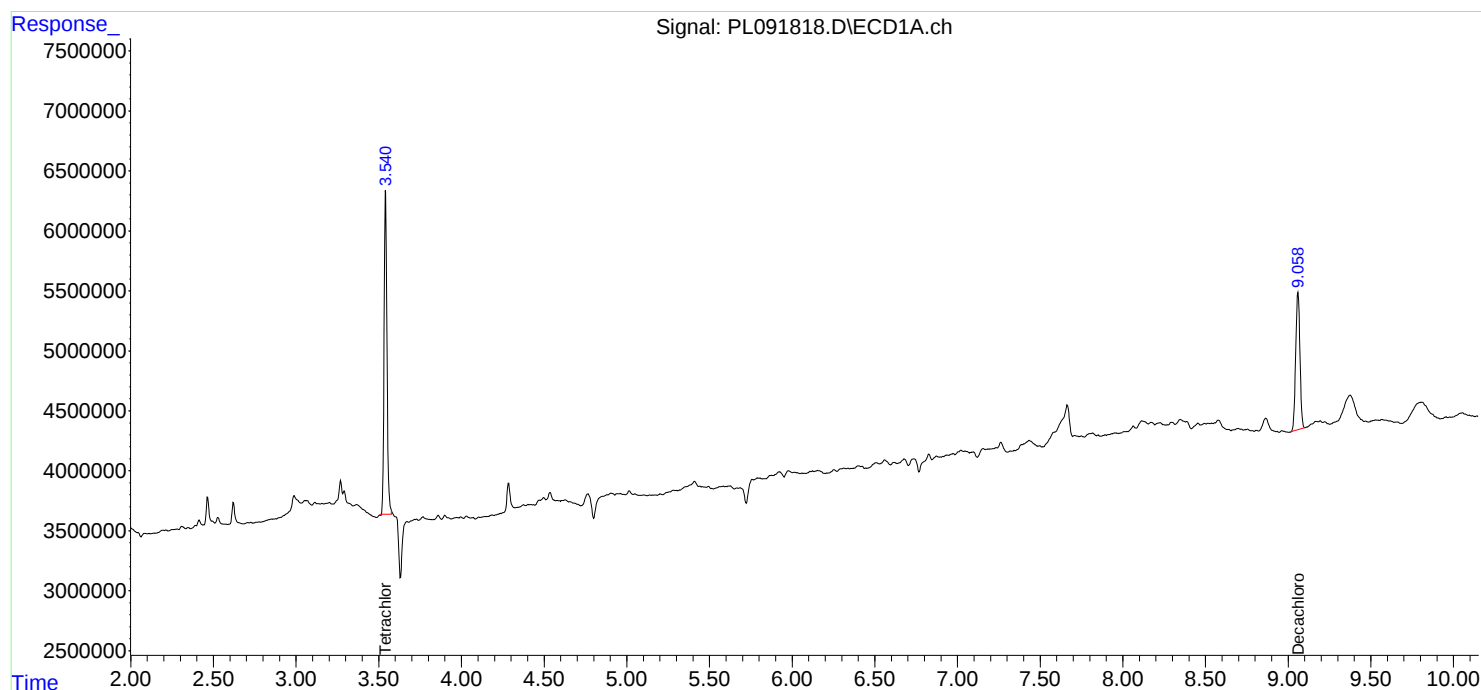

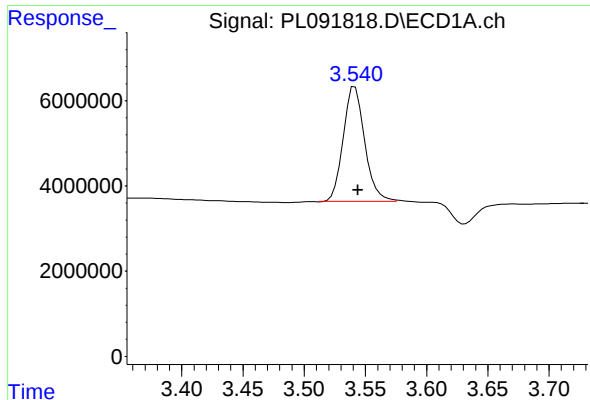


#1 Tetrachloro-m-xylene

R.T.: 3.540 min
Delta R.T.: -0.004 min
Response: 32929810
Conc: 21.13 ng/ml

Instrument :
ECD_L
ClientSampleId :
NB-614-COMP-08


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/19/2024
Supervised By :Ankita Jodhani 09/19/2024

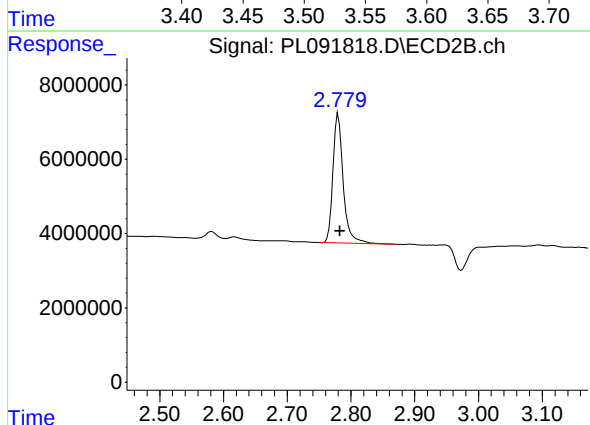


#1 Tetrachloro-m-xylene

R.T.: 2.780 min
Delta R.T.: -0.002 min
Response: 39116788
Conc: 20.91 ng/ml

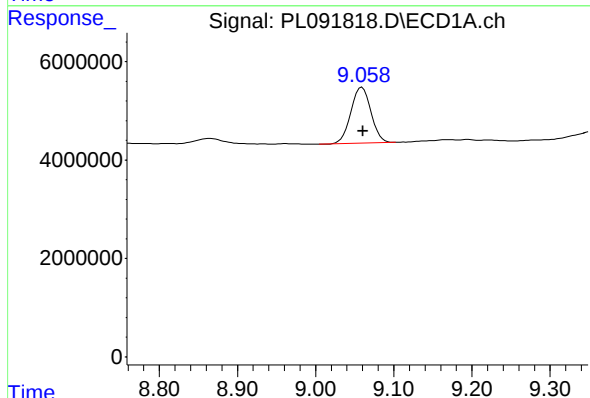

#28 Decachlorobiphenyl

R.T.: 9.059 min
Delta R.T.: -0.001 min
Response: 20299446
Conc: 16.70 ng/ml

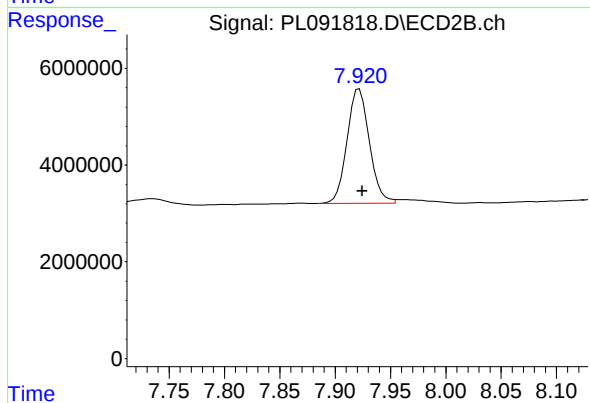

#28 Decachlorobiphenyl

R.T.: 7.920 min
Delta R.T.: -0.004 min
Response: 33336544
Conc: 18.05 ng/ml m