

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082218\
 Data File : PL039416.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2018 15:52
 Operator : AJ\SJ
 Sample : PB112284BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 01:01:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.314	3.905	133.7E6	61291486	19.129	22.862
28)	SA Decachlor...	7.974	8.900	135.8E6	50498208	19.330	21.761
Target Compounds							
4)	MA Heptachlor	4.228f	0.000	5149100	0	0.489	N.D. #
6)	B beta-BHC	4.228f	0.000	5149100	0	1.108	N.D. #
9)	A Endosulfan I	5.322	0.000	3493175	0	0.399	N.D. #
17)	MA 4,4'-DDT	6.143	0.000	6743145	0	0.890	N.D. #
23)	Chlordane-1	4.079	0.000	8492525	0	26.825	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082218\
Data File : PL039416.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2018 15:52
Operator : AJ\SJ
Sample : PB112284BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 01:01:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

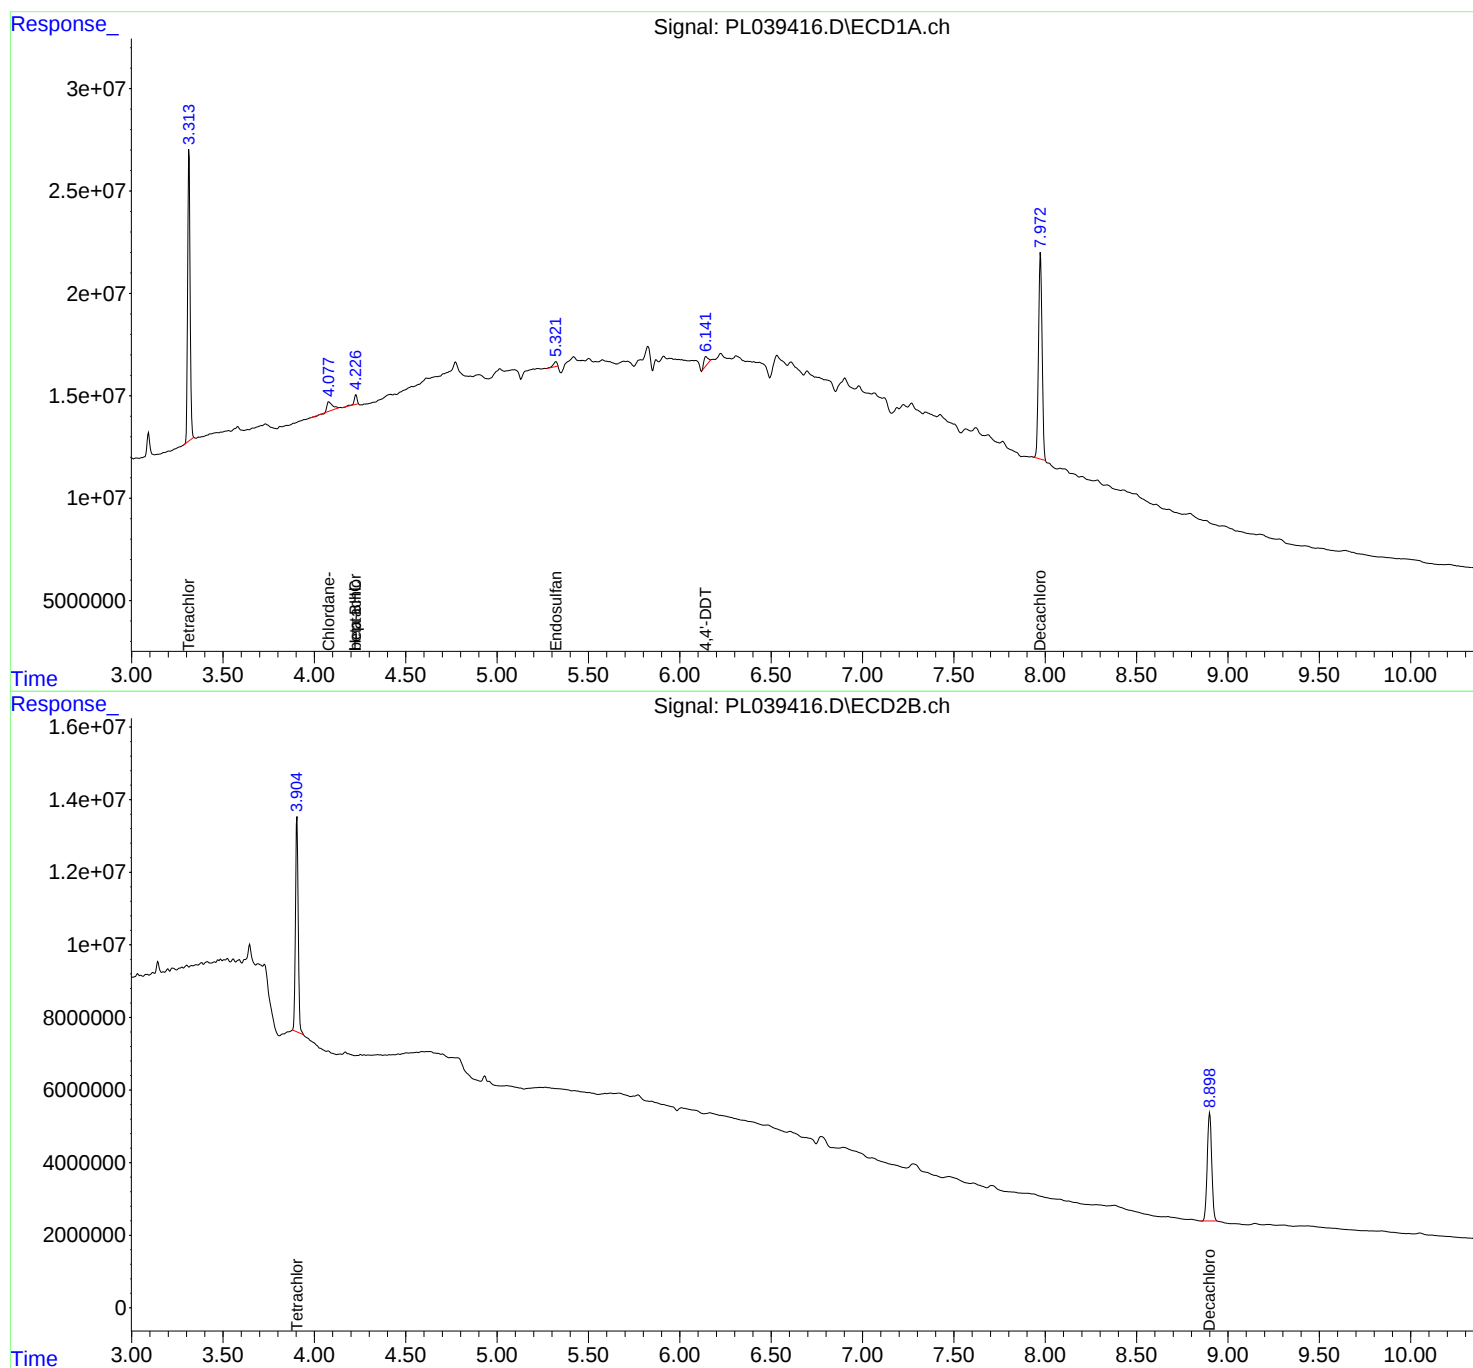


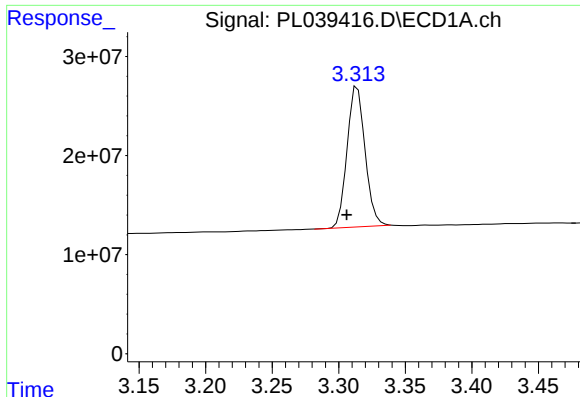

#1 Tetrachloro-m-xylene


R.T.: 3.314 min
Delta R.T.: 0.008 min
Response: 133719976
Conc: 19.13 ng/ml

Instrument :
ECD_L
ClientSampleId :

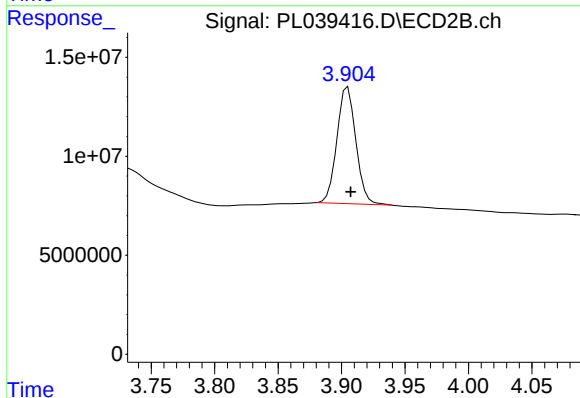


#1 Tetrachloro-m-xylene

R.T.: 3.905 min
Delta R.T.: -0.002 min
Response: 61291486
Conc: 22.86 ng/ml

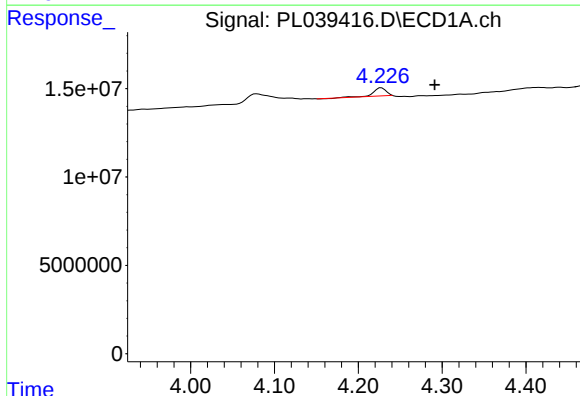


#4 Heptachlor

R.T.: 4.228 min
Delta R.T.: -0.064 min
Response: 5149100
Conc: 0.49 ng/ml

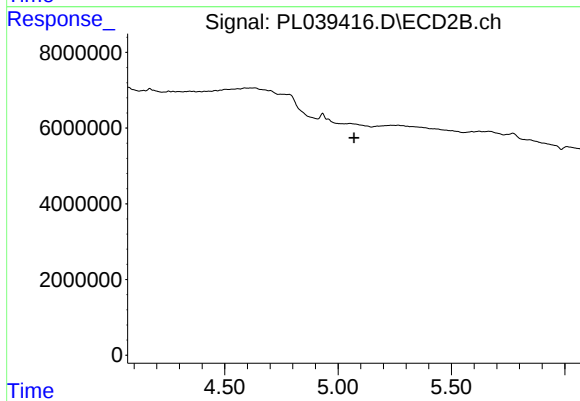

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.071 min
Response: 0
Conc: N.D.

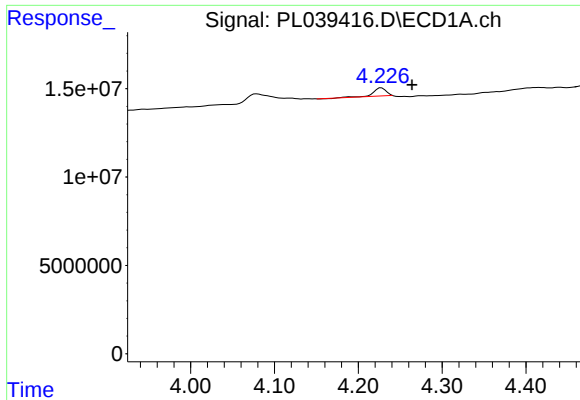

#6 beta-BHC


R.T.: 4.228 min
Delta R.T.: -0.037 min
Response: 5149100
Conc: 1.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

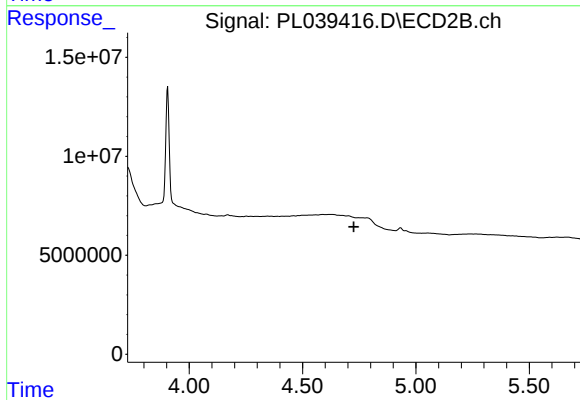


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

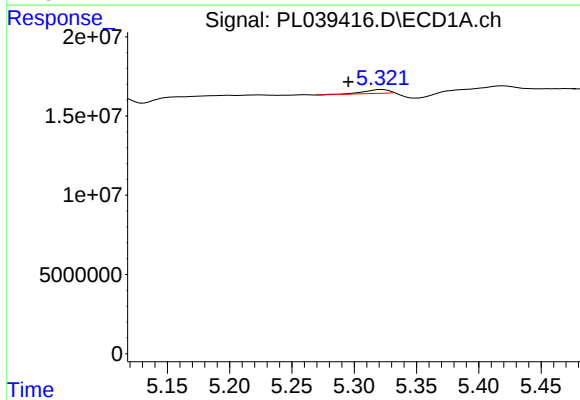


#9 Endosulfan I

R.T.: 5.322 min
Delta R.T.: 0.027 min
Response: 3493175
Conc: 0.40 ng/ml

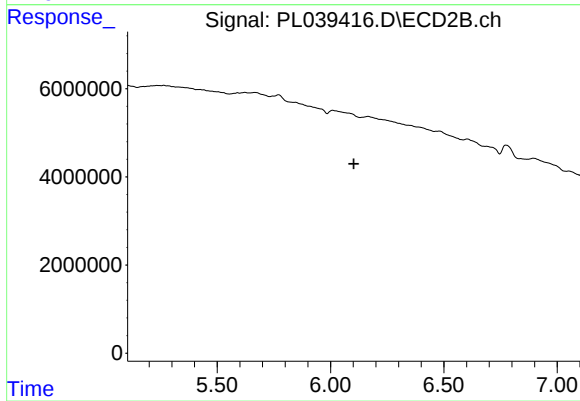

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

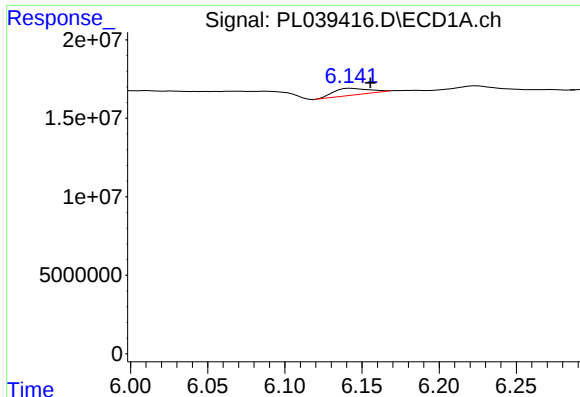

#17 4,4'-DDT


R.T.: 6.143 min
Delta R.T.: -0.012 min
Response: 6743145
Conc: 0.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

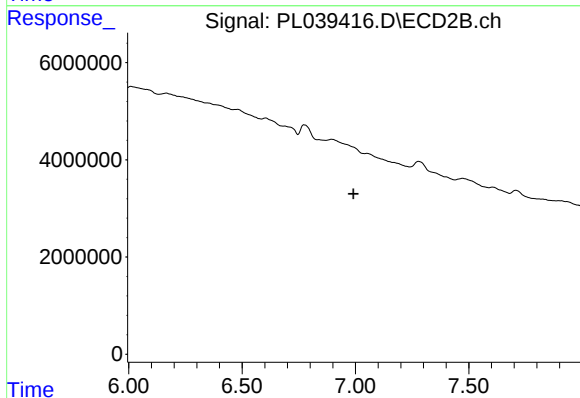


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.991 min
Response: 0
Conc: N.D.

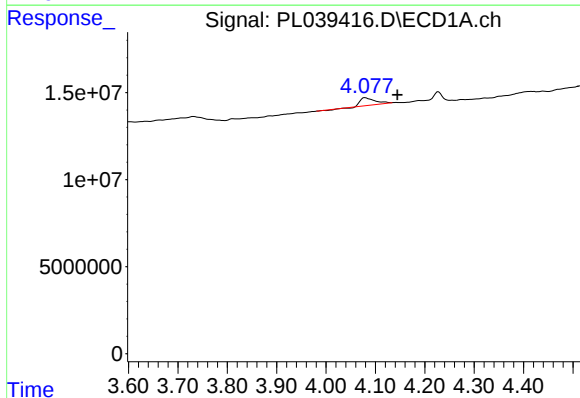


#23 Chlordane-1

R.T.: 4.079 min
Delta R.T.: -0.066 min
Response: 8492525
Conc: 26.83 ng/ml

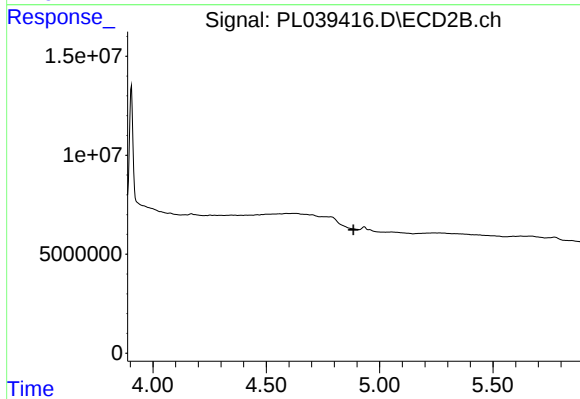

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

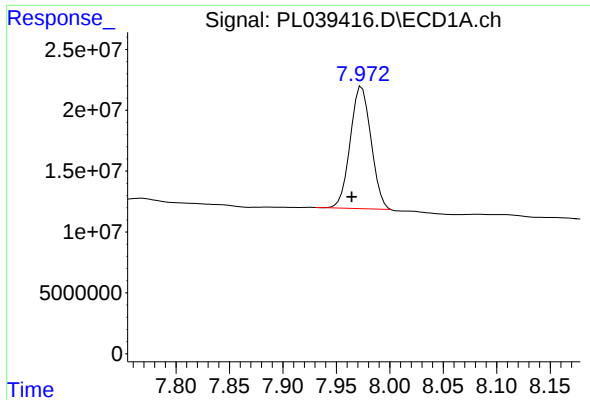

#28 Decachlorobiphenyl

R.T.: 7.974 min
Delta R.T.: 0.009 min
Response: 135760093
Conc: 19.33 ng/ml

Instrument :
ECD_L
ClientSampleId :

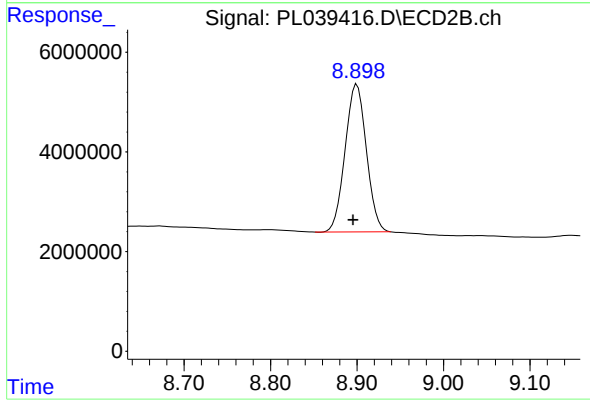

#28 Decachlorobiphenyl

R.T.: 8.900 min
Delta R.T.: 0.004 min
Response: 50498208
Conc: 21.76 ng/ml