

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082218\
 Data File : PL039422.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2018 17:47
 Operator : AJ\SJ
 Sample : J4573-07
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 01:03:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.303	3.906	108.8E6	44227404	15.557	16.497
28)	SA Decachlor...	7.961	8.896	90743077	37162952	12.920	16.014
Target Compounds							
6)	B beta-BHC	4.215f	4.751	21397122	-3599235	4.606	N.D. #
8)	B Heptachlo...	4.917f	0.000	2963847	0	0.310	N.D. #
23)	Chlordane-1	4.151	0.000	15058121	0	47.564	N.D. #
24)	Chlordane-2	4.665	0.000	18252581	0	52.211	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082218\
Data File : PL039422.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2018 17:47
Operator : AJ\SJ
Sample : J4573-07
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 01:03:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

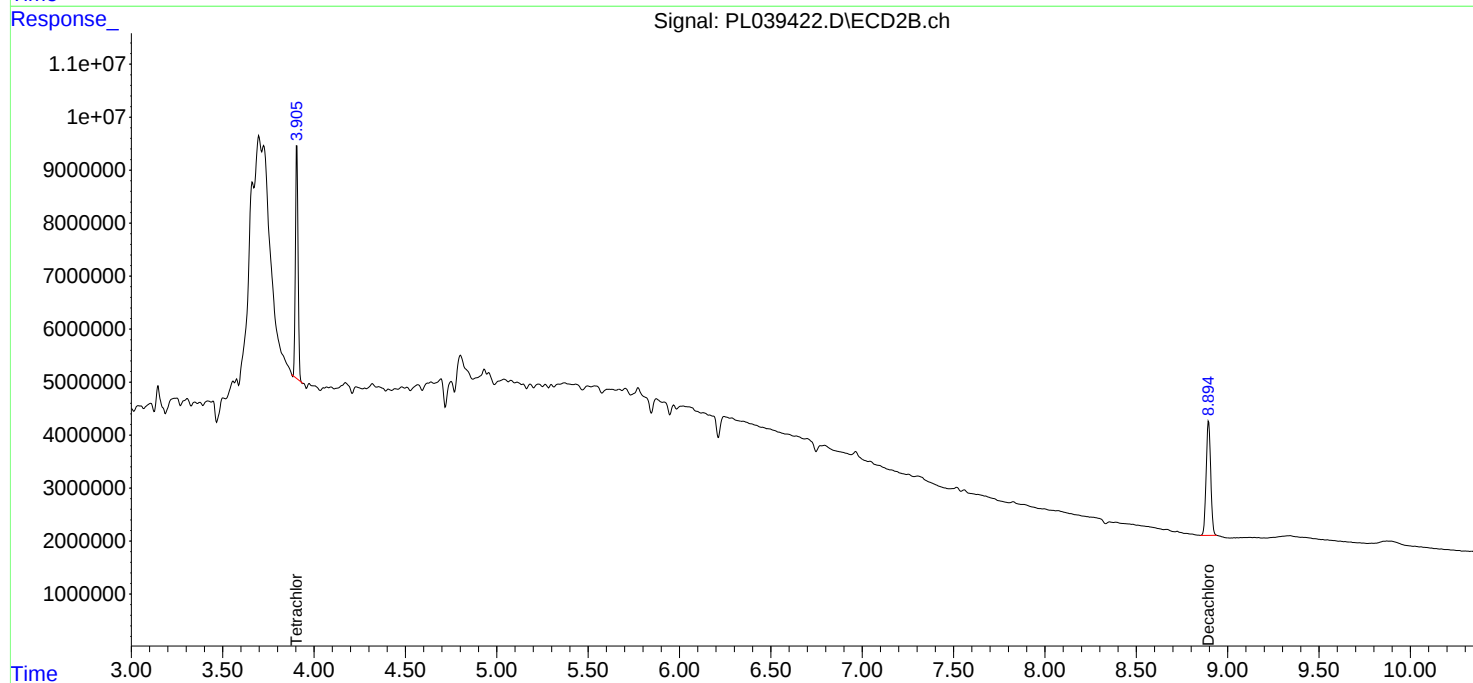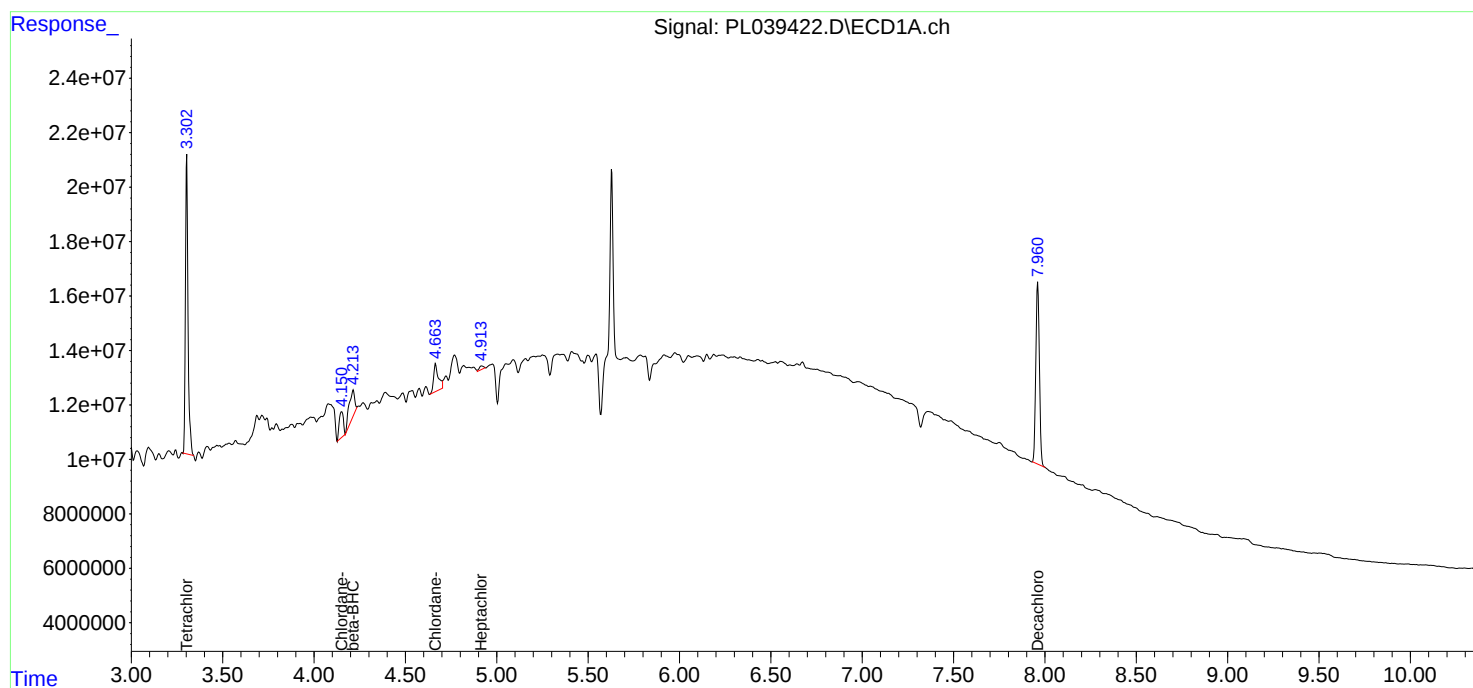


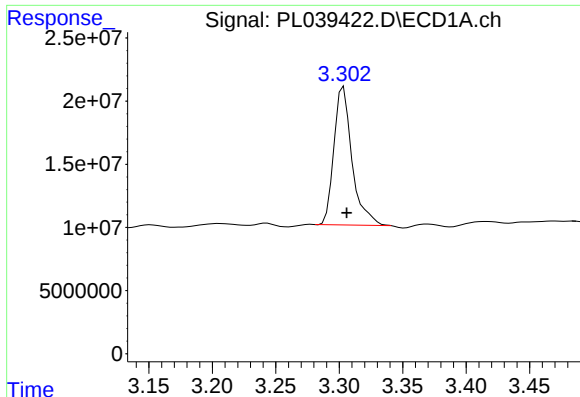

#1 Tetrachloro-m-xylene


R.T.: 3.303 min
Delta R.T.: -0.003 min
Response: 108750336
Conc: 15.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

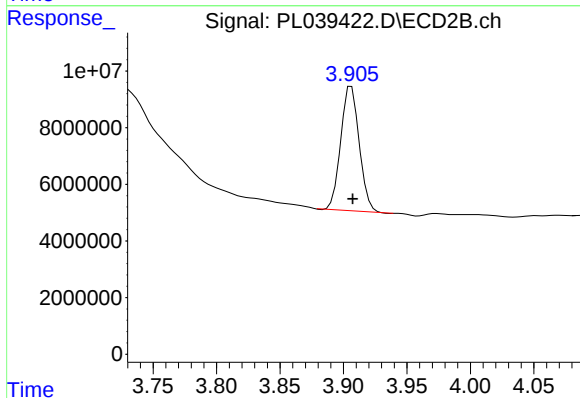


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: 0.000 min
Response: 44227404
Conc: 16.50 ng/ml

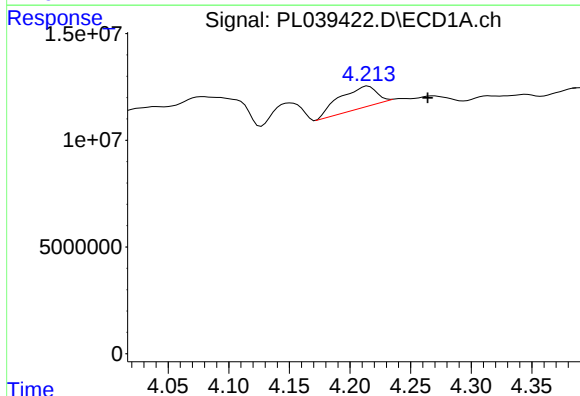


#6 beta-BHC

R.T.: 4.215 min
Delta R.T.: -0.049 min
Response: 21397122
Conc: 4.61 ng/ml

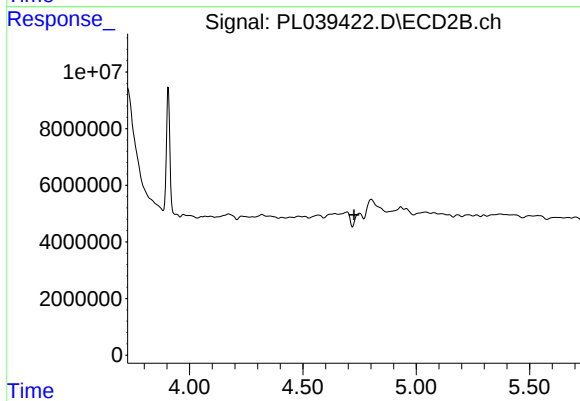

#6 beta-BHC


R.T.: 4.751 min
Delta R.T.: 0.025 min
Response: -3599235
Conc: N.D.

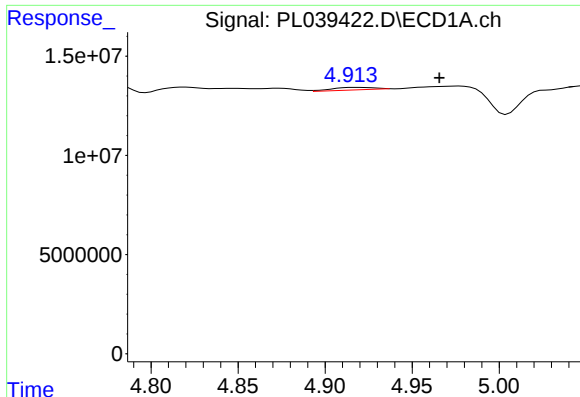

#8 Heptachlor epoxide


R.T.: 4.917 min
Delta R.T.: -0.049 min
Response: 2963847
Conc: 0.31 ng/ml

Instrument :
ECD_L
ClientSampleId :

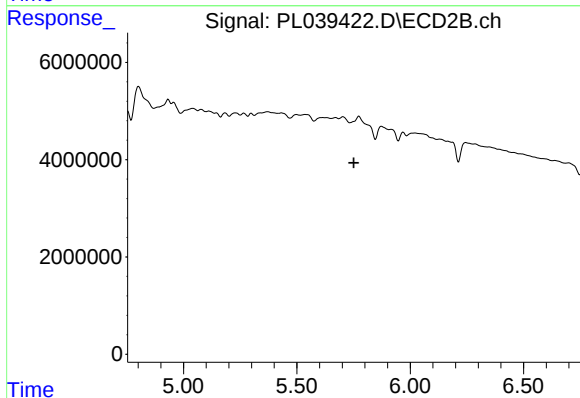


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.751 min
Response: 0
Conc: N.D.

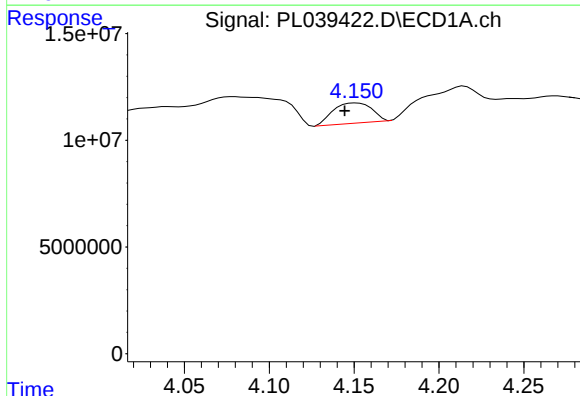


#23 Chlordane-1

R.T.: 4.151 min
Delta R.T.: 0.007 min
Response: 15058121
Conc: 47.56 ng/ml

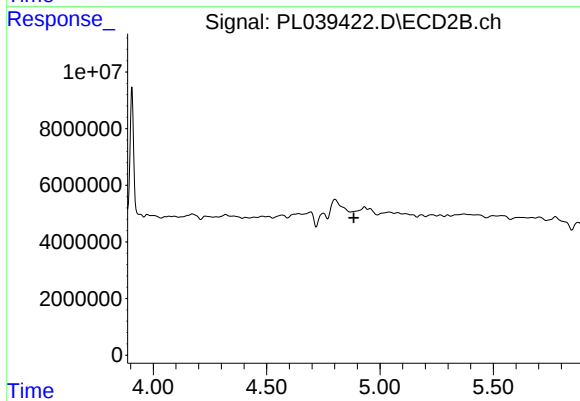

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

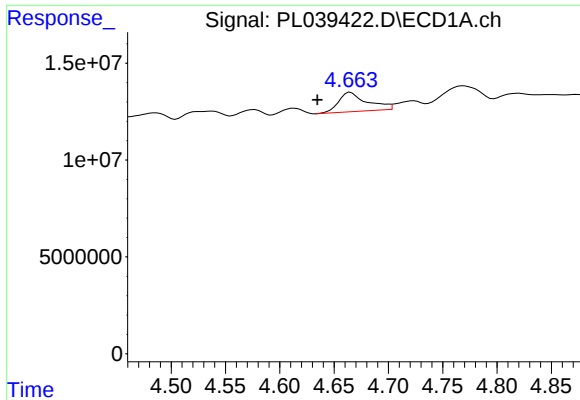

#24 Chlordane-2


R.T.: 4.665 min
Delta R.T.: 0.030 min
Response: 18252581
Conc: 52.21 ng/ml

Instrument :
ECD_L
ClientSampleId :

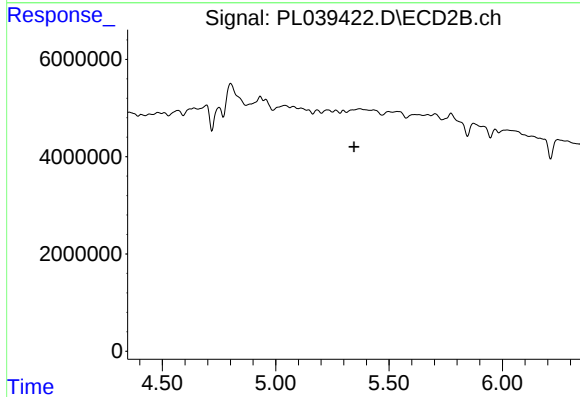


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.346 min
Response: 0
Conc: N.D.

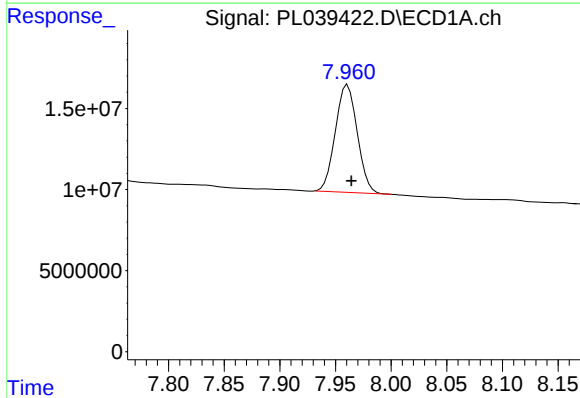

#28 Decachlorobiphenyl

R.T.: 7.961 min
Delta R.T.: -0.003 min
Response: 90743077
Conc: 12.92 ng/ml

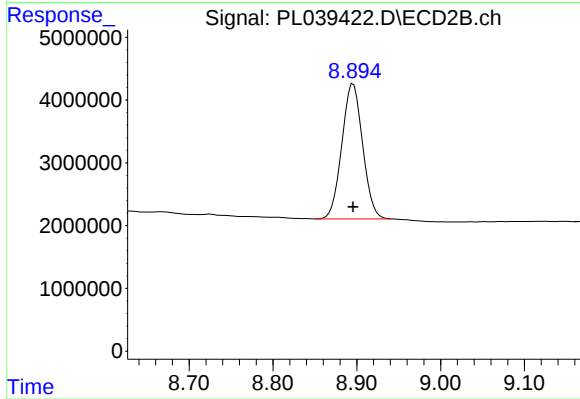

#28 Decachlorobiphenyl

R.T.: 8.896 min
Delta R.T.: 0.000 min
Response: 37162952
Conc: 16.01 ng/ml