

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082218\
 Data File : PL039429.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2018 19:26
 Operator : AJ\SJ
 Sample : J4583-06
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 01:05:16 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.305	3.907	188.0E6	82274178	26.900	30.689
28)	SA Decachlor...	7.962	8.897	148.3E6	58810800	21.119	25.343
Target Compounds							
2)	A alpha-BHC	3.687f	0.000	494898	0	0.042	N.D. #
3)	MA gamma-BHC...	4.057f	0.000	157.7E6	0	14.869	N.D. #
6)	B beta-BHC	4.217f	0.000	10033723	0	2.160	N.D. #
7)	B delta-BHC	0.000	4.958	0	17131139	N.D.	4.303 #
8)	B Heptachlo...	4.914f	5.776	3041571	9763826	0.319	2.903 #
15)	B Endosulfa...	0.000	6.799	0	9421991	N.D.	3.668 #
19)	B Endosulfa...	6.468	0.000	10021700	0	1.232	N.D. #
23)	Chlordane-1	4.157	0.000	13687706	0	43.235	N.D. #
27)	Chlordane-5	0.000	6.799	0	9421991	N.D.	101.855 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082218\
Data File : PL039429.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2018 19:26
Operator : AJ\SJ
Sample : J4583-06
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 01:05:16 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

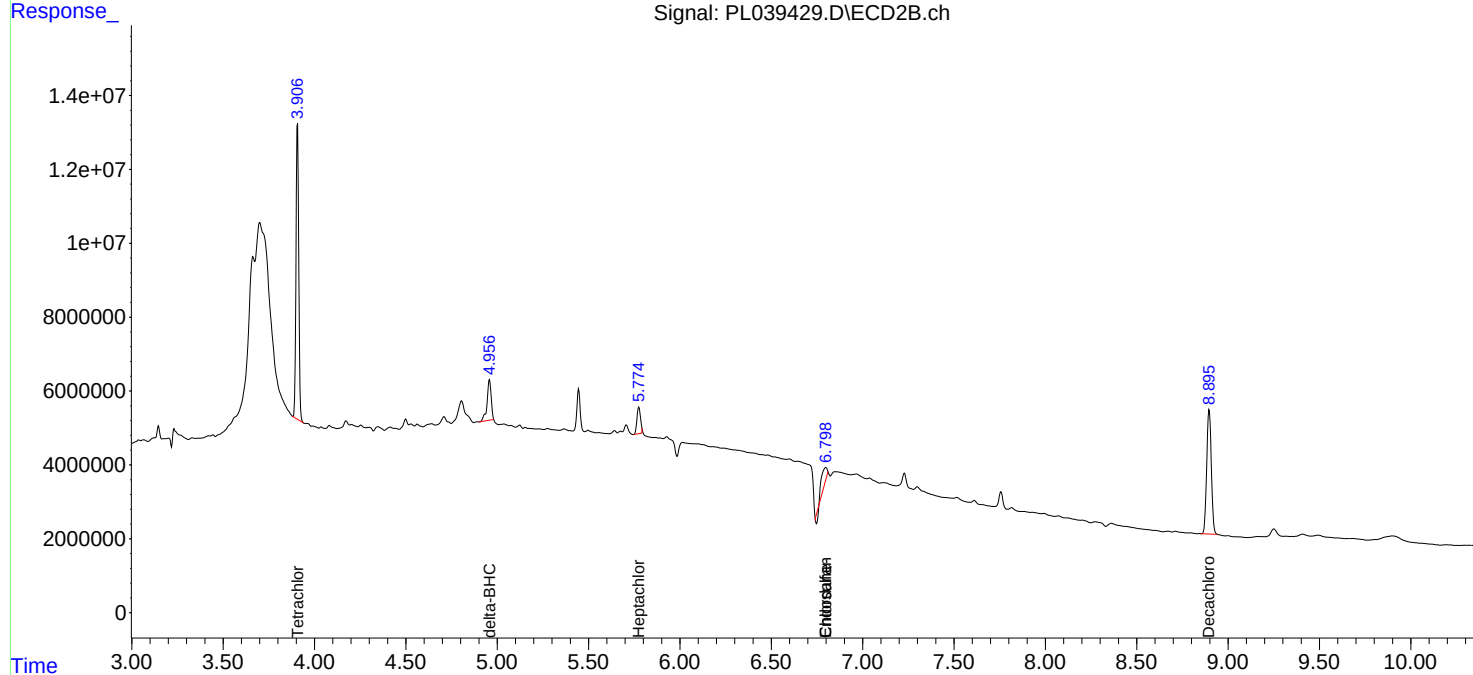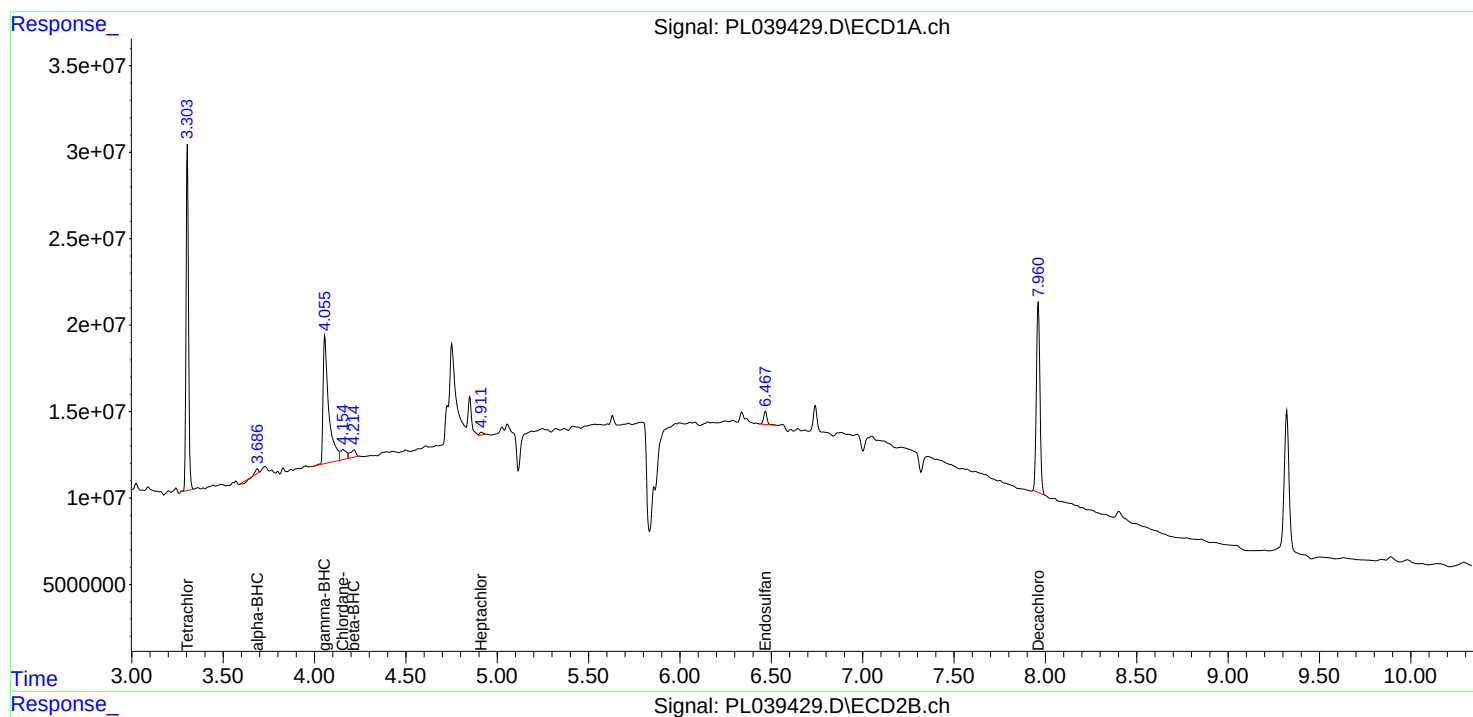


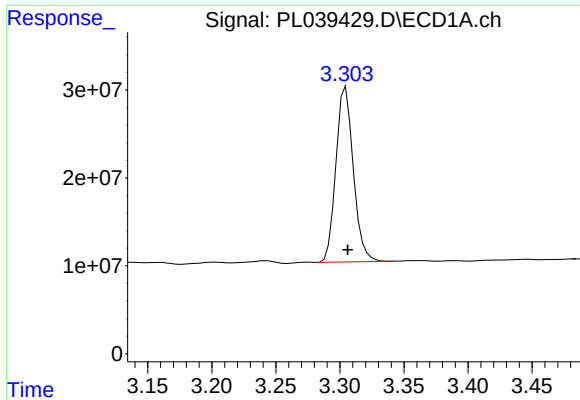

#1 Tetrachloro-m-xylene


R.T.: 3.305 min
Delta R.T.: -0.001 min
Response: 188044008
Conc: 26.90 ng/ml

Instrument :
ECD_L
ClientSampleId :

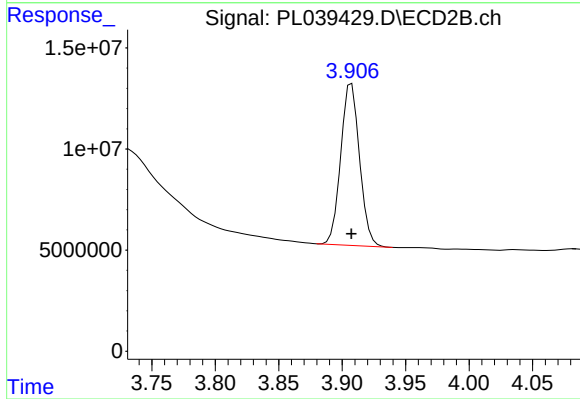


#1 Tetrachloro-m-xylene

R.T.: 3.907 min
Delta R.T.: 0.000 min
Response: 82274178
Conc: 30.69 ng/ml

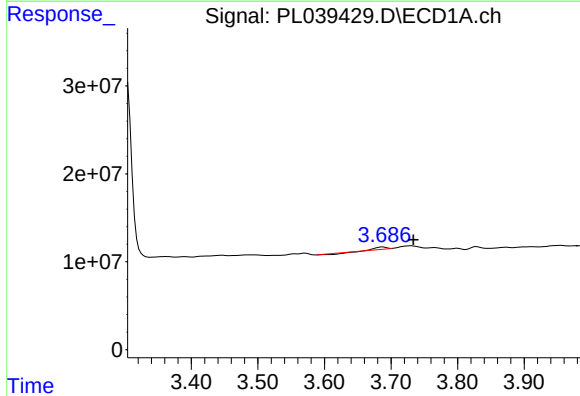


#2 alpha-BHC

R.T.: 3.687 min
Delta R.T.: -0.046 min
Response: 494898
Conc: 0.04 ng/ml

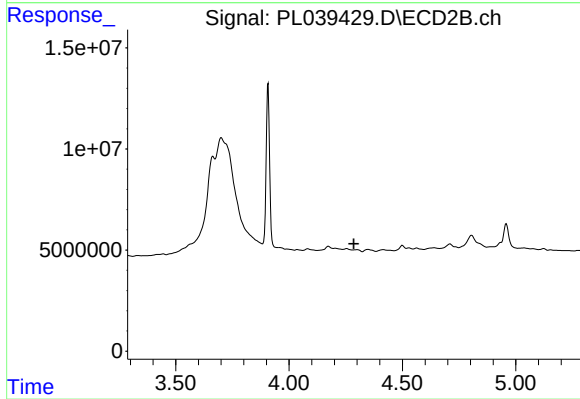

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T. : 4.285 min
Response: 0
Conc: N.D.

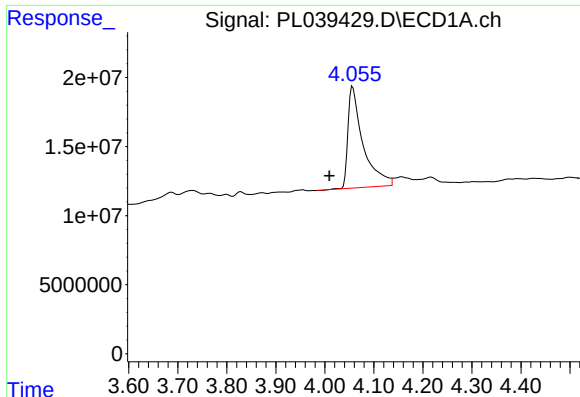

#3 gamma-BHC (Lindane)


R.T.: 4.057 min
Delta R.T.: 0.047 min
Response: 157713213
Conc: 14.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

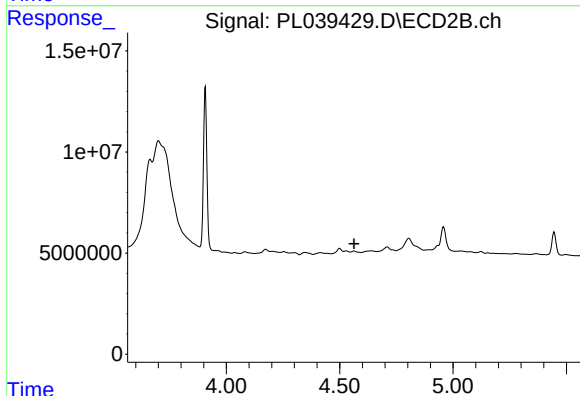


#3 gamma-BHC (Lindane)

R.T.: 0.000 min
Exp R.T. : 4.563 min
Response: 0
Conc: N.D.

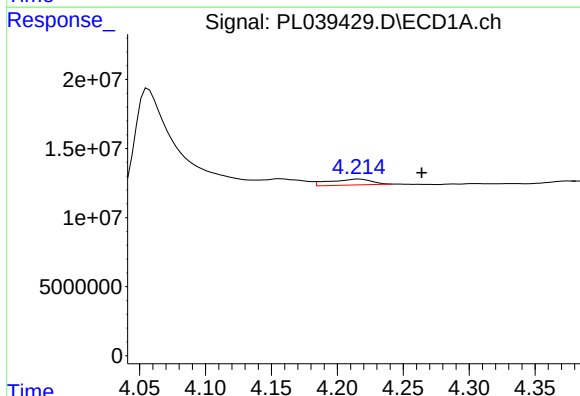


#6 beta-BHC

R.T.: 4.217 min
Delta R.T.: -0.047 min
Response: 10033723
Conc: 2.16 ng/ml

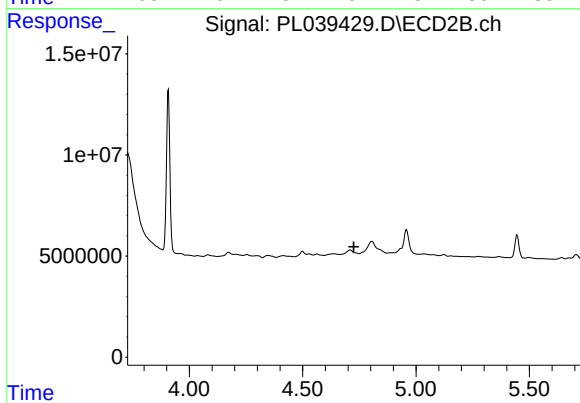

#6 beta-BHC


R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

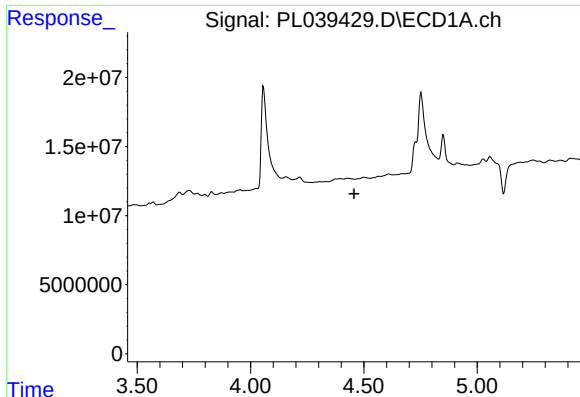

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.457 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

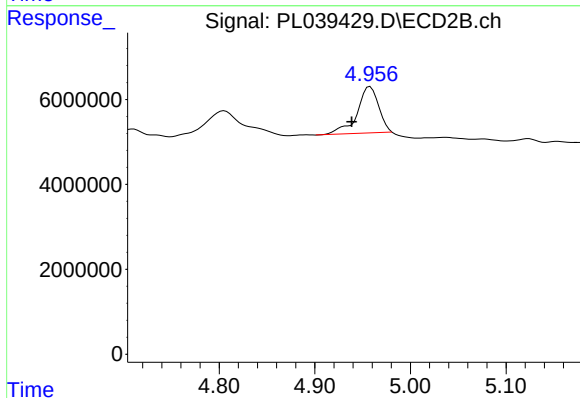


#7 delta-BHC

R.T.: 4.958 min
Delta R.T.: 0.019 min
Response: 17131139
Conc: 4.30 ng/ml

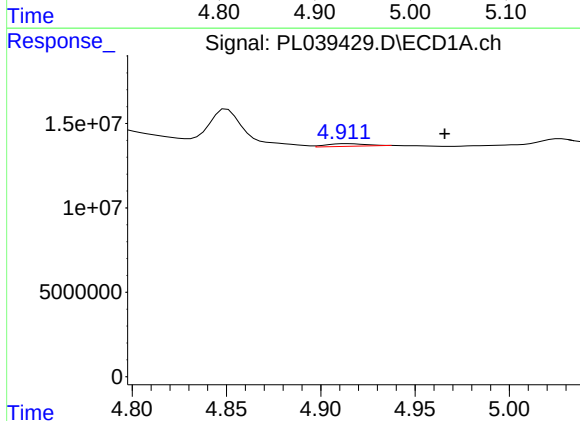


#8 Heptachlor epoxide

R.T.: 4.914 min
Delta R.T.: -0.052 min
Response: 3041571
Conc: 0.32 ng/ml

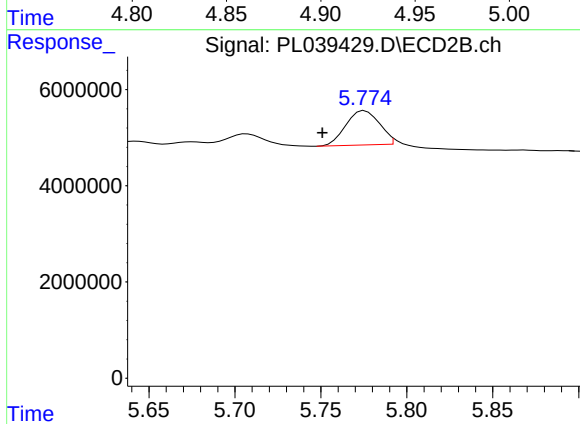

#8 Heptachlor epoxide


R.T.: 5.776 min
Delta R.T.: 0.025 min
Response: 9763826
Conc: 2.90 ng/ml

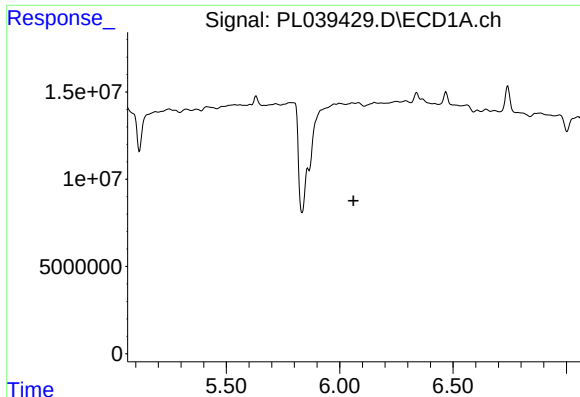

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 6.061 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

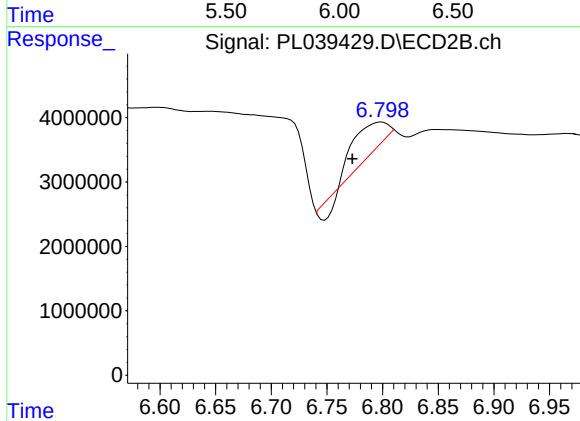


#15 Endosulfan II

R.T.: 6.799 min
Delta R.T.: 0.026 min
Response: 9421991
Conc: 3.67 ng/ml

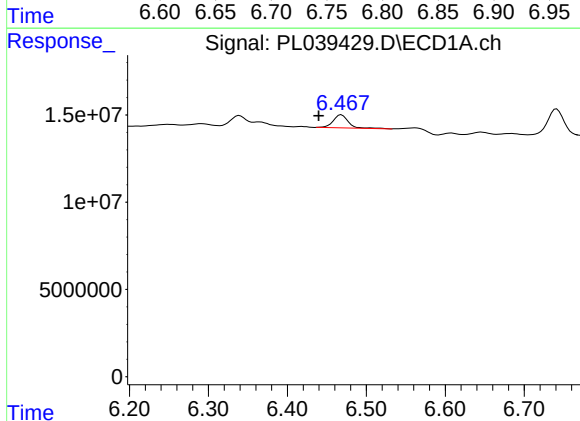


#19 Endosulfan Sulfate

R.T.: 6.468 min
Delta R.T.: 0.029 min
Response: 10021700
Conc: 1.23 ng/ml

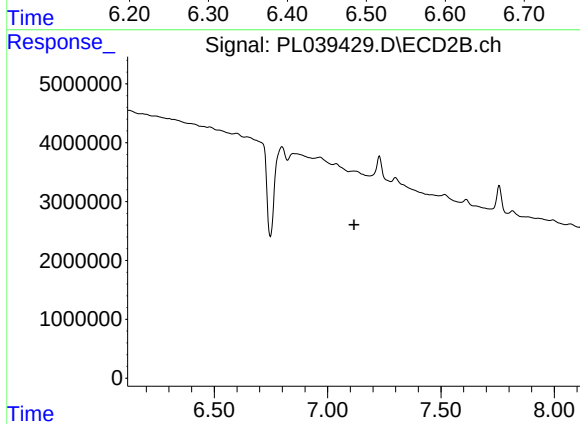

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.117 min
Response: 0
Conc: N.D.

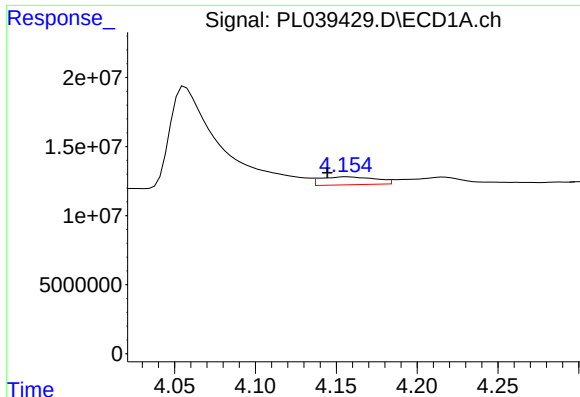

#23 Chlordane-1


R.T.: 4.157 min
Delta R.T.: 0.013 min
Response: 13687706
Conc: 43.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

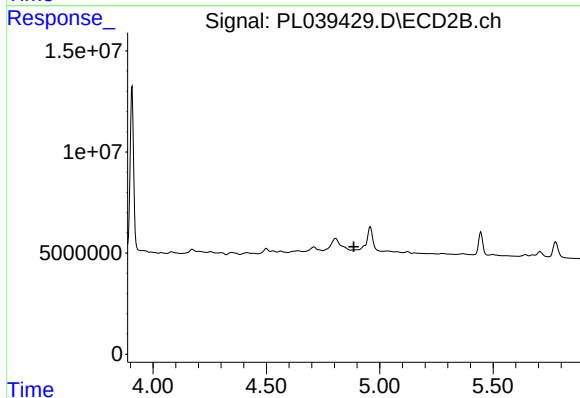


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

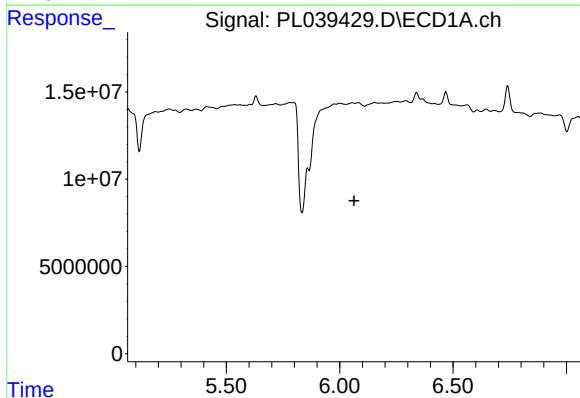


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.064 min
Response: 0
Conc: N.D.

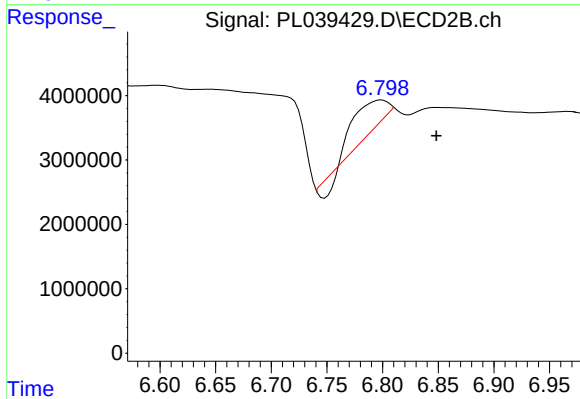

#27 Chlordane-5


R.T.: 6.799 min
Delta R.T.: -0.049 min
Response: 9421991
Conc: 101.86 ng/ml

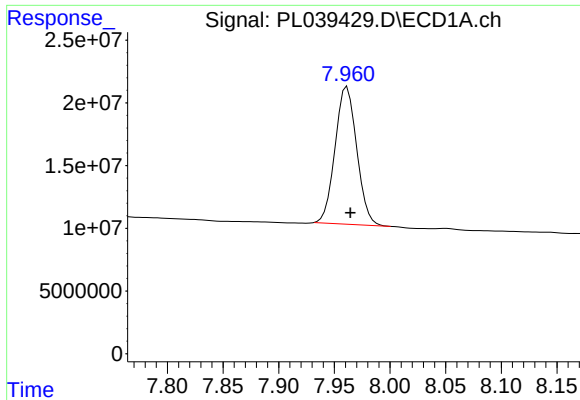

#28 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: -0.003 min
Response: 148327580
Conc: 21.12 ng/ml

Instrument :
ECD_L
ClientSampleId :

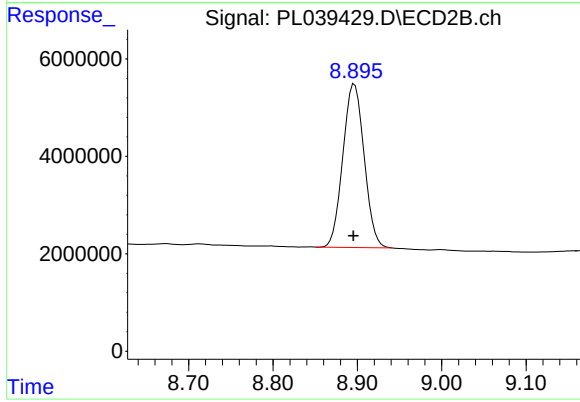

#28 Decachlorobiphenyl

R.T.: 8.897 min
Delta R.T.: 0.001 min
Response: 58810800
Conc: 25.34 ng/ml