

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082218\
 Data File : PL039443.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2018 22:45
 Operator : AJ\SJ
 Sample : J4585-02
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 01:09:12 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.907	123.1E6	53882894	17.614	20.099
28)	SA Decachlor...	7.961	8.897	116.6E6	46606115	16.603	20.084
Target Compounds							
3)	MA gamma-BHC...	4.045f	0.000	17994762	0	1.697	N.D. #
6)	B beta-BHC	4.219f	0.000	35093359	0	7.554	N.D. #
7)	B delta-BHC	0.000	4.932	0	18217595	N.D.	4.575 #
9)	A Endosulfan I	5.326	0.000	11122398	0	1.270	N.D. #
15)	B Endosulfa...	6.057	0.000	13330402	0	1.533	N.D. #
19)	B Endosulfa...	6.456	0.000	42626962	0	5.239	N.D. #
20)	A Methoxychlor	6.637f	0.000	64425899	0	15.744	N.D. #
21)	B Endrin ke...	6.981f	0.000	8786820	0	1.021	N.D. #
23)	Chlordane-1	4.077	4.932	12858710	18217595	40.617	145.817 #
27)	Chlordane-5	6.057	0.000	13330402	0	41.101	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082218\
Data File : PL039443.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2018 22:45
Operator : AJ\SJ
Sample : J4585-02
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 01:09:12 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

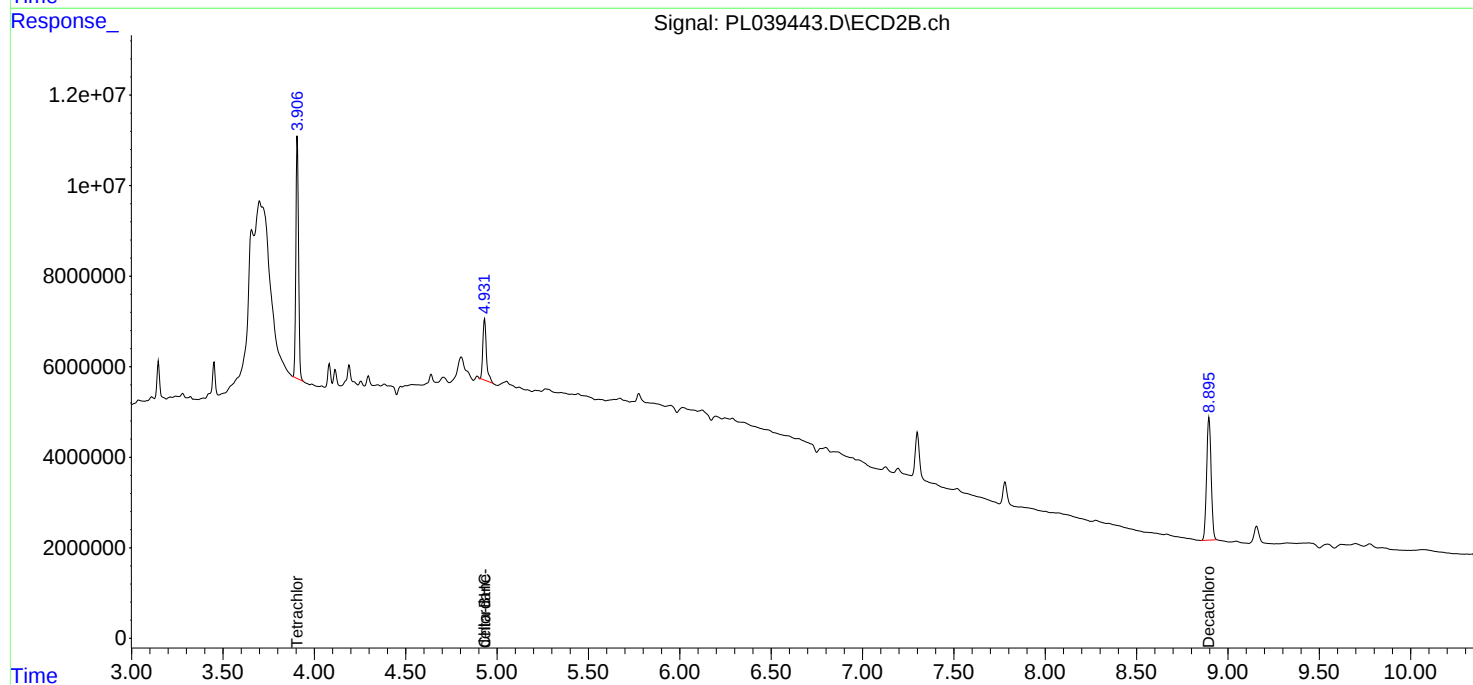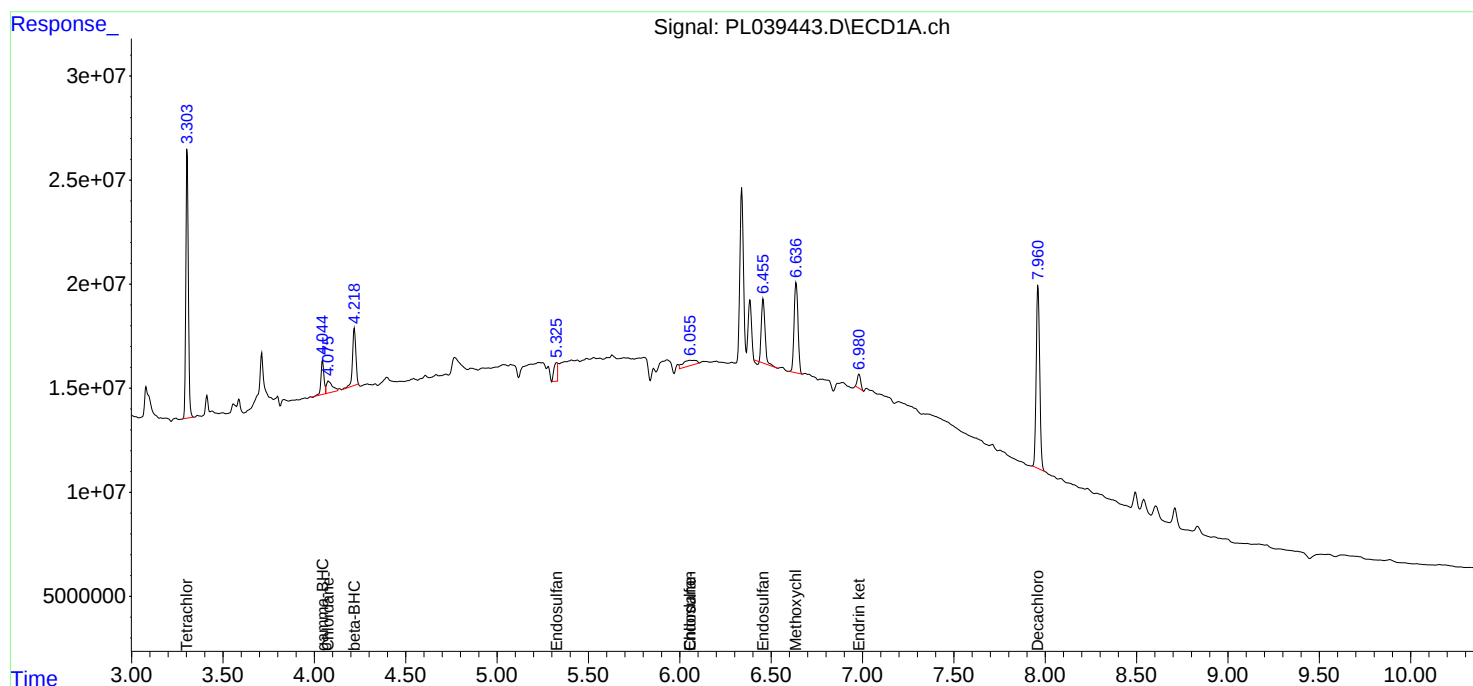


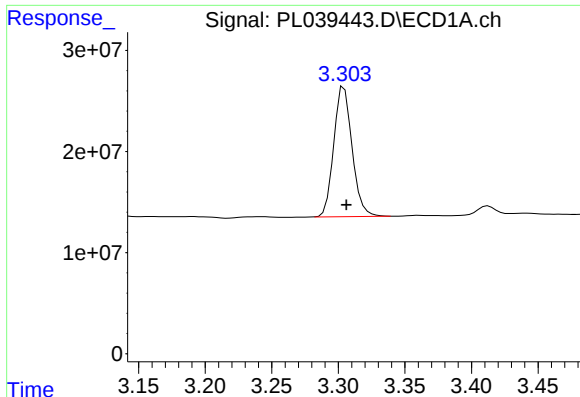

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: -0.002 min
Response: 123130442
Conc: 17.61 ng/ml

Instrument :
ECD_L
ClientSampleId :

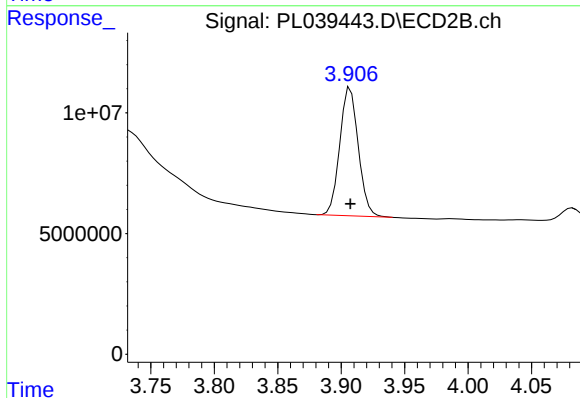


#1 Tetrachloro-m-xylene

R.T.: 3.907 min
Delta R.T.: 0.000 min
Response: 53882894
Conc: 20.10 ng/ml

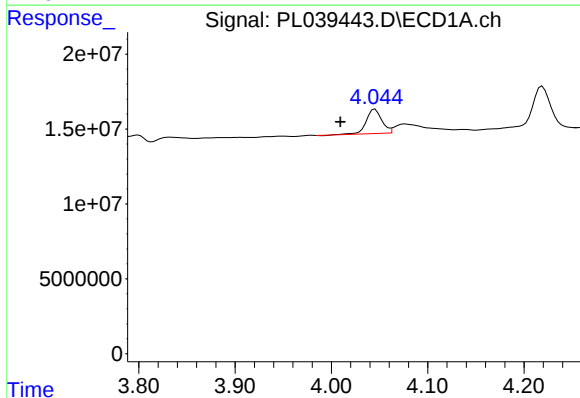


#3 gamma-BHC (Lindane)

R.T.: 4.045 min
Delta R.T.: 0.036 min
Response: 17994762
Conc: 1.70 ng/ml

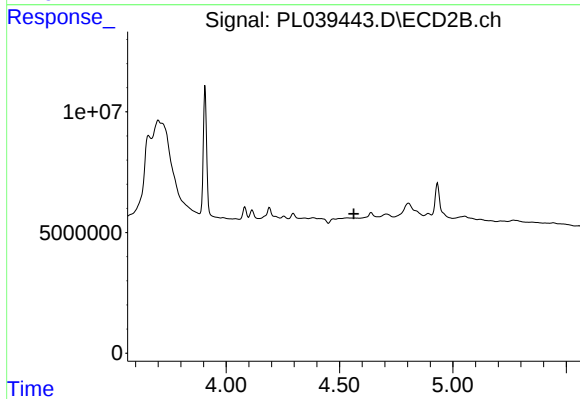

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.563 min
Response: 0
Conc: N.D.

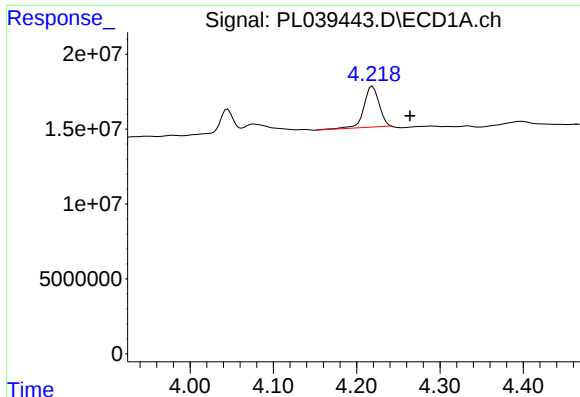

#6 beta-BHC


R.T.: 4.219 min
Delta R.T.: -0.045 min
Response: 35093359
Conc: 7.55 ng/ml

Instrument :
ECD_L
ClientSampleId :

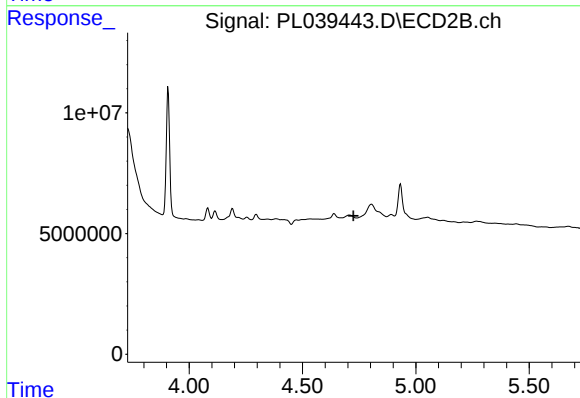


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

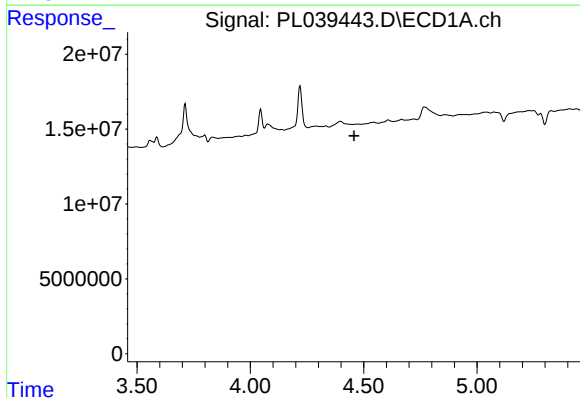


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.457 min
Response: 0
Conc: N.D.

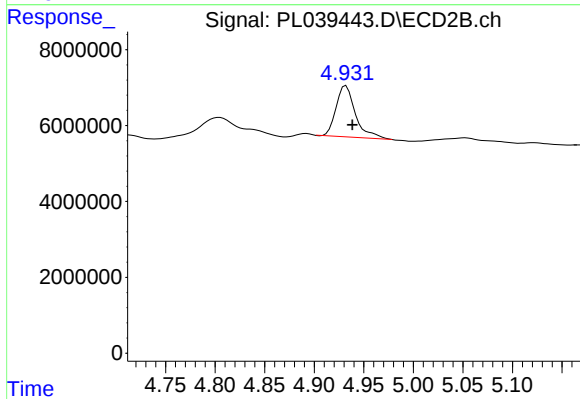

#7 delta-BHC


R.T.: 4.932 min
Delta R.T.: -0.007 min
Response: 18217595
Conc: 4.58 ng/ml

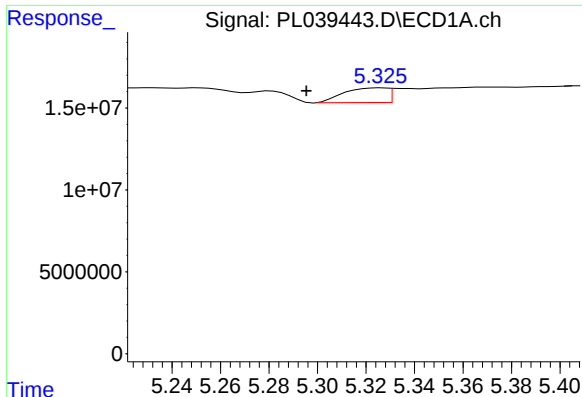

#9 Endosulfan I


R.T.: 5.326 min
Delta R.T.: 0.031 min
Response: 11122398
Conc: 1.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

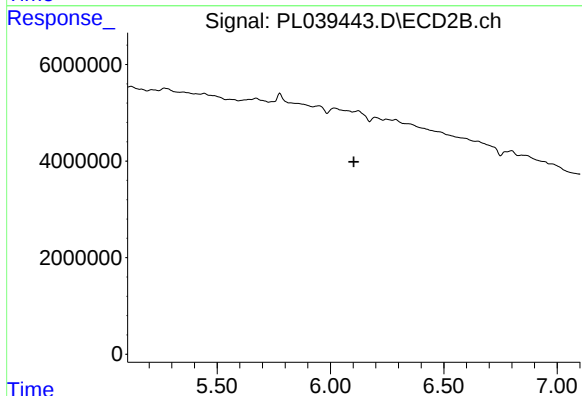


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

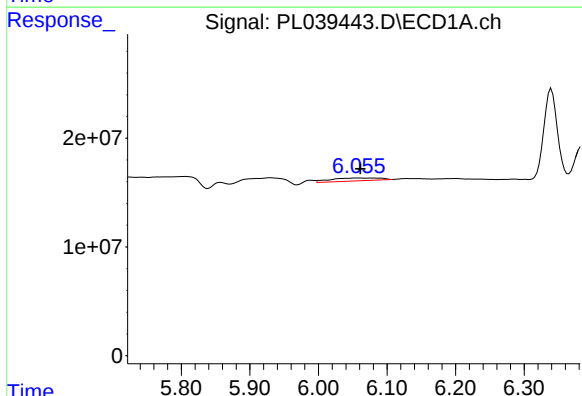


#15 Endosulfan II

R.T.: 6.057 min
Delta R.T.: -0.005 min
Response: 13330402
Conc: 1.53 ng/ml

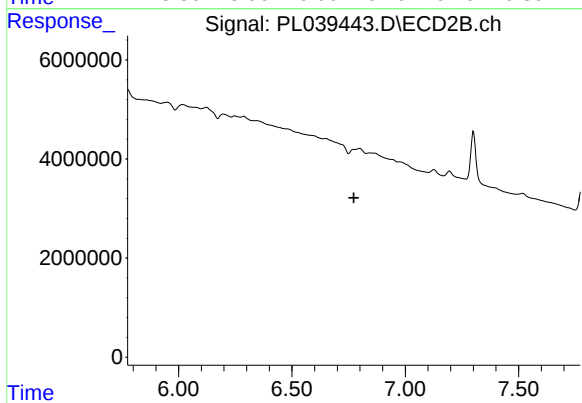

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.773 min
Response: 0
Conc: N.D.

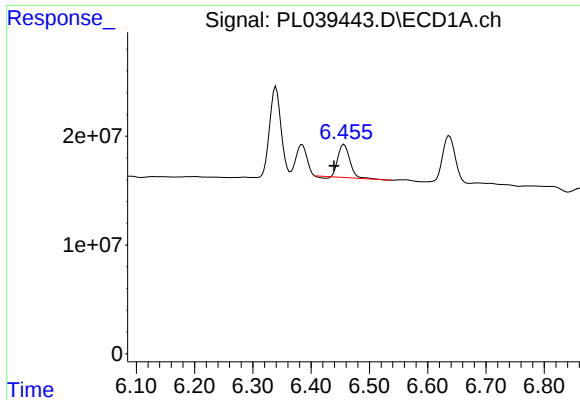

#19 Endosulfan Sulfate


R.T.: 6.456 min
Delta R.T.: 0.017 min
Response: 42626962
Conc: 5.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

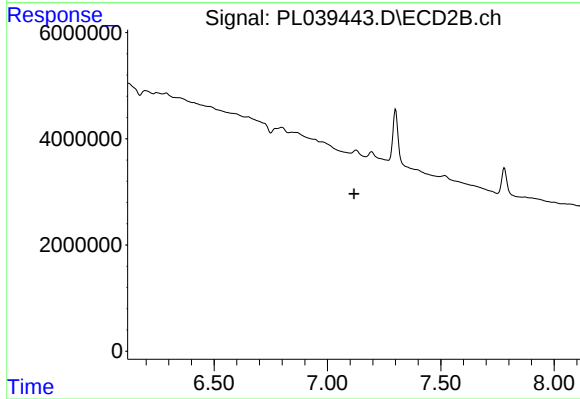


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

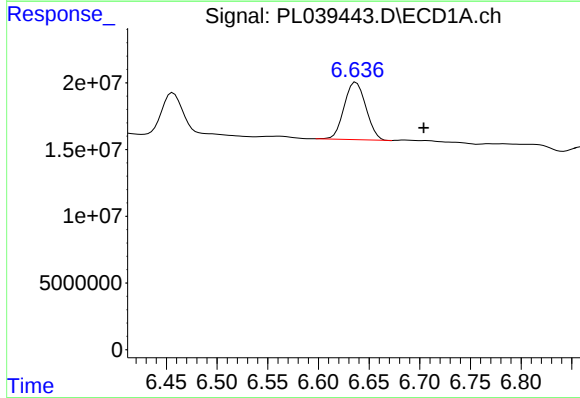


#20 Methoxychlor

R.T.: 6.637 min
Delta R.T.: -0.067 min
Response: 64425899
Conc: 15.74 ng/ml

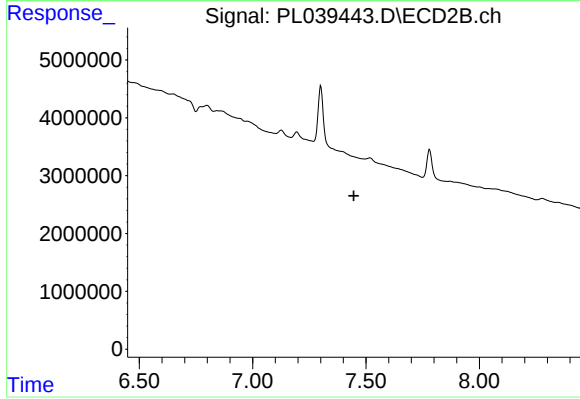

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

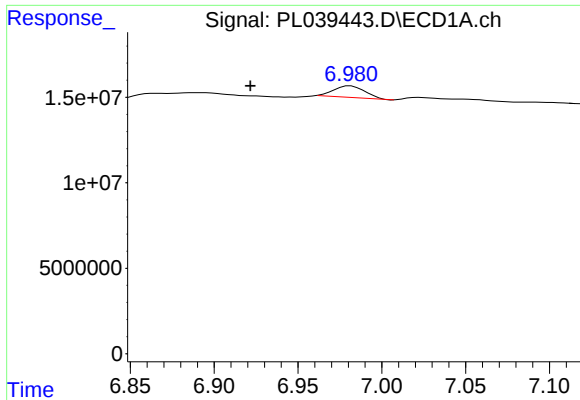

#21 Endrin ketone


R.T.: 6.981 min
Delta R.T.: 0.060 min
Response: 8786820
Conc: 1.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

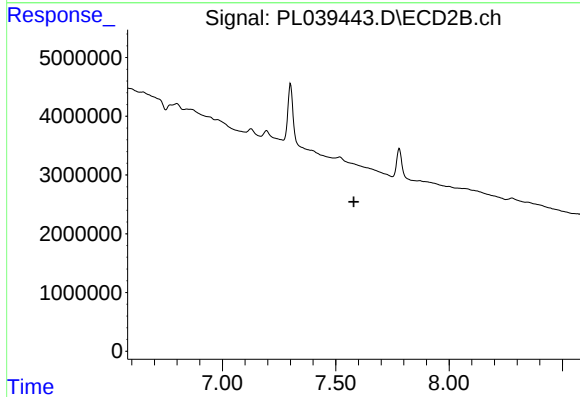


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.580 min
Response: 0
Conc: N.D.

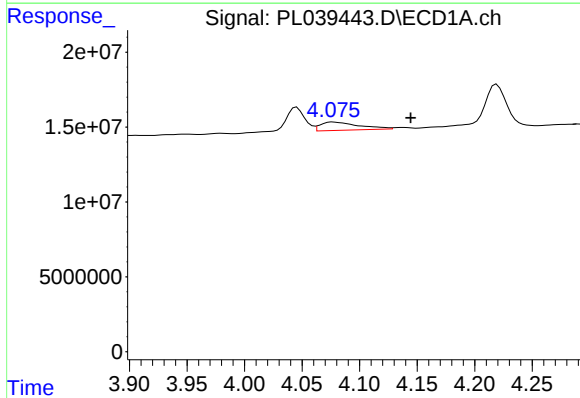


#23 Chlordane-1

R.T.: 4.077 min
Delta R.T.: -0.067 min
Response: 12858710
Conc: 40.62 ng/ml

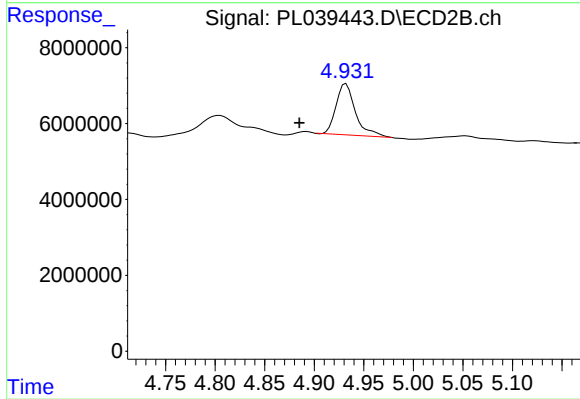

#23 Chlordane-1


R.T.: 4.932 min
Delta R.T.: 0.047 min
Response: 18217595
Conc: 145.82 ng/ml

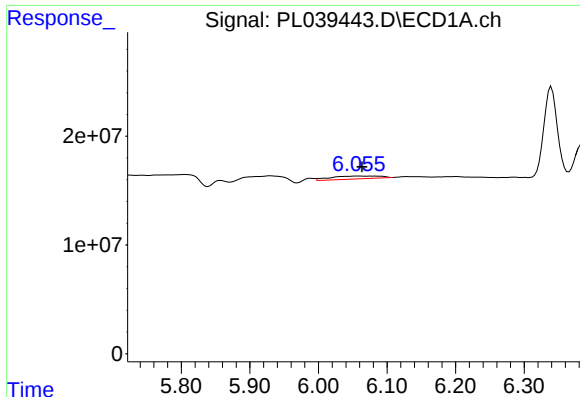

#27 Chlordane-5


R.T.: 6.057 min
Delta R.T.: -0.007 min
Response: 13330402
Conc: 41.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

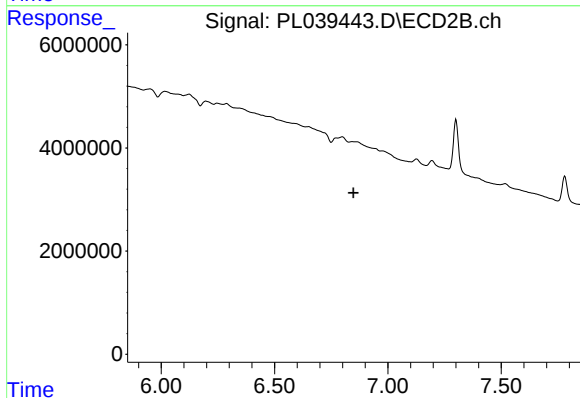


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 6.848 min
Response: 0
Conc: N.D.

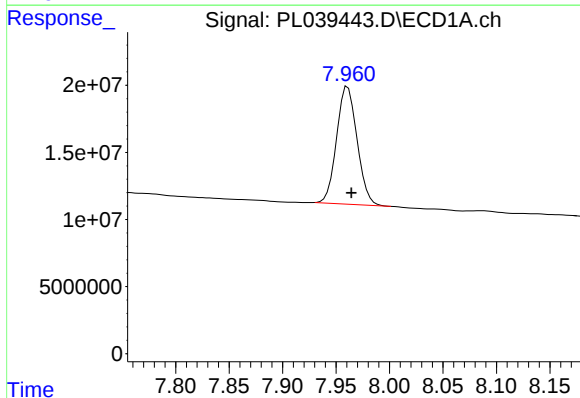

#28 Decachlorobiphenyl

R.T.: 7.961 min
Delta R.T.: -0.003 min
Response: 116610708
Conc: 16.60 ng/ml

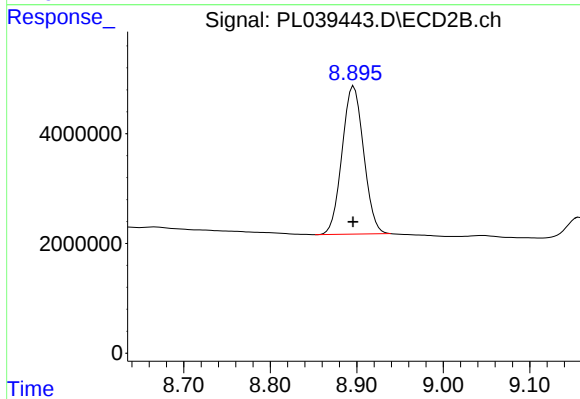

#28 Decachlorobiphenyl

R.T.: 8.897 min
Delta R.T.: 0.001 min
Response: 46606115
Conc: 20.08 ng/ml