

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082218\
 Data File : PL039447.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 22 Aug 2018 23:41
 Operator : AJ\SJ
 Sample : J4283-06
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 01:10:13 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.907	120.4E6	52138723	17.223	19.448
28)	SA Decachlor...	7.962	8.896	117.4E6	45445540	16.716	19.583
Target Compounds							
3)	MA gamma-BHC...	4.046f	0.000	12519094	0	1.180	N.D. #
6)	B beta-BHC	4.219f	0.000	21104167	0	4.543	N.D. #
7)	B delta-BHC	0.000	4.932	0	10569403	N.D.	2.655 #
9)	A Endosulfan I	5.325	0.000	9184474	0	1.049	N.D. #
19)	B Endosulfa...	6.456	0.000	28309279	0	3.479	N.D. #
20)	A Methoxychlor	6.637f	0.000	42780526	0	10.454	N.D. #
23)	Chlordane-1	4.157	4.932	5372425	10569403	16.970	84.599 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082218\
Data File : PL039447.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 22 Aug 2018 23:41
Operator : AJ\SJ
Sample : J4283-06
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 01:10:13 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

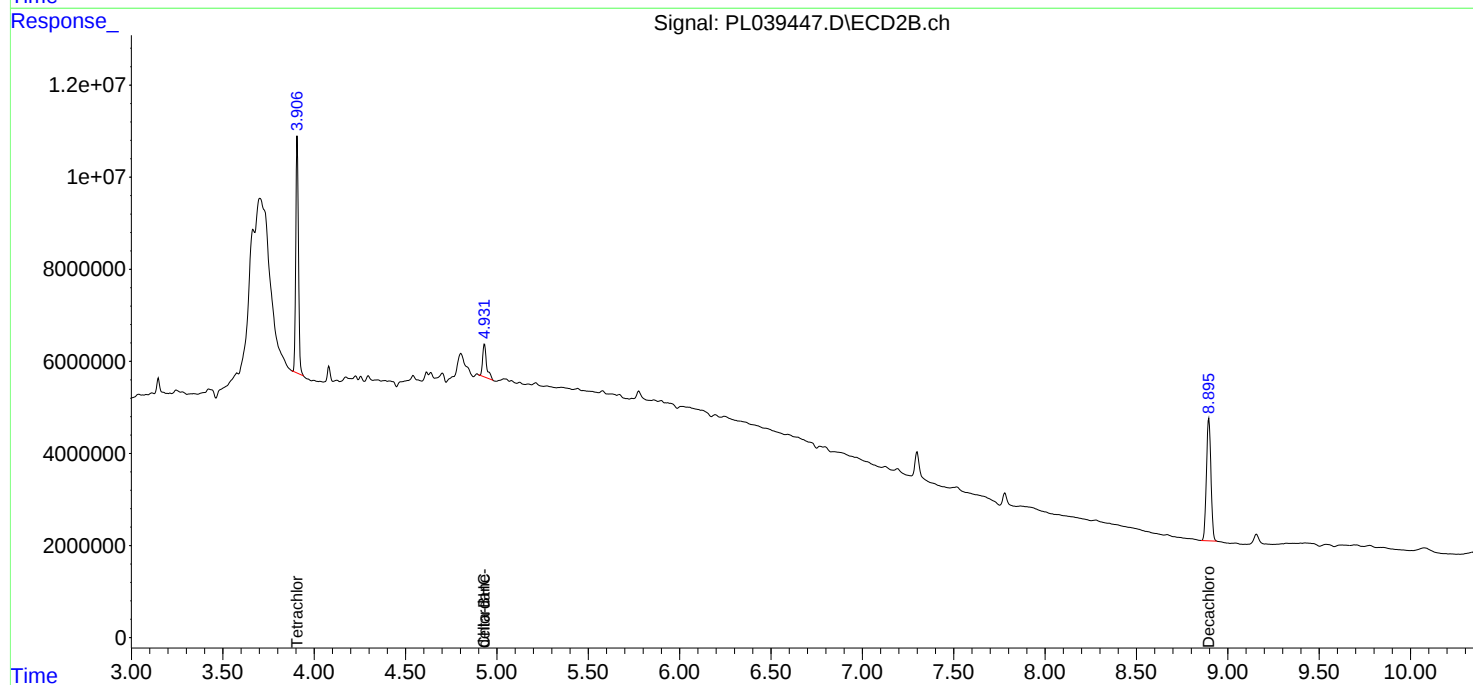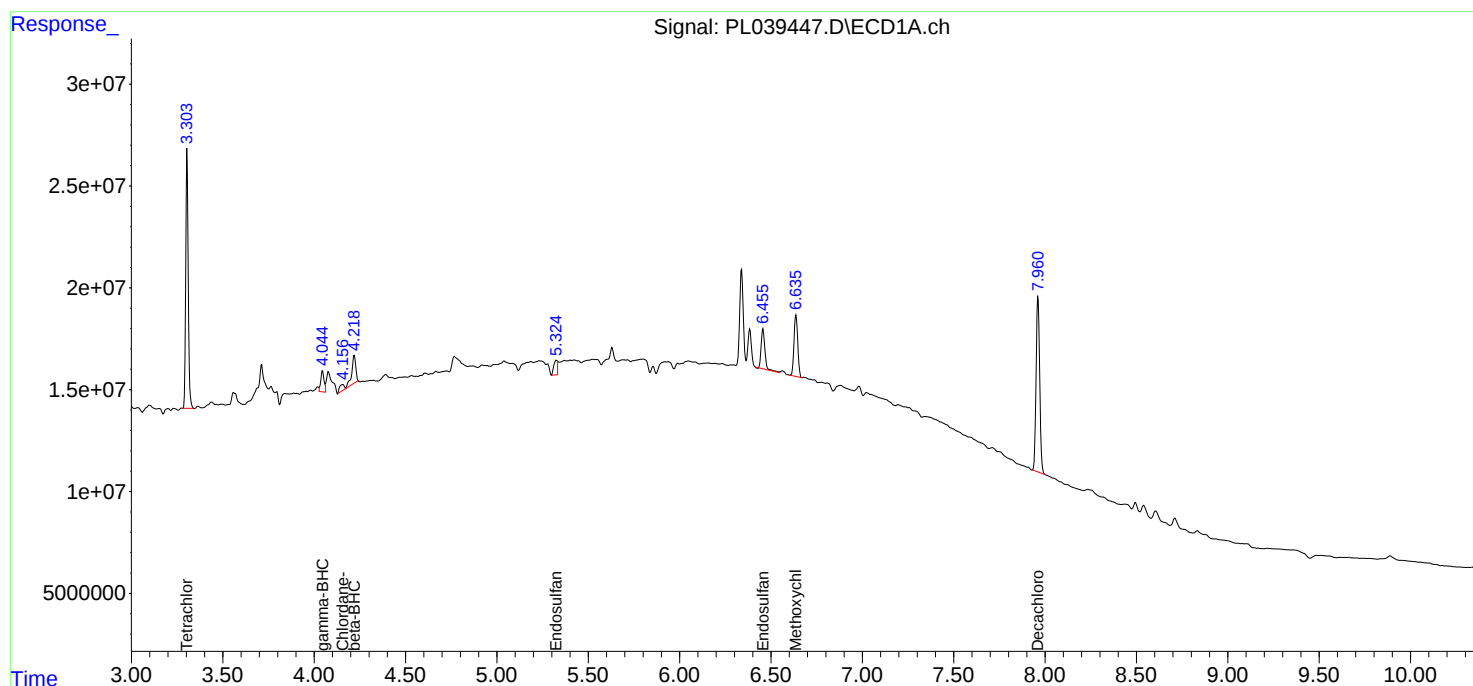


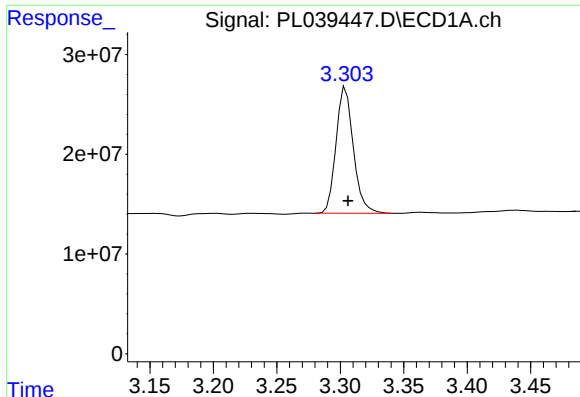

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: -0.002 min
Response: 120394129
Conc: 17.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

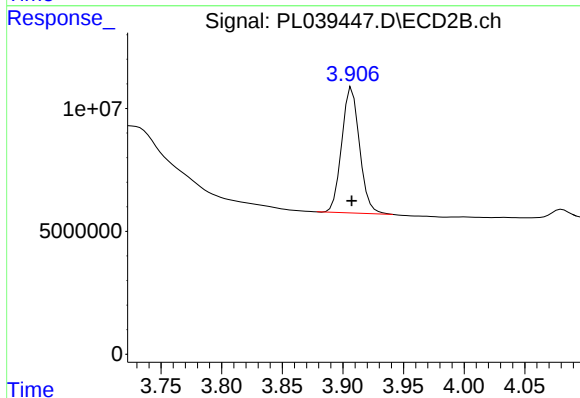


#1 Tetrachloro-m-xylene

R.T.: 3.907 min
Delta R.T.: 0.000 min
Response: 52138723
Conc: 19.45 ng/ml

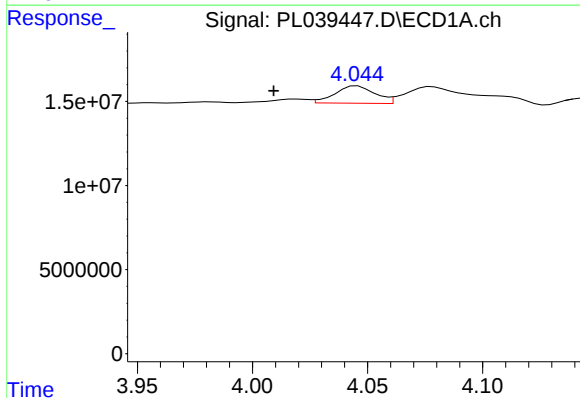


#3 gamma-BHC (Lindane)

R.T.: 4.046 min
Delta R.T.: 0.036 min
Response: 12519094
Conc: 1.18 ng/ml

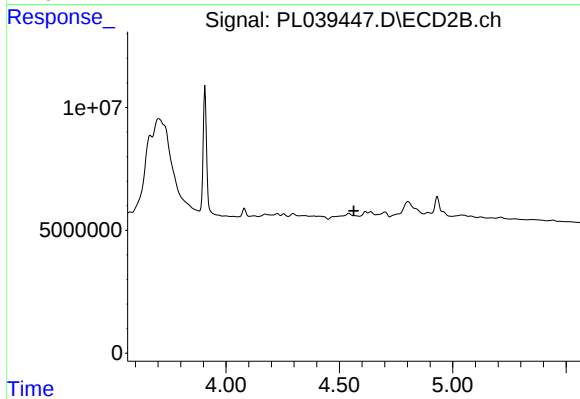

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.563 min
Response: 0
Conc: N.D.

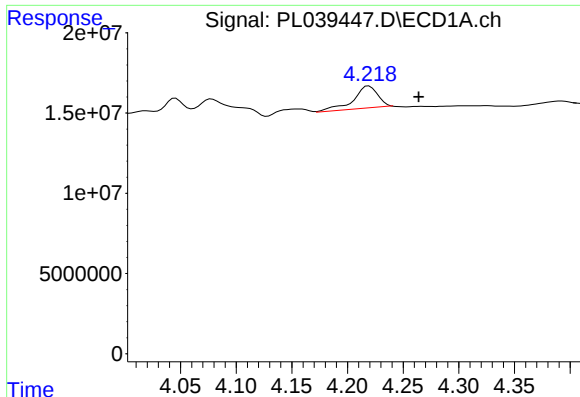

#6 beta-BHC


R.T.: 4.219 min
Delta R.T.: -0.045 min
Response: 21104167
Conc: 4.54 ng/ml

Instrument :
ECD_L
ClientSampleId :

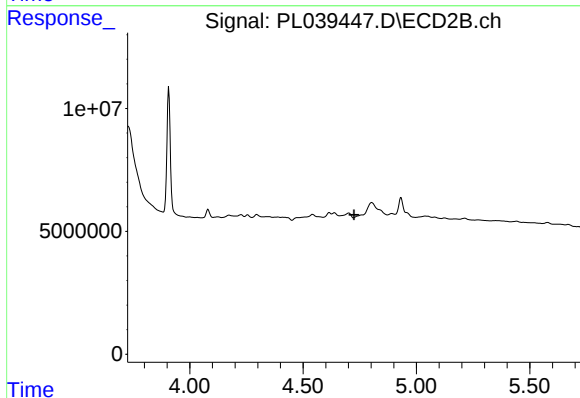


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

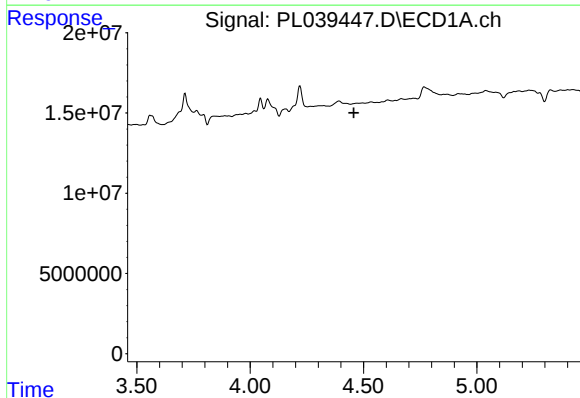


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.457 min
Response: 0
Conc: N.D.

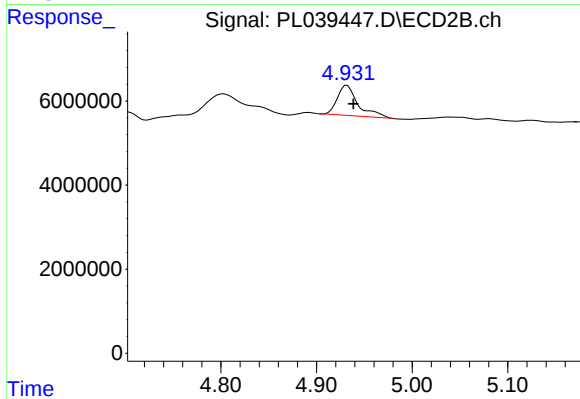

#7 delta-BHC


R.T.: 4.932 min
Delta R.T.: -0.007 min
Response: 10569403
Conc: 2.65 ng/ml

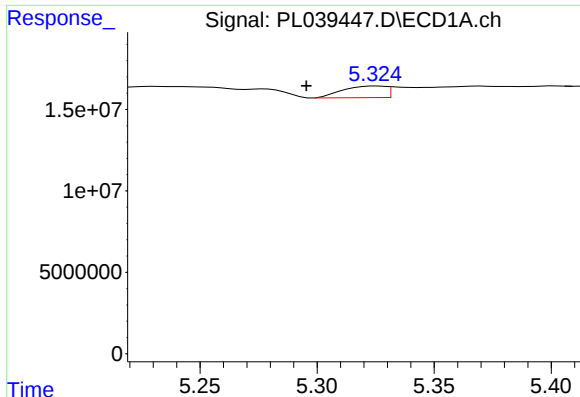

#9 Endosulfan I


R.T.: 5.325 min
Delta R.T.: 0.030 min
Response: 9184474
Conc: 1.05 ng/ml

Instrument :
ECD_L
ClientSampleId :

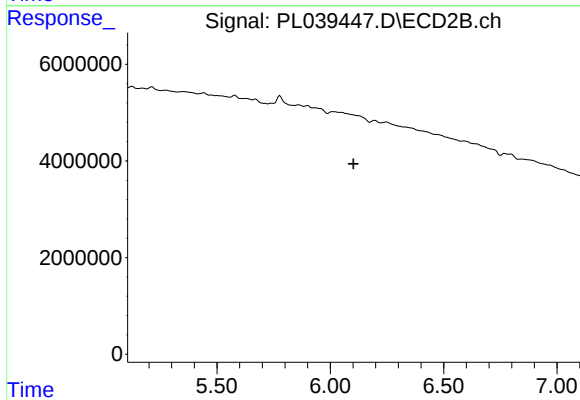


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

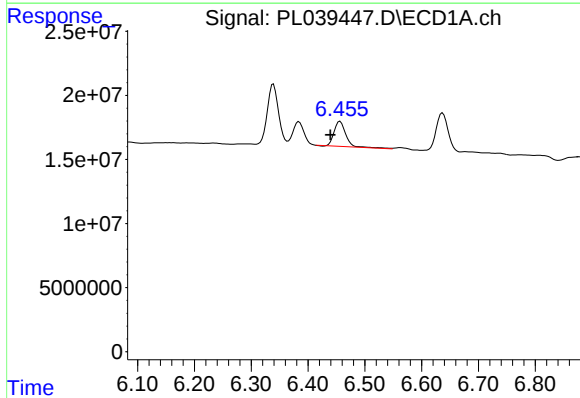


#19 Endosulfan Sulfate

R.T.: 6.456 min
Delta R.T.: 0.017 min
Response: 28309279
Conc: 3.48 ng/ml

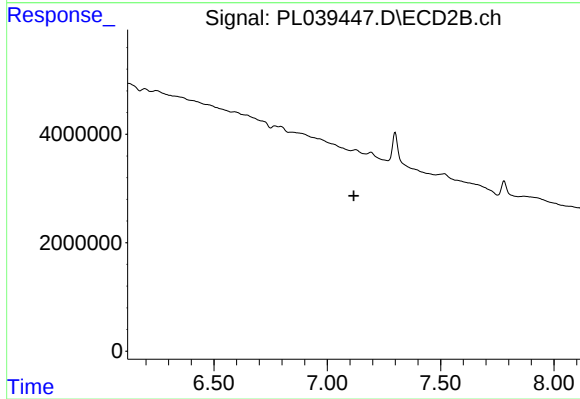

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.117 min
Response: 0
Conc: N.D.

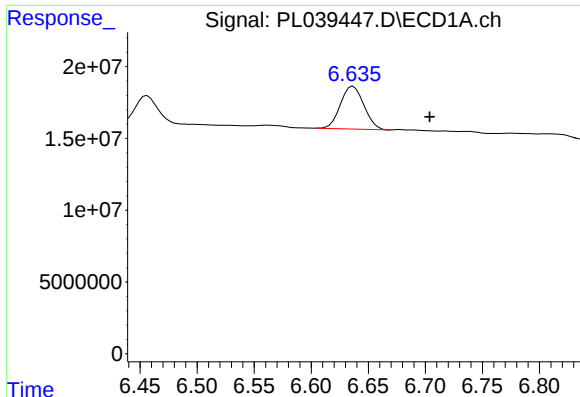

#20 Methoxychlor


R.T.: 6.637 min
Delta R.T.: -0.067 min
Response: 42780526
Conc: 10.45 ng/ml

Instrument :
ECD_L
ClientSampleId :

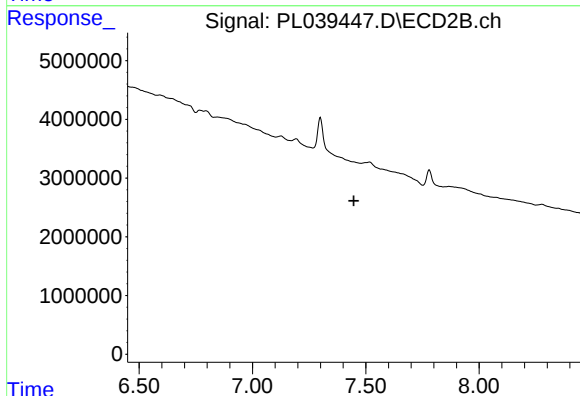


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.446 min
Response: 0
Conc: N.D.

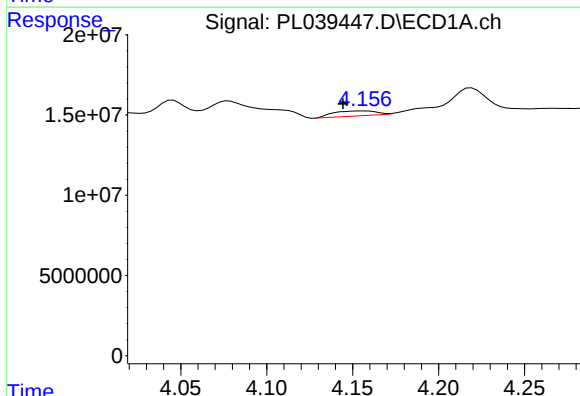


#23 Chlordane-1

R.T.: 4.157 min
Delta R.T.: 0.013 min
Response: 5372425
Conc: 16.97 ng/ml

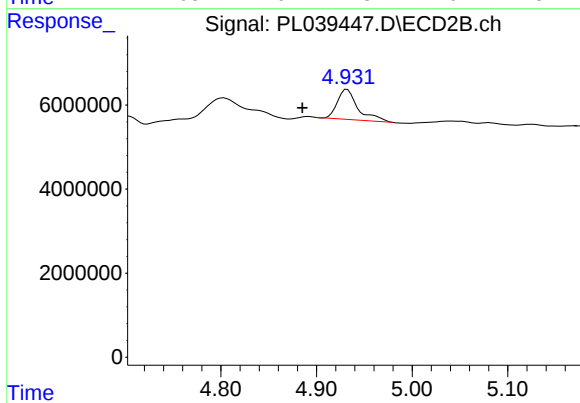

#23 Chlordane-1


R.T.: 4.932 min
Delta R.T.: 0.047 min
Response: 10569403
Conc: 84.60 ng/ml

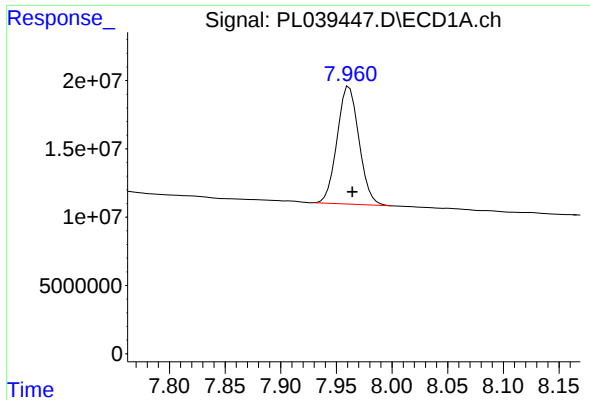

#28 Decachlorobiphenyl

R.T.: 7.962 min
Delta R.T.: -0.003 min
Response: 117403080
Conc: 16.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

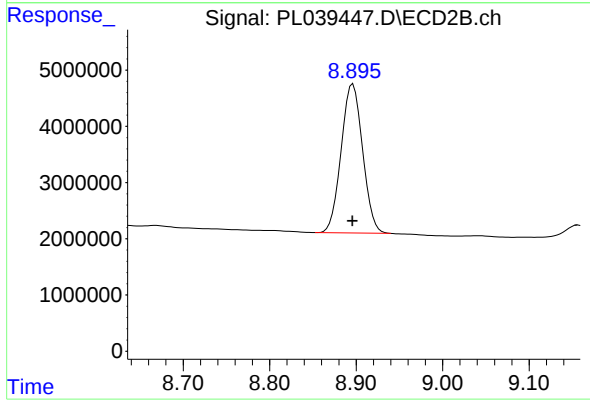

#28 Decachlorobiphenyl

R.T.: 8.896 min
Delta R.T.: 0.000 min
Response: 45445540
Conc: 19.58 ng/ml