

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082218\
 Data File : PL039451.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2018 00:38
 Operator : AJ\SJ
 Sample : J4276-03 5X
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 01:11:20 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.907	18319875	6489669	2.621	2.421
28)	SA Decachlor...	7.961	8.896	17683624	7733551	2.518	3.333 #
Target Compounds							
6)	B beta-BHC	4.216f	0.000	20905926	0	4.500	N.D. #
9)	A Endosulfan I	5.325	0.000	17241992	0	1.969	N.D. #
15)	B Endosulfa...	6.060	0.000	2723171	0	0.313	N.D. #
23)	Chlordane-1	4.152	0.000	13957706	0	44.088	N.D. #
24)	Chlordane-2	4.665	0.000	15257901	0	43.645	N.D. #
27)	Chlordane-5	6.060	0.000	2723171	0	8.396	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082218\
Data File : PL039451.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2018 00:38
Operator : AJ\SJ
Sample : J4276-03 5X
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 01:11:20 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

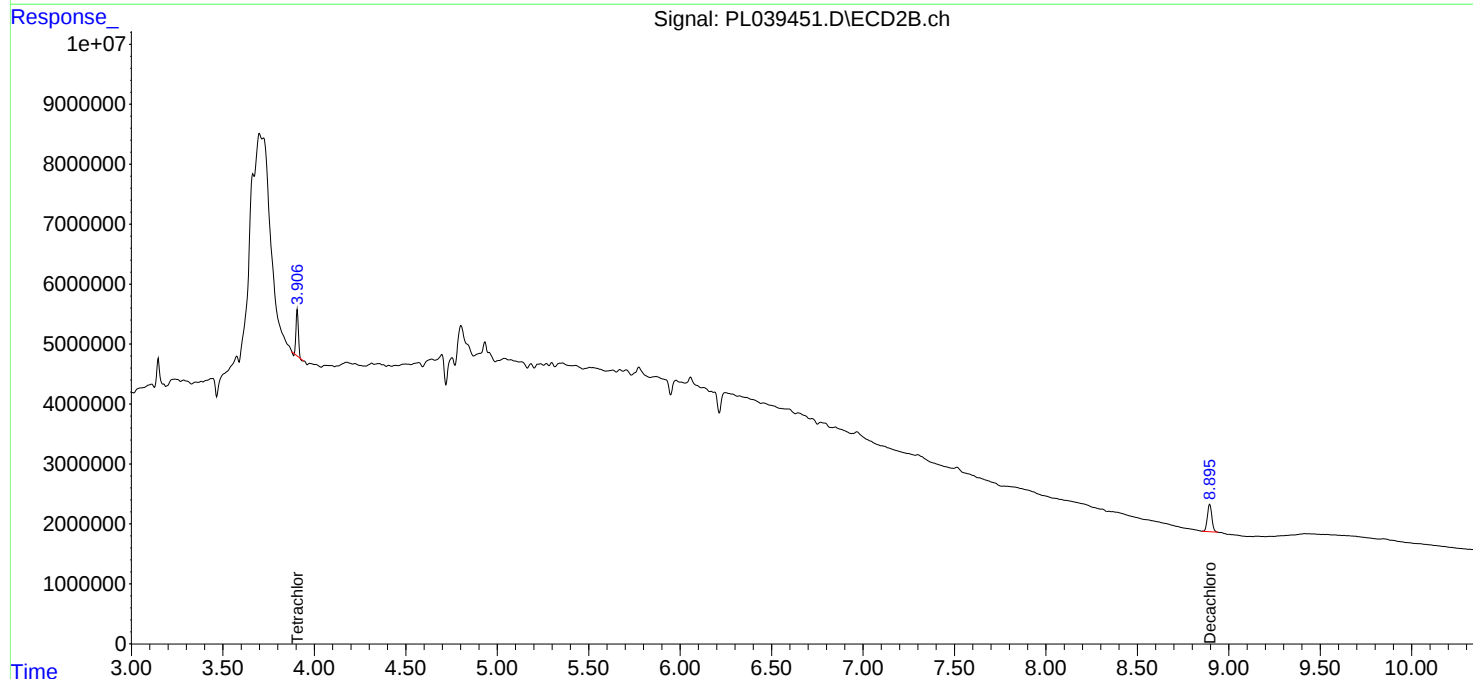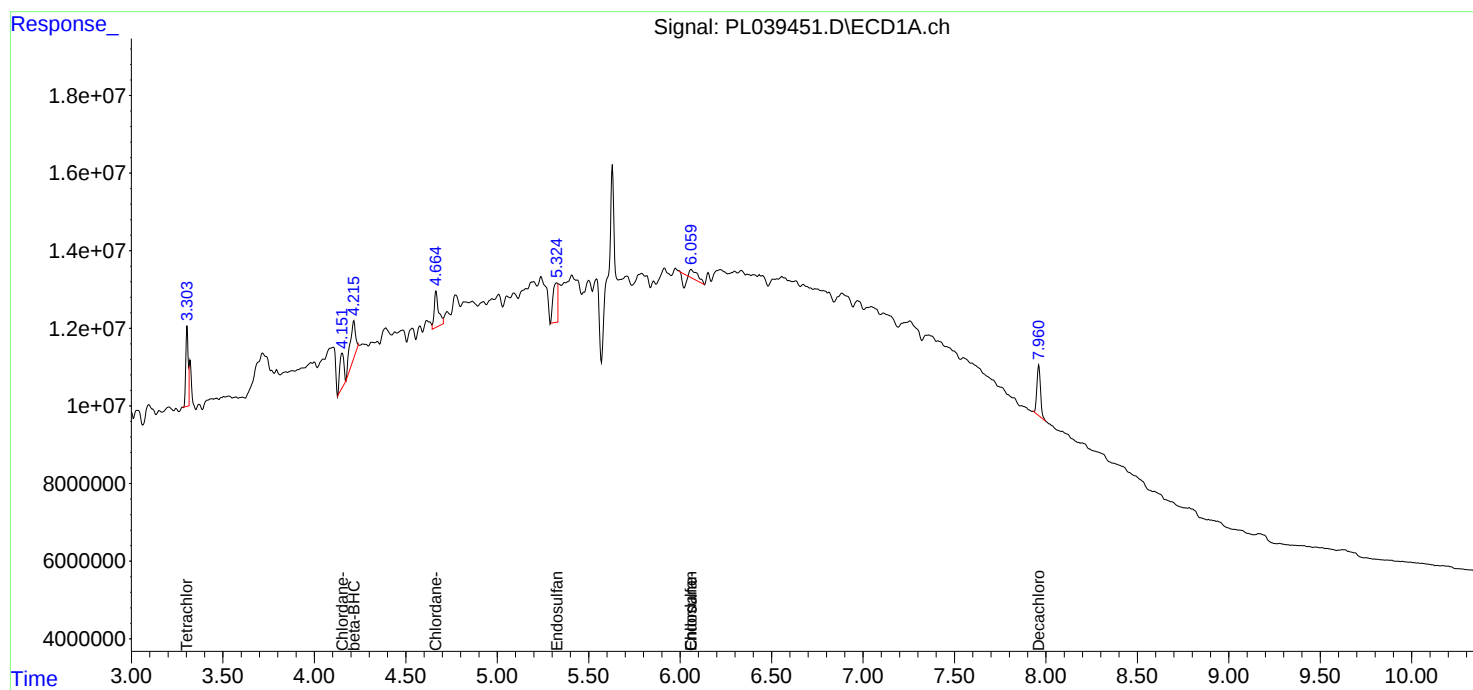


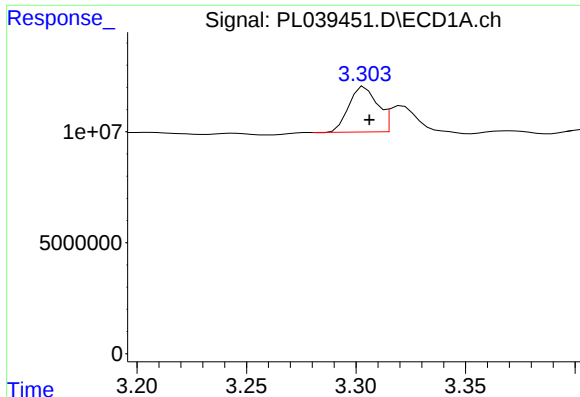

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: -0.002 min
Response: 18319875
Conc: 2.62 ng/ml

Instrument :
ECD_L
ClientSampleId :

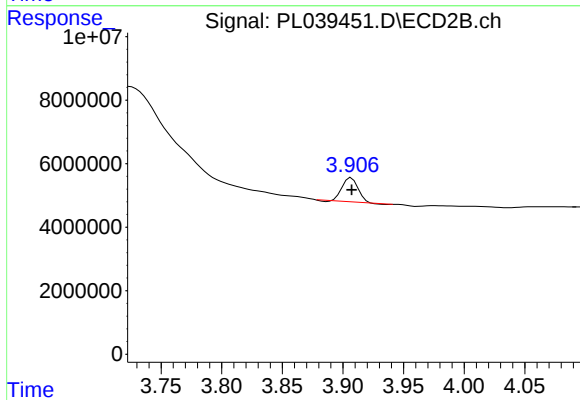


#1 Tetrachloro-m-xylene

R.T.: 3.907 min
Delta R.T.: 0.000 min
Response: 6489669
Conc: 2.42 ng/ml

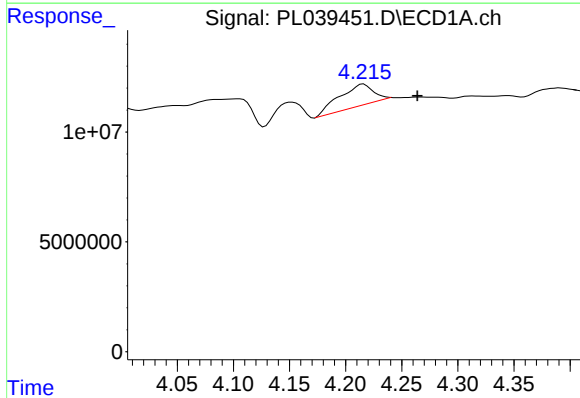


#6 beta-BHC

R.T.: 4.216 min
Delta R.T.: -0.048 min
Response: 20905926
Conc: 4.50 ng/ml

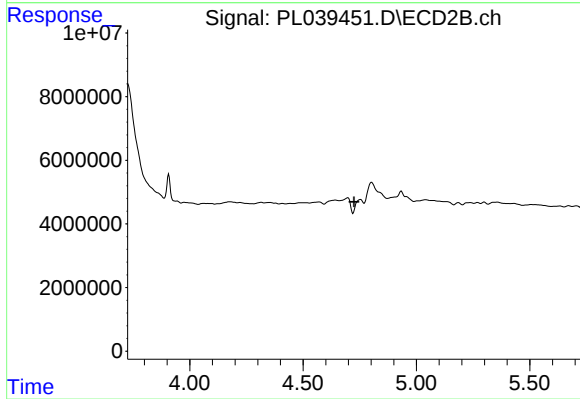

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.726 min
Response: 0
Conc: N.D.

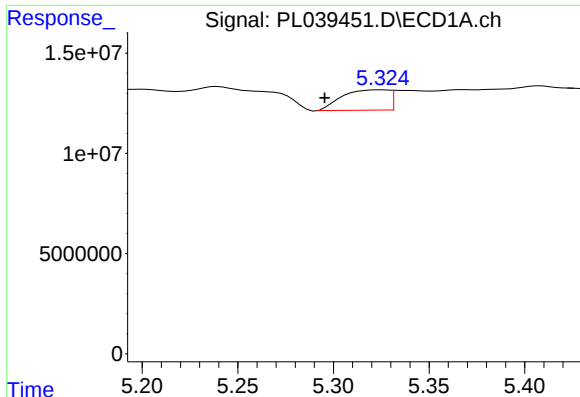

#9 Endosulfan I


R.T.: 5.325 min
Delta R.T.: 0.030 min
Response: 17241992
Conc: 1.97 ng/ml

Instrument :
ECD_L
ClientSampleId :

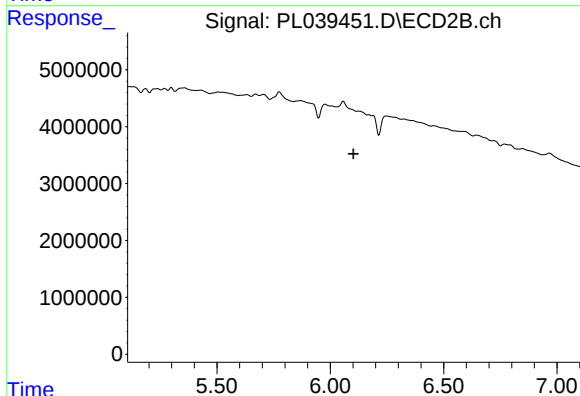


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.102 min
Response: 0
Conc: N.D.

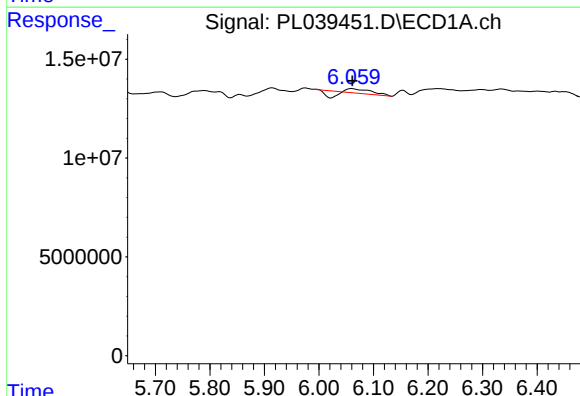


#15 Endosulfan II

R.T.: 6.060 min
Delta R.T.: 0.000 min
Response: 2723171
Conc: 0.31 ng/ml

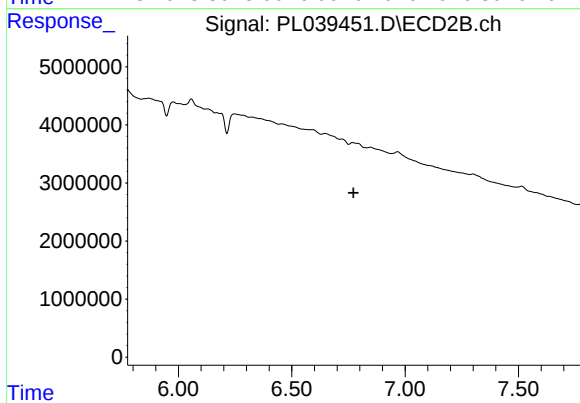

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 6.773 min
Response: 0
Conc: N.D.

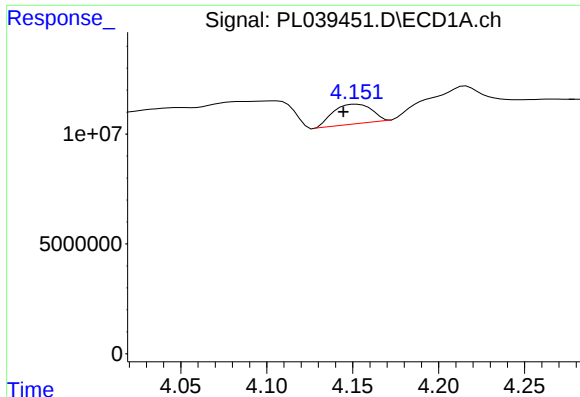

#23 Chlordane-1


R.T.: 4.152 min
Delta R.T.: 0.008 min
Response: 13957706
Conc: 44.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

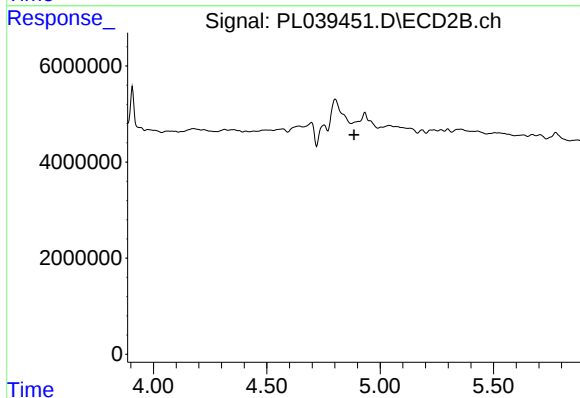


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

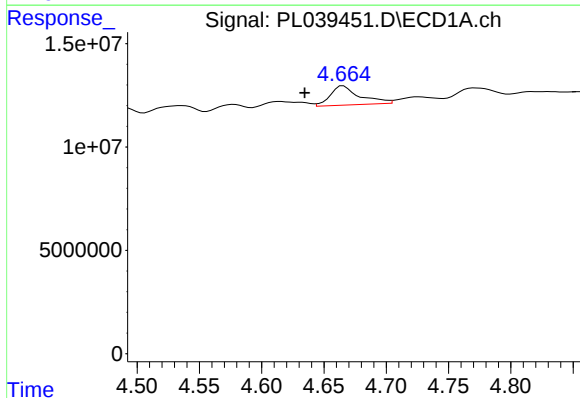


#24 Chlordane-2

R.T.: 4.665 min
Delta R.T.: 0.031 min
Response: 15257901
Conc: 43.64 ng/ml

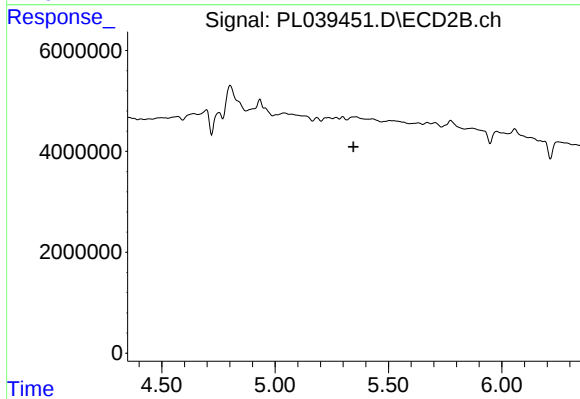

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T. : 5.346 min
Response: 0
Conc: N.D.

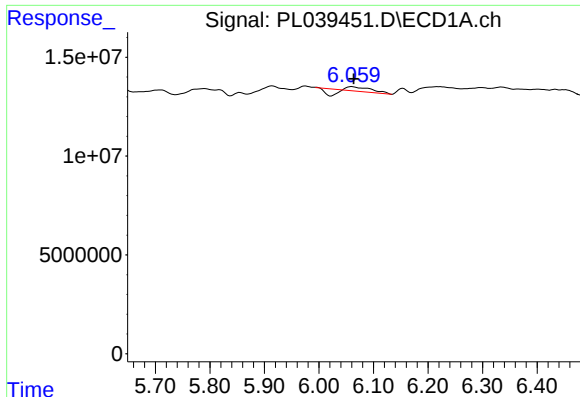

#27 Chlordane-5


R.T.: 6.060 min
Delta R.T.: -0.003 min
Response: 2723171
Conc: 8.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

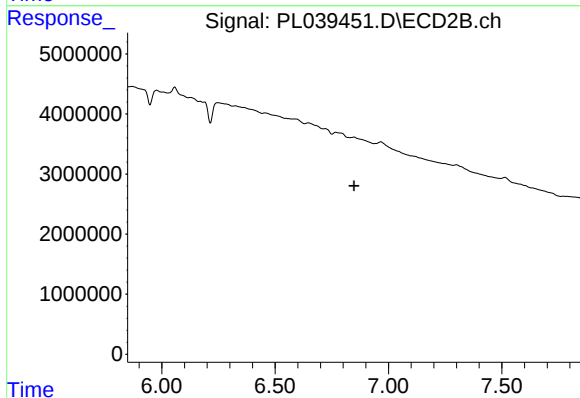


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 6.848 min
Response: 0
Conc: N.D.

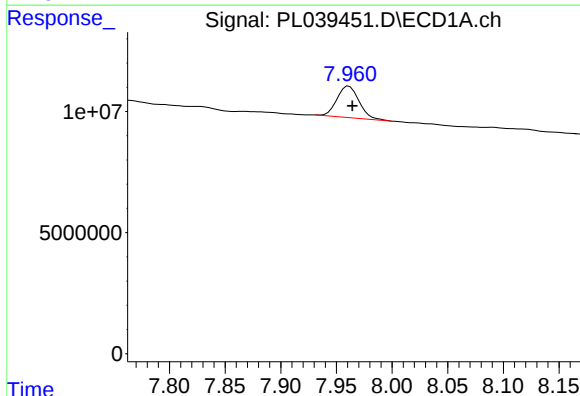

#28 Decachlorobiphenyl

R.T.: 7.961 min
Delta R.T.: -0.003 min
Response: 17683624
Conc: 2.52 ng/ml

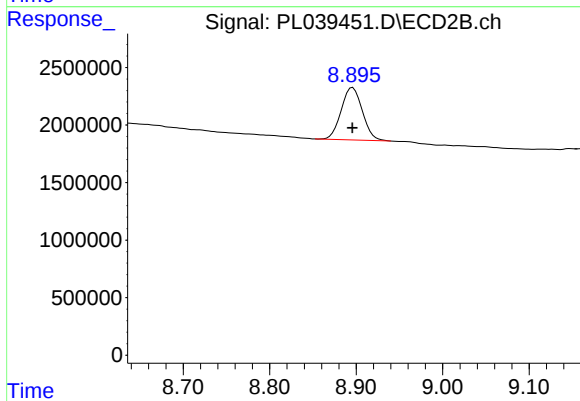

#28 Decachlorobiphenyl

R.T.: 8.896 min
Delta R.T.: 0.000 min
Response: 7733551
Conc: 3.33 ng/ml