

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082218\
 Data File : PL039453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 23 Aug 2018 01:07
 Operator : AJ\SJ
 Sample : J4278-09 5X
 Misc :
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Aug 23 03:51:49 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
 Quant Title : GC Extractables
 QLast Update : Wed Aug 15 15:04:22 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.304	3.906	24050826	7550443	3.441	2.816
28)	SA Decachlor...	7.961	8.896	23462001	10763486	3.341	4.638 #
Target Compounds							
3)	MA gamma-BHC...	3.968f	0.000	17079361	0	1.610	N.D. #
6)	B beta-BHC	4.217f	0.000	14433761	0	3.107	N.D. #
8)	B Heptachlo...	4.931	0.000	2993232	0	0.313	N.D. #
23)	Chlordane-1	4.082	0.000	6462772	0	20.414	N.D. #
24)	Chlordane-2	4.585	0.000	26452839	0	75.668	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL082218\
Data File : PL039453.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 23 Aug 2018 01:07
Operator : AJ\SJ
Sample : J4278-09 5X
Misc :
ALS Vial : 36 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Aug 23 03:51:49 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL081318.M
Quant Title : GC Extractables
QLast Update : Wed Aug 15 15:04:22 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

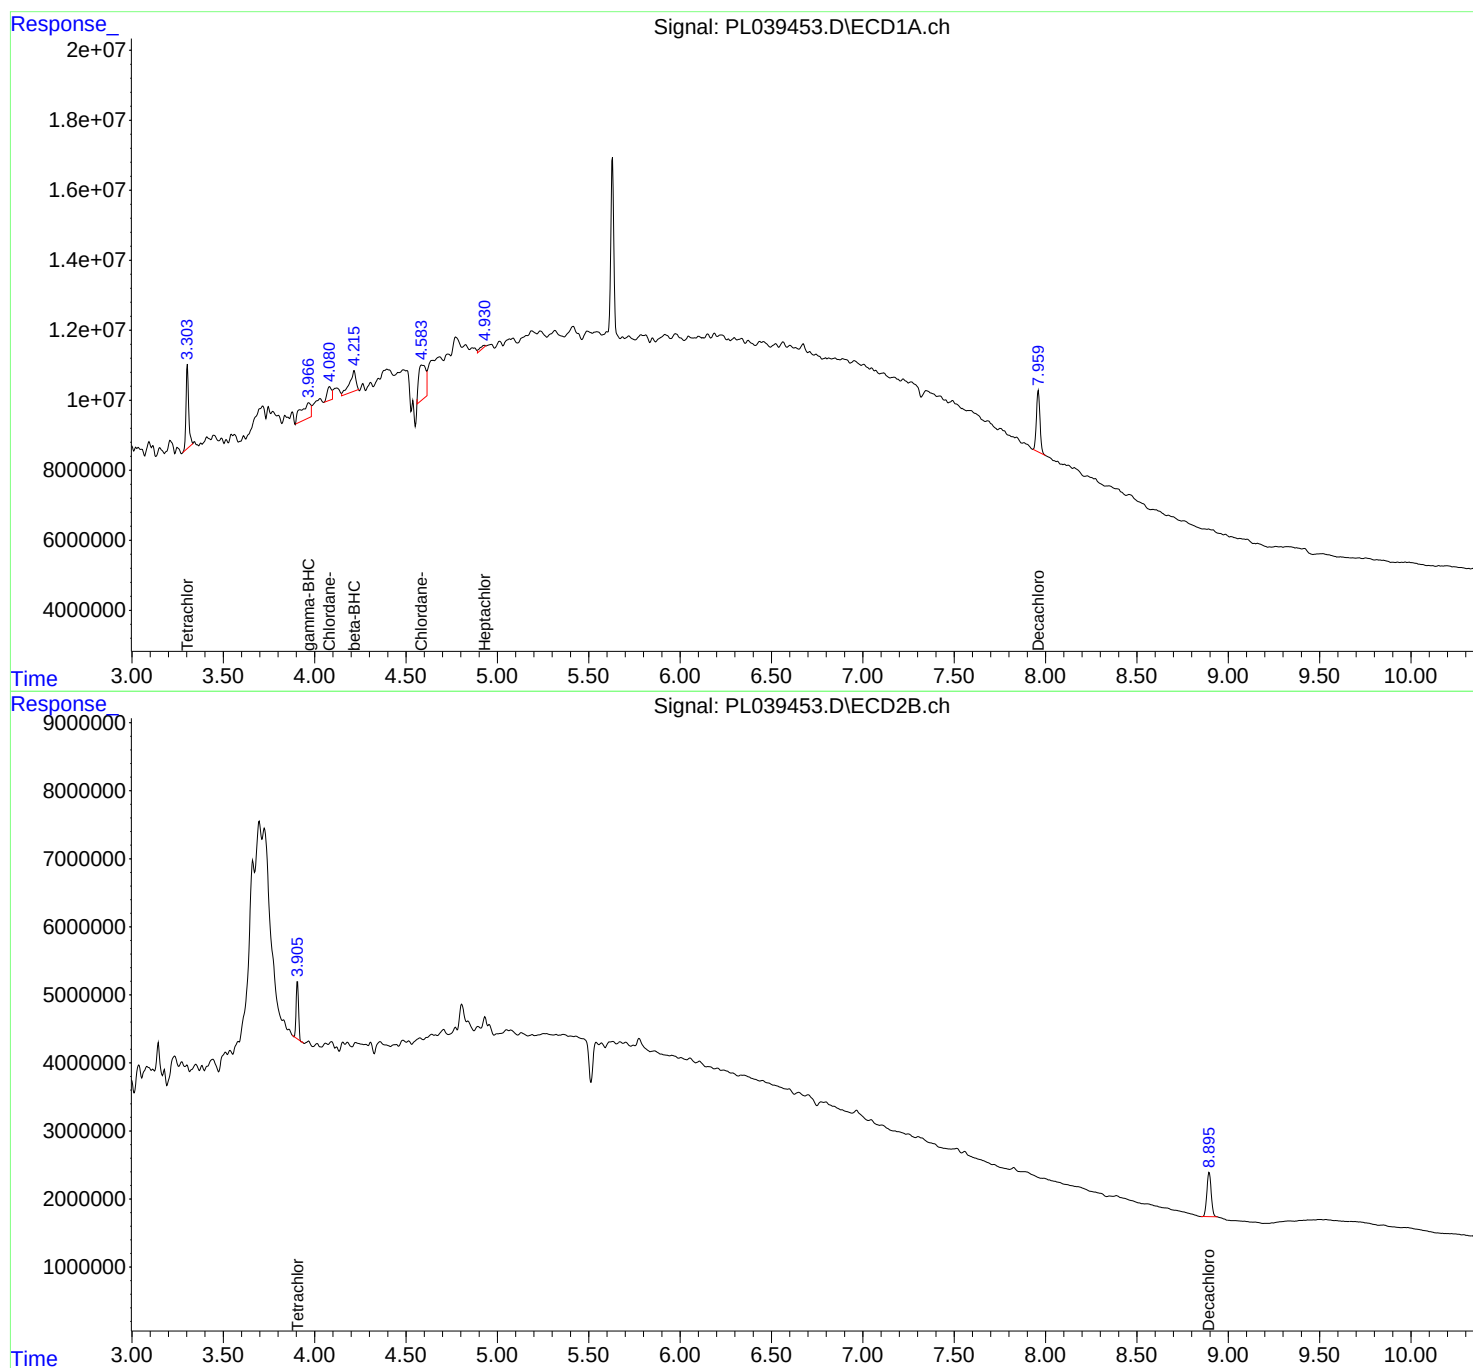


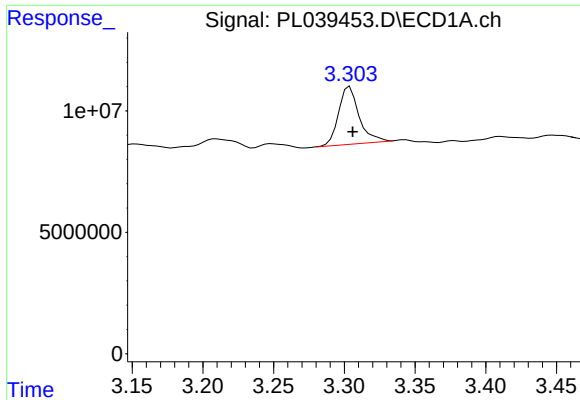

#1 Tetrachloro-m-xylene


R.T.: 3.304 min
Delta R.T.: -0.002 min
Response: 24050826
Conc: 3.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

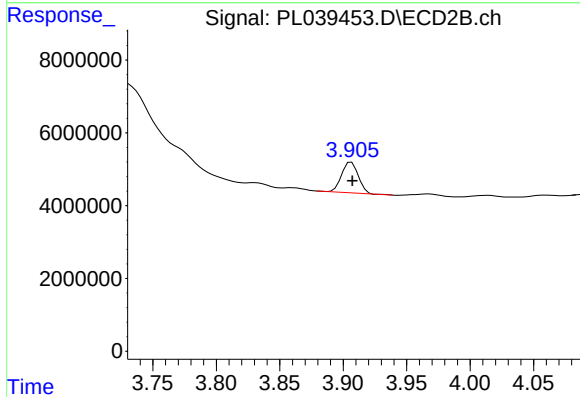


#1 Tetrachloro-m-xylene

R.T.: 3.906 min
Delta R.T.: 0.000 min
Response: 7550443
Conc: 2.82 ng/ml

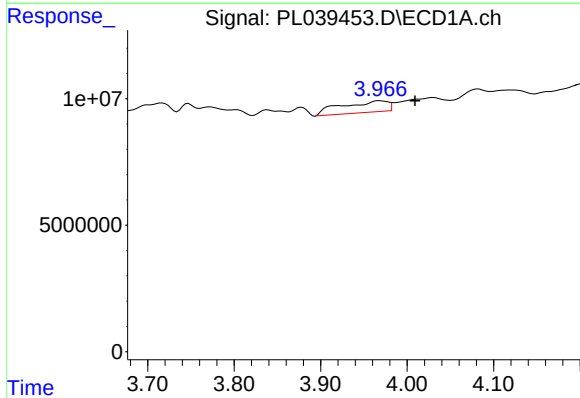


#3 gamma-BHC (Lindane)

R.T.: 3.968 min
Delta R.T.: -0.042 min
Response: 17079361
Conc: 1.61 ng/ml

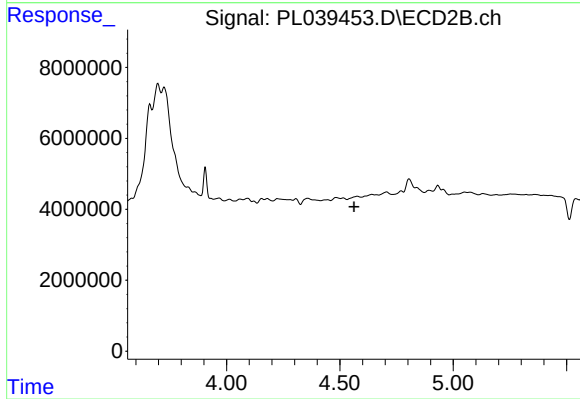

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.563 min
Response: 0
Conc: N.D.

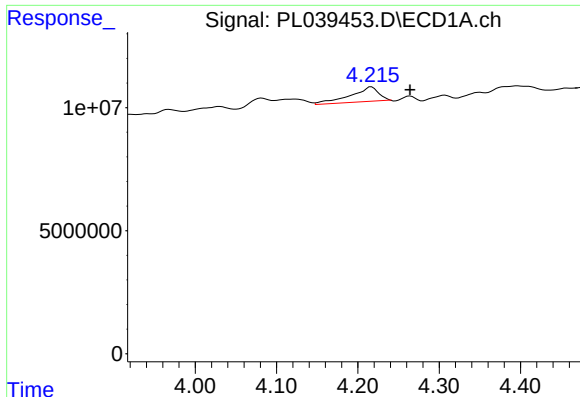

#6 beta-BHC


R.T.: 4.217 min
Delta R.T.: -0.047 min
Response: 14433761
Conc: 3.11 ng/ml

Instrument :
ECD_L
ClientSampleId :

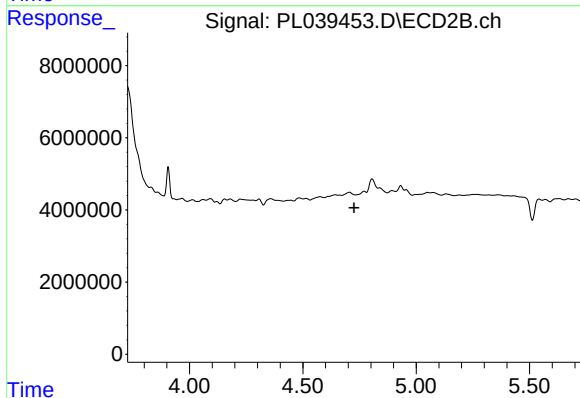


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.726 min
Response: 0
Conc: N.D.

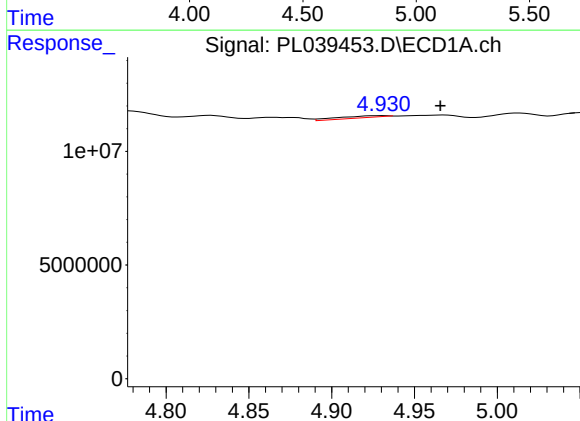


#8 Heptachlor epoxide

R.T.: 4.931 min
Delta R.T.: -0.035 min
Response: 2993232
Conc: 0.31 ng/ml

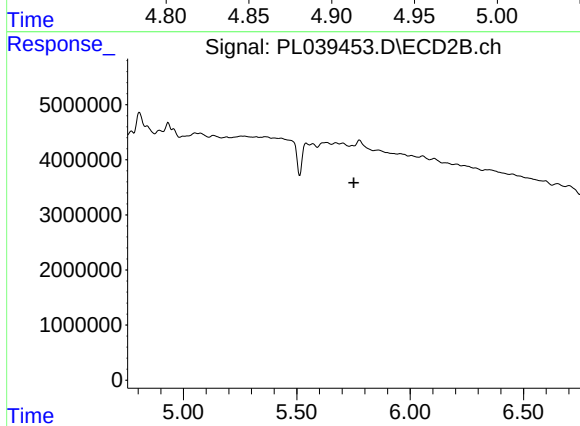

#8 Heptachlor epoxide


R.T.: 0.000 min
Exp R.T. : 5.751 min
Response: 0
Conc: N.D.

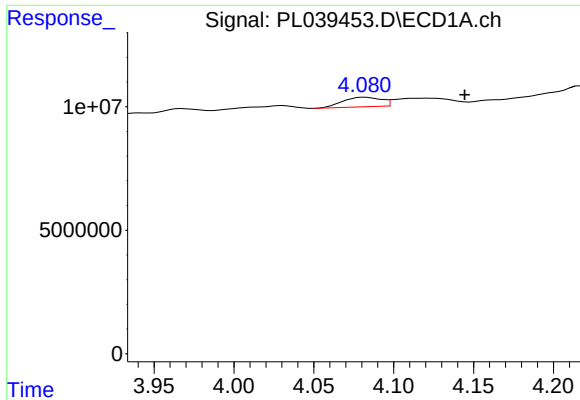

#23 Chlordane-1


R.T.: 4.082 min
Delta R.T.: -0.062 min
Response: 6462772
Conc: 20.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

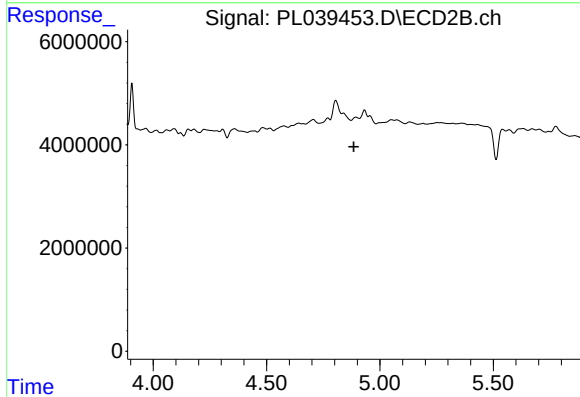


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.885 min
Response: 0
Conc: N.D.

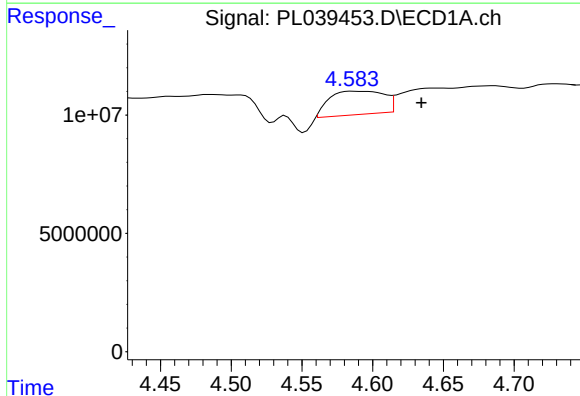


#24 Chlordane-2

R.T.: 4.585 min
Delta R.T.: -0.049 min
Response: 26452839
Conc: 75.67 ng/ml

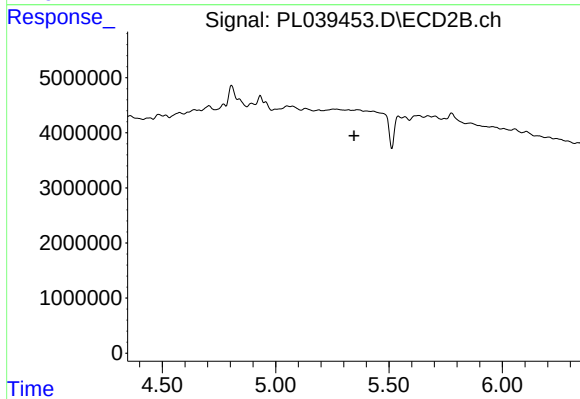

#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 5.346 min
Response: 0
Conc: N.D.

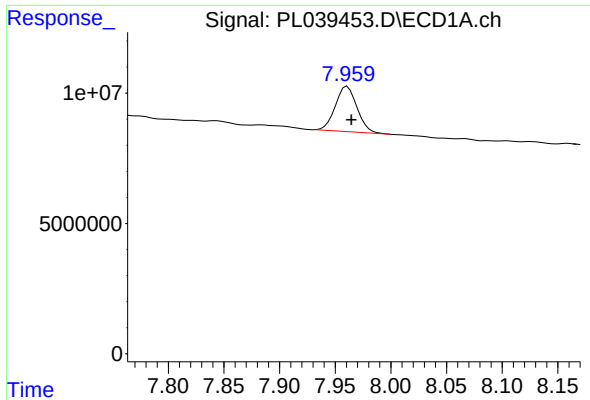

#28 Decachlorobiphenyl


R.T.: 7.961 min

Delta R.T.: -0.004 min

Response: 23462001

Conc: 3.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

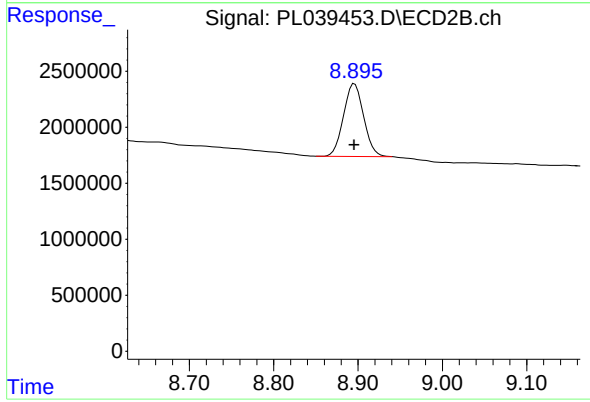

#28 Decachlorobiphenyl

R.T.: 8.896 min

Delta R.T.: 0.000 min

Response: 10763486

Conc: 4.64 ng/ml