

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010623\
 Data File : PL080150.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jan 2023 14:53
 Operator : AR\AJ
 Sample : 01023-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 QUARTERLY-INFLUENT

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 01/09/2023
 Supervised By :Ankita Jodhani 01/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 21:03:00 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 05 05:11:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.381	2.690	28699976	23183171	14.428	10.196 #
2)	SA Decachlor...	8.908f	7.847	35190812	28039805	20.511m	12.411 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010623\
Data File : PL080150.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jan 2023 14:53
Operator : AR\AJ
Sample : 01023-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
QUARTERLY-INFLUENT


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/09/2023
Supervised By : Ankita Jodhani 01/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 21:03:00 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
Quant Title : GC Extractables
QLast Update : Thu Jan 05 05:11:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

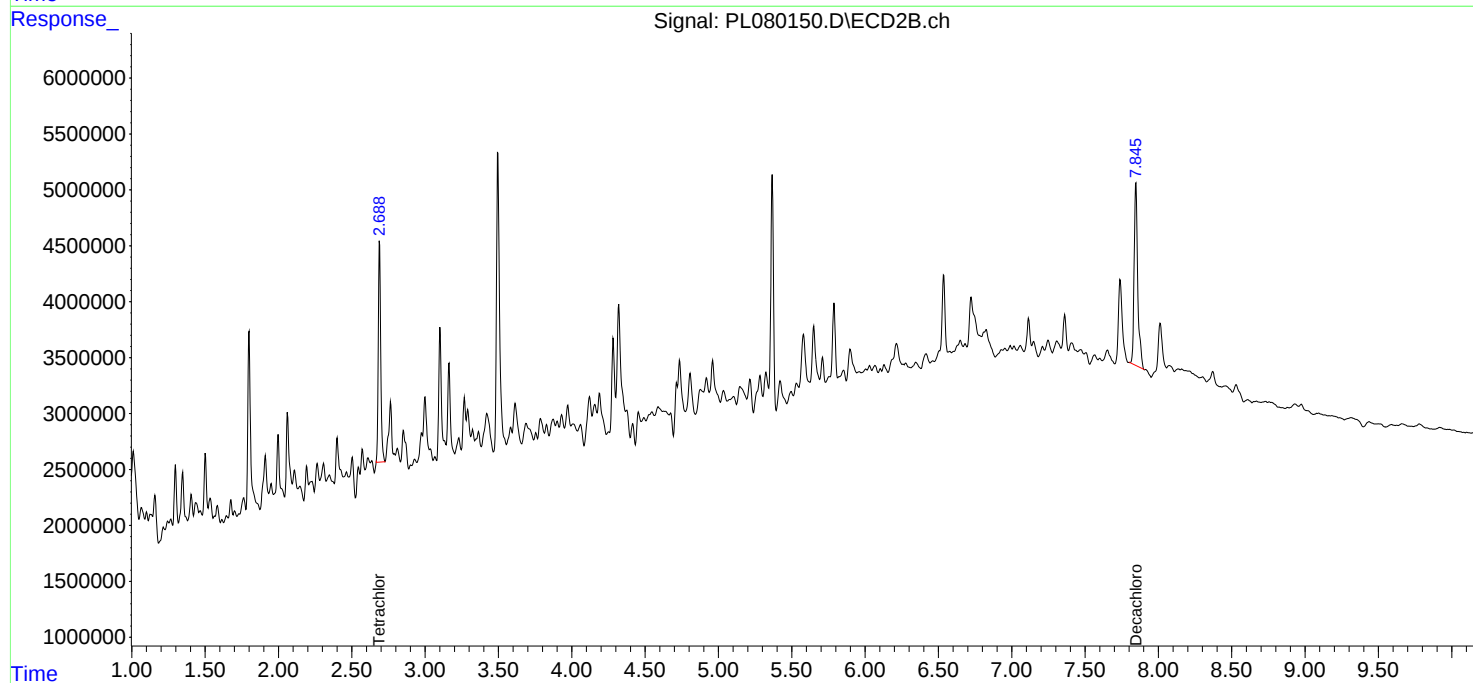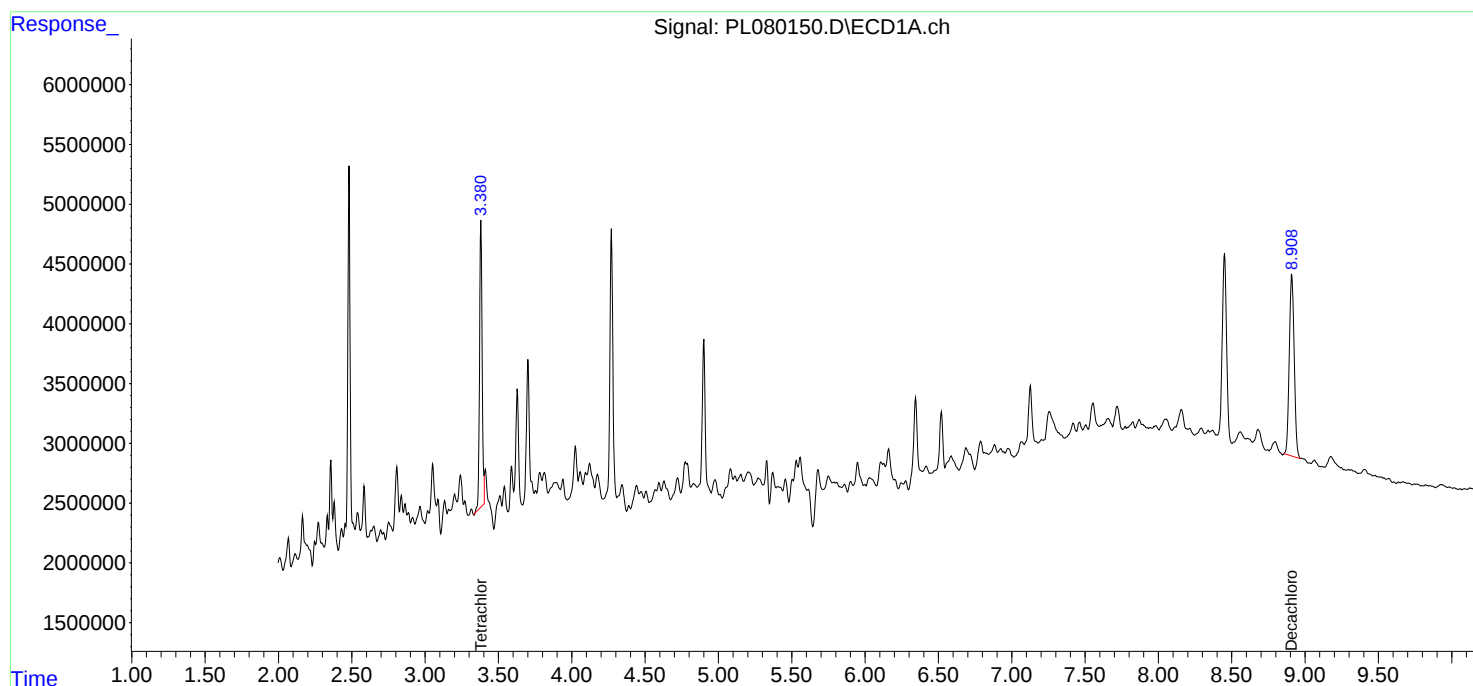

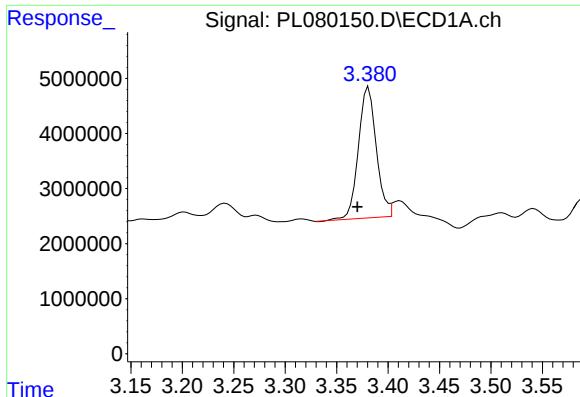


#1 Tetrachloro-m-xylene

R.T.: 3.381 min
Delta R.T.: 0.011 min
Response: 28699976
Conc: 14.43 ng/ml

Instrument :
ECD_L
ClientSampleId :
QUARTERLY-INFLUENT


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/09/2023
Supervised By :Ankita Jodhani 01/09/2023

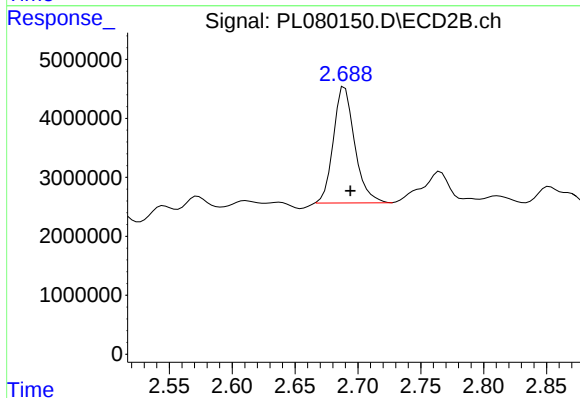


#1 Tetrachloro-m-xylene

R.T.: 2.690 min
Delta R.T.: -0.004 min
Response: 23183171
Conc: 10.20 ng/ml

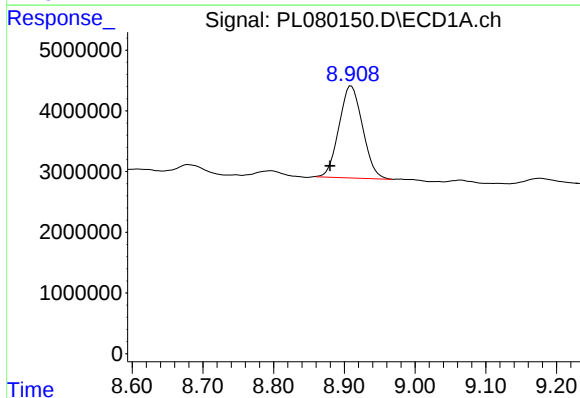

#28 Decachlorobiphenyl

R.T.: 8.908 min
Delta R.T.: 0.028 min
Response: 35190812
Conc: 20.51 ng/ml m

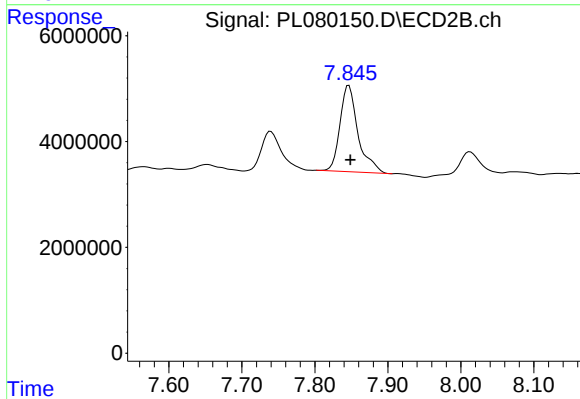

#28 Decachlorobiphenyl

R.T.: 7.847 min
Delta R.T.: -0.002 min
Response: 28039805
Conc: 12.41 ng/ml