

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010623\
 Data File : PL080151.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jan 2023 15:06
 Operator : AR\AJ
 Sample : 01025-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 QUARTERLY-OUTFALL-002

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/09/2023
 Supervised By : Ankita Jodhani 01/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 21:04:22 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 05 05:11:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.372	2.691	35727755	33609256	17.961	14.781m
28) SA Decachlor...	8.890	7.845	30780494	38144427	17.940	16.883

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010623\
Data File : PL080151.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jan 2023 15:06
Operator : AR\AJ
Sample : 01025-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
QUARTERLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/09/2023
Supervised By : Ankita Jodhani 01/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 21:04:22 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
Quant Title : GC Extractables
QLast Update : Thu Jan 05 05:11:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

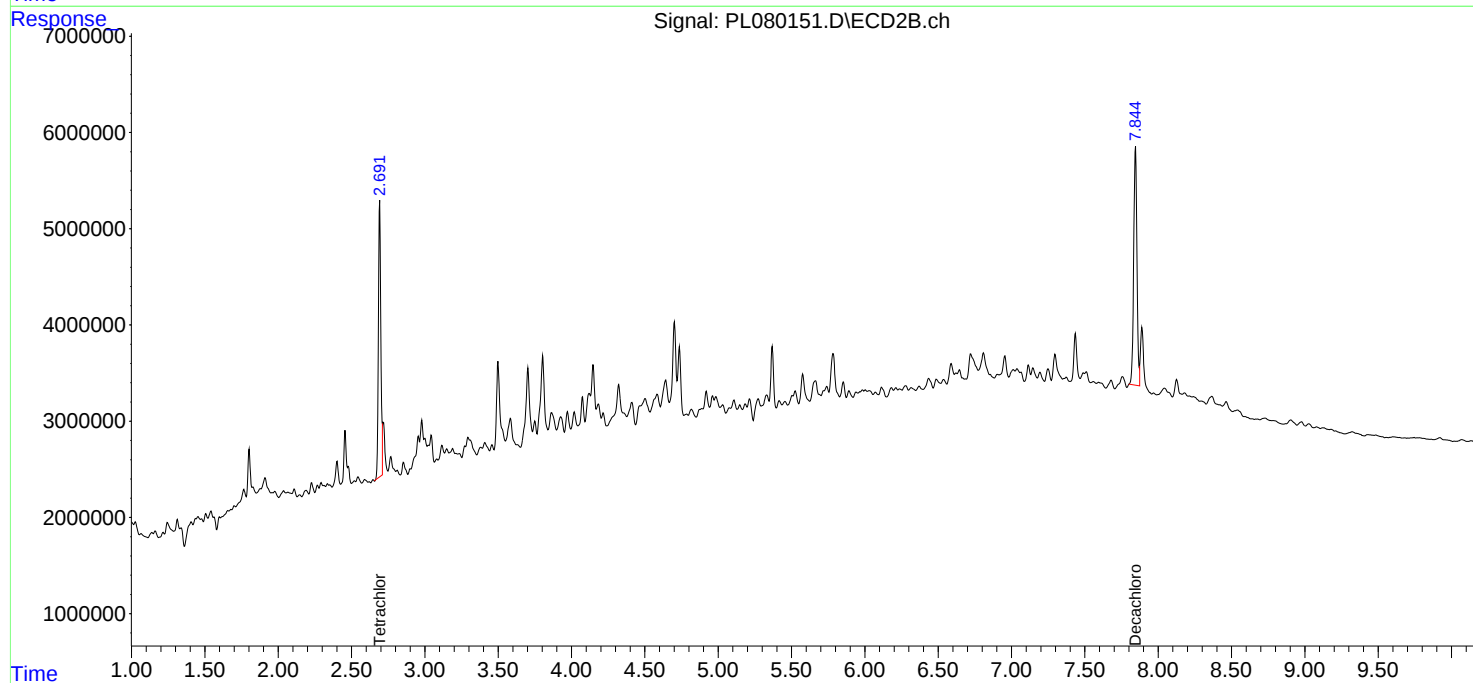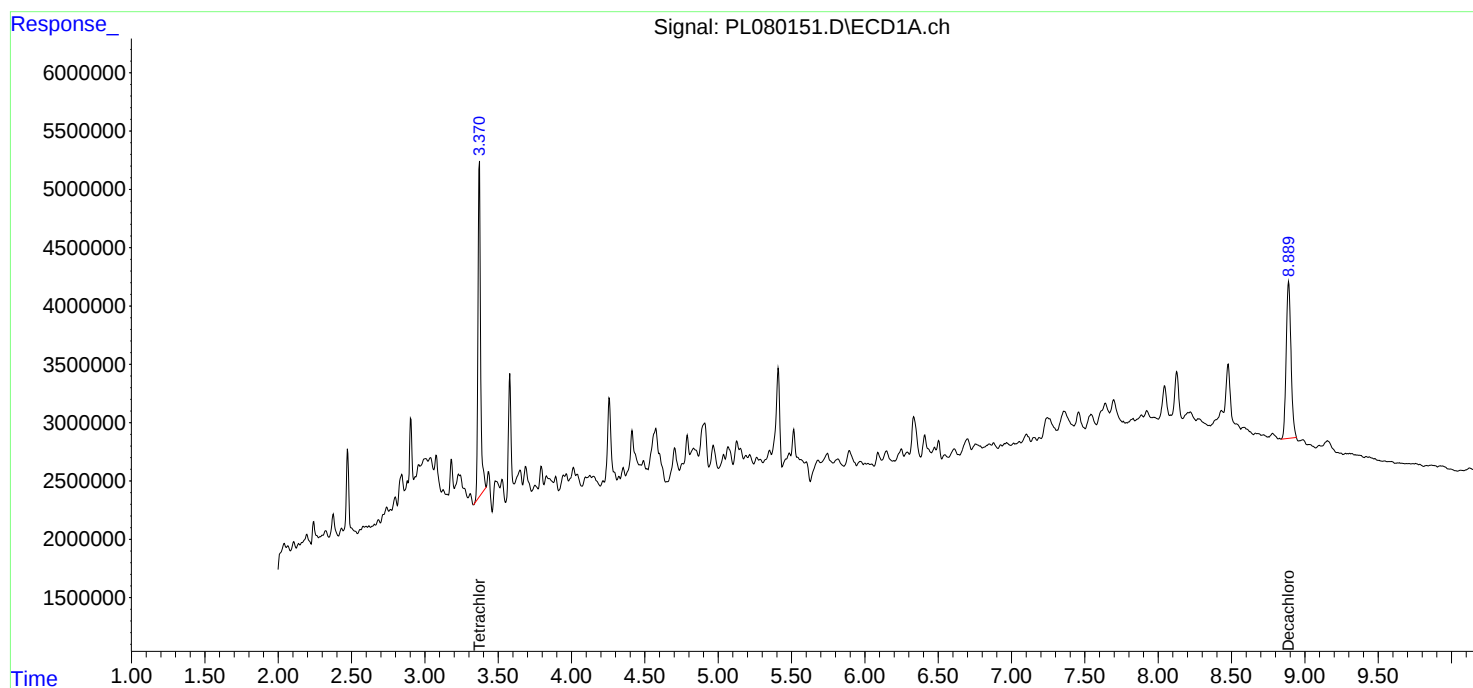

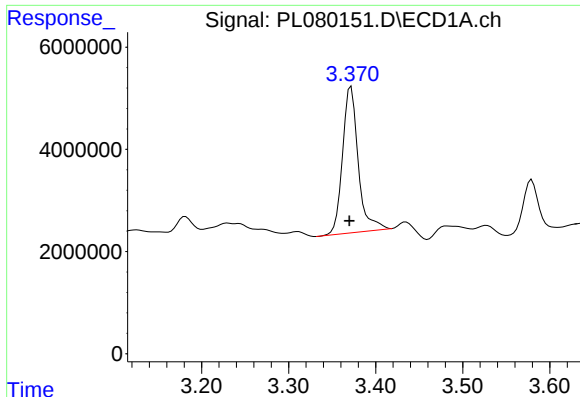


#1 Tetrachloro-m-xylene

R.T.: 3.372 min
Delta R.T.: 0.002 min
Response: 35727755
Conc: 17.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
QUARTERLY-OUTFALL-002


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/09/2023
Supervised By :Ankita Jodhani 01/09/2023

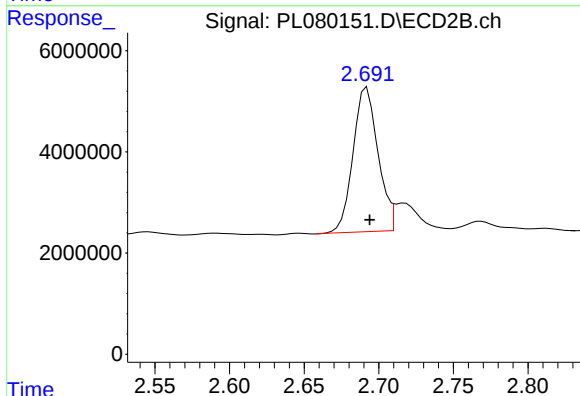


#1 Tetrachloro-m-xylene

R.T.: 2.691 min
Delta R.T.: -0.003 min
Response: 33609256
Conc: 14.78 ng/ml m

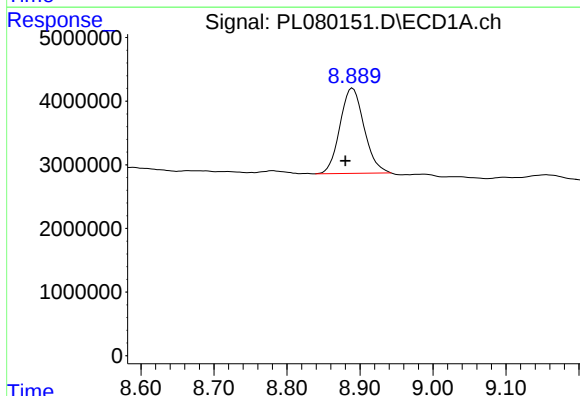

#28 Decachlorobiphenyl

R.T.: 8.890 min
Delta R.T.: 0.010 min
Response: 30780494
Conc: 17.94 ng/ml

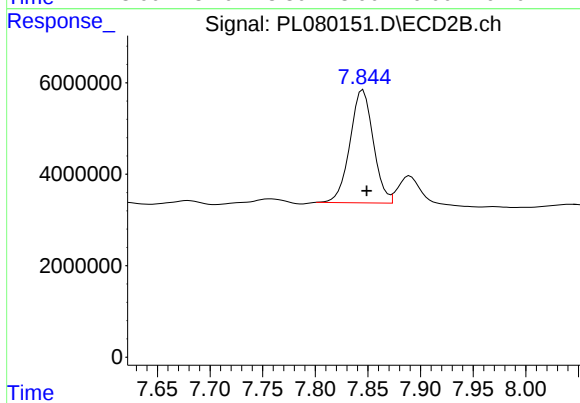

#28 Decachlorobiphenyl

R.T.: 7.845 min
Delta R.T.: -0.004 min
Response: 38144427
Conc: 16.88 ng/ml