

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010623\
 Data File : PL080156.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 06 Jan 2023 16:16
 Operator : AR\AJ
 Sample : 01033-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 VNJ-228

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/09/2023
 Supervised By : Ankita Jodhani 01/09/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 06 21:09:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 05 05:11:24 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.370	2.692	17261681	16484701	8.678m	7.250m
28)	SA Decachlor...	8.888	7.846	15733280	20189626	9.170	8.936
Target Compounds							
17)	MA 4,4'-DDT	6.871	5.960	2958618	4871252	1.979m	2.392

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010623\
Data File : PL080156.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 06 Jan 2023 16:16
Operator : AR\AJ
Sample : 01033-01
Misc :
ALS Vial : 16 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
VNJ-228


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/09/2023
Supervised By : Ankita Jodhani 01/09/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 06 21:09:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010423.M
Quant Title : GC Extractables
QLast Update : Thu Jan 05 05:11:24 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

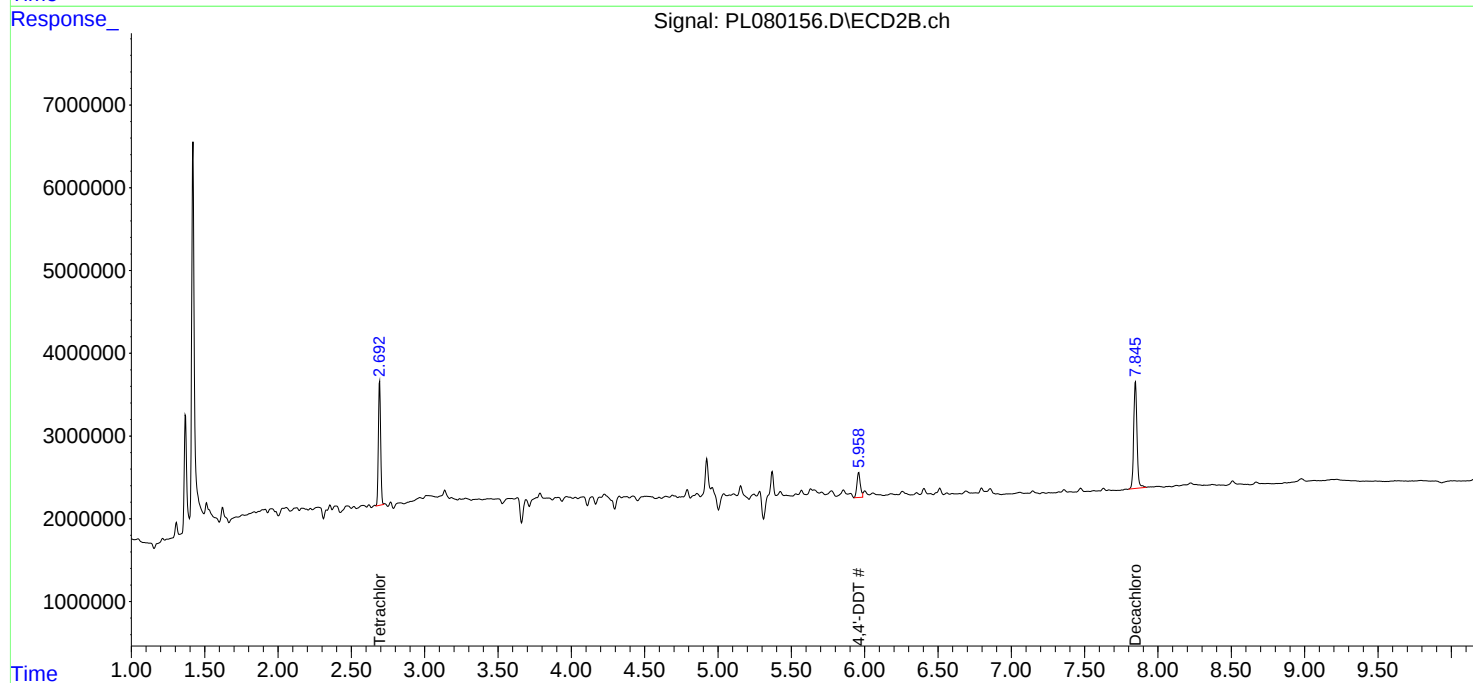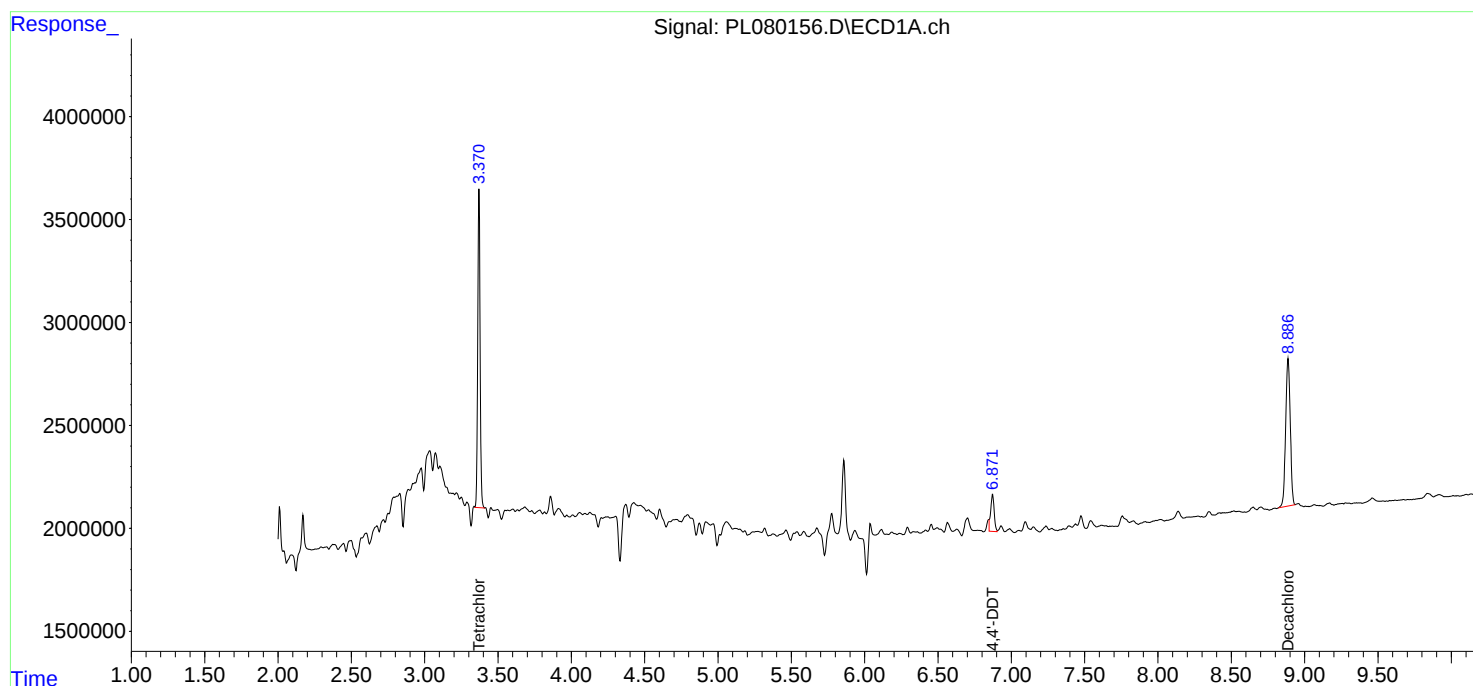

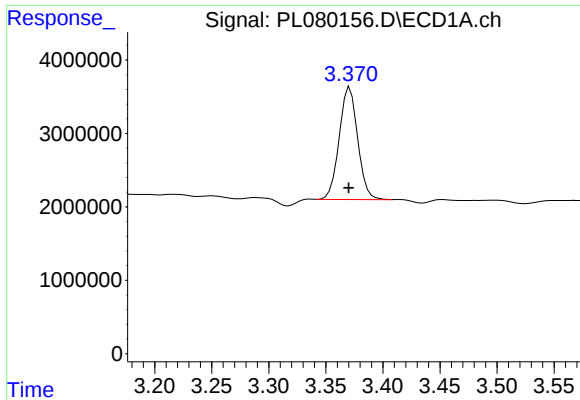


#1 Tetrachloro-m-xylene

R.T.: 3.370 min
Delta R.T.: 0.000 min
Response: 17261681
Conc: 8.68 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-228


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/09/2023
Supervised By :Ankita Jodhani 01/09/2023

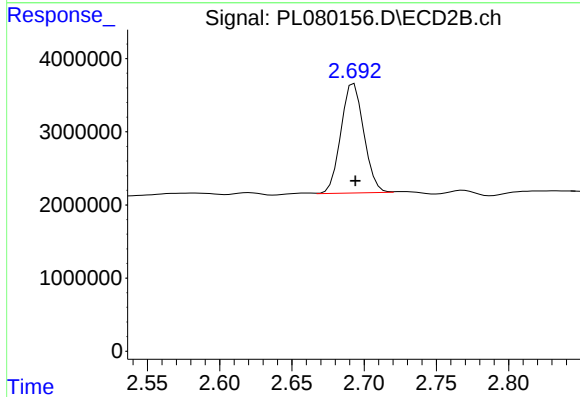


#1 Tetrachloro-m-xylene

R.T.: 2.692 min
Delta R.T.: -0.002 min
Response: 16484701
Conc: 7.25 ng/ml m

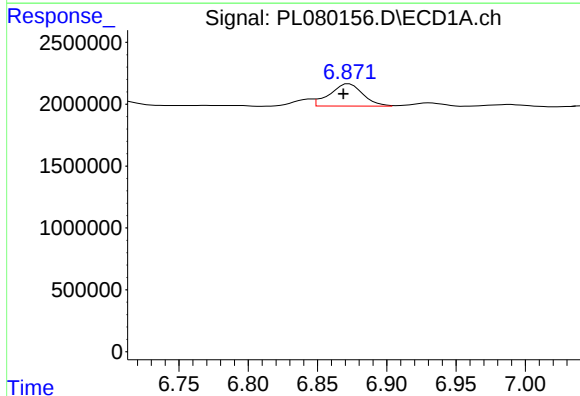


#17 4,4'-DDT

R.T.: 6.871 min
Delta R.T.: 0.002 min
Response: 2958618
Conc: 1.98 ng/ml m

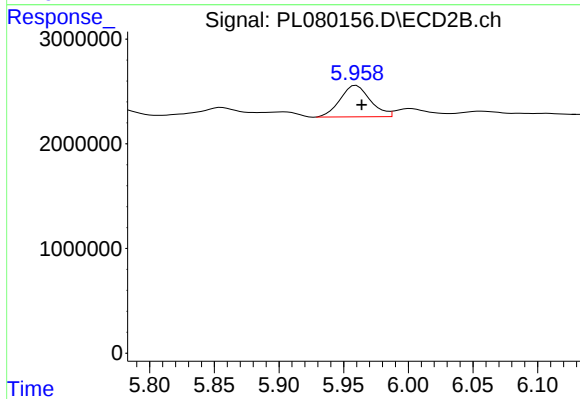

#17 4,4'-DDT

R.T.: 5.960 min
Delta R.T.: -0.004 min
Response: 4871252
Conc: 2.39 ng/ml

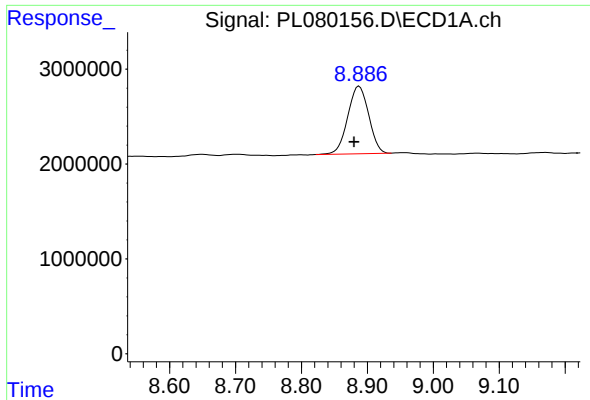


#28 Decachlorobiphenyl

R.T.: 8.888 min
Delta R.T.: 0.008 min
Response: 15733280
Conc: 9.17 ng/ml

Instrument :
ECD_L
ClientSampleId :
VNJ-228

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/09/2023
Supervised By :Ankita Jodhani 01/09/2023

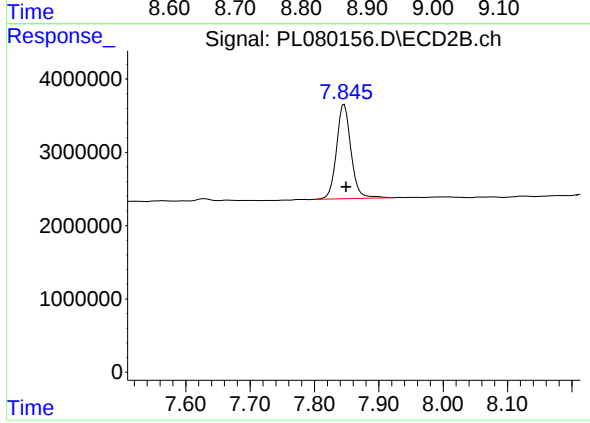

#28 Decachlorobiphenyl

R.T.: 7.846 min
Delta R.T.: -0.003 min
Response: 20189626
Conc: 8.94 ng/ml