

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010722\
 Data File : PL071859.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2022 09:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 23:35:25 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.562	5.496	9352409	26028333	20.246	21.185
28)	SA Decachlor...	10.326	11.393	14695110	23616673	20.324	19.929
Target Compounds							
6)	B beta-BHC	6.041f	0.000	184306	0	0.681	N.D. #
7)	B delta-BHC	0.000	6.975f	0	404855	N.D.	0.264 #
9)	A Endosulfan I	0.000	8.355	0	118621	N.D.	0.096 #
10)	B gamma-Chl...	0.000	8.216	0	59462	N.D.	0.043 #
17)	MA 4,4'-DDT	0.000	9.327f	0	80549	N.D.	0.085 #
18)	B Endrin al...	0.000	9.283f	0	191419	N.D.	0.226 #
24)	Chlordane-2	0.000	7.437f	0	662499	N.D.	12.240 #
25)	Chlordane-3	0.000	8.216	0	59462	N.D.	0.291 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010722\
Data File : PL071859.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2022 09:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 23:35:25 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

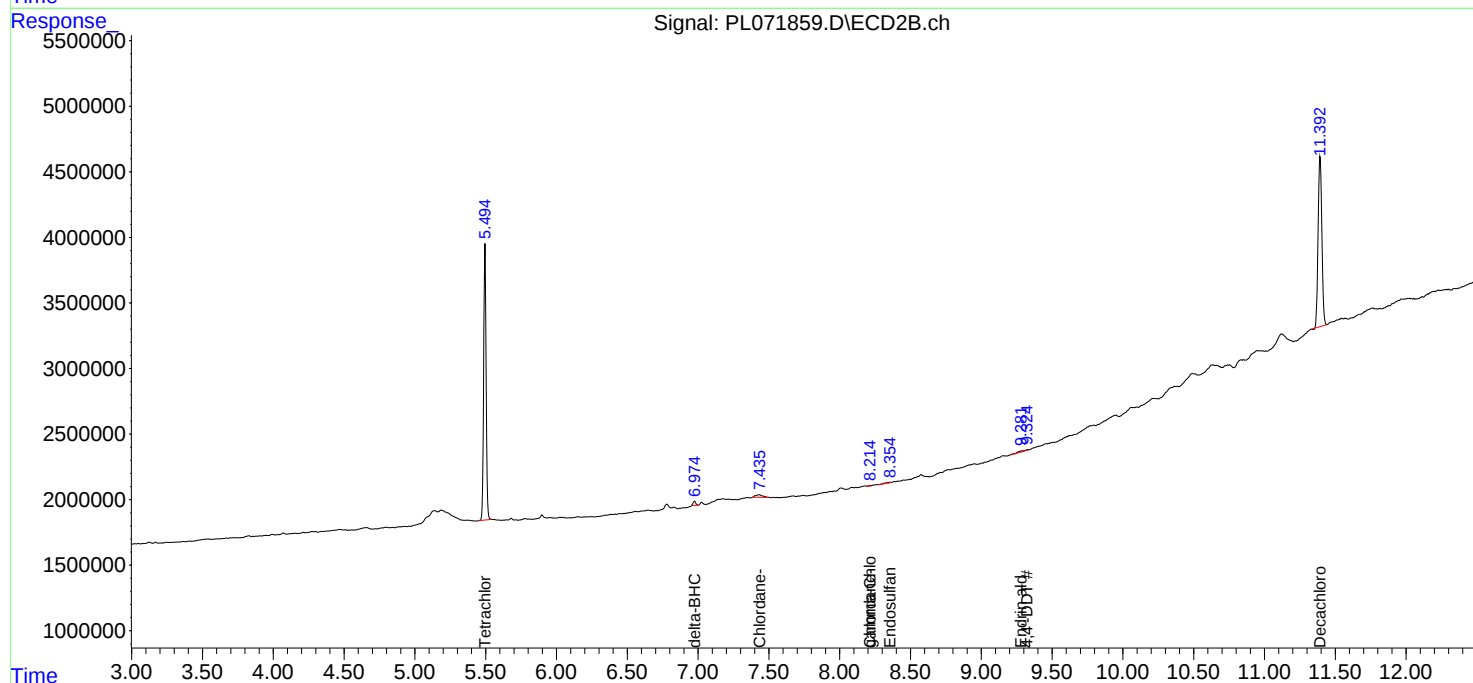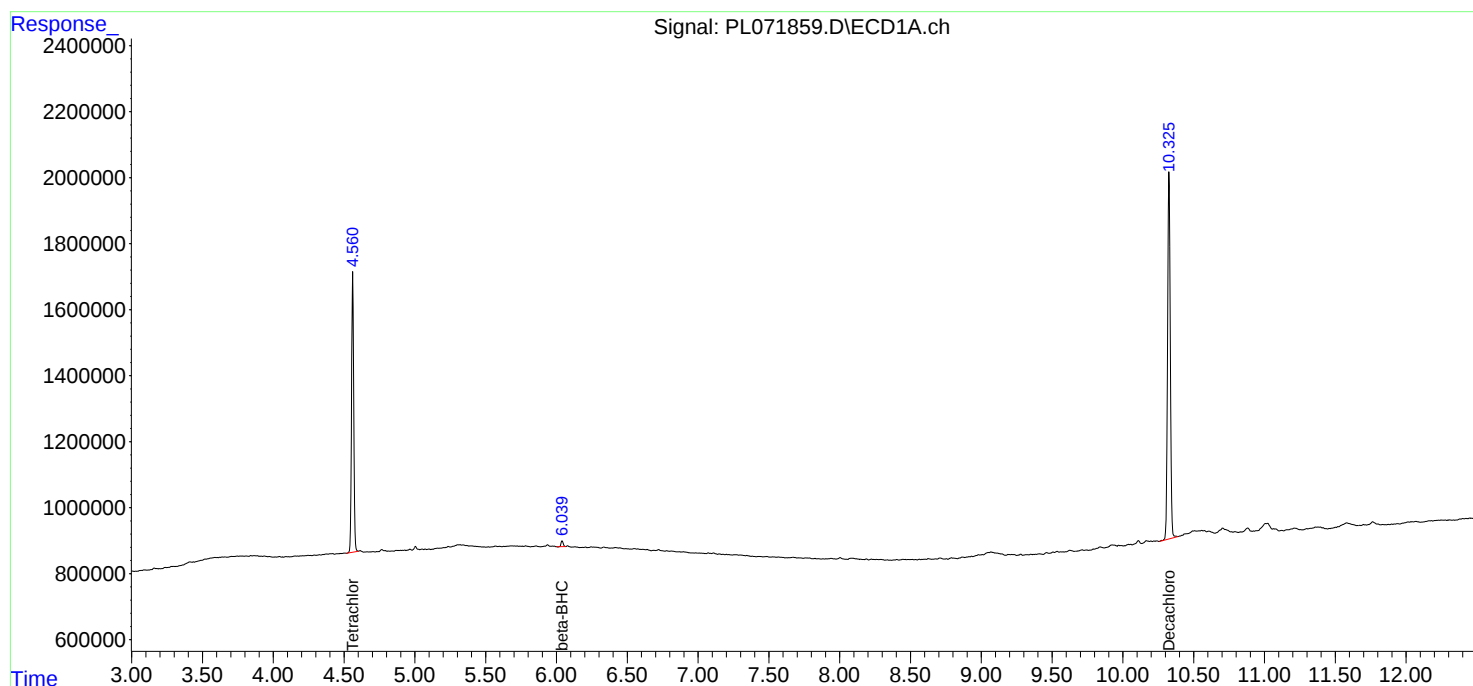


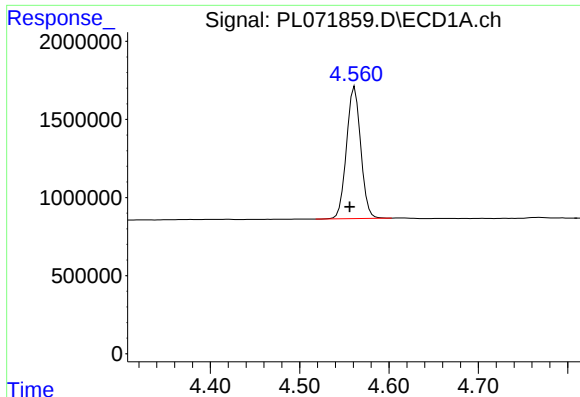

#1 Tetrachloro-m-xylene


R.T.: 4.562 min
Delta R.T.: 0.006 min
Response: 9352409
Conc: 20.25 ng/ml

Instrument :
ECD_L
ClientSampleId :

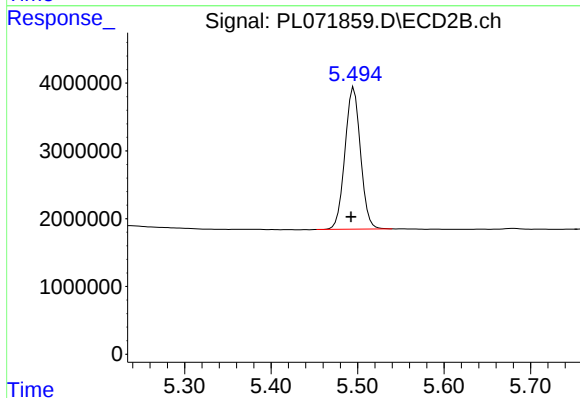


#1 Tetrachloro-m-xylene

R.T.: 5.496 min
Delta R.T.: 0.003 min
Response: 26028333
Conc: 21.18 ng/ml

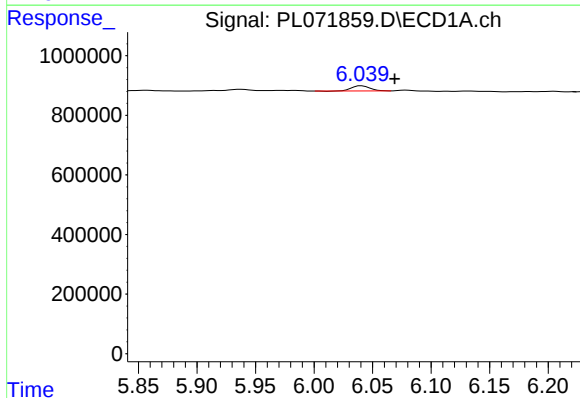


#6 beta-BHC

R.T.: 6.041 min
Delta R.T.: -0.028 min
Response: 184306
Conc: 0.68 ng/ml

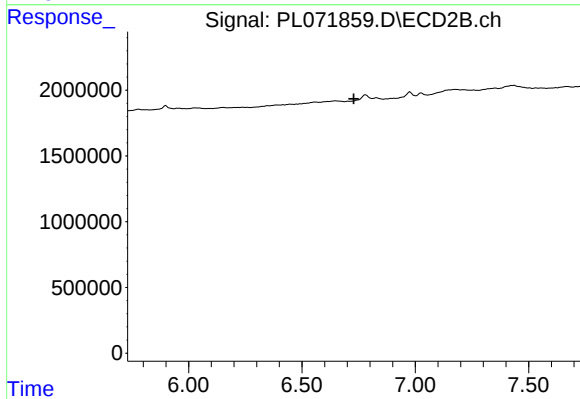

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 6.729 min
Response: 0
Conc: N.D.

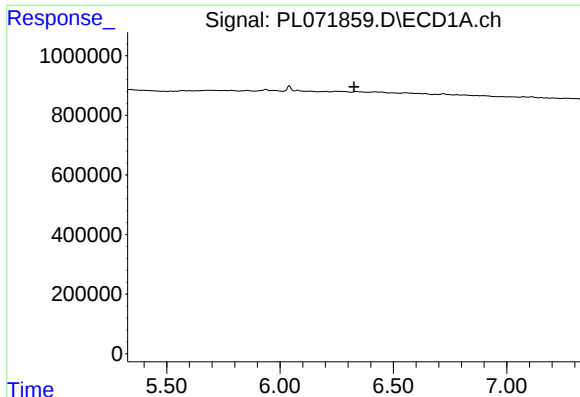

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.327 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

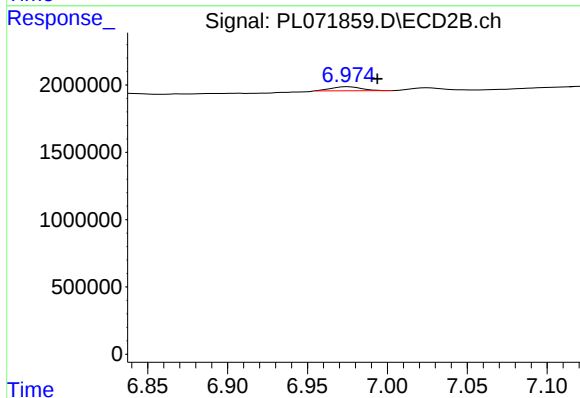


#7 delta-BHC

R.T.: 6.975 min
Delta R.T.: -0.018 min
Response: 404855
Conc: 0.26 ng/ml

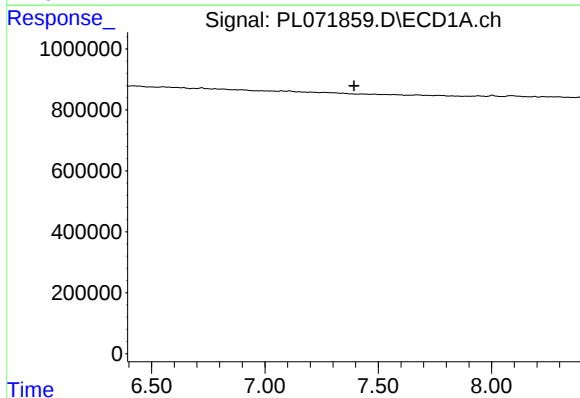


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

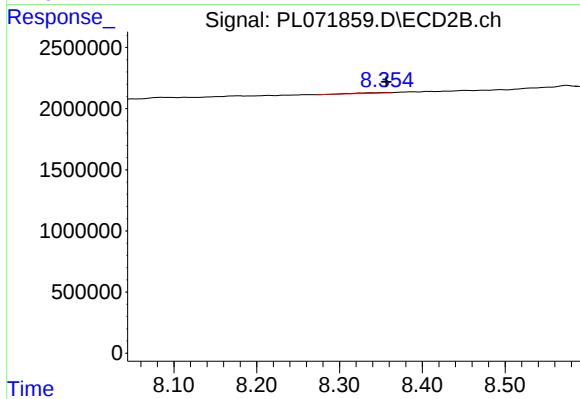

#9 Endosulfan I


R.T.: 8.355 min
Delta R.T.: -0.002 min
Response: 118621
Conc: 0.10 ng/ml

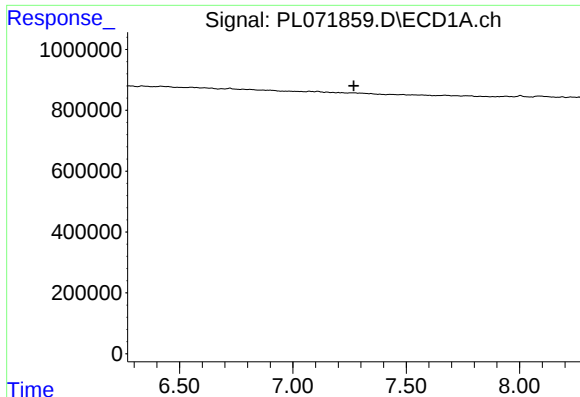

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

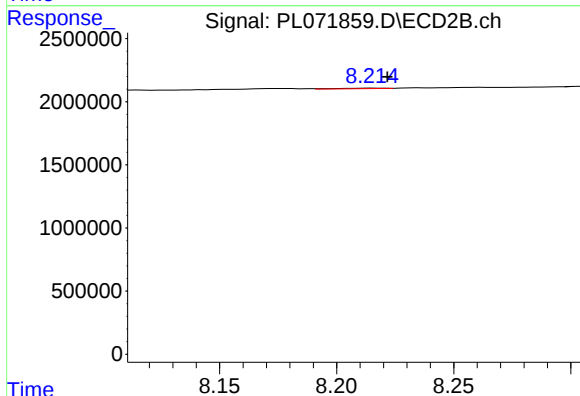


#10 gamma-Chlordane

R.T.: 8.216 min
Delta R.T.: -0.006 min
Response: 59462
Conc: 0.04 ng/ml

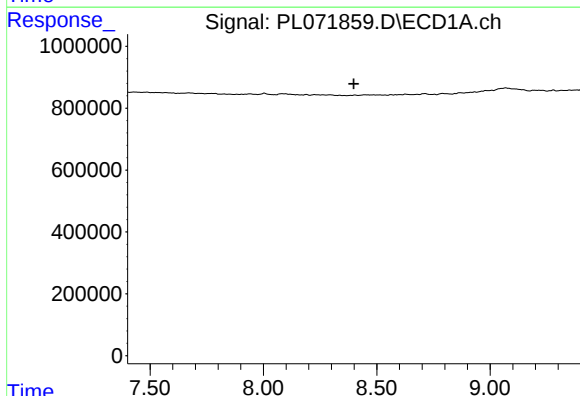


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

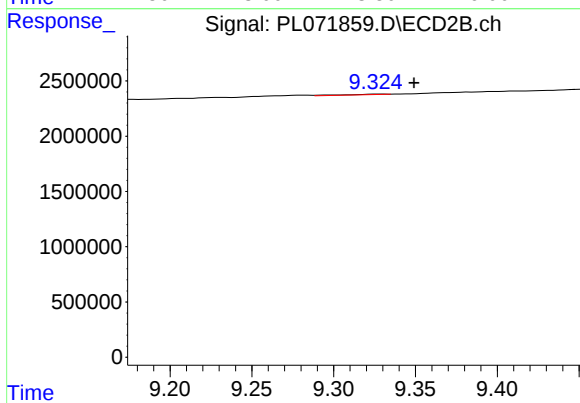

#17 4,4'-DDT


R.T.: 9.327 min
Delta R.T.: -0.022 min
Response: 80549
Conc: 0.09 ng/ml

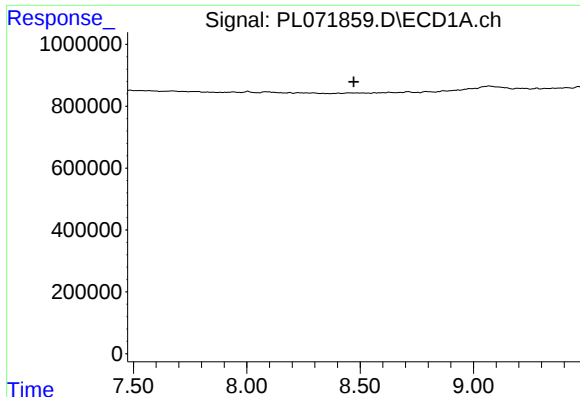

#18 Endrin aldehyde


R.T.: 0.000 min
Exp R.T.: 8.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

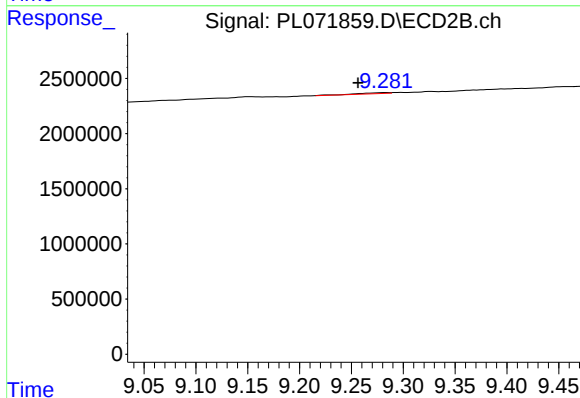


#18 Endrin aldehyde

R.T.: 9.283 min
Delta R.T.: 0.026 min
Response: 191419
Conc: 0.23 ng/ml

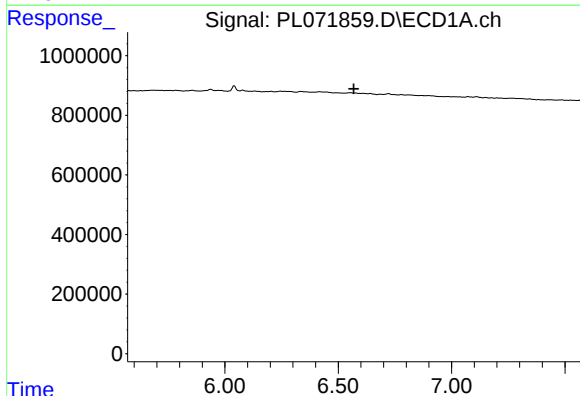


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T.: 6.569 min
Response: 0
Conc: N.D.

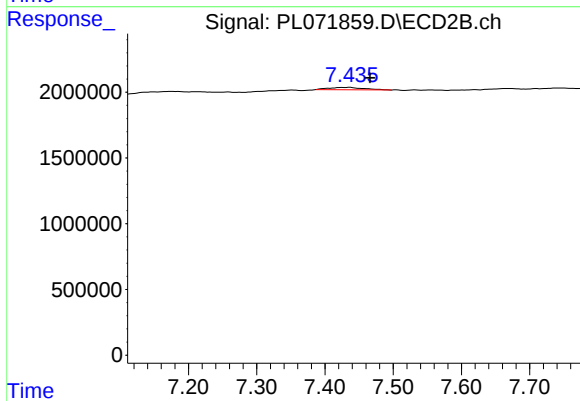

#24 Chlordane-2


R.T.: 7.437 min
Delta R.T.: -0.030 min
Response: 662499
Conc: 12.24 ng/ml

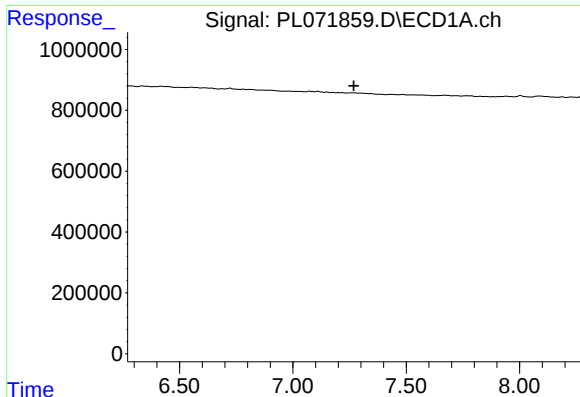

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

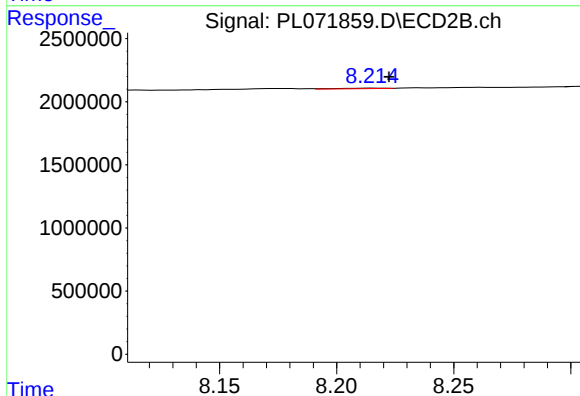


#25 Chlordane-3

R.T.: 8.216 min
Delta R.T.: -0.007 min
Response: 59462
Conc: 0.29 ng/ml

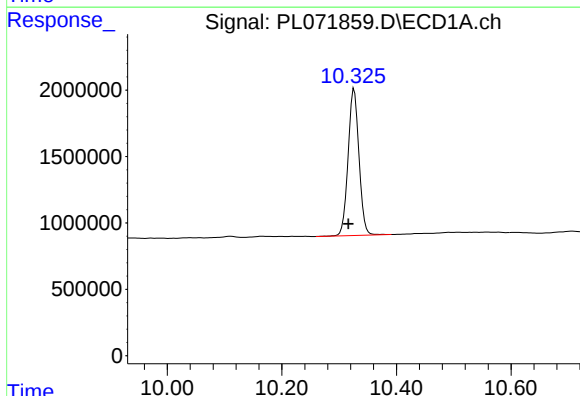

#28 Decachlorobiphenyl

R.T.: 10.326 min
Delta R.T.: 0.010 min
Response: 14695110
Conc: 20.32 ng/ml

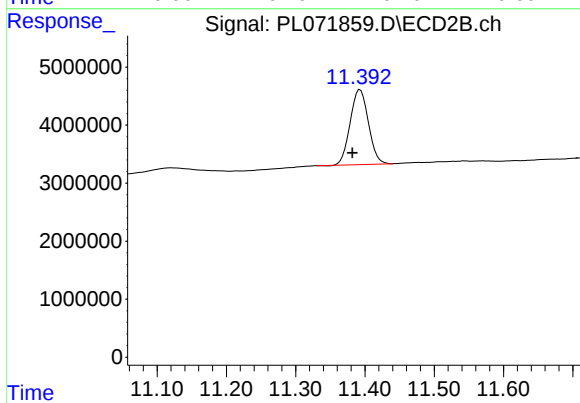

#28 Decachlorobiphenyl

R.T.: 11.393 min
Delta R.T.: 0.011 min
Response: 23616673
Conc: 19.93 ng/ml