

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010722\
 Data File : PL071869.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2022 15:37
 Operator : AR\AJ
 Sample : N1065-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 23:38:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.559	5.495	10884007	29123632	23.561	23.704
28)	SA Decachlor...	10.322	11.391	11231262	20481494	15.534	17.284
Target Compounds							
5)	MB Aldrin	0.000	7.490	0	202527	N.D.	0.131 #
7)	B delta-BHC	0.000	6.975f	0	315517	N.D.	0.206 #
8)	B Heptachlo...	0.000	7.930f	0	193057	N.D.	0.138 #
11)	B alpha-Chl...	0.000	8.314	0	181512	N.D.	0.136 #
12)	B 4,4'-DDE	0.000	8.500	0	248152	N.D.	0.197 #
15)	B Endosulfa...	0.000	9.092f	0	1732518	N.D.	1.543 #
16)	A 4,4'-DDD	0.000	9.029	0	781559	N.D.	0.813 #
17)	MA 4,4'-DDT	0.000	9.353	0	671597	N.D.	0.712 #
22)	Mirex	0.000	10.458	0	2662160	N.D.	3.099 #
24)	Chlordane-2	0.000	7.490f	0	202527	N.D.	3.742 #
26)	Chlordane-4	0.000	8.314	0	181512	N.D.	0.746 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010722\
Data File : PL071869.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2022 15:37
Operator : AR\AJ
Sample : N1065-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 23:38:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

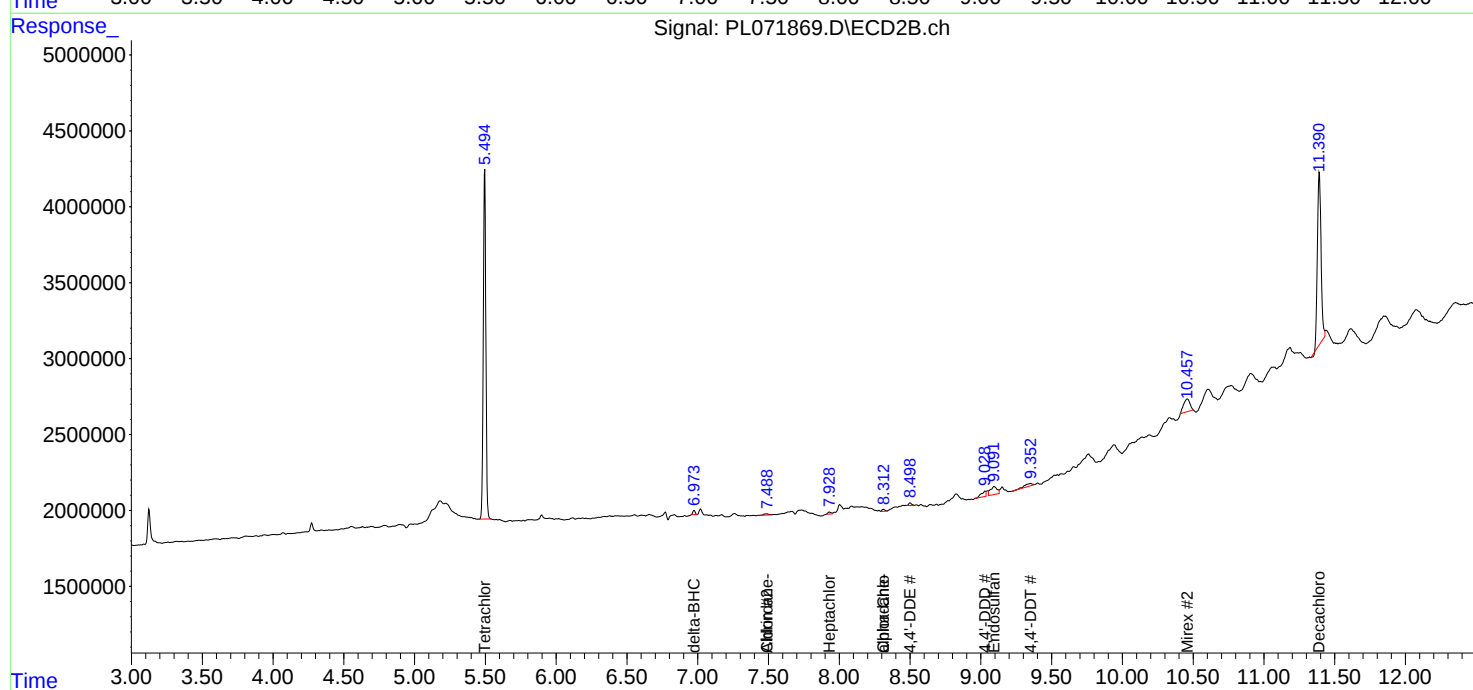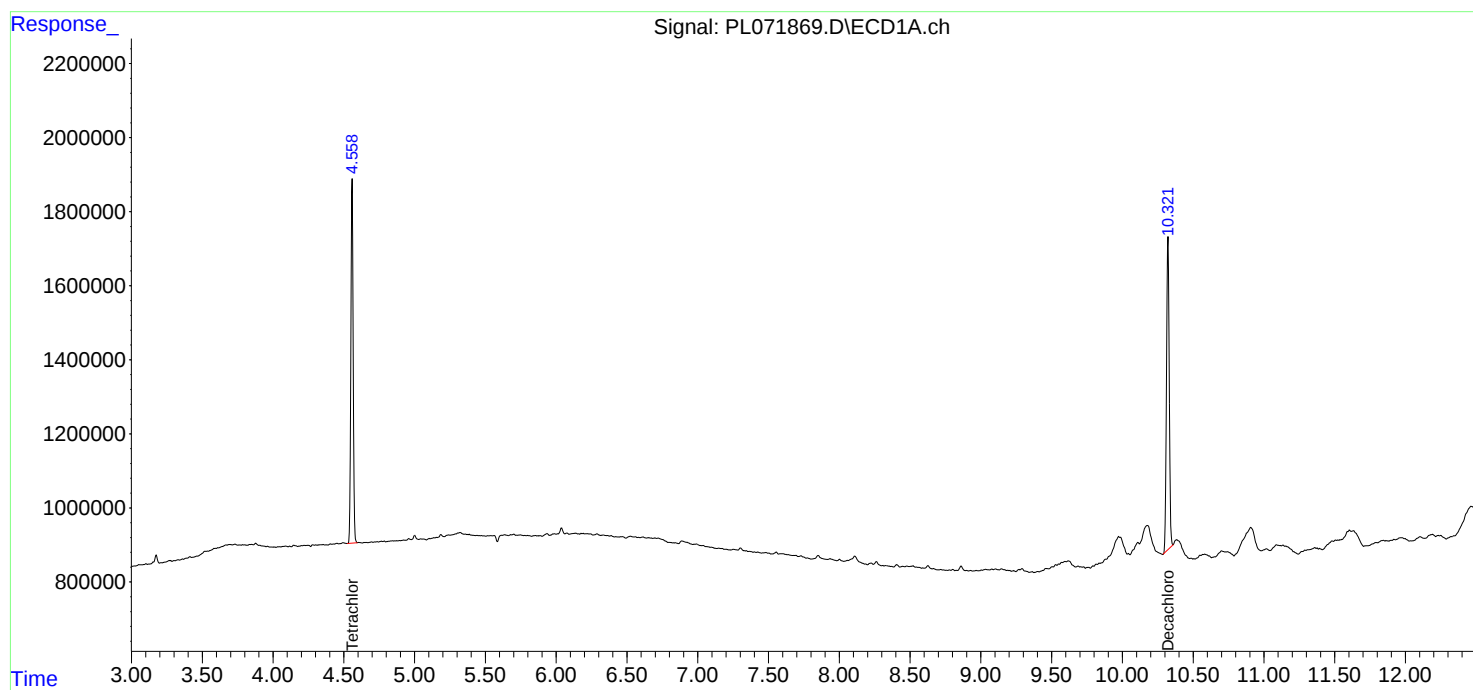


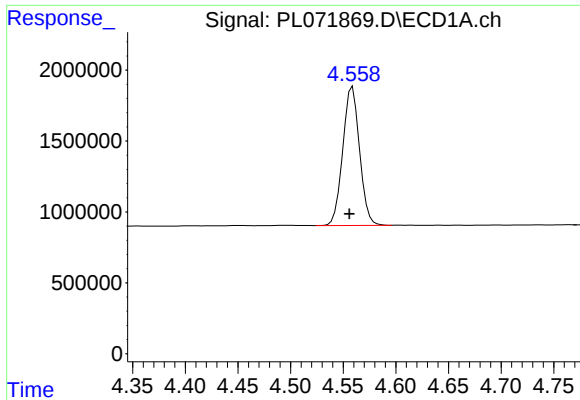

#1 Tetrachloro-m-xylene


R.T.: 4.559 min
Delta R.T.: 0.003 min
Response: 10884007
Conc: 23.56 ng/ml

Instrument :
ECD_L
ClientSampleId :

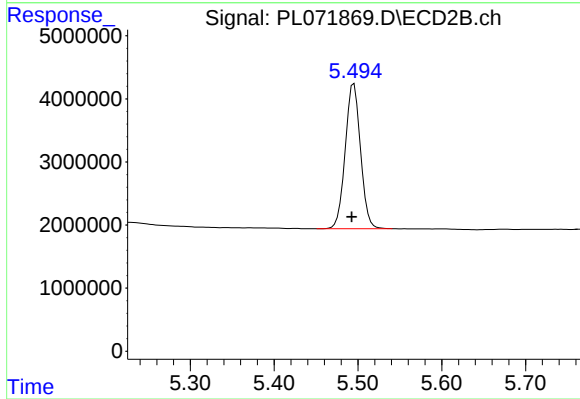


#1 Tetrachloro-m-xylene

R.T.: 5.495 min
Delta R.T.: 0.003 min
Response: 29123632
Conc: 23.70 ng/ml

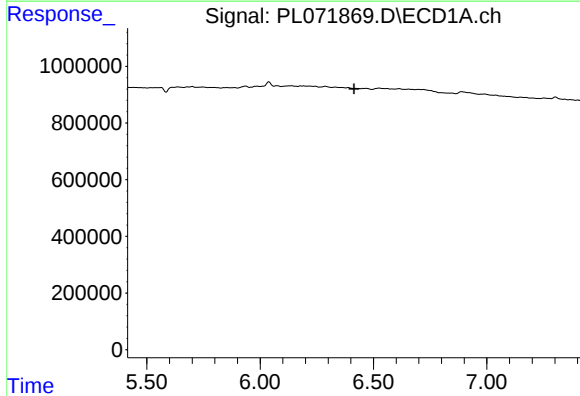


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.414 min
Response: 0
Conc: N.D.

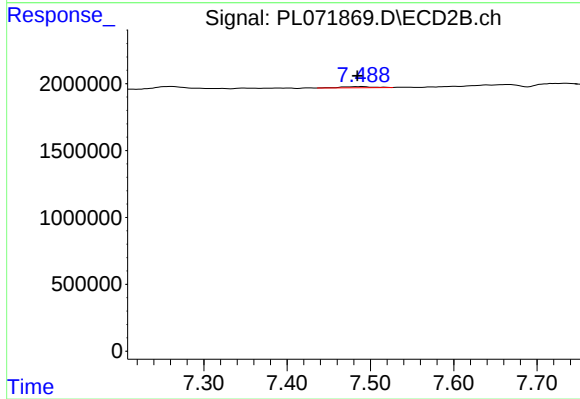

#5 Aldrin


R.T.: 7.490 min
Delta R.T.: 0.006 min
Response: 202527
Conc: 0.13 ng/ml

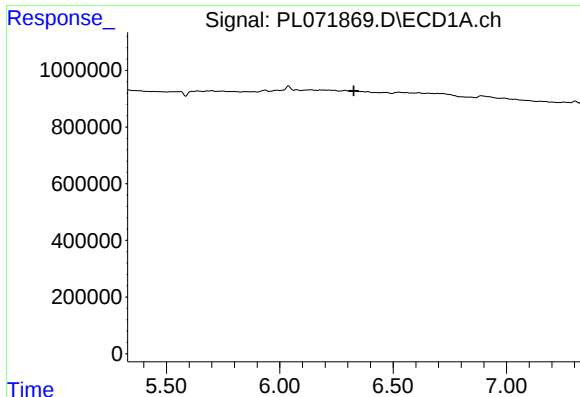

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 6.327 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

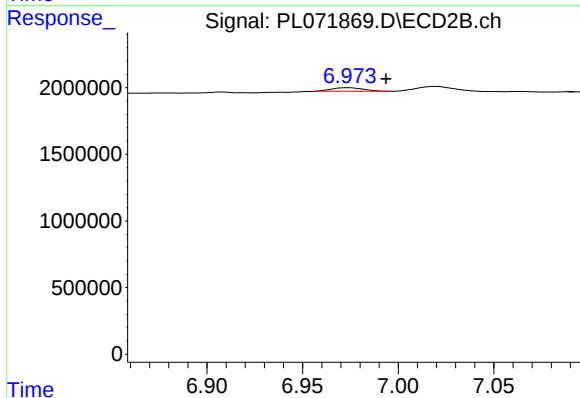


#7 delta-BHC

R.T.: 6.975 min
Delta R.T.: -0.019 min
Response: 315517
Conc: 0.21 ng/ml

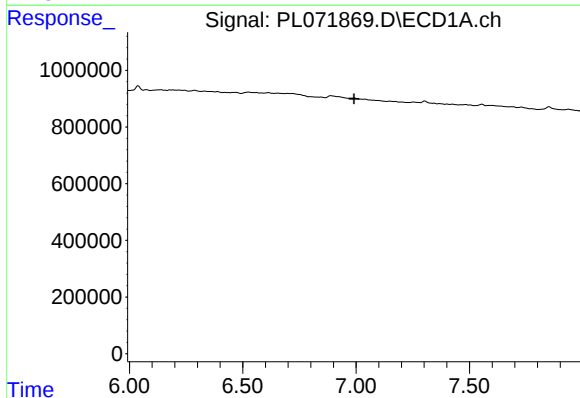


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 6.992 min
Response: 0
Conc: N.D.

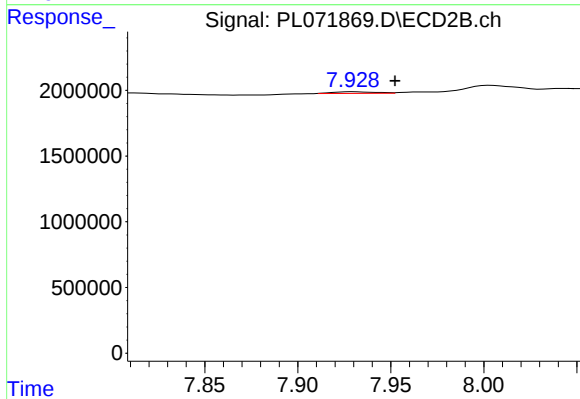

#8 Heptachlor epoxide


R.T.: 7.930 min
Delta R.T.: -0.023 min
Response: 193057
Conc: 0.14 ng/ml

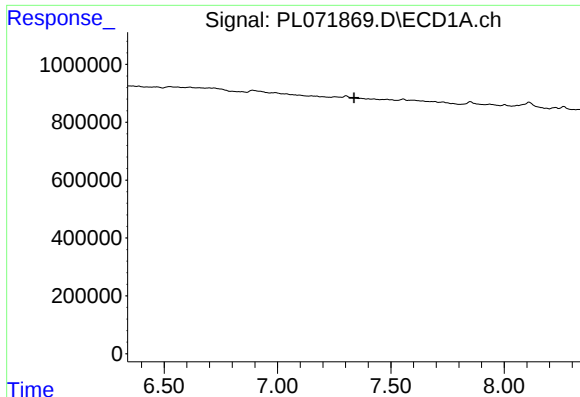

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

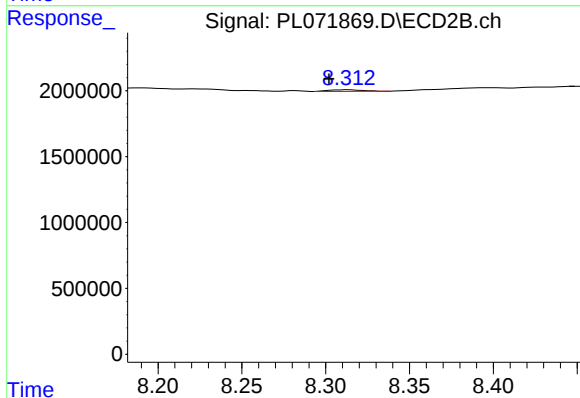


#11 alpha-Chlordane

R.T.: 8.314 min
Delta R.T.: 0.012 min
Response: 181512
Conc: 0.14 ng/ml

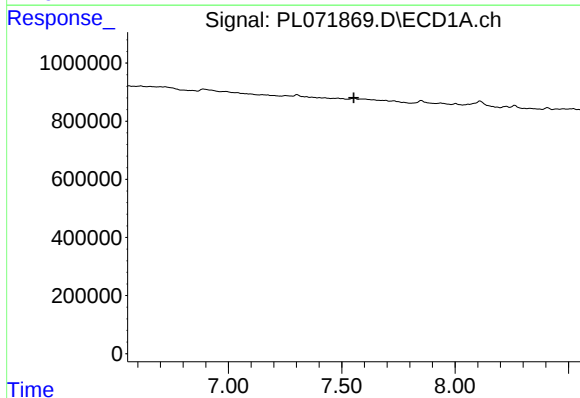


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 7.553 min
Response: 0
Conc: N.D.

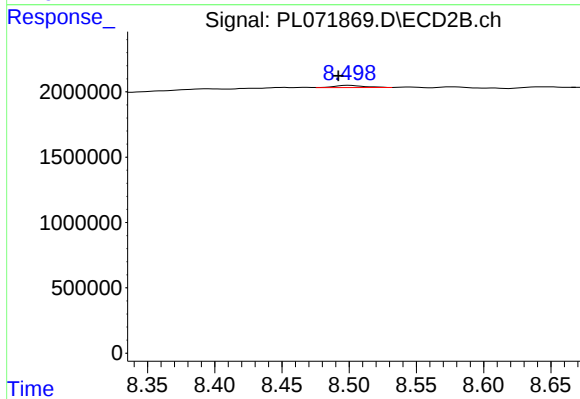

#12 4,4'-DDE


R.T.: 8.500 min
Delta R.T.: 0.008 min
Response: 248152
Conc: 0.20 ng/ml

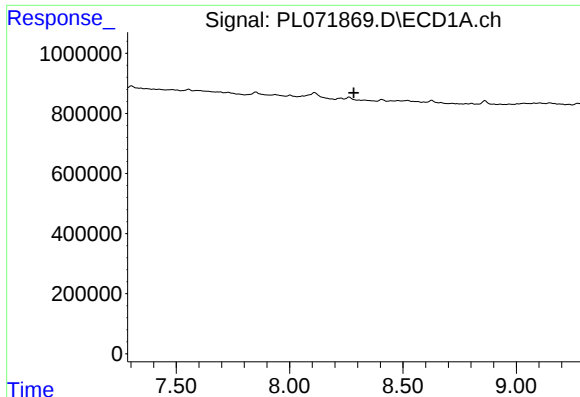

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

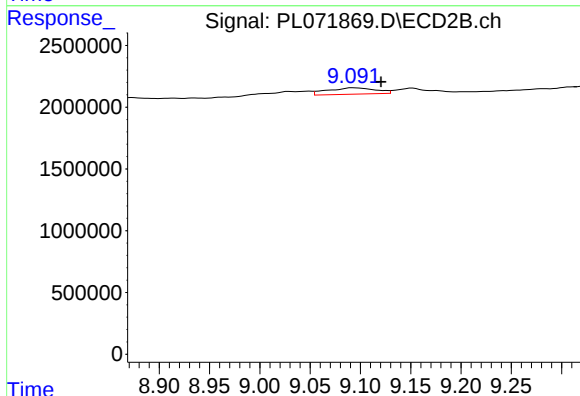


#15 Endosulfan II

R.T.: 9.092 min
Delta R.T.: -0.028 min
Response: 1732518
Conc: 1.54 ng/ml

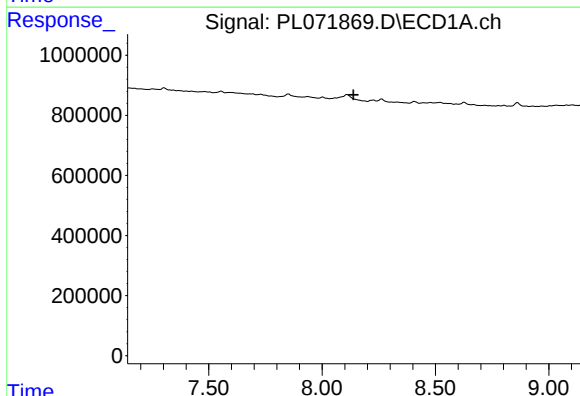


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T.: 8.139 min
Response: 0
Conc: N.D.

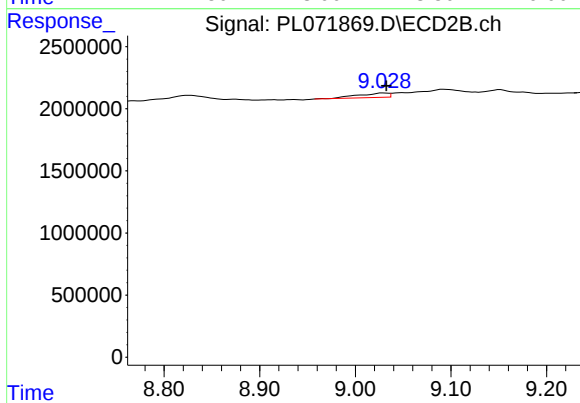

#16 4,4'-DDD


R.T.: 9.029 min
Delta R.T.: -0.003 min
Response: 781559
Conc: 0.81 ng/ml

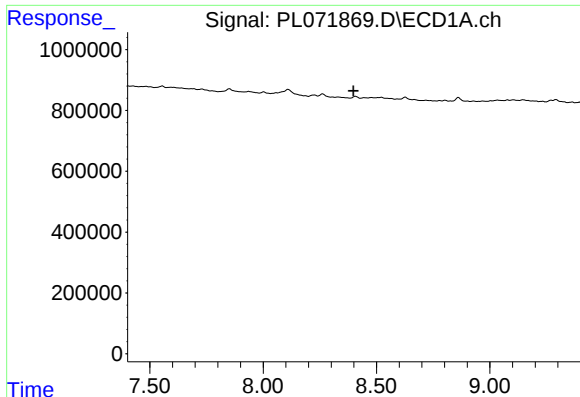

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

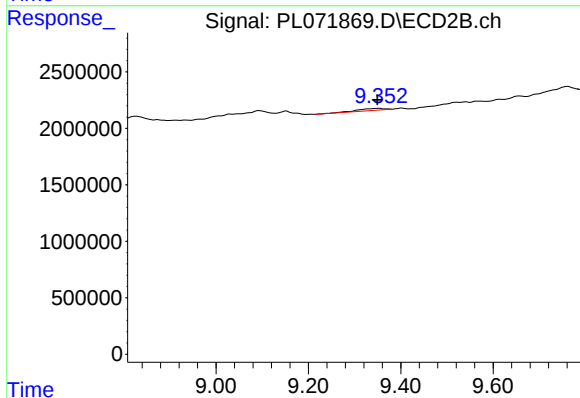


#17 4,4'-DDT

R.T.: 9.353 min
Delta R.T.: 0.003 min
Response: 671597
Conc: 0.71 ng/ml

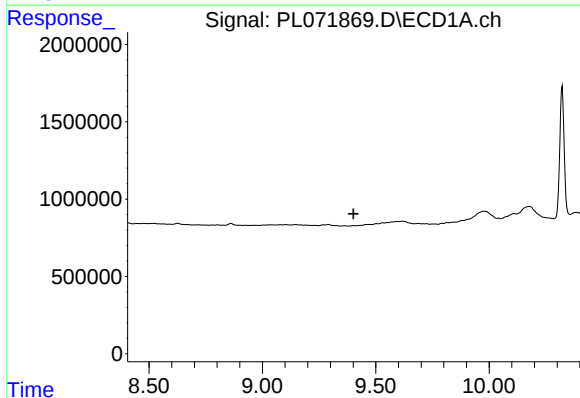


#22 Mirex

R.T.: 0.000 min
Exp R.T.: 9.402 min
Response: 0
Conc: N.D.

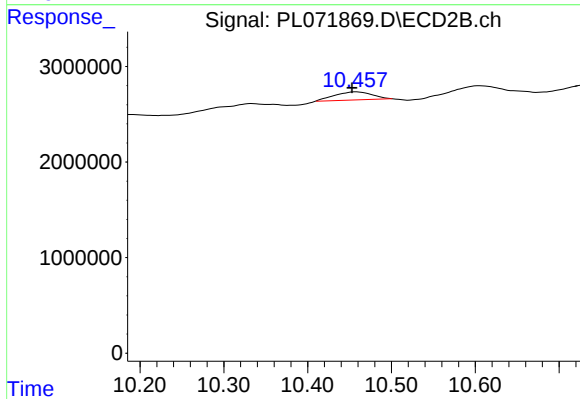

#22 Mirex


R.T.: 10.458 min
Delta R.T.: 0.005 min
Response: 2662160
Conc: 3.10 ng/ml

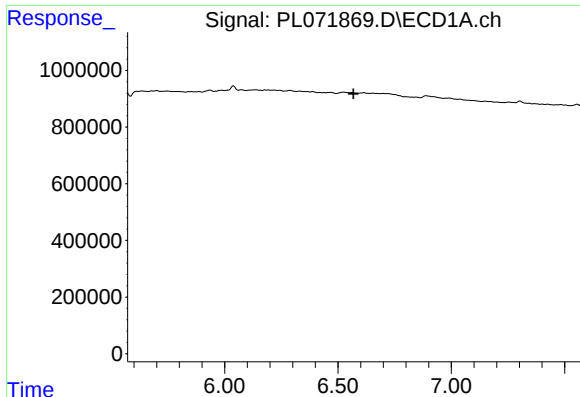

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 6.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

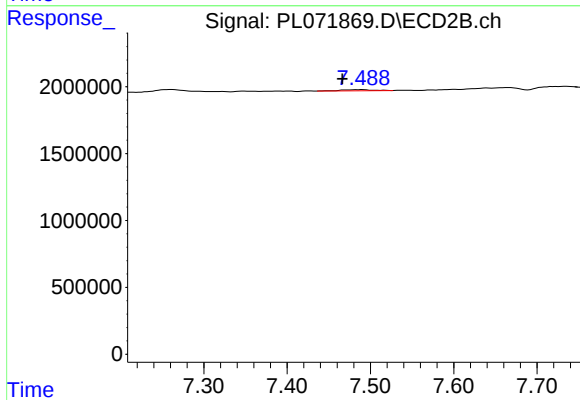


#24 Chlordane-2

R.T.: 7.490 min
Delta R.T.: 0.024 min
Response: 202527
Conc: 3.74 ng/ml

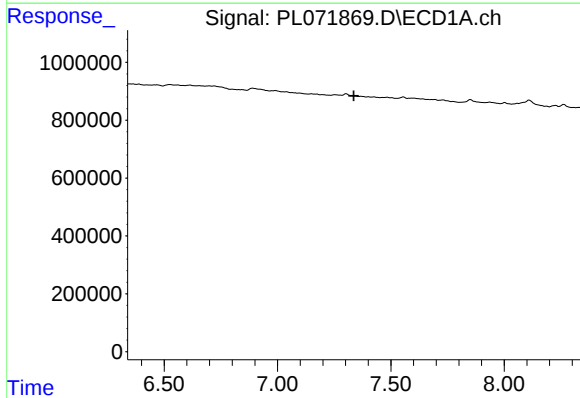


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.336 min
Response: 0
Conc: N.D.

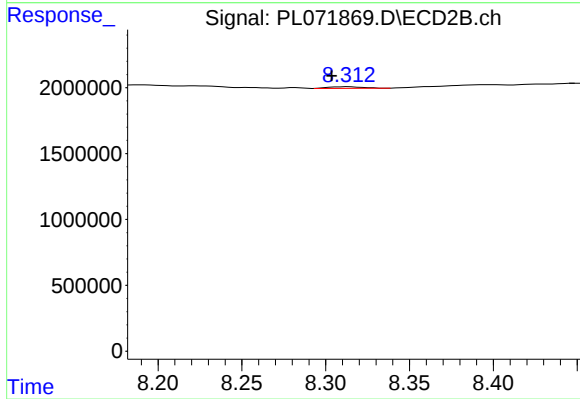

#26 Chlordane-4


R.T.: 8.314 min
Delta R.T.: 0.010 min
Response: 181512
Conc: 0.75 ng/ml

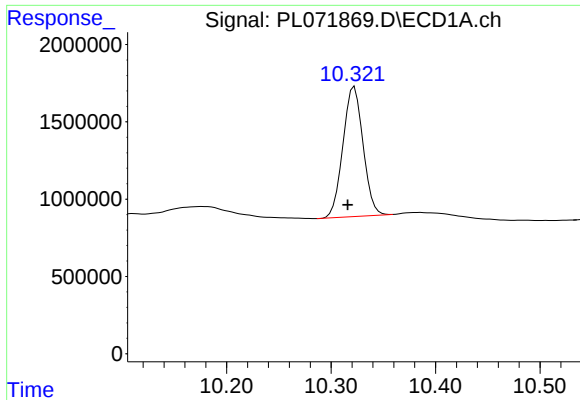

#28 Decachlorobiphenyl

R.T.: 10.322 min
Delta R.T.: 0.006 min
Response: 11231262
Conc: 15.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

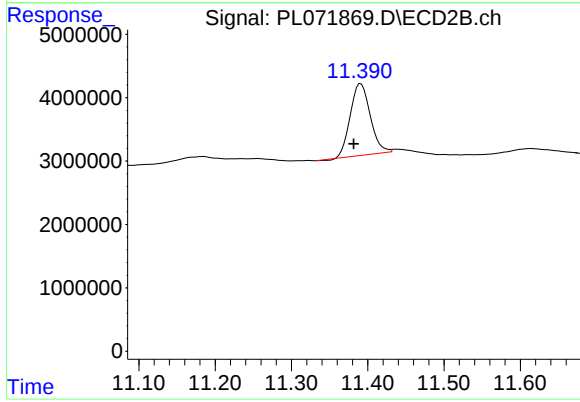

#28 Decachlorobiphenyl

R.T.: 11.391 min
Delta R.T.: 0.009 min
Response: 20481494
Conc: 17.28 ng/ml