

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010722\
 Data File : PL071881.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2022 18:53
 Operator : AR\AJ
 Sample : N1065-38
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 23:42:36 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.494	10569396	29195154	22.880	23.762
28)	SA Decachlor...	10.321	11.389	16966699	29173045	23.466	24.618
Target Compounds							
7)	B delta-BHC	0.000	6.973f	0	374389	N.D.	0.244 #
9)	A Endosulfan I	0.000	8.351	0	28011	N.D.	0.023 #
10)	B gamma-Chl...	0.000	8.227	0	428293	N.D.	0.313 #
11)	B alpha-Chl...	0.000	8.309	0	647640	N.D.	0.487 #
12)	B 4,4'-DDE	0.000	8.497	0	258395	N.D.	0.205 #
15)	B Endosulfa...	0.000	9.094f	0	329204	N.D.	0.293 #
17)	MA 4,4'-DDT	0.000	9.356	0	123608	N.D.	0.131 #
25)	Chlordane-3	0.000	8.227	0	428293	N.D.	2.098 #
26)	Chlordane-4	0.000	8.309	0	647640	N.D.	2.661 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010722\
Data File : PL071881.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2022 18:53
Operator : AR\AJ
Sample : N1065-38
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 23:42:36 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

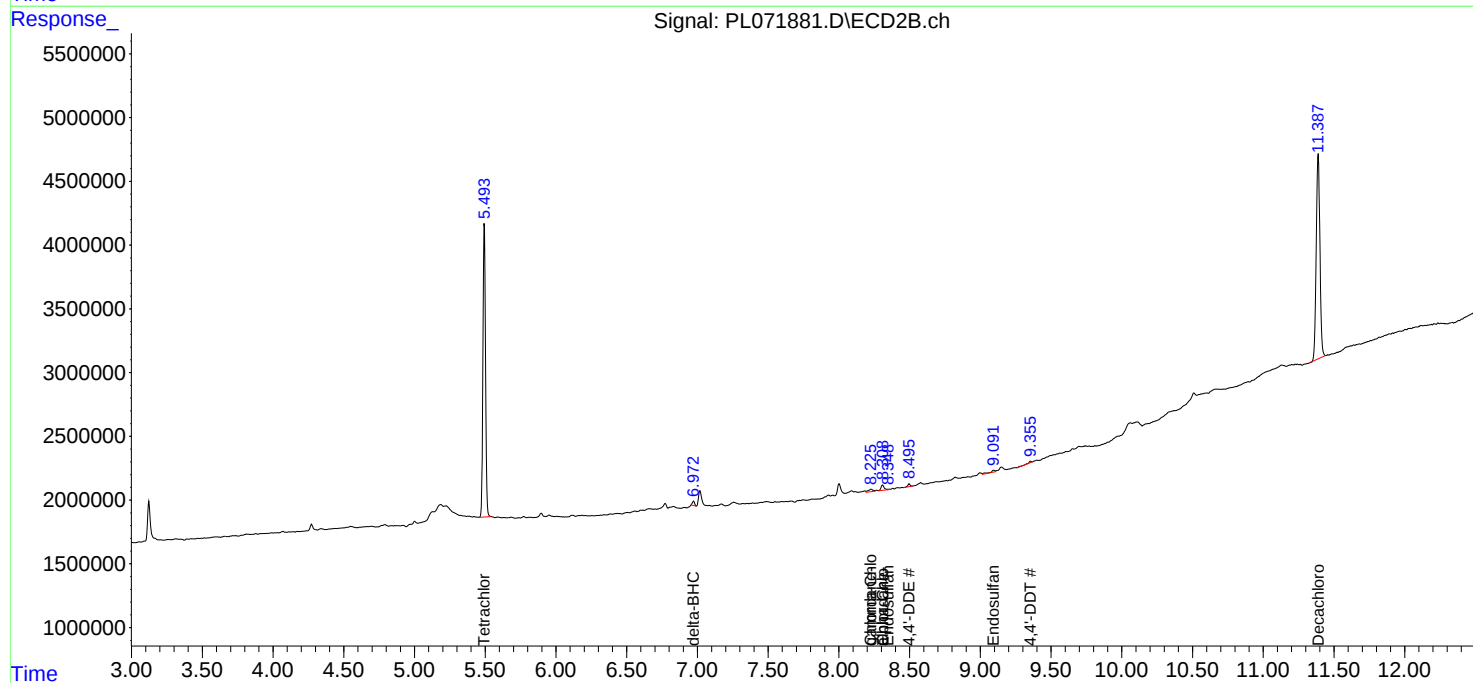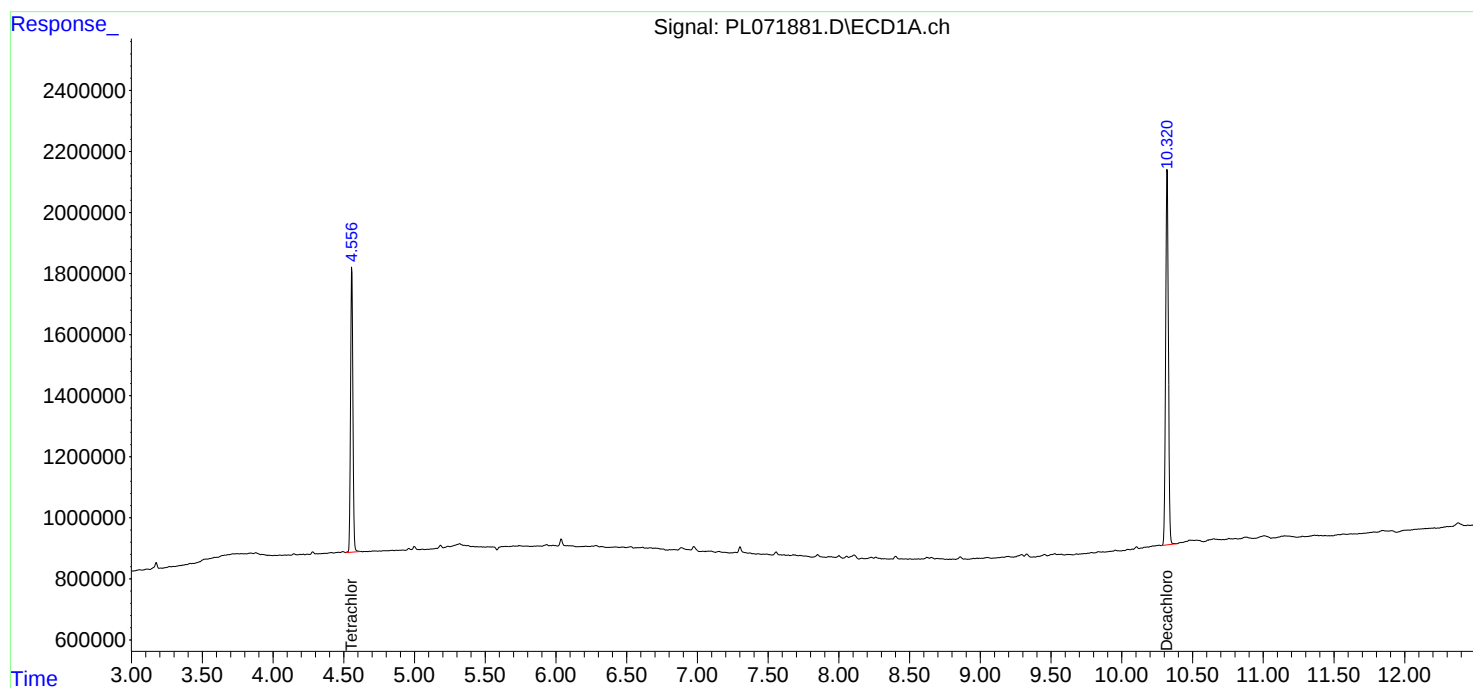


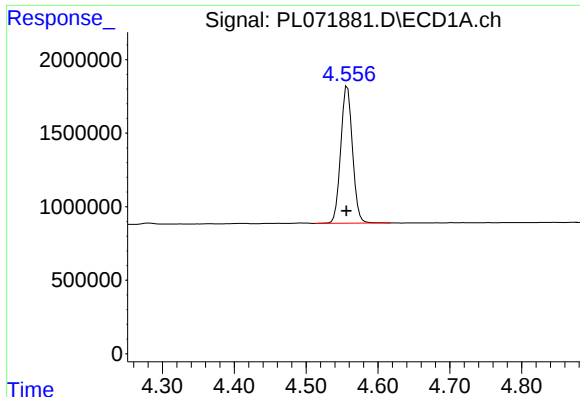

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: 0.002 min
Response: 10569396
Conc: 22.88 ng/ml

Instrument :
ECD_L
ClientSampleId :

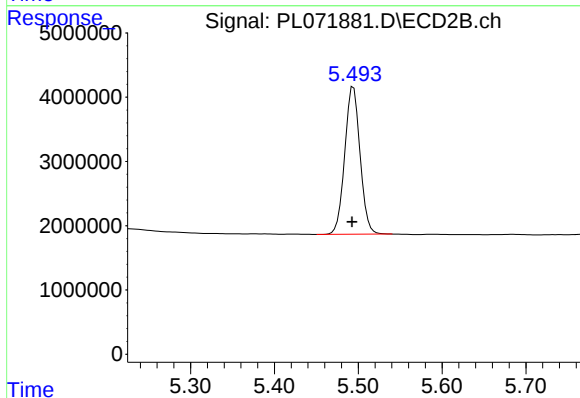


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.002 min
Response: 29195154
Conc: 23.76 ng/ml

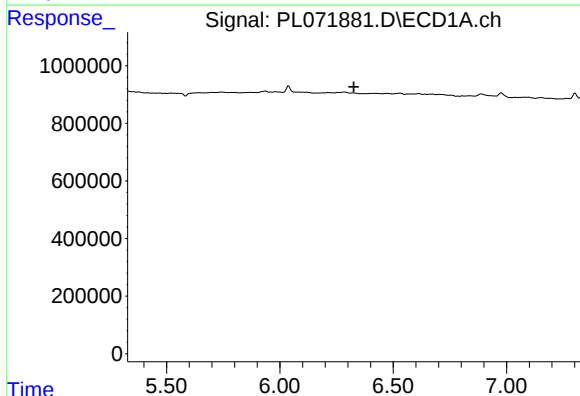


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

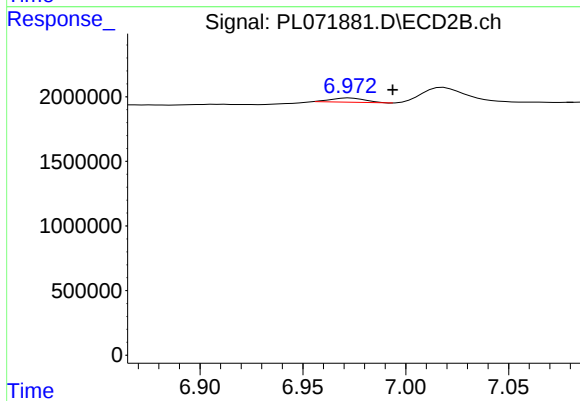

#7 delta-BHC


R.T.: 6.973 min
Delta R.T.: -0.021 min
Response: 374389
Conc: 0.24 ng/ml

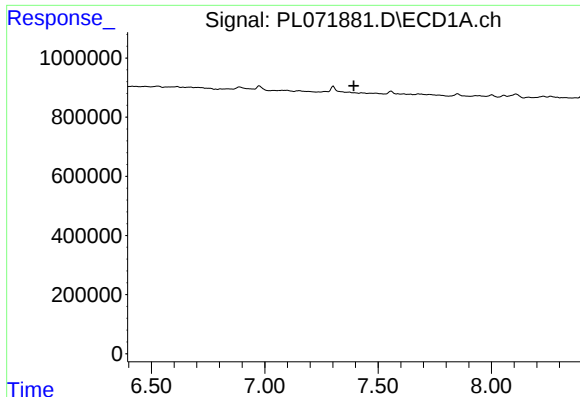

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 7.393 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

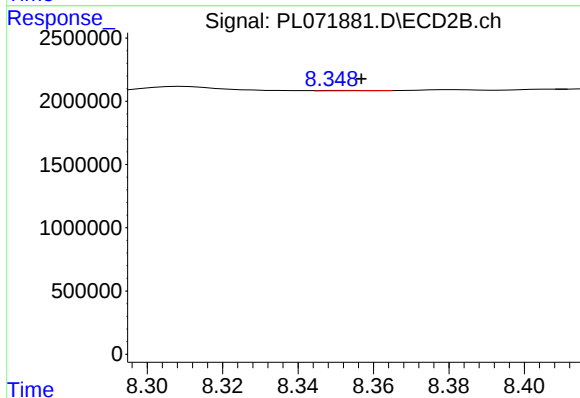


#9 Endosulfan I

R.T.: 8.351 min
Delta R.T.: -0.006 min
Response: 28011
Conc: 0.02 ng/ml

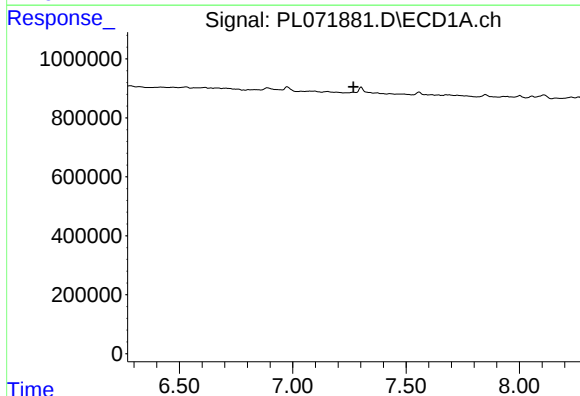


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

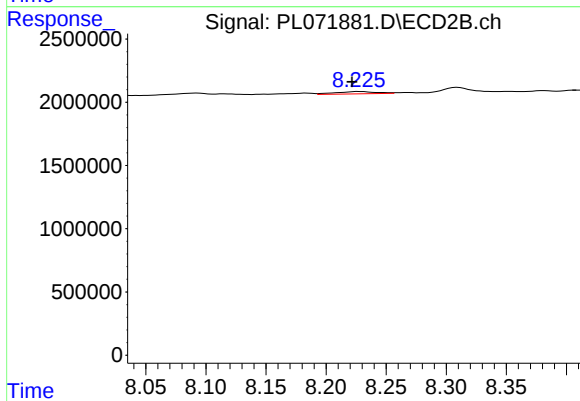

#10 gamma-Chlordane


R.T.: 8.227 min
Delta R.T.: 0.005 min
Response: 428293
Conc: 0.31 ng/ml

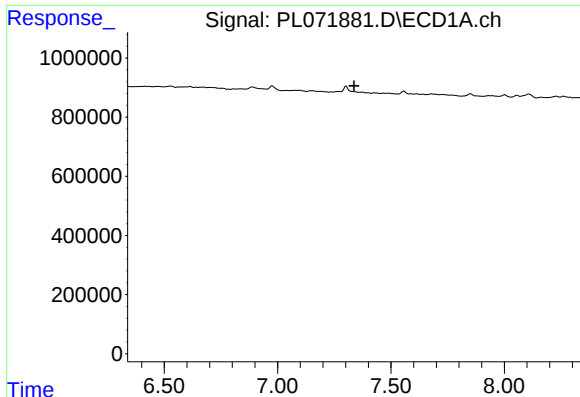

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

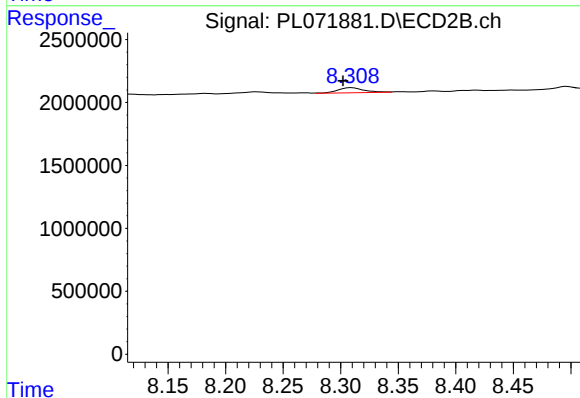


#11 alpha-Chlordane

R.T.: 8.309 min
Delta R.T.: 0.007 min
Response: 647640
Conc: 0.49 ng/ml

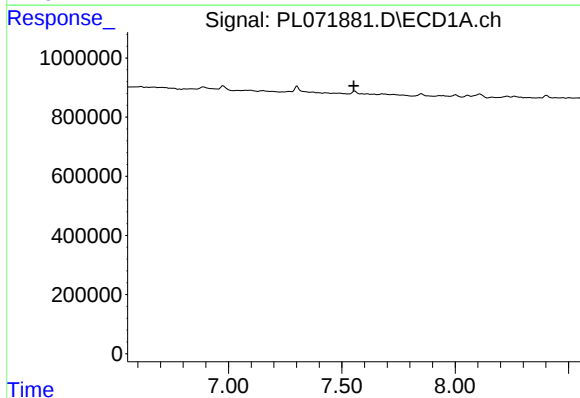


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T.: 7.553 min
Response: 0
Conc: N.D.

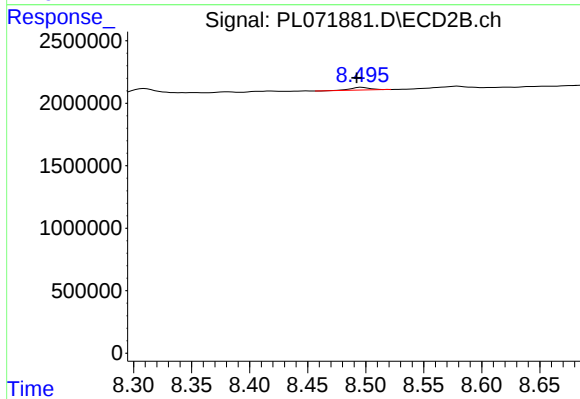

#12 4,4'-DDE


R.T.: 8.497 min
Delta R.T.: 0.005 min
Response: 258395
Conc: 0.21 ng/ml

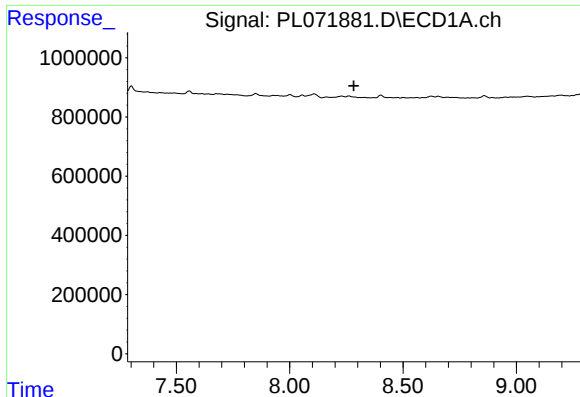

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

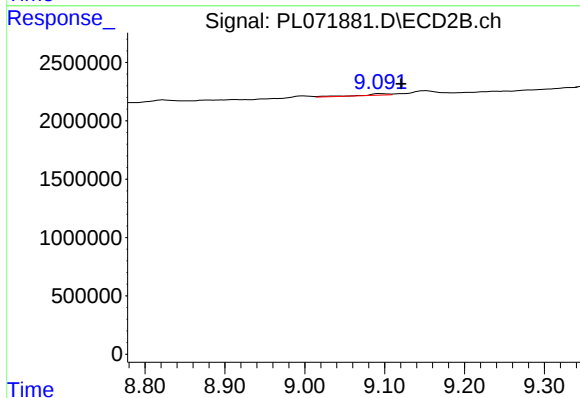


#15 Endosulfan II

R.T.: 9.094 min
Delta R.T.: -0.027 min
Response: 329204
Conc: 0.29 ng/ml

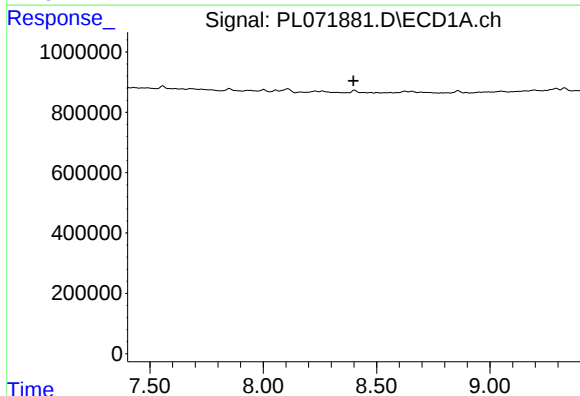


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T.: 8.398 min
Response: 0
Conc: N.D.

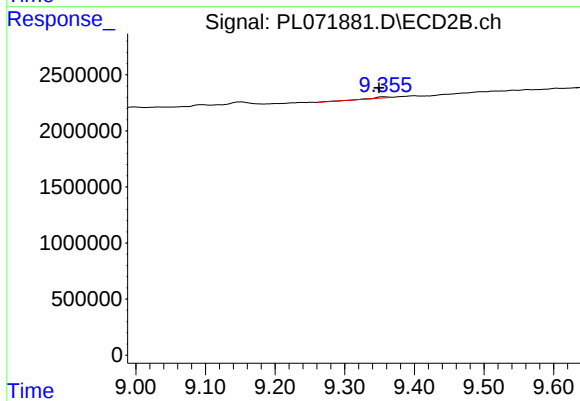

#17 4,4'-DDT


R.T.: 9.356 min
Delta R.T.: 0.007 min
Response: 123608
Conc: 0.13 ng/ml

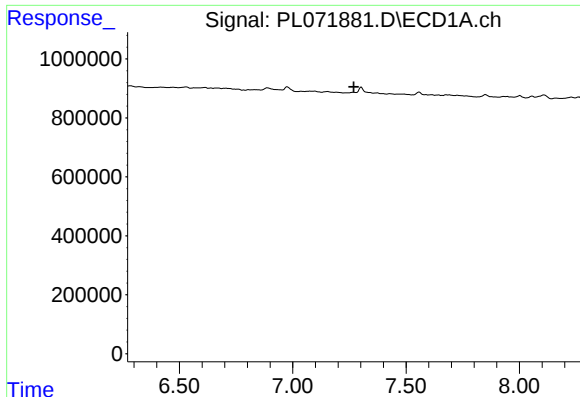

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

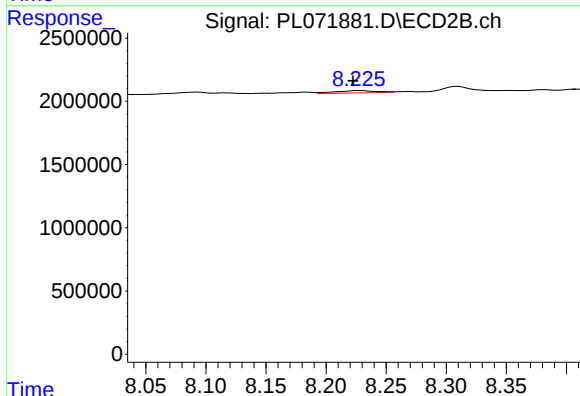


#25 Chlordane-3

R.T.: 8.227 min
Delta R.T.: 0.005 min
Response: 428293
Conc: 2.10 ng/ml

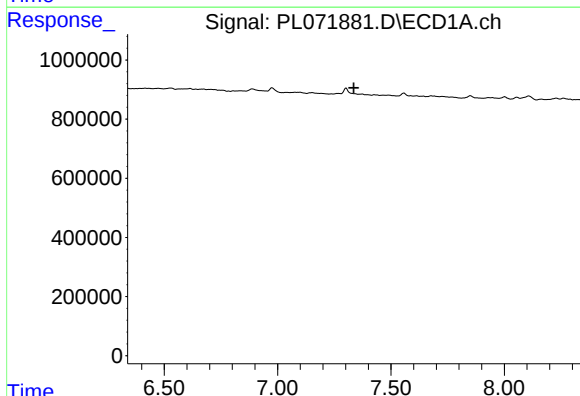


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 7.336 min
Response: 0
Conc: N.D.

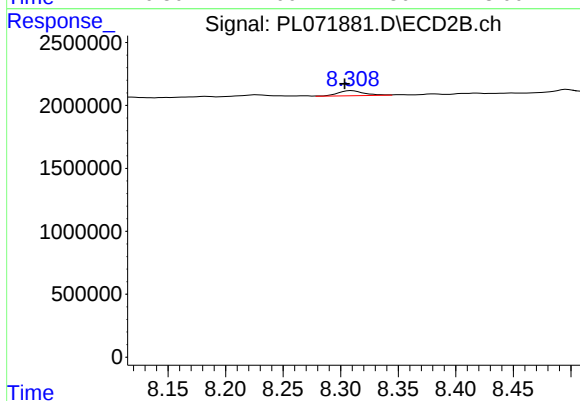

#26 Chlordane-4


R.T.: 8.309 min
Delta R.T.: 0.006 min
Response: 647640
Conc: 2.66 ng/ml

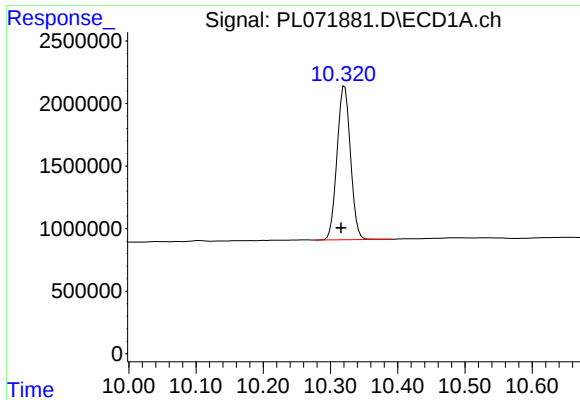

#28 Decachlorobiphenyl

R.T.: 10.321 min
Delta R.T.: 0.005 min
Response: 16966699
Conc: 23.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

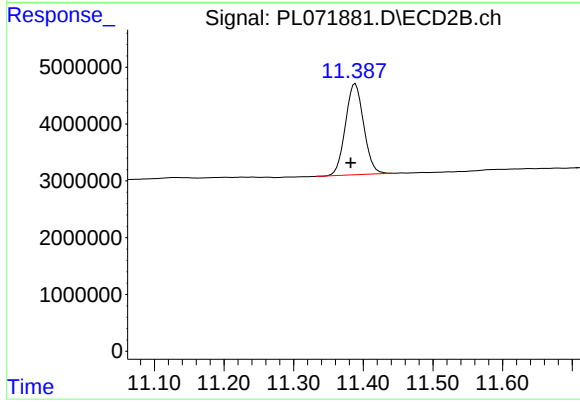

#28 Decachlorobiphenyl

R.T.: 11.389 min
Delta R.T.: 0.007 min
Response: 29173045
Conc: 24.62 ng/ml