

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010722\
 Data File : PL071890.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Jan 2022 22:23
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 07 23:45:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
 Quant Title : GC Extractables
 QLast Update : Thu Jan 06 10:33:37 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.558	5.494	9442940	26183834	20.442	21.311
28)	SA Decachlor...	10.321	11.388	13854841	24107471	19.162	20.344
Target Compounds							
5)	MB Aldrin	0.000	7.493	0	160931	N.D.	0.104 #
7)	B delta-BHC	0.000	6.973f	0	379303	N.D.	0.247 #
8)	B Heptachlo...	0.000	7.965	0	244004	N.D.	0.175 #
10)	B gamma-Chl...	0.000	8.221	0	559524	N.D.	0.409 #
11)	B alpha-Chl...	0.000	8.297	0	133344	N.D.	0.100 #
15)	B Endosulfa...	0.000	9.101f	0	1169871	N.D.	1.042 #
21)	B Endrin ke...	0.000	9.968f	0	25268	N.D.	0.022 #
24)	Chlordane-2	0.000	7.493f	0	160931	N.D.	2.973 #
25)	Chlordane-3	0.000	8.221	0	559524	N.D.	2.741 #
26)	Chlordane-4	0.000	8.297	0	133344	N.D.	0.548 #
27)	Chlordane-5	0.000	9.179	0	22581	N.D.	0.564 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL010722\
Data File : PL071890.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Jan 2022 22:23
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 07 23:45:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL010422.M
Quant Title : GC Extractables
QLast Update : Thu Jan 06 10:33:37 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

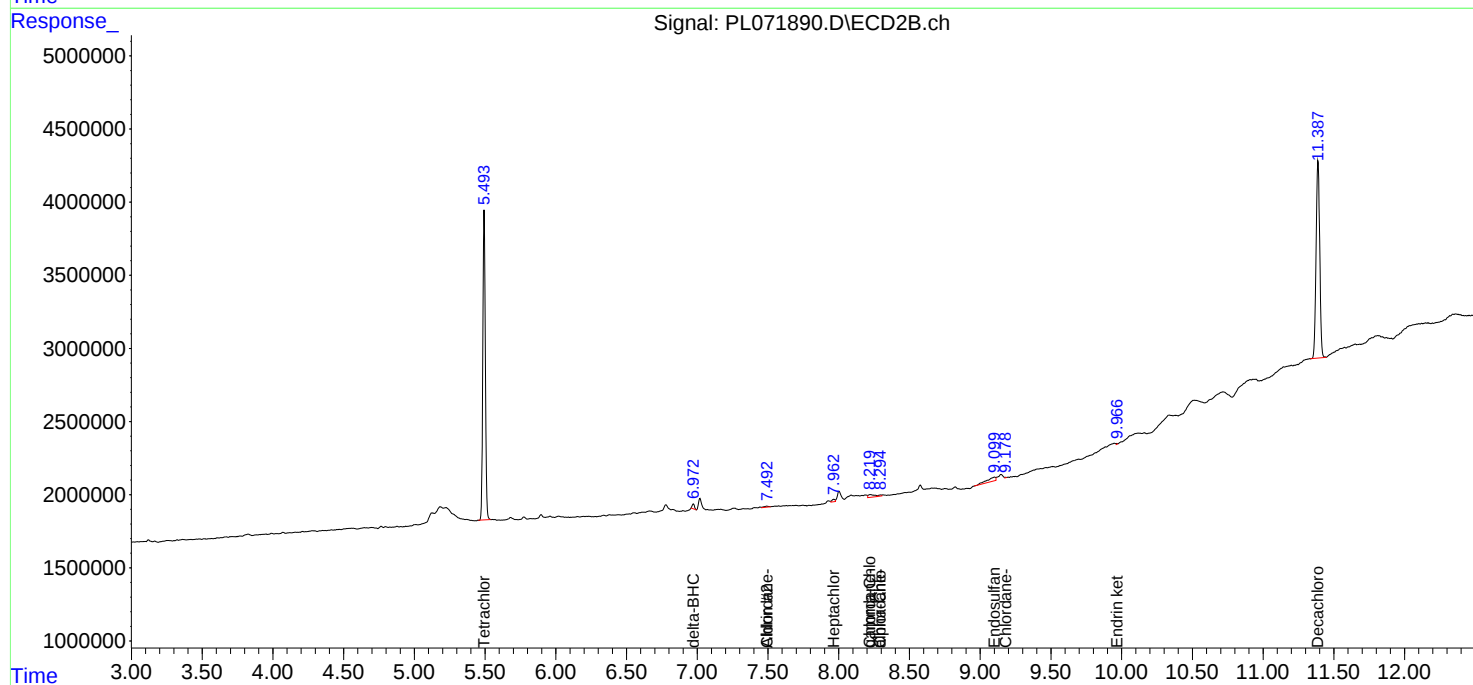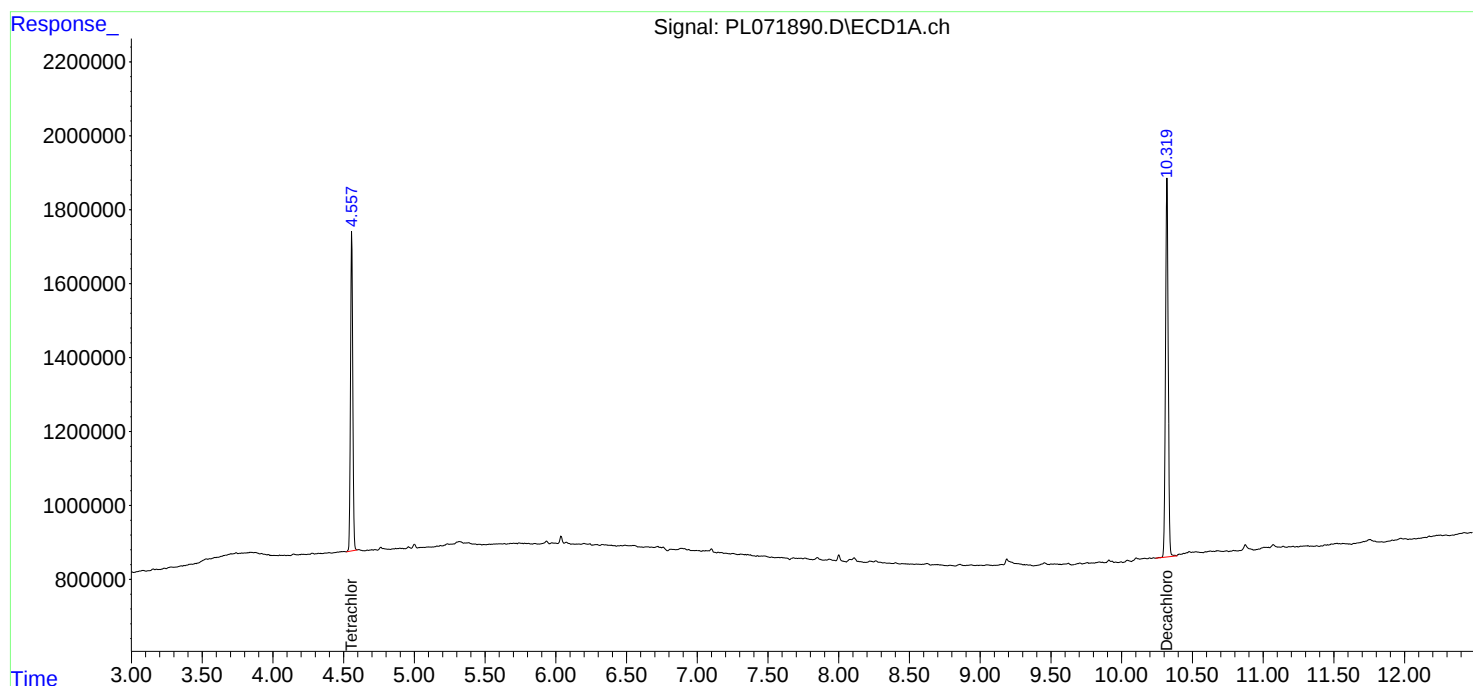


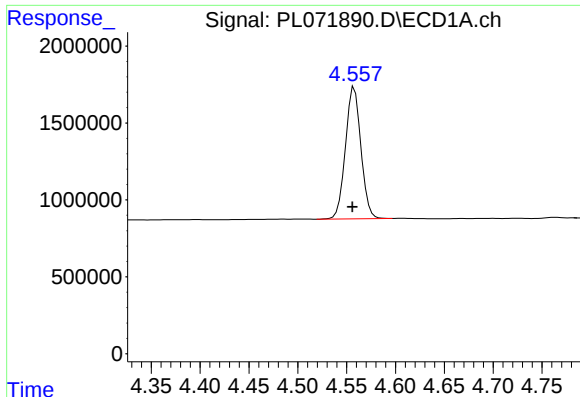

#1 Tetrachloro-m-xylene


R.T.: 4.558 min
Delta R.T.: 0.002 min
Response: 9442940
Conc: 20.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

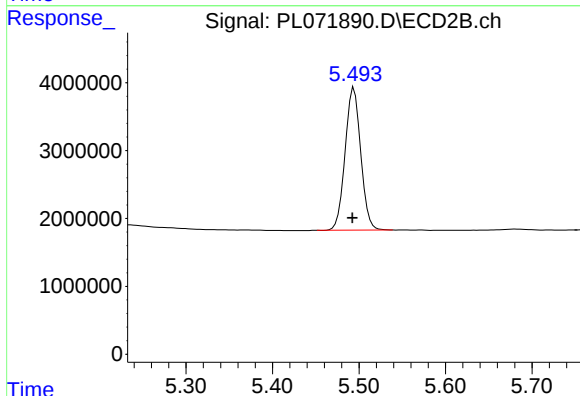


#1 Tetrachloro-m-xylene

R.T.: 5.494 min
Delta R.T.: 0.002 min
Response: 26183834
Conc: 21.31 ng/ml

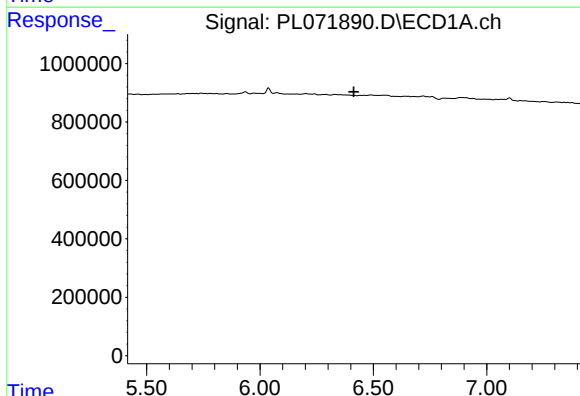


#5 Aldrin

R.T.: 0.000 min
Exp R.T. : 6.414 min
Response: 0
Conc: N.D.

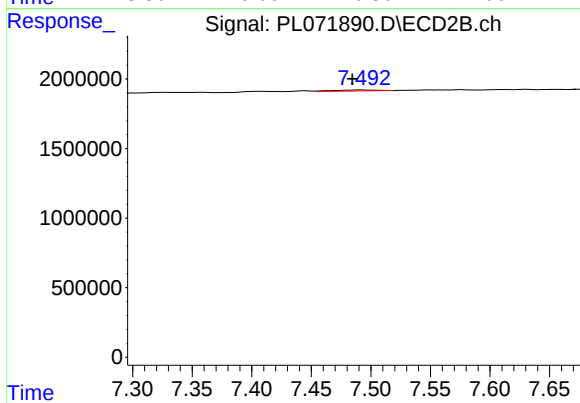

#5 Aldrin


R.T.: 7.493 min
Delta R.T.: 0.009 min
Response: 160931
Conc: 0.10 ng/ml

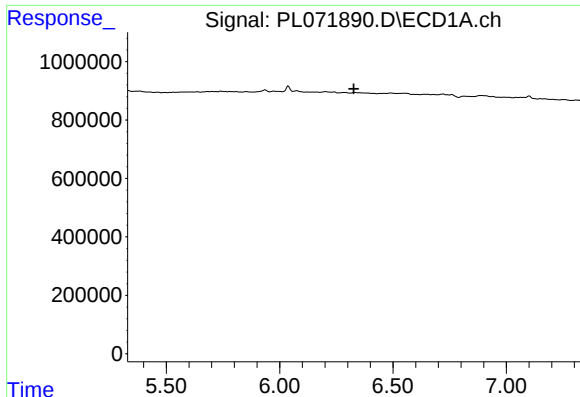

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 6.327 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

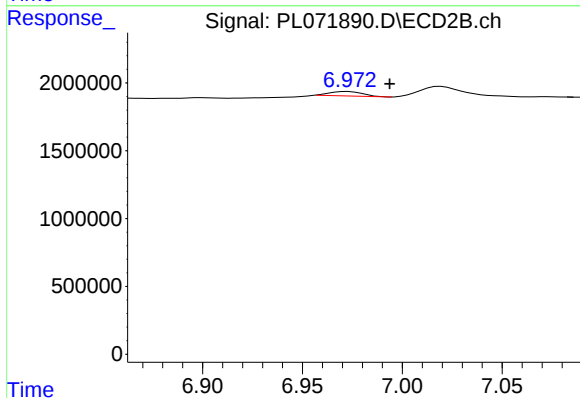


#7 delta-BHC

R.T.: 6.973 min
Delta R.T.: -0.021 min
Response: 379303
Conc: 0.25 ng/ml

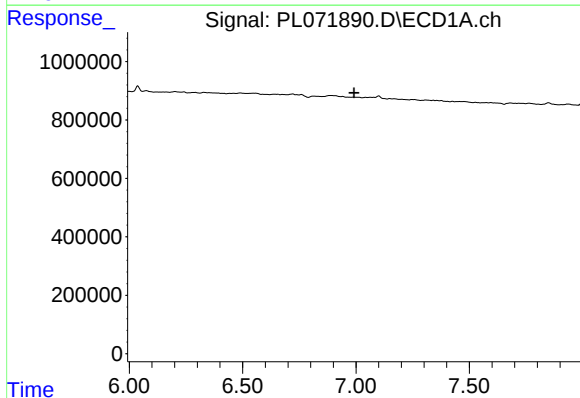


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 6.992 min
Response: 0
Conc: N.D.

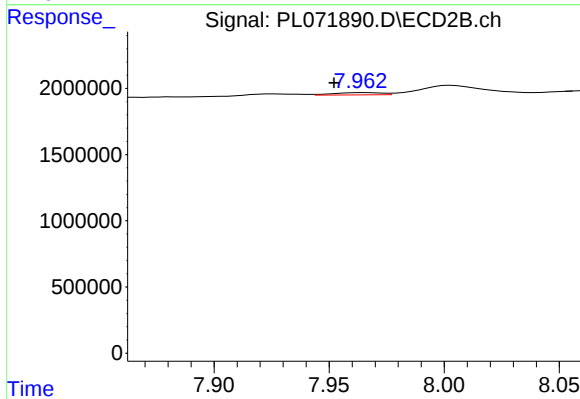

#8 Heptachlor epoxide


R.T.: 7.965 min
Delta R.T.: 0.013 min
Response: 244004
Conc: 0.17 ng/ml

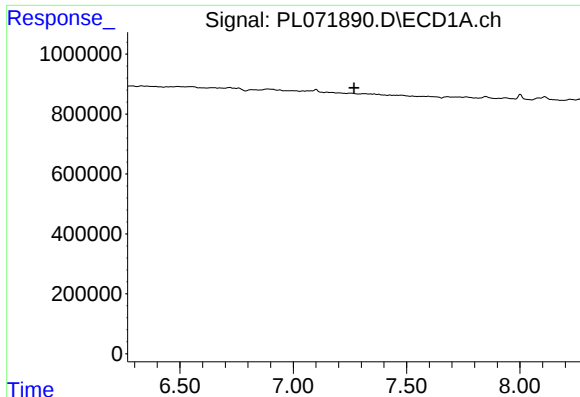

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 7.268 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

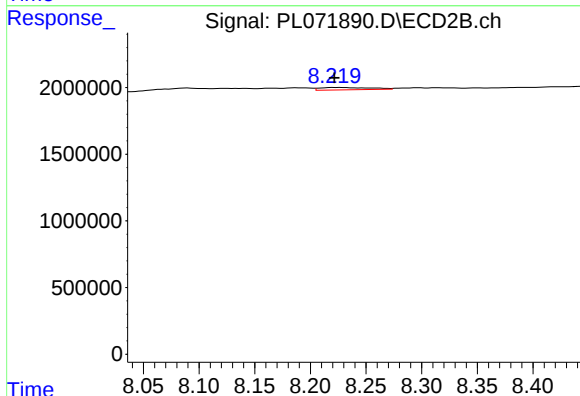


#10 gamma-Chlordane

R.T.: 8.221 min
Delta R.T.: 0.000 min
Response: 559524
Conc: 0.41 ng/ml

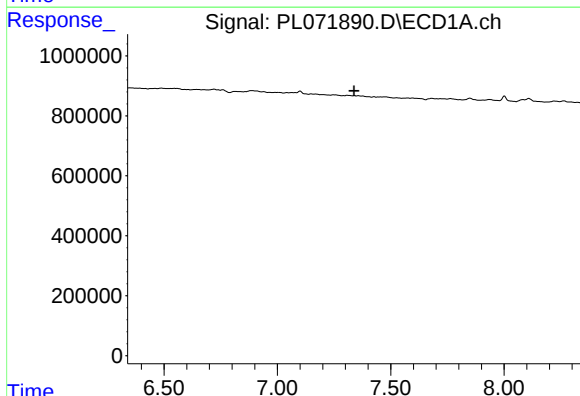


#11 alpha-Chlordane

R.T.: 0.000 min
Exp R.T.: 7.338 min
Response: 0
Conc: N.D.

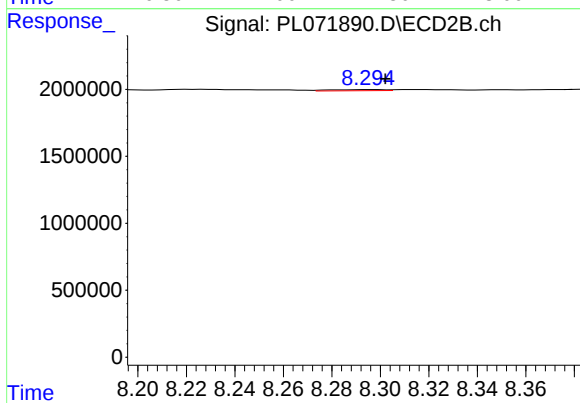

#11 alpha-Chlordane


R.T.: 8.297 min
Delta R.T.: -0.006 min
Response: 133344
Conc: 0.10 ng/ml

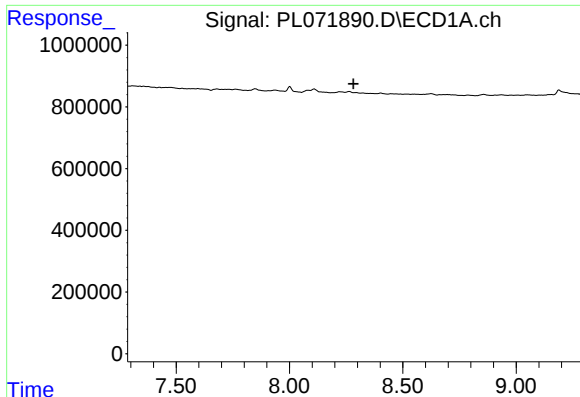

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.283 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

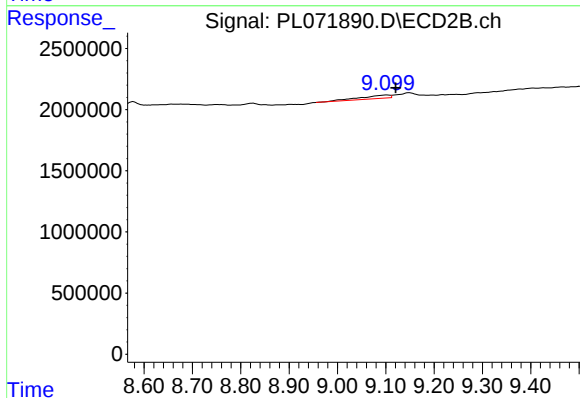


#15 Endosulfan II

R.T.: 9.101 min
Delta R.T.: -0.019 min
Response: 1169871
Conc: 1.04 ng/ml

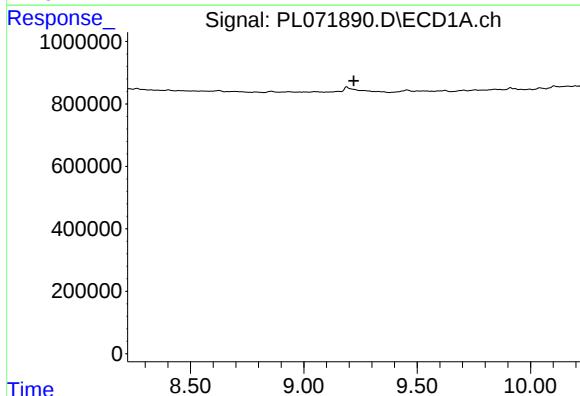


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T.: 9.220 min
Response: 0
Conc: N.D.

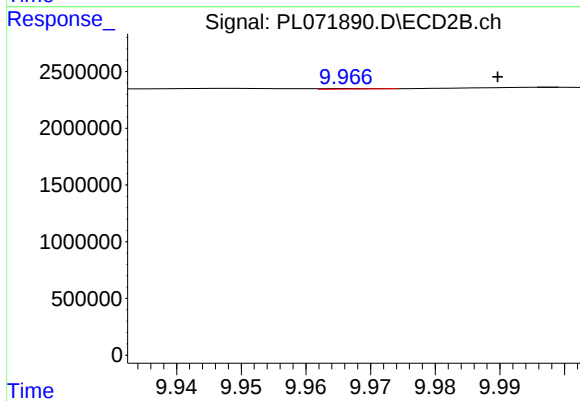

#21 Endrin ketone


R.T.: 9.968 min
Delta R.T.: -0.022 min
Response: 25268
Conc: 0.02 ng/ml

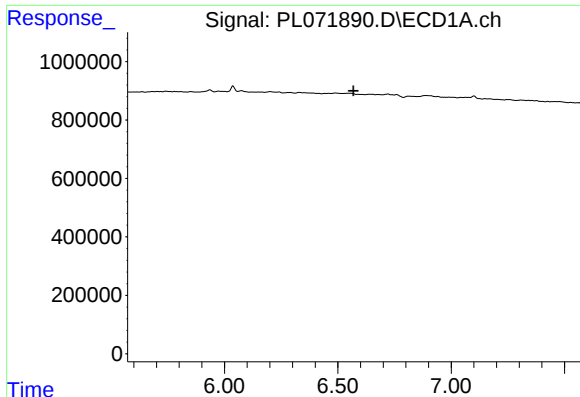

#24 Chlordane-2


R.T.: 0.000 min
Exp R.T.: 6.569 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

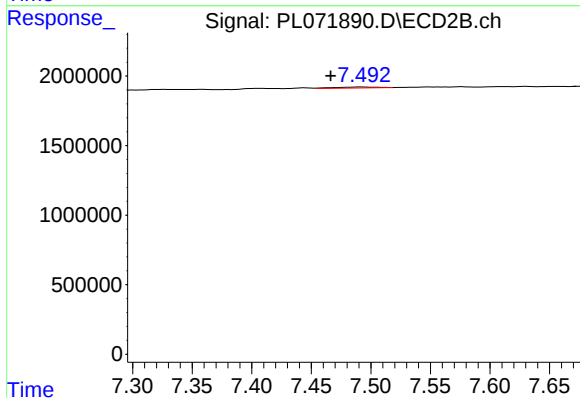


#24 Chlordane-2

R.T.: 7.493 min
Delta R.T.: 0.027 min
Response: 160931
Conc: 2.97 ng/ml

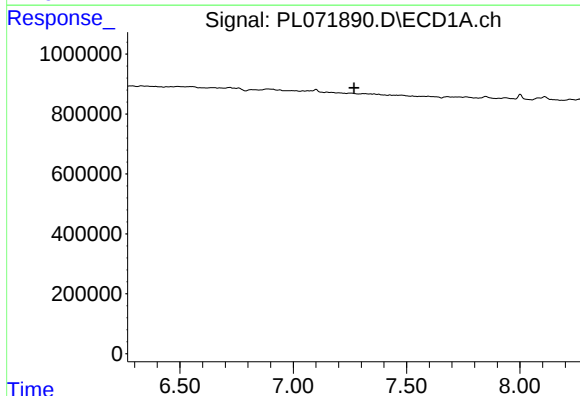


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 7.269 min
Response: 0
Conc: N.D.

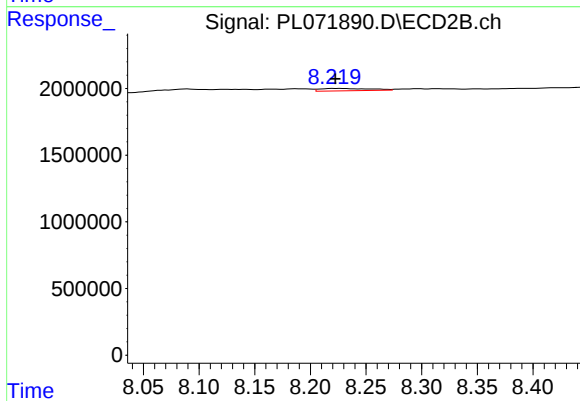

#25 Chlordane-3


R.T.: 8.221 min
Delta R.T.: -0.001 min
Response: 559524
Conc: 2.74 ng/ml

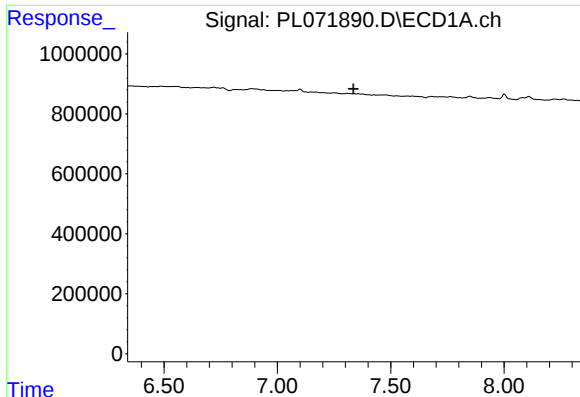

#26 Chlordane-4


R.T.: 0.000 min
Exp R.T.: 7.336 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

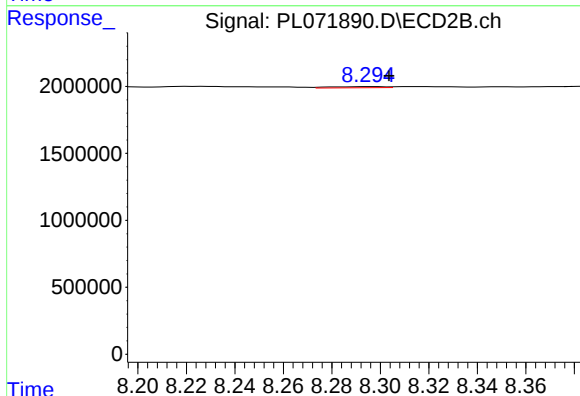


#26 Chlordane-4

R.T.: 8.297 min
Delta R.T.: -0.007 min
Response: 133344
Conc: 0.55 ng/ml

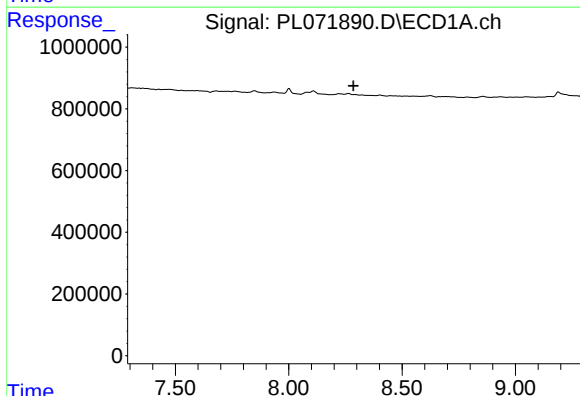


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T.: 8.286 min
Response: 0
Conc: N.D.

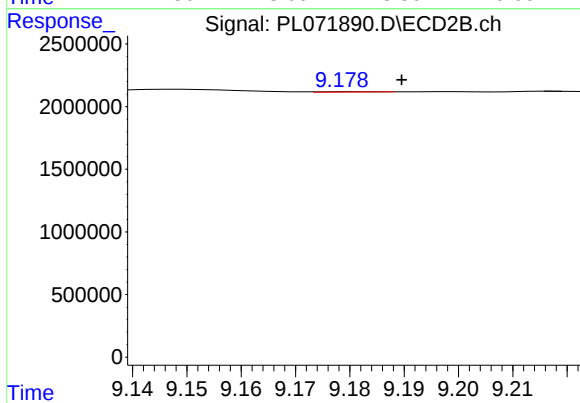

#27 Chlordane-5


R.T.: 9.179 min
Delta R.T.: -0.010 min
Response: 22581
Conc: 0.56 ng/ml

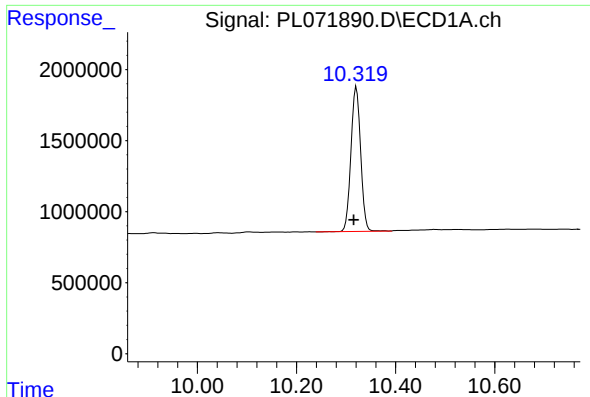

#28 Decachlorobiphenyl

R.T.: 10.321 min
Delta R.T.: 0.005 min
Response: 13854841
Conc: 19.16 ng/ml

Instrument :
ECD_L
ClientSampleId :

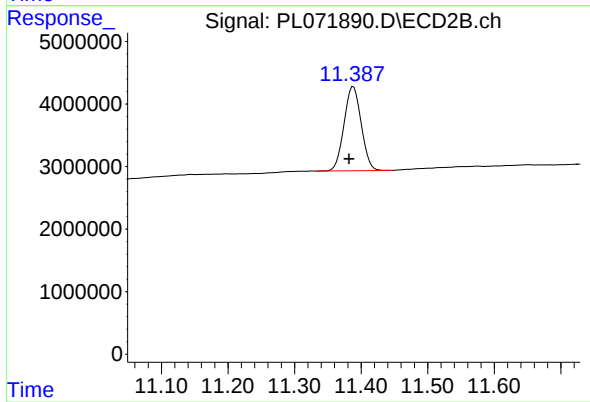

#28 Decachlorobiphenyl

R.T.: 11.388 min
Delta R.T.: 0.006 min
Response: 24107471
Conc: 20.34 ng/ml