

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011325\
 Data File : PL093643.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Jan 2025 13:40
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 01/13/2025
 Supervised By : Ankita Jodhani 01/14/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 13 13:50:11 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
 Quant Title : GC Extractables
 QLast Update : Tue Dec 24 15:29:41 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.539	2.775	52651429	60057060	21.267	20.630
2)	SA Decachlor...	9.057	7.914	37918695	61545637	20.507m	20.612

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL011325\
Data File : PL093643.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Jan 2025 13:40
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 01/13/2025
Supervised By : Ankita Jodhani 01/14/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 13 13:50:11 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL122324.M
Quant Title : GC Extractables
QLast Update : Tue Dec 24 15:29:41 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

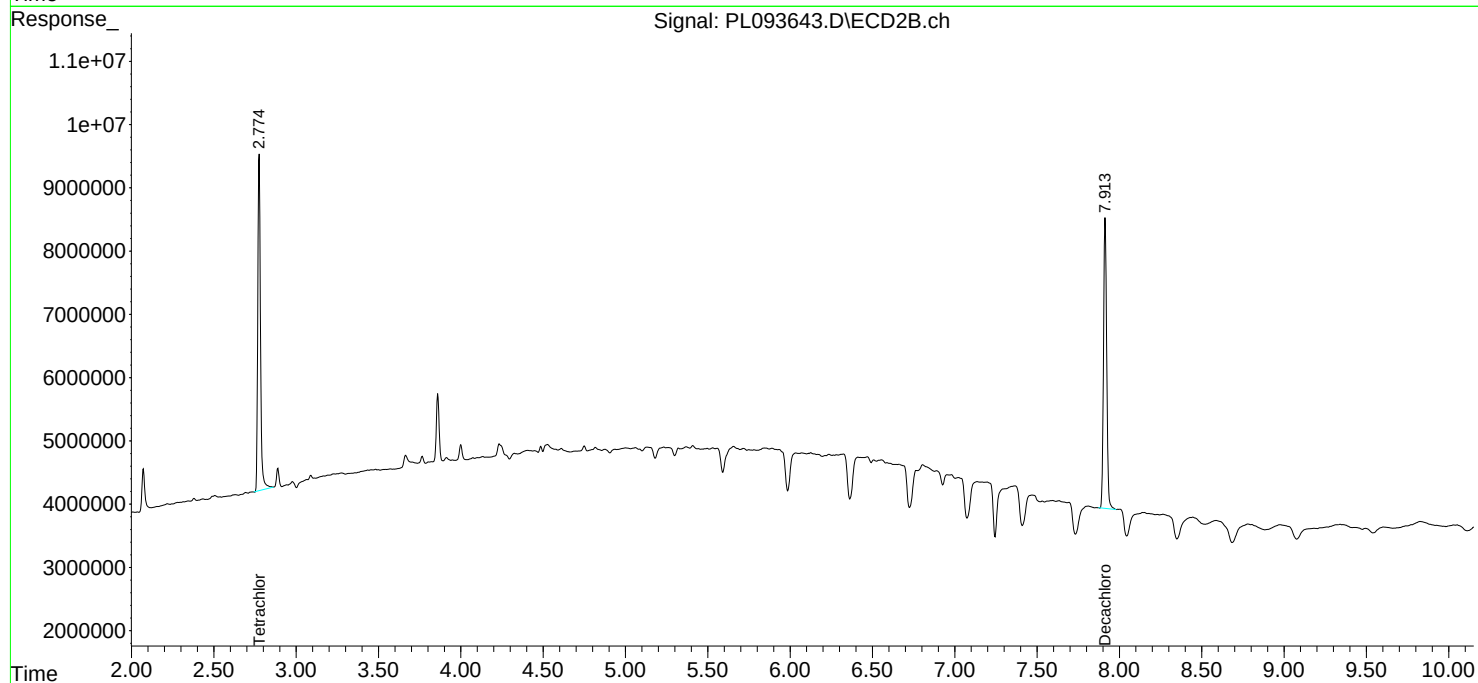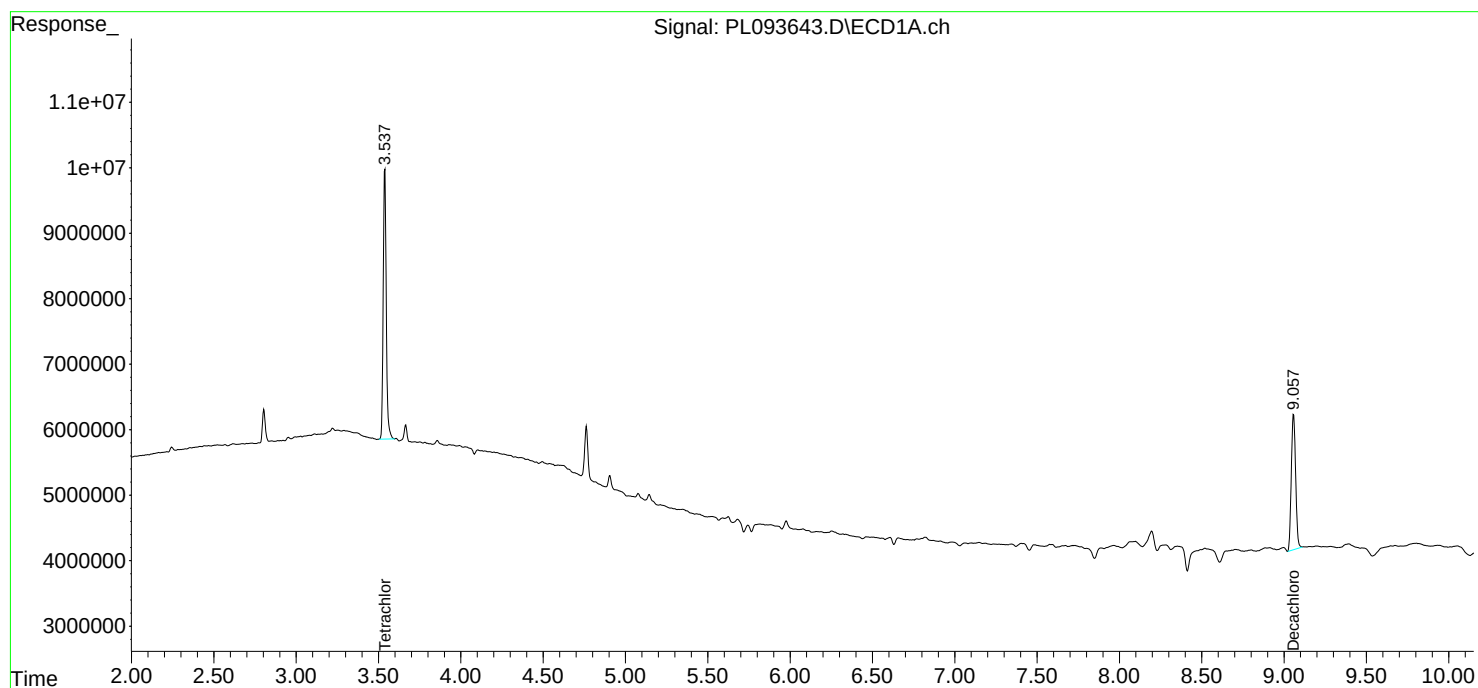

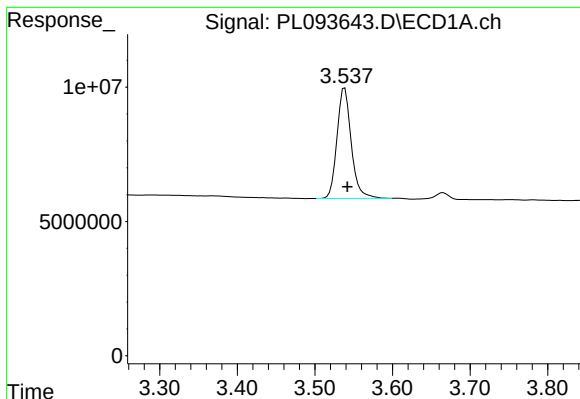


#1 Tetrachloro-m-xylene

R.T.: 3.539 min
Delta R.T.: -0.003 min
Response: 52651429
Conc: 21.27 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 01/13/2025
Supervised By :Ankita Jodhani 01/14/2025

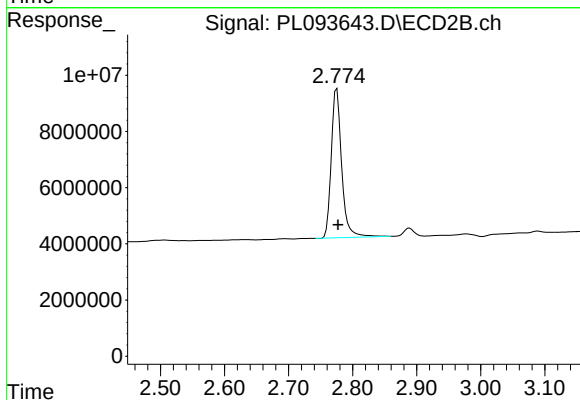


#1 Tetrachloro-m-xylene

R.T.: 2.775 min
Delta R.T.: -0.002 min
Response: 60057060
Conc: 20.63 ng/ml

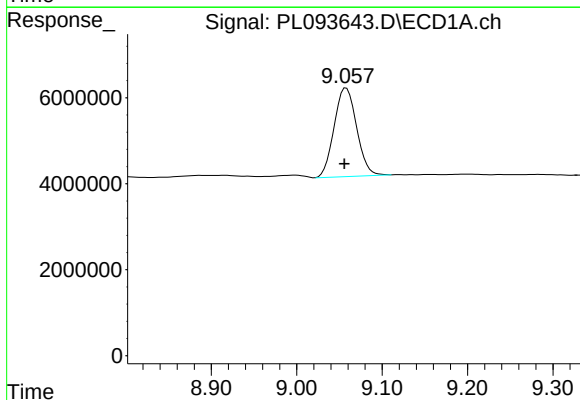

#28 Decachlorobiphenyl

R.T.: 9.057 min
Delta R.T.: 0.000 min
Response: 37918695
Conc: 20.51 ng/ml m

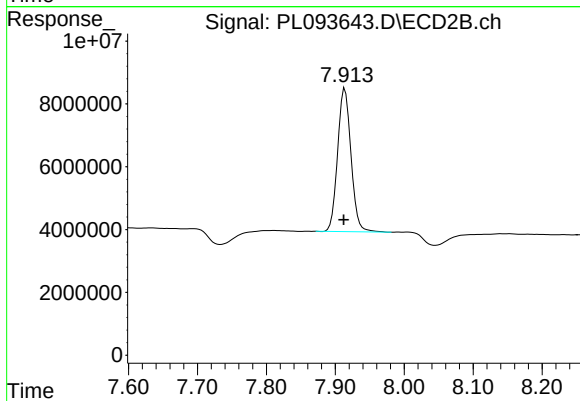

#28 Decachlorobiphenyl

R.T.: 7.914 min
Delta R.T.: 0.002 min
Response: 61545637
Conc: 20.61 ng/ml