

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012621\
 Data File : PL064437.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2021 15:16
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 26 16:34:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	4.108	56293165	45058042	18.774	17.625
28)	SA Decachlor...	8.165	9.271	37186473	31085534	12.184	13.097
Target Compounds							
4)	MA Heptachlor	0.000	5.303	0	7387161	N.D.	2.057 #
7)	B delta-BHC	0.000	5.224f	0	2335133	N.D.	0.736 #
8)	B Heptachlo...	0.000	6.020	0	1911232	N.D.	0.734 #
10)	B gamma-Chl...	0.000	6.260	0	3470913	N.D.	1.155 #
14)	MA Endrin	5.969	6.880f	900264	2063627	0.259	0.904 #
17)	MA 4,4'-DDT	0.000	7.250f	0	1419439	N.D.	0.627 #
23)	Chlordane-1	4.326f	5.145f	2029413	8548091	17.426	76.542 #
25)	Chlordane-3	0.000	6.260	0	3470913	N.D.	8.584 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012621\
Data File : PL064437.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2021 15:16
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 26 16:34:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

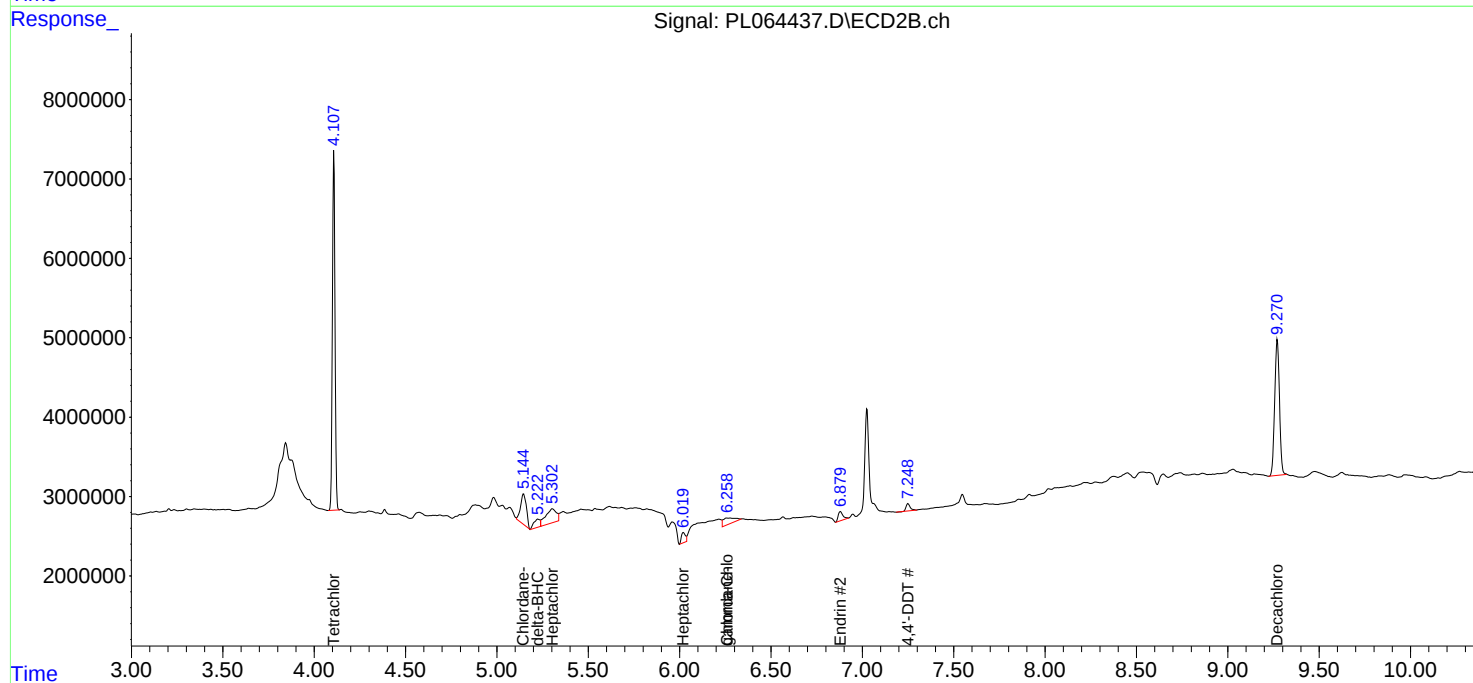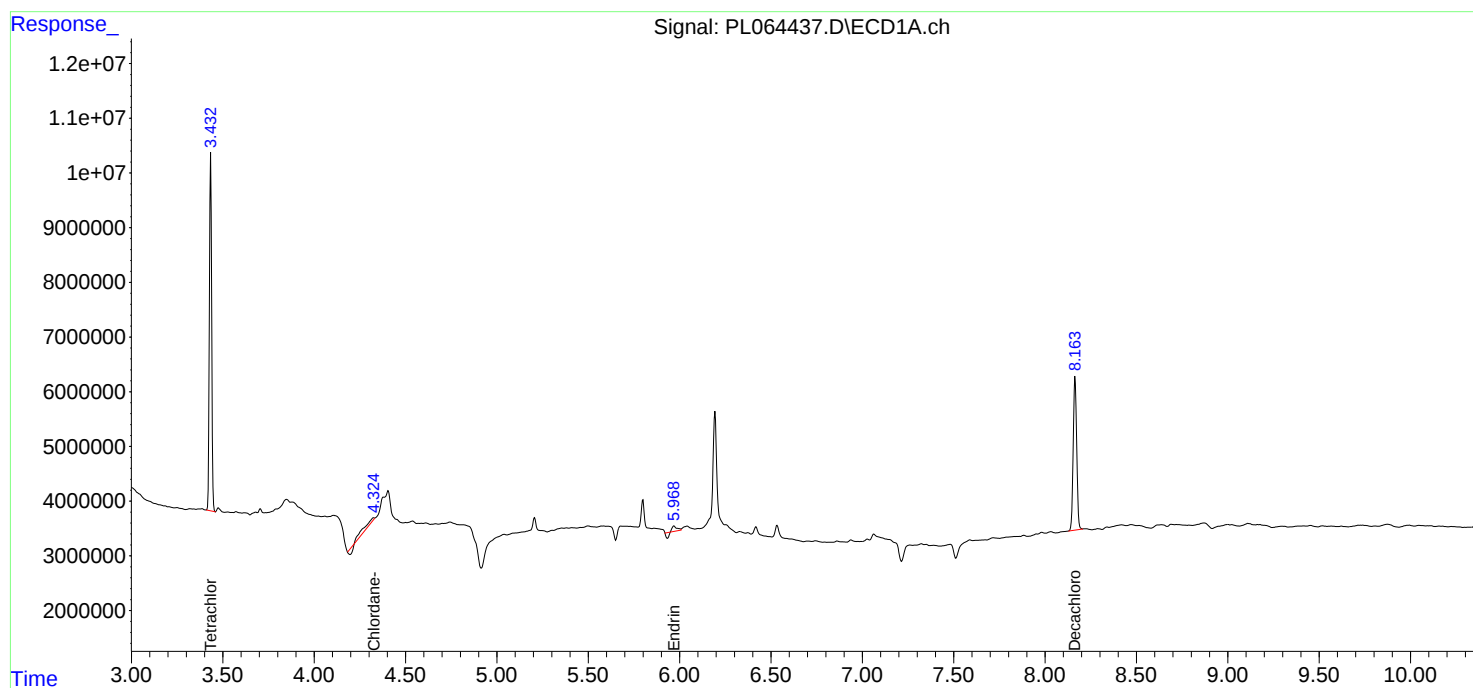


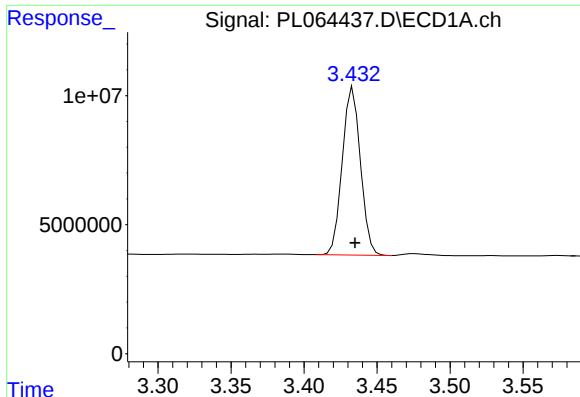

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: -0.001 min
Response: 56293165
Conc: 18.77 ng/ml

Instrument :
ECD_L
ClientSampleId :

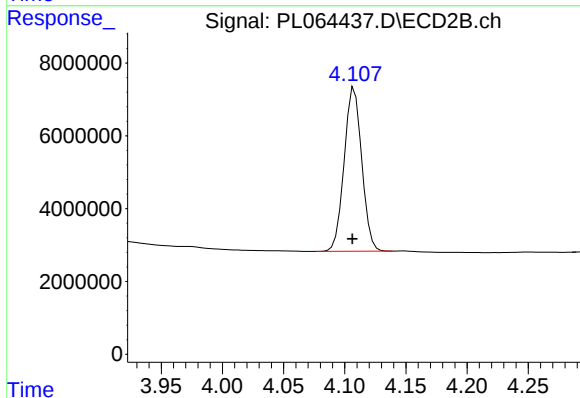


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.002 min
Response: 45058042
Conc: 17.63 ng/ml

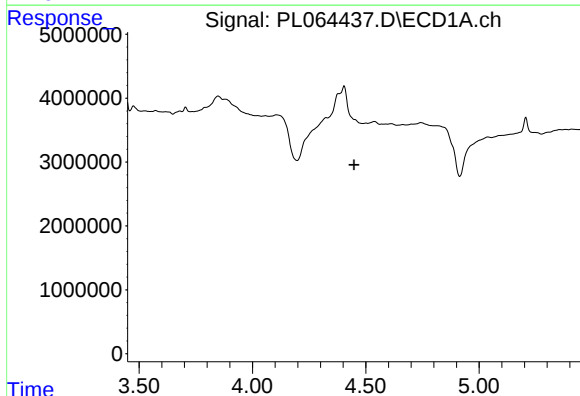


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.449 min
Response: 0
Conc: N.D.

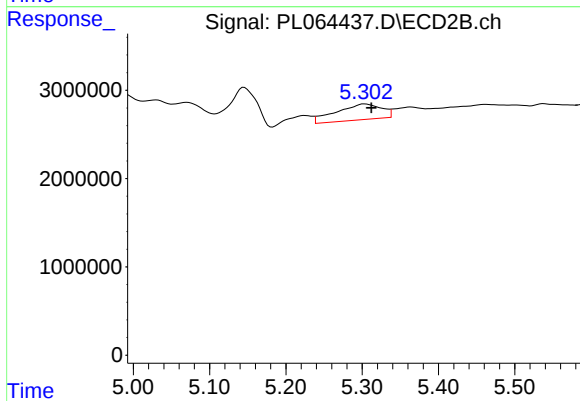

#4 Heptachlor


R.T.: 5.303 min
Delta R.T.: -0.009 min
Response: 7387161
Conc: 2.06 ng/ml

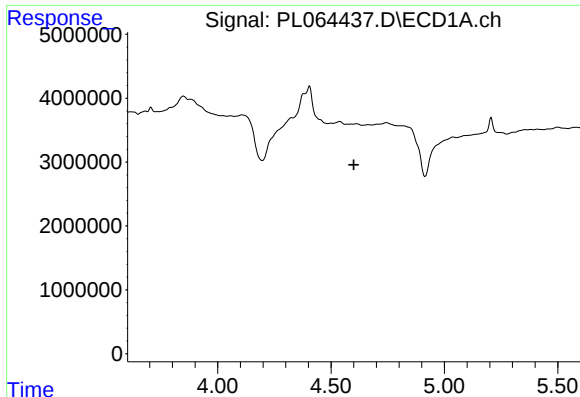

#7 delta-BHC


R.T.: 0.000 min
Exp R.T.: 4.601 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

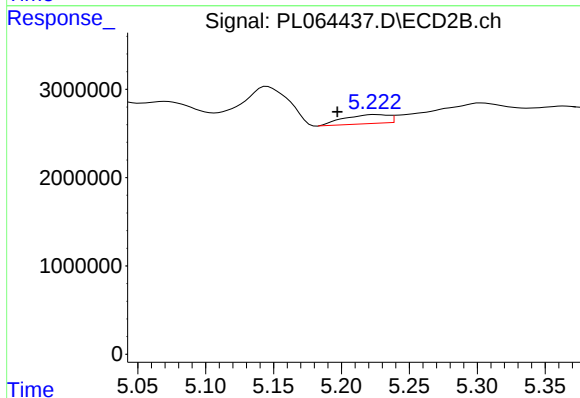


#7 delta-BHC

R.T.: 5.224 min
Delta R.T.: 0.027 min
Response: 2335133
Conc: 0.74 ng/ml

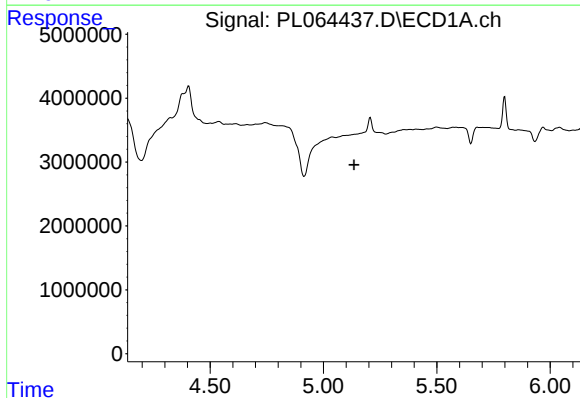


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T.: 5.135 min
Response: 0
Conc: N.D.

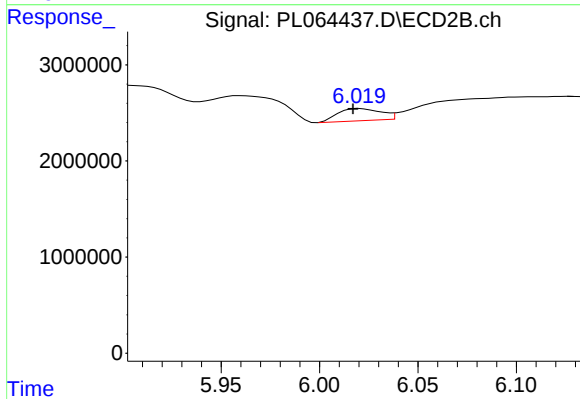

#8 Heptachlor epoxide


R.T.: 6.020 min
Delta R.T.: 0.003 min
Response: 1911232
Conc: 0.73 ng/ml

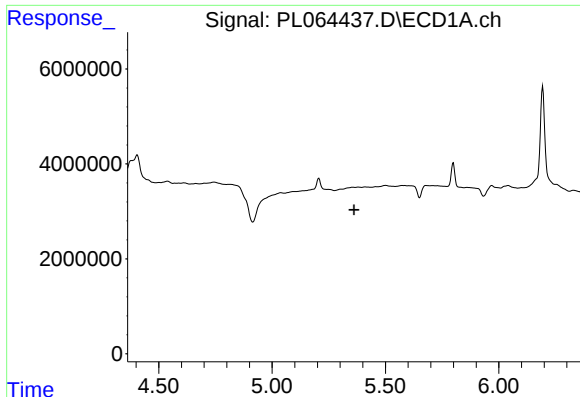

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

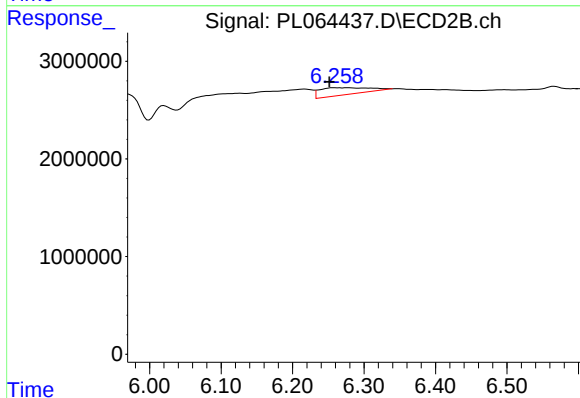


#10 gamma-Chlordane

R.T.: 6.260 min
Delta R.T.: 0.008 min
Response: 3470913
Conc: 1.16 ng/ml

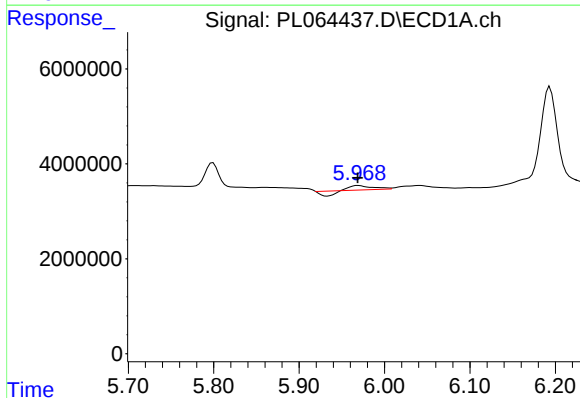


#14 Endrin

R.T.: 5.969 min
Delta R.T.: 0.000 min
Response: 900264
Conc: 0.26 ng/ml

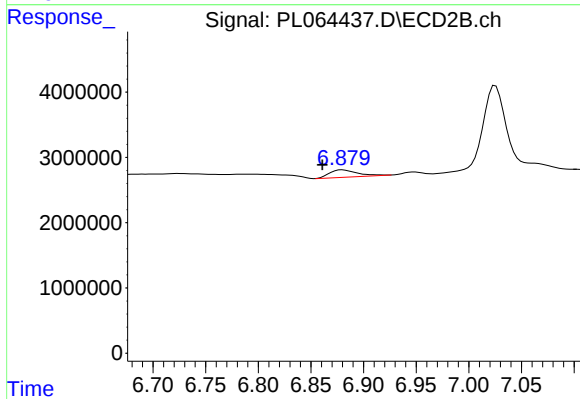

#14 Endrin


R.T.: 6.880 min
Delta R.T.: 0.019 min
Response: 2063627
Conc: 0.90 ng/ml

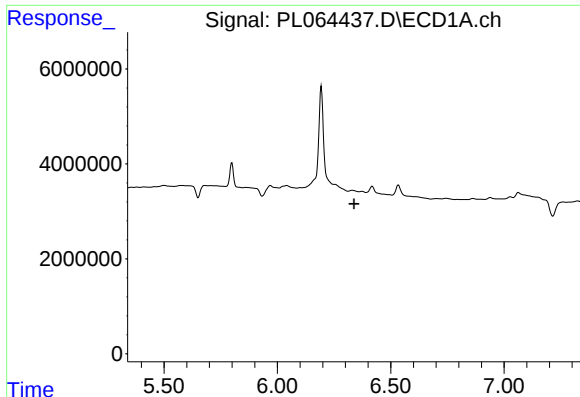

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.339 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

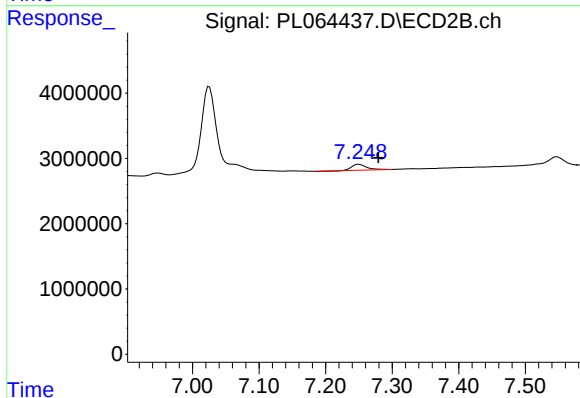


#17 4,4'-DDT

R.T.: 7.250 min
Delta R.T.: -0.029 min
Response: 1419439
Conc: 0.63 ng/ml

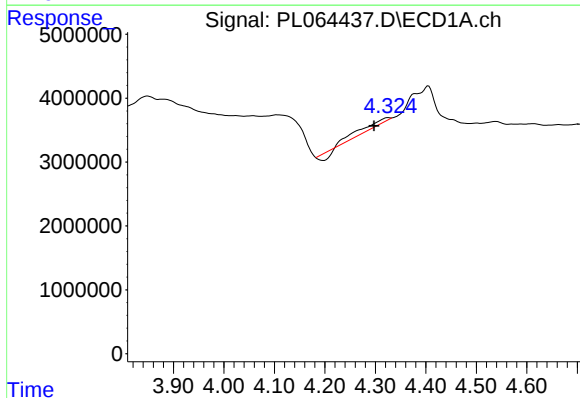


#23 Chlordane-1

R.T.: 4.326 min
Delta R.T.: 0.028 min
Response: 2029413
Conc: 17.43 ng/ml

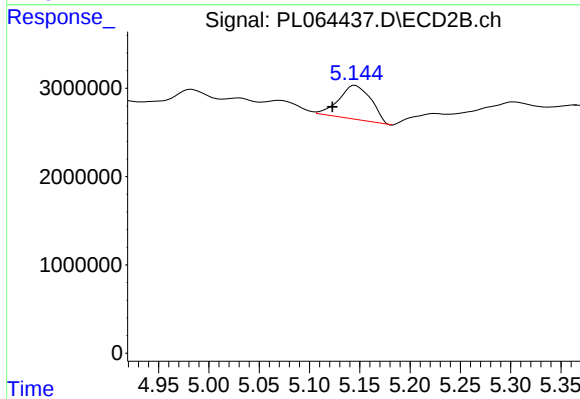

#23 Chlordane-1


R.T.: 5.145 min
Delta R.T.: 0.023 min
Response: 8548091
Conc: 76.54 ng/ml

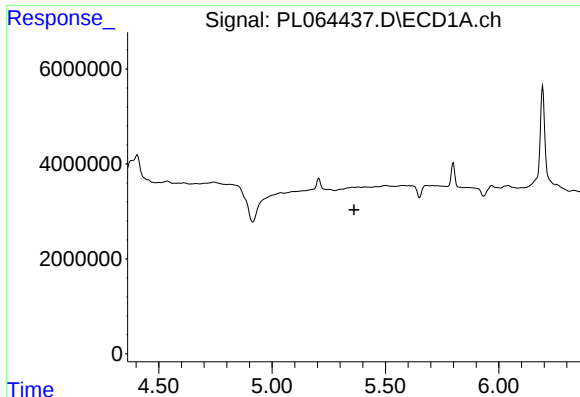

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

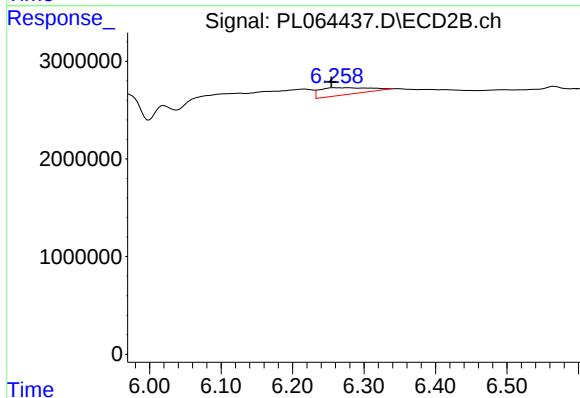


#25 Chlordane-3

R.T.: 6.260 min
Delta R.T.: 0.005 min
Response: 3470913
Conc: 8.58 ng/ml

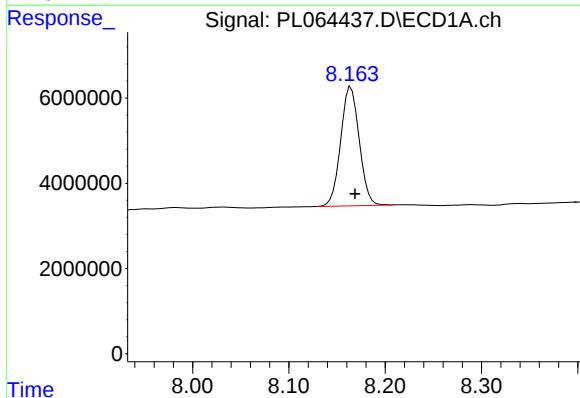

#28 Decachlorobiphenyl

R.T.: 8.165 min
Delta R.T.: -0.004 min
Response: 37186473
Conc: 12.18 ng/ml

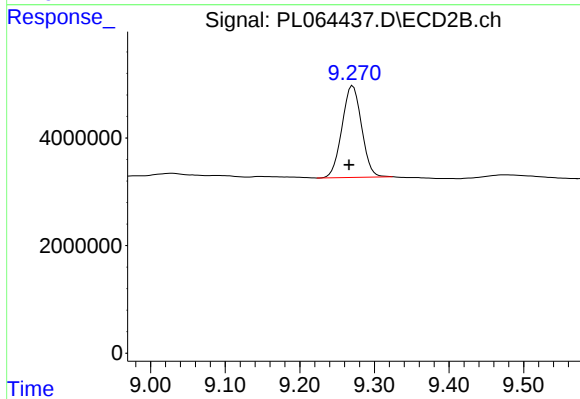

#28 Decachlorobiphenyl

R.T.: 9.271 min
Delta R.T.: 0.005 min
Response: 31085534
Conc: 13.10 ng/ml