

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012621\
 Data File : PL064423.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Jan 2021 11:11
 Operator : AR\AJ
 Sample : M1208-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-SF-03-011-A

Manual Integrations
 APPROVED

Ankita
 1/29/2021 11:12:35 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 04:15:03 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.435	4.108	36663208	27893131	12.227	10.911
28)	SA Decachlor...	8.166	9.271	23648554	20048496	7.748	8.447
Target Compounds							
4)	MA Heptachlor	4.447	5.313	11535561	8867147	2.633	2.469m
5)	MB Aldrin	4.693	5.622	26607443	20134847	6.640	6.487m
10)	B gamma-Chl...	5.359	6.254	24196673	25300268	6.246m	8.420 #
11)	B alpha-Chl...	5.418	6.327	26176475	40954047	6.841	13.453 #
12)	B 4,4'-DDE	5.583	6.484	22185966	20705428	6.298m	7.773
14)	MA Endrin	5.971	6.849	5062190	3017327	1.458	1.321
17)	MA 4,4'-DDT	6.334	7.282	14237172	4713932	4.769	2.081 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012621\
Data File : PL064423.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Jan 2021 11:11
Operator : AR\AJ
Sample : M1208-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampled :
FK-SF-03-011-A


Manual Integrations
APPROVED

Ankita
1/29/2021 11:12:35 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 04:15:03 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

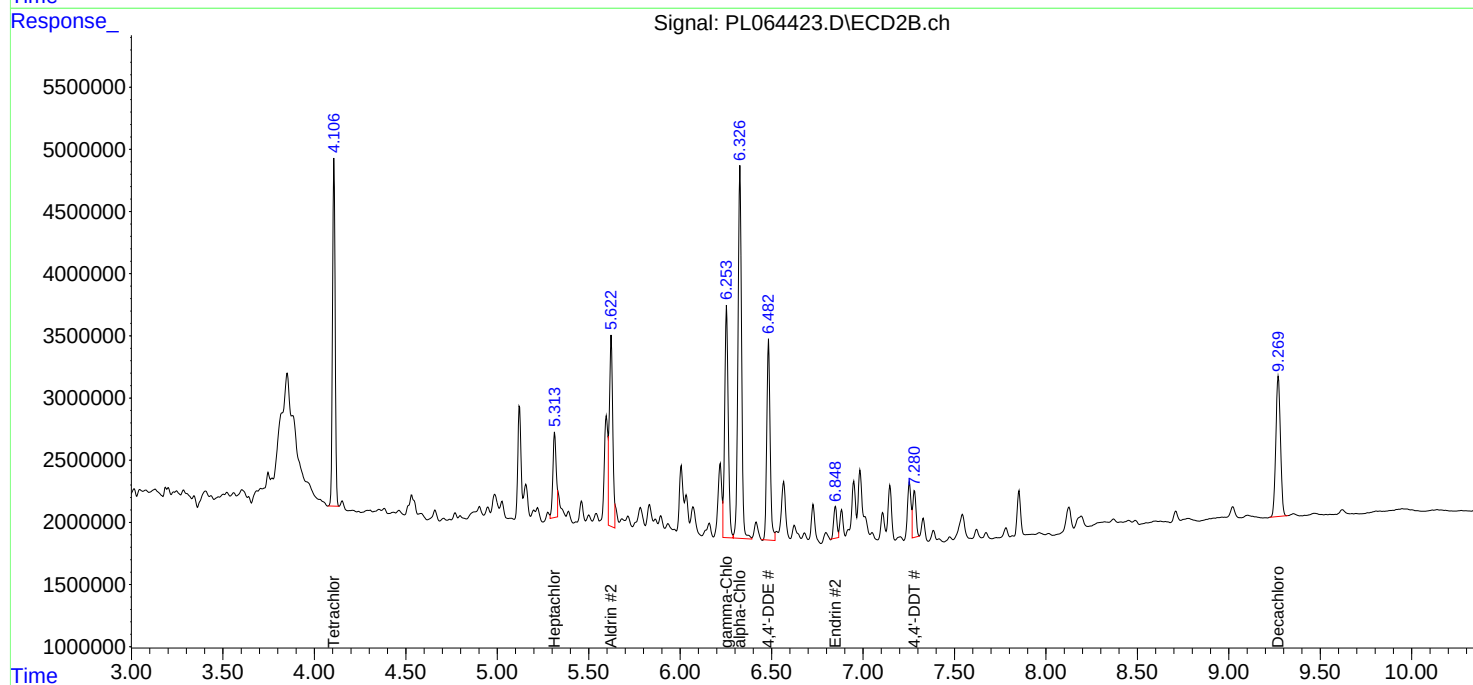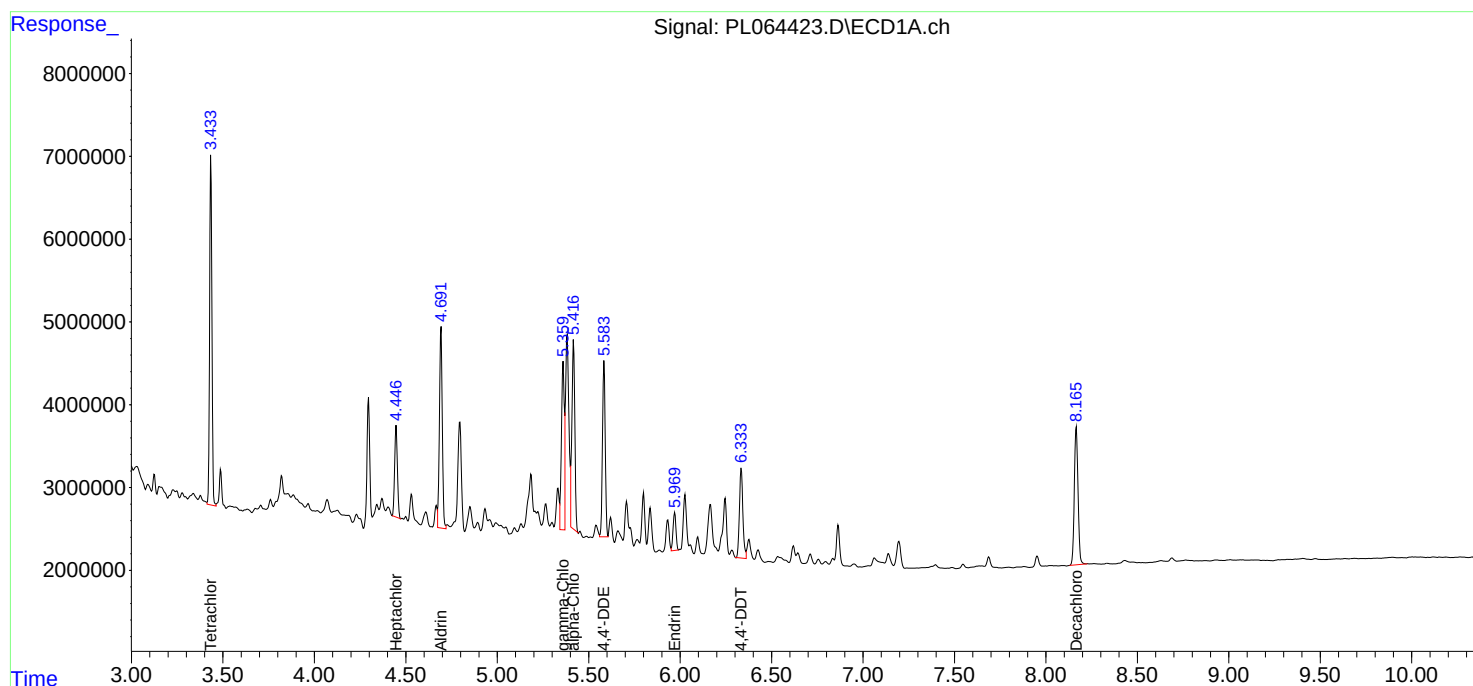

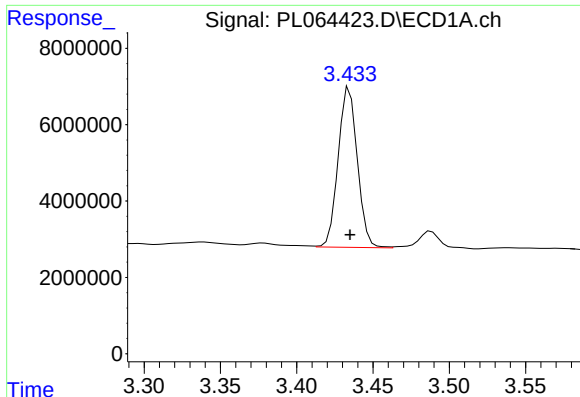


#1 Tetrachloro-m-xylene

R.T.: 3.435 min
Delta R.T.: 0.000 min
Response: 36663208
Conc: 12.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-SF-03-011-A


Manual Integrations
APPROVED

Ankita
1/29/2021 11:12:35 AM

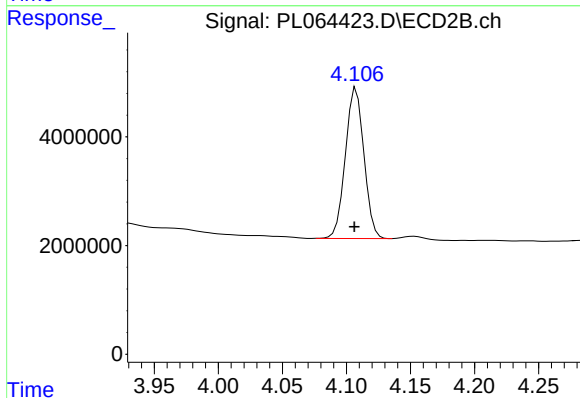


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.001 min
Response: 27893131
Conc: 10.91 ng/ml

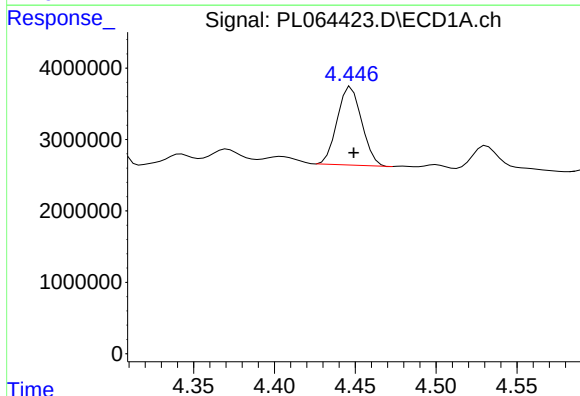


#4 Heptachlor

R.T.: 4.447 min
Delta R.T.: -0.002 min
Response: 11535561
Conc: 2.63 ng/ml

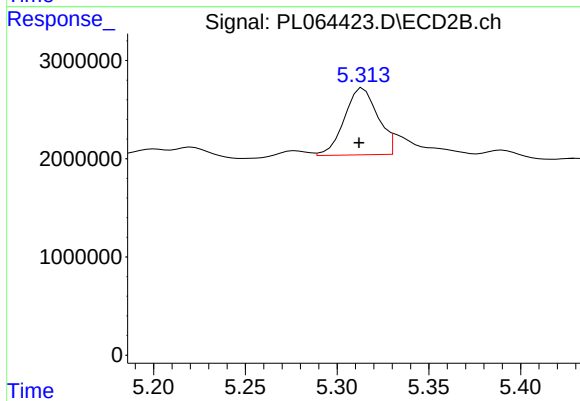

#4 Heptachlor

R.T.: 5.313 min
Delta R.T.: 0.000 min
Response: 8867147
Conc: 2.47 ng/ml m

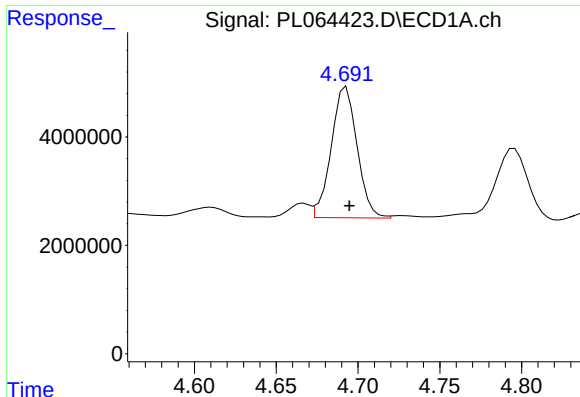


#5 Aldrin

R.T.: 4.693 min
Delta R.T.: -0.002 min
Response: 26607443
Conc: 6.64 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-SF-03-011-A


Manual Integrations
APPROVED

Ankita
1/29/2021 11:12:35 AM

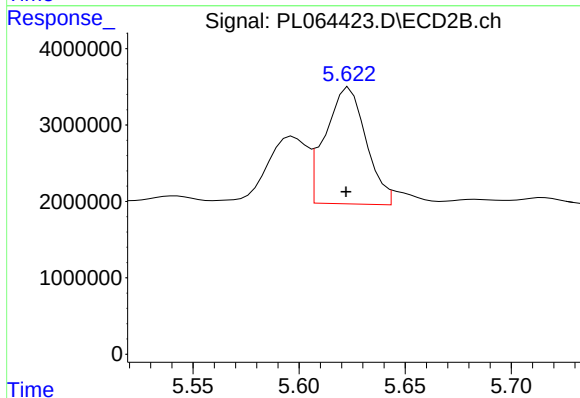


#5 Aldrin

R.T.: 5.622 min
Delta R.T.: 0.000 min
Response: 20134847
Conc: 6.49 ng/ml m

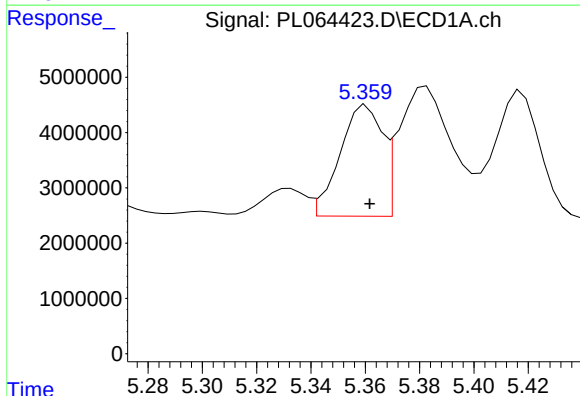


#10 gamma-Chlordane

R.T.: 5.359 min
Delta R.T.: -0.003 min
Response: 24196673
Conc: 6.25 ng/ml m

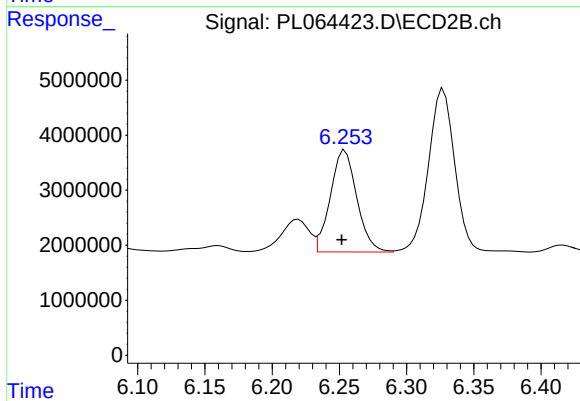

#10 gamma-Chlordane

R.T.: 6.254 min
Delta R.T.: 0.002 min
Response: 25300268
Conc: 8.42 ng/ml

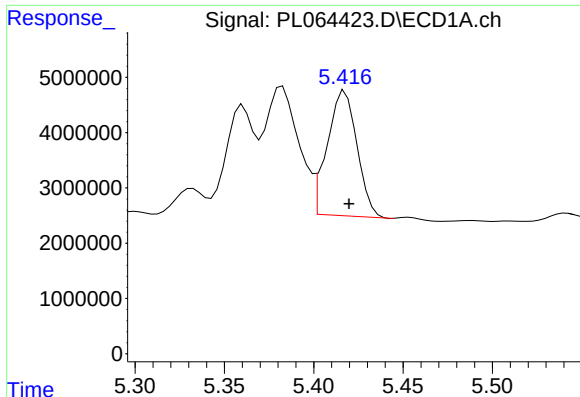


#11 alpha-Chlordane

R.T.: 5.418 min
Delta R.T.: -0.002 min
Response: 26176475
Conc: 6.84 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-SF-03-011-A


Manual Integrations
APPROVED

Ankita
1/29/2021 11:12:35 AM

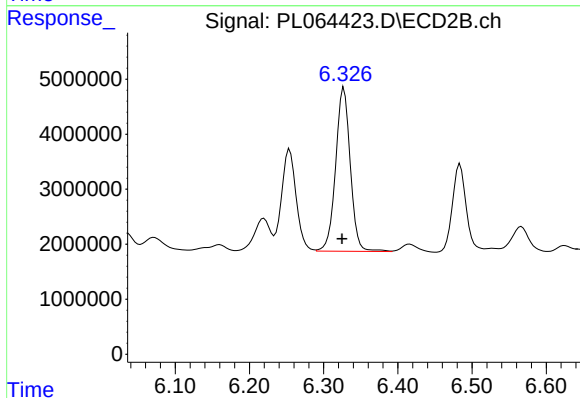


#11 alpha-Chlordane

R.T.: 6.327 min
Delta R.T.: 0.002 min
Response: 40954047
Conc: 13.45 ng/ml

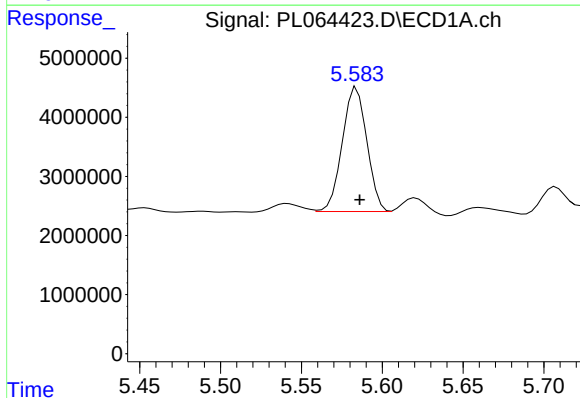


#12 4,4'-DDE

R.T.: 5.583 min
Delta R.T.: -0.003 min
Response: 22185966
Conc: 6.30 ng/ml m

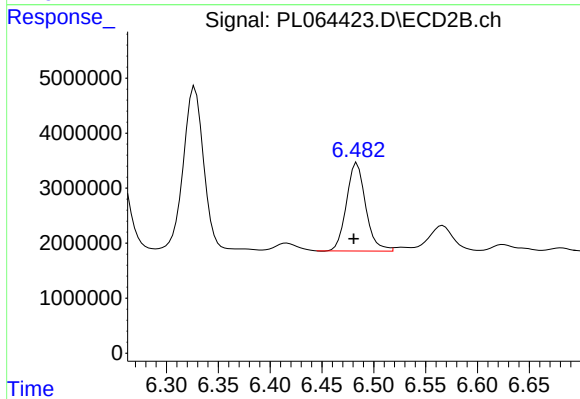

#12 4,4'-DDE

R.T.: 6.484 min
Delta R.T.: 0.003 min
Response: 20705428
Conc: 7.77 ng/ml

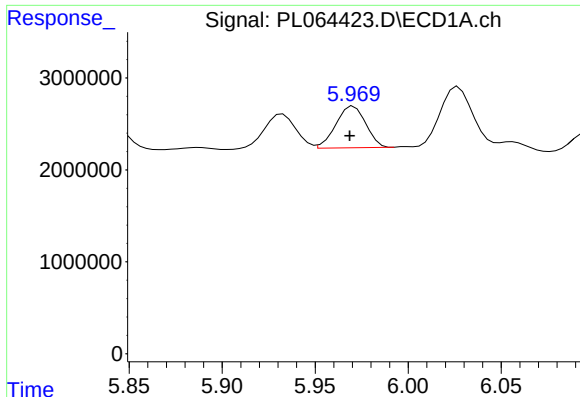


#14 Endrin

R.T.: 5.971 min
Delta R.T.: 0.002 min
Response: 5062190
Conc: 1.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-SF-03-011-A


Manual Integrations
APPROVED

Ankita
1/29/2021 11:12:35 AM

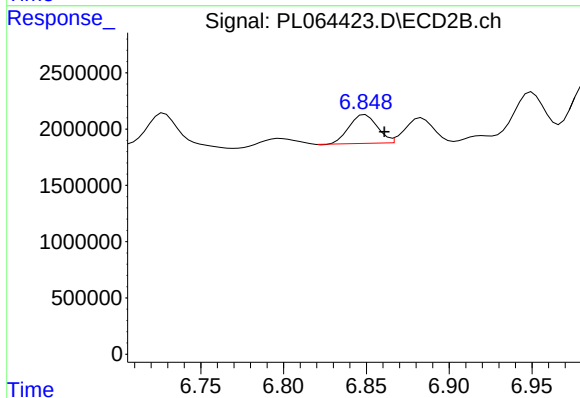


#14 Endrin

R.T.: 6.849 min
Delta R.T.: -0.012 min
Response: 3017327
Conc: 1.32 ng/ml

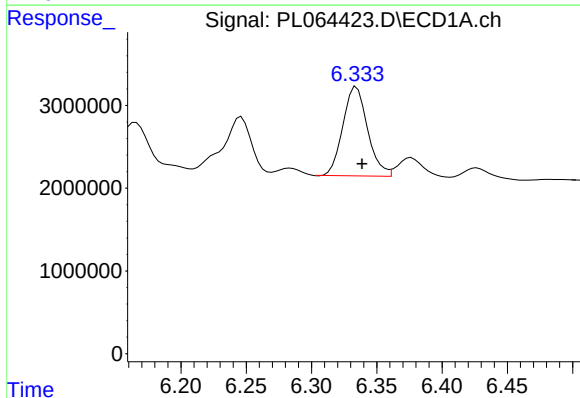


#17 4,4'-DDT

R.T.: 6.334 min
Delta R.T.: -0.004 min
Response: 14237172
Conc: 4.77 ng/ml

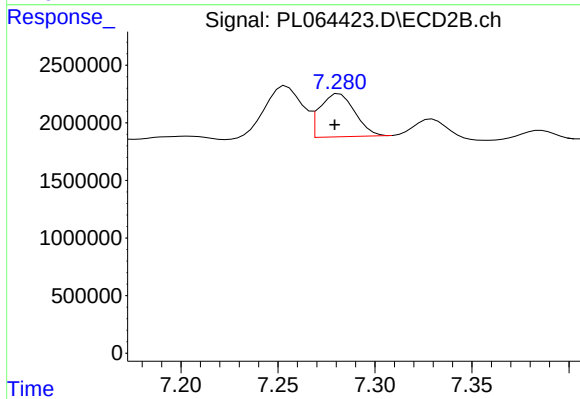

#17 4,4'-DDT

R.T.: 7.282 min
Delta R.T.: 0.002 min
Response: 4713932
Conc: 2.08 ng/ml

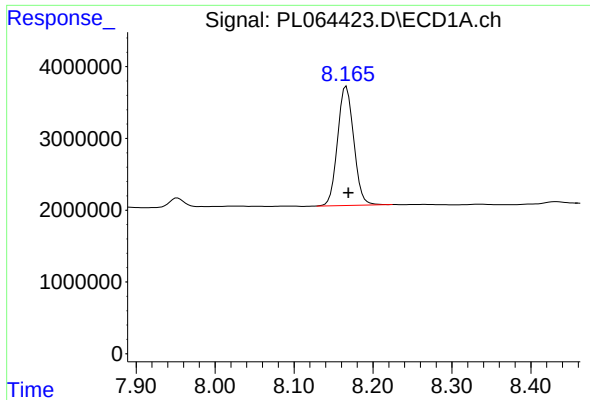


#28 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: -0.003 min
Response: 23648554
Conc: 7.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-SF-03-011-A

Manual Integrations
APPROVED

Ankita
1/29/2021 11:12:35 AM

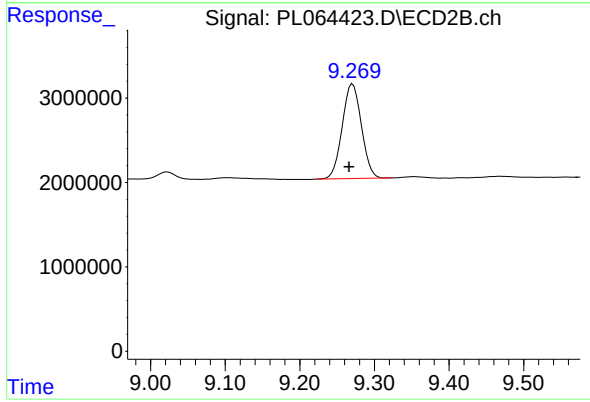

#28 Decachlorobiphenyl

R.T.: 9.271 min
Delta R.T.: 0.005 min
Response: 20048496
Conc: 8.45 ng/ml