

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012721\
 Data File : PL064440.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2021 10:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 15:53:20 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	4.108	55416433	45183273	18.481	17.674
28)	SA Decachlor...	8.164	9.269	51478570	36954161	16.867	15.570
Target Compounds							
23)	Chlordane-1	4.321f	5.153f	-3798585	16278995	N.D.	145.767



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012721\
Data File : PL064440.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2021 10:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 15:53:20 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

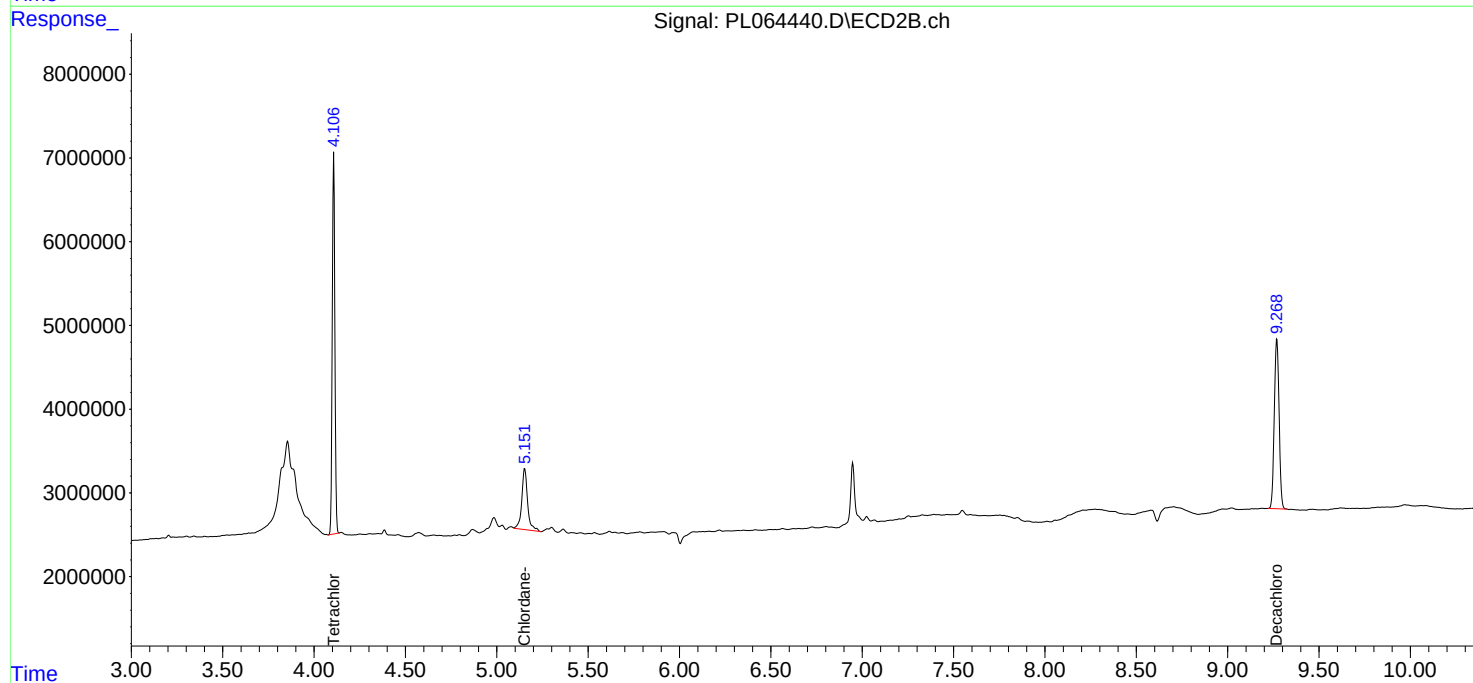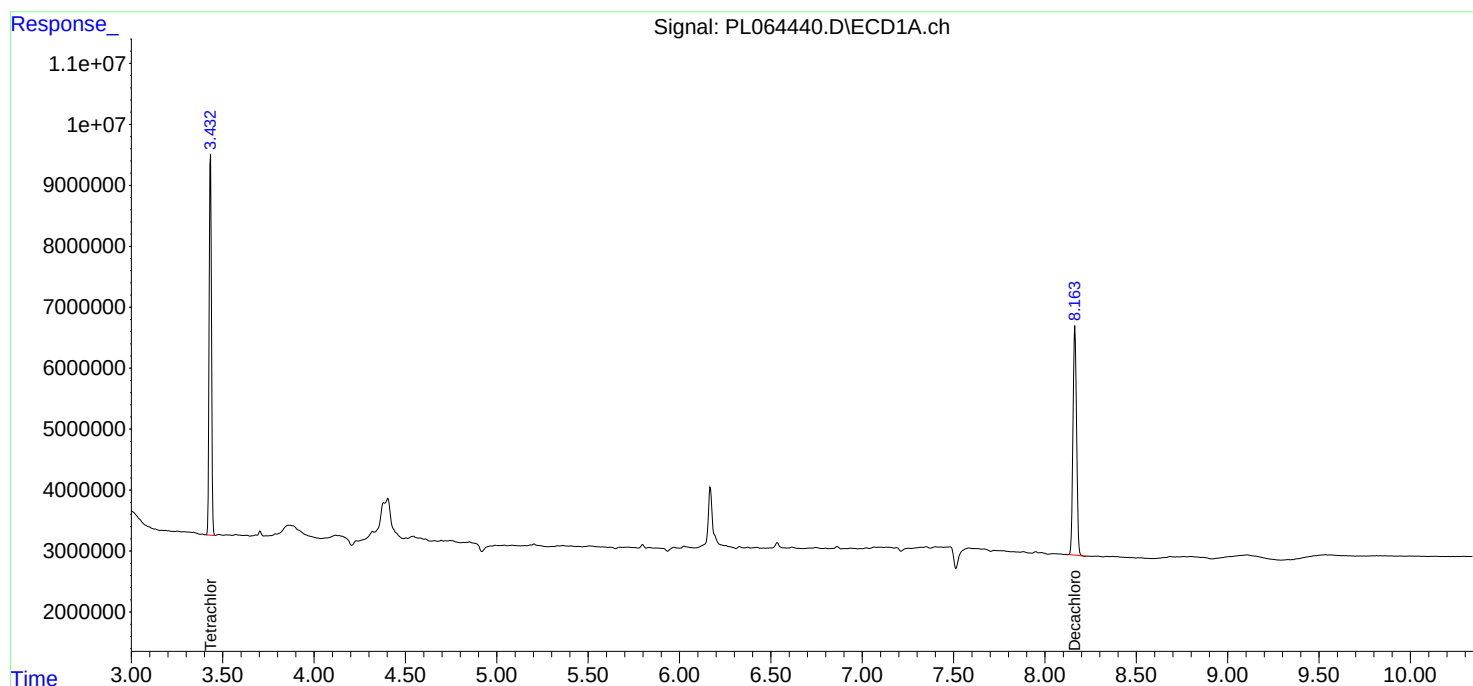


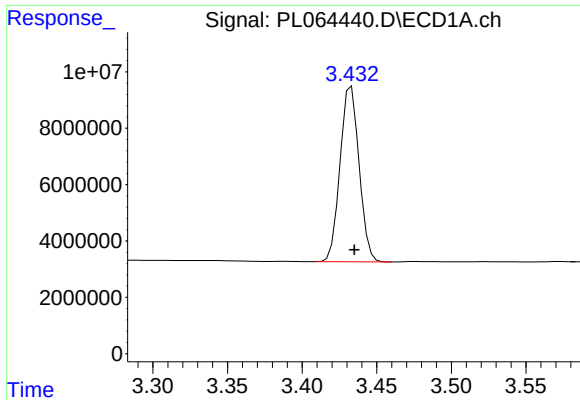

#1 Tetrachloro-m-xylene


R.T.: 3.433 min
Delta R.T.: -0.002 min
Response: 55416433
Conc: 18.48 ng/ml

Instrument :
ECD_L
ClientSampleId :

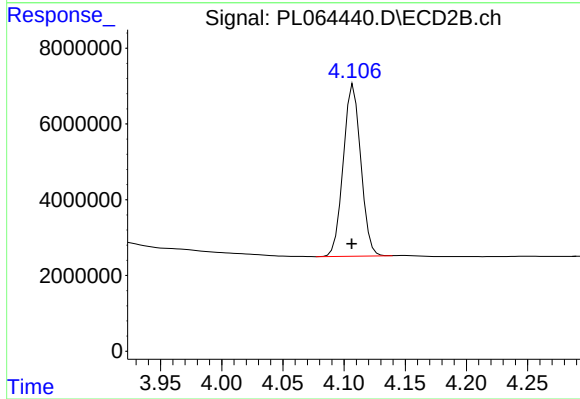


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.001 min
Response: 45183273
Conc: 17.67 ng/ml

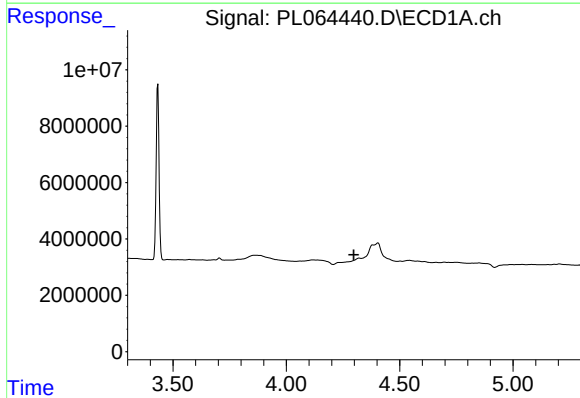


#23 Chlordane-1

R.T.: 4.321 min
Delta R.T.: 0.023 min
Response: -3798585
Conc: N.D.

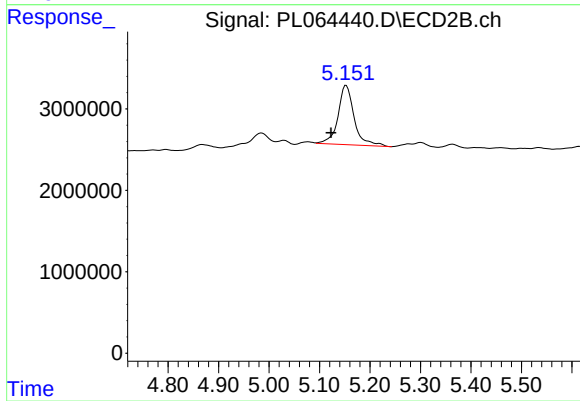

#23 Chlordane-1


R.T.: 5.153 min
Delta R.T.: 0.030 min
Response: 16278995
Conc: 145.77 ng/ml

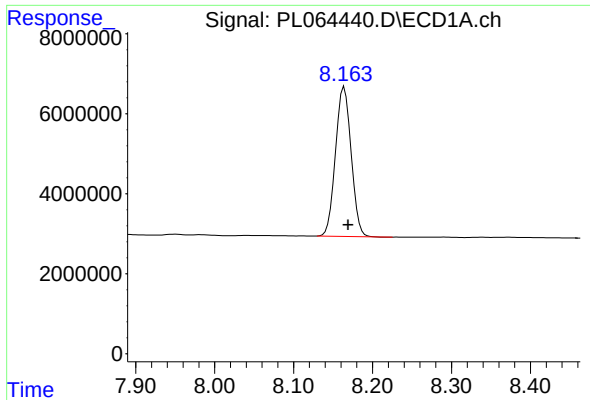

#28 Decachlorobiphenyl

R.T.: 8.164 min
Delta R.T.: -0.005 min
Response: 51478570
Conc: 16.87 ng/ml

Instrument :
ECD_L
ClientSampleId :

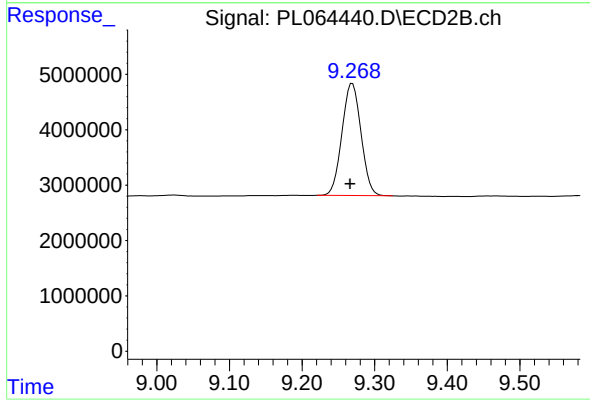

#28 Decachlorobiphenyl

R.T.: 9.269 min
Delta R.T.: 0.003 min
Response: 36954161
Conc: 15.57 ng/ml