

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012721\
 Data File : PL064443.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2021 11:17
 Operator : AR\AJ
 Sample : PB134320BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 15:53:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.439	4.109	58709568	49673014	19.580	19.430
28)	SA Decachlor...	8.172	9.274	56776628	40370289	18.603	17.009
Target Compounds							
23)	Chlordane-1	0.000	5.145f	0	35051459	N.D.	313.861 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012721\
Data File : PL064443.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2021 11:17
Operator : AR\AJ
Sample : PB134320BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 15:53:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

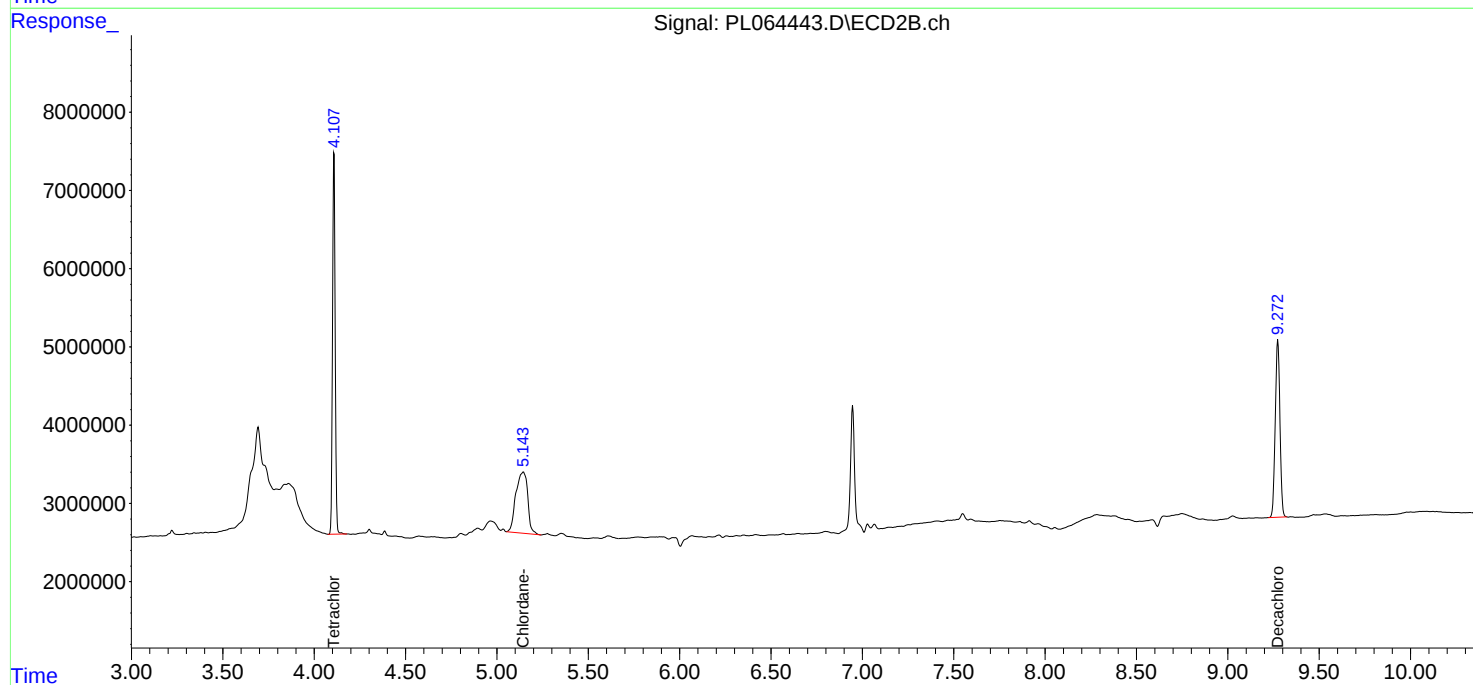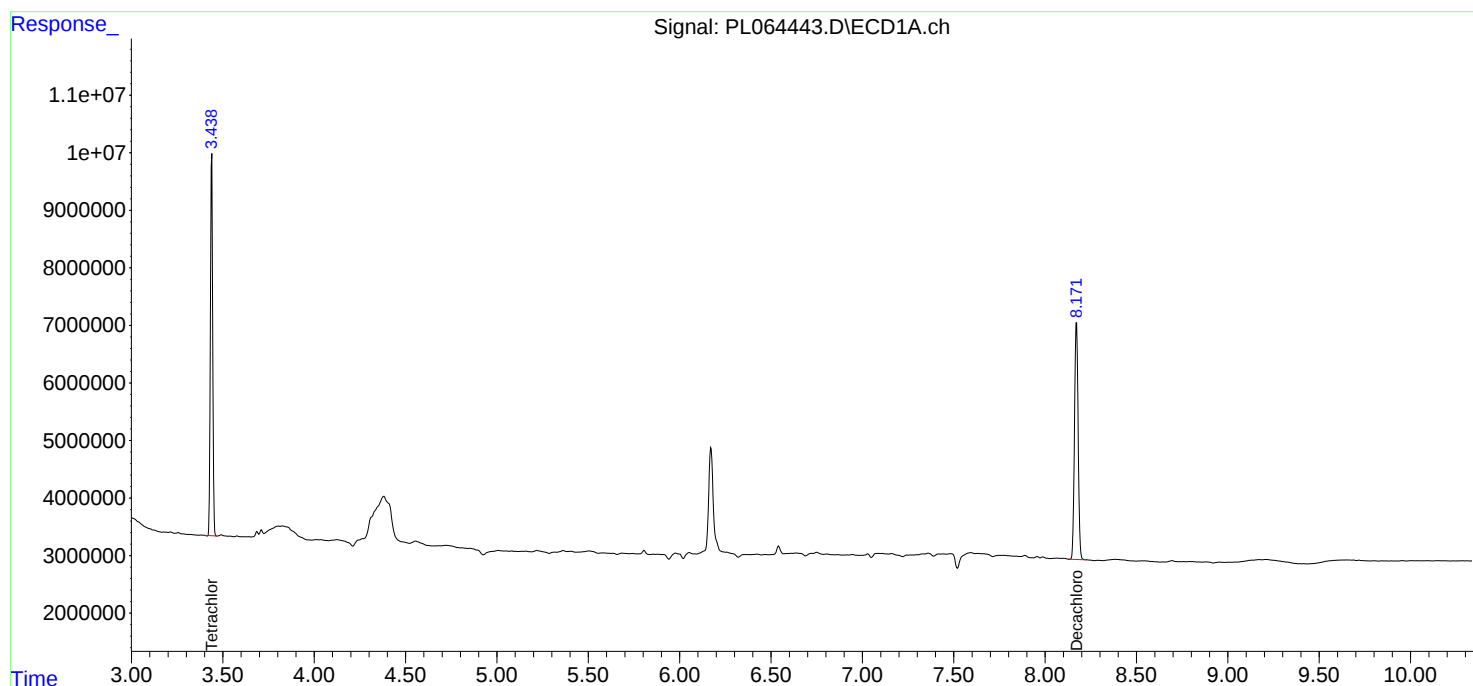


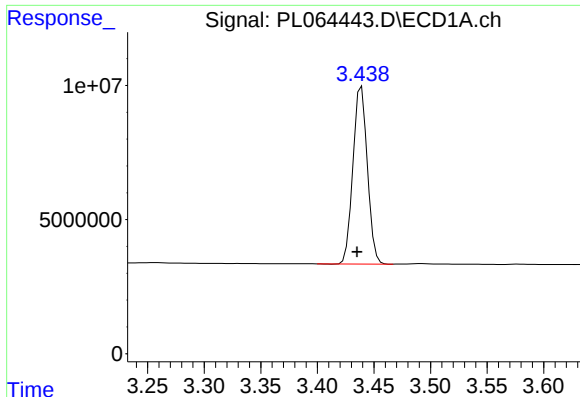

#1 Tetrachloro-m-xylene


R.T.: 3.439 min
Delta R.T.: 0.004 min
Response: 58709568
Conc: 19.58 ng/ml

Instrument :
ECD_L
ClientSampleId :

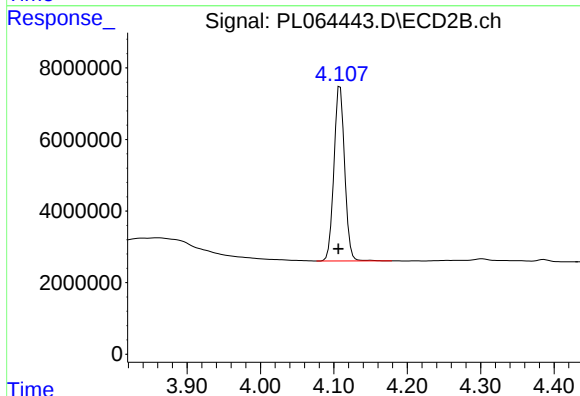


#1 Tetrachloro-m-xylene

R.T.: 4.109 min
Delta R.T.: 0.002 min
Response: 49673014
Conc: 19.43 ng/ml

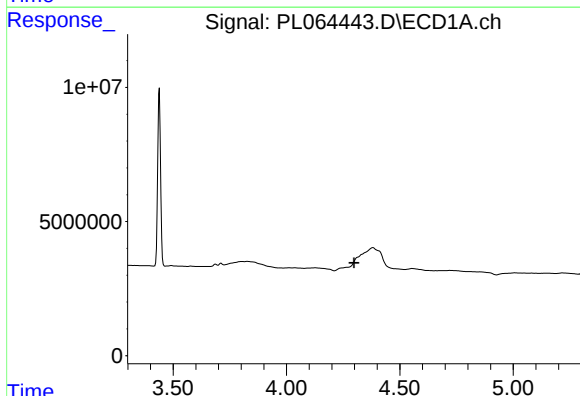


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 4.298 min
Response: 0
Conc: N.D.

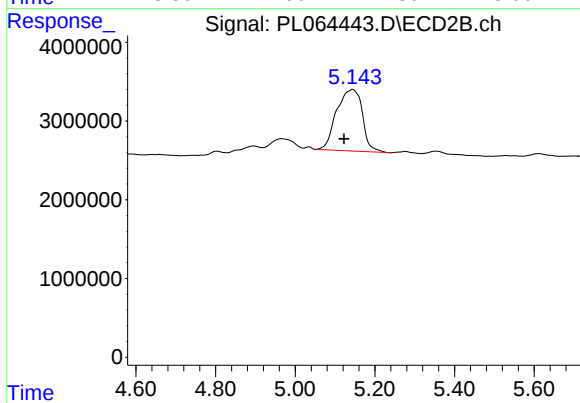

#23 Chlordane-1


R.T.: 5.145 min
Delta R.T.: 0.022 min
Response: 35051459
Conc: 313.86 ng/ml

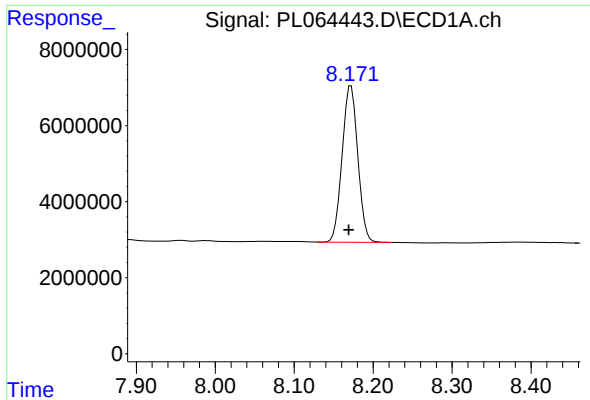

#28 Decachlorobiphenyl

R.T.: 8.172 min
Delta R.T.: 0.003 min
Response: 56776628
Conc: 18.60 ng/ml

Instrument :
ECD_L
ClientSampleId :

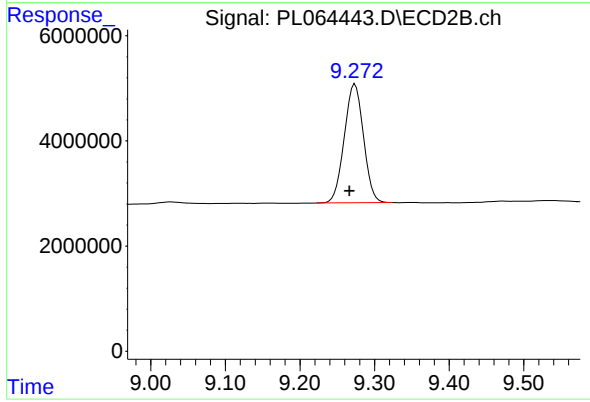

#28 Decachlorobiphenyl

R.T.: 9.274 min
Delta R.T.: 0.008 min
Response: 40370289
Conc: 17.01 ng/ml