

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012721\
 Data File : PL064458.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2021 15:48
 Operator : AR\AJ
 Sample : M1236-08
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 16:32:30 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.434	4.108	62511919	50729377	20.848	19.844
28)	SA Decachlor...	8.166	9.270	51263739	36575965	16.796	15.411
Target Compounds							
10)	B gamma-Chl...	0.000	6.256	0	871877	N.D.	0.290 #
17)	MA 4,4'-DDT	0.000	7.277	0	2607813	N.D.	1.151 #
23)	Chlordane-1	4.299	0.000	1127677	0	9.683	N.D. #
25)	Chlordane-3	0.000	6.256	0	871877	N.D.	2.156 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012721\
Data File : PL064458.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2021 15:48
Operator : AR\AJ
Sample : M1236-08
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 16:32:30 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

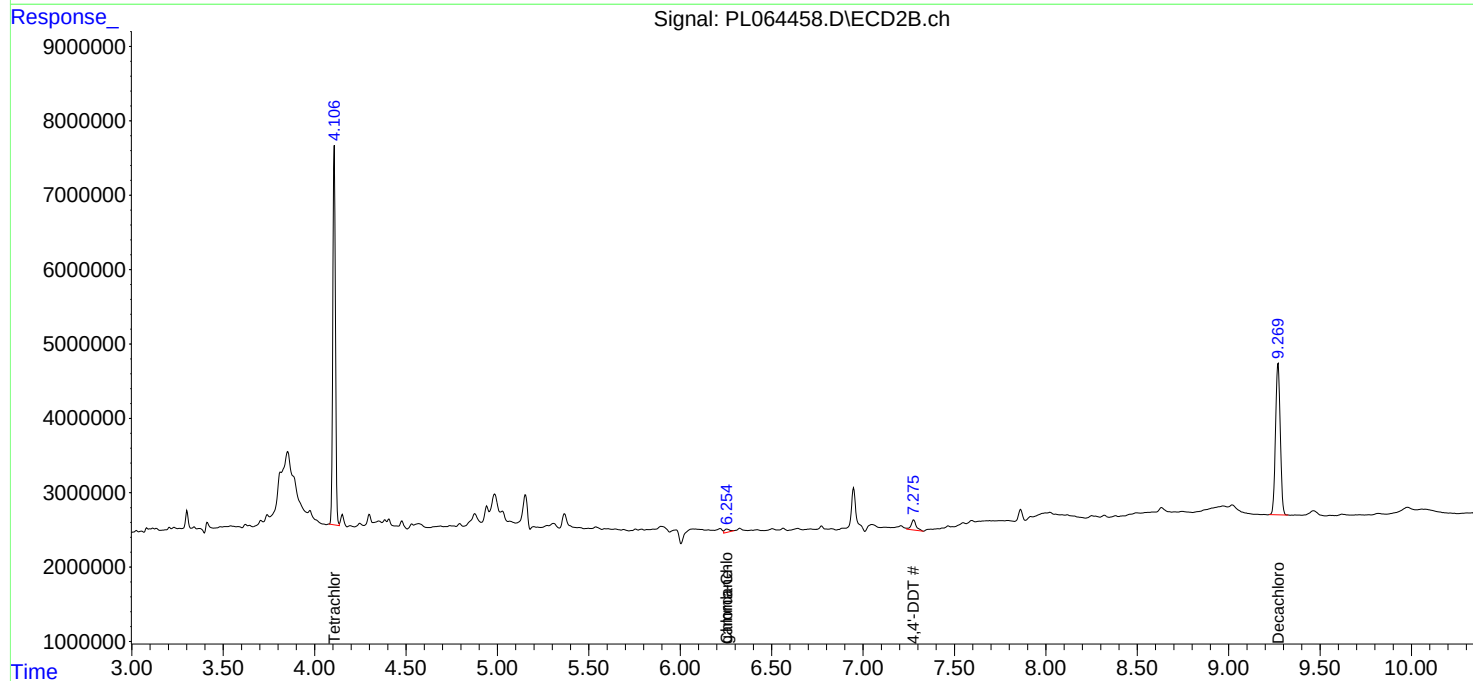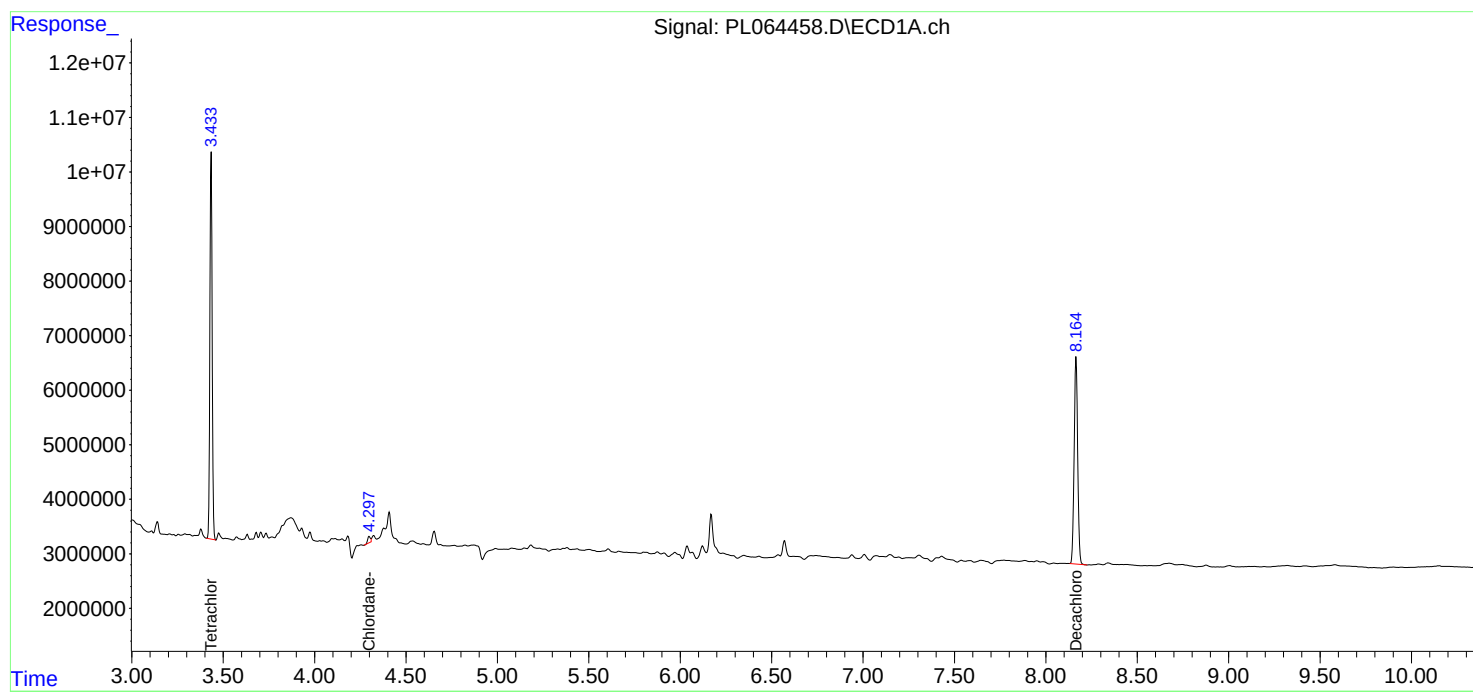


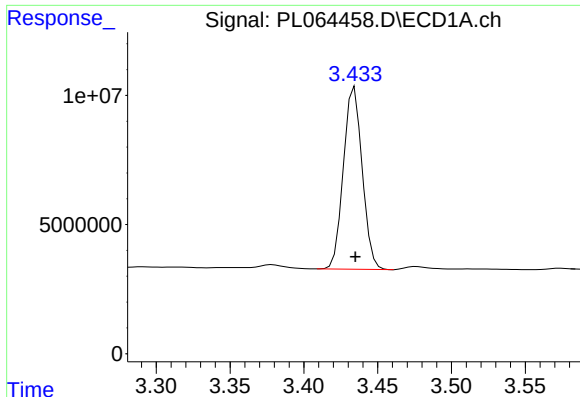

#1 Tetrachloro-m-xylene


R.T.: 3.434 min
Delta R.T.: 0.000 min
Response: 62511919
Conc: 20.85 ng/ml

Instrument :
ECD_L
ClientSampleId :

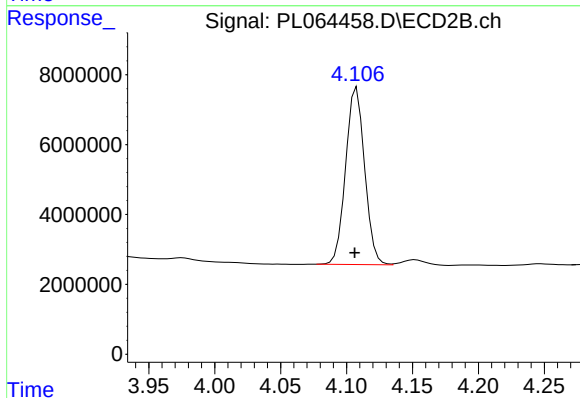


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.001 min
Response: 50729377
Conc: 19.84 ng/ml

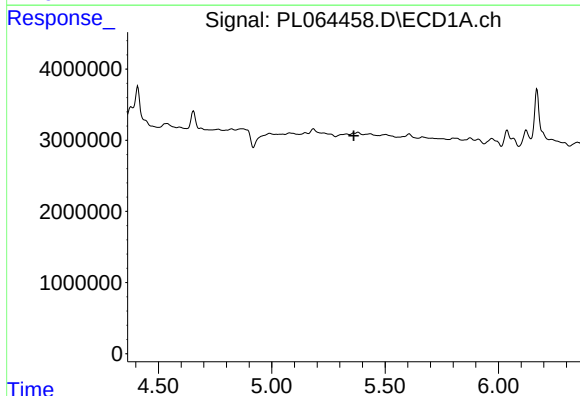


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.362 min
Response: 0
Conc: N.D.

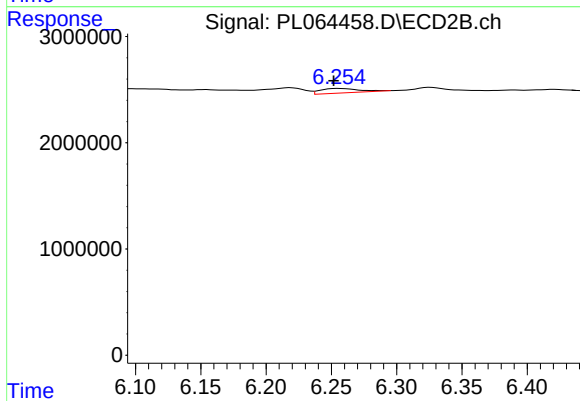

#10 gamma-Chlordane


R.T.: 6.256 min
Delta R.T.: 0.004 min
Response: 871877
Conc: 0.29 ng/ml

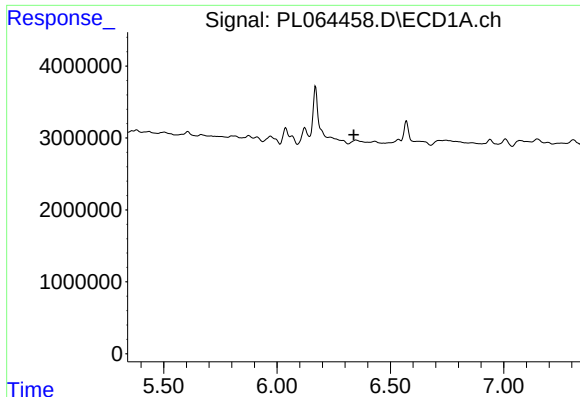

#17 4,4'-DDT


R.T.: 0.000 min
Exp R.T.: 6.339 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

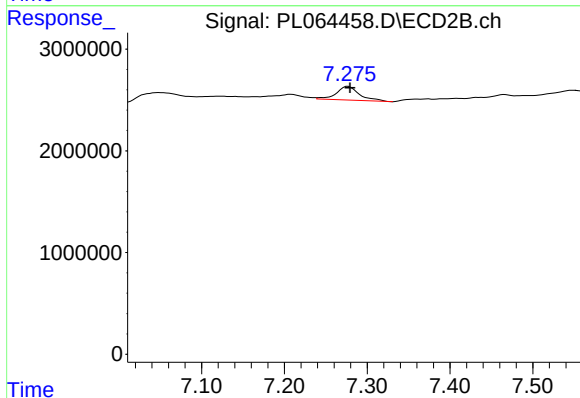


#17 4,4'-DDT

R.T.: 7.277 min
Delta R.T.: -0.002 min
Response: 2607813
Conc: 1.15 ng/ml

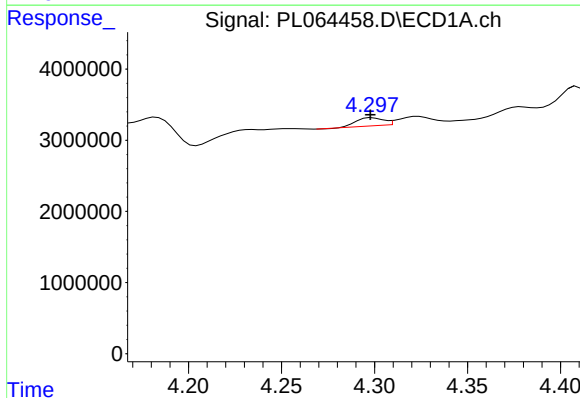


#23 Chlordane-1

R.T.: 4.299 min
Delta R.T.: 0.001 min
Response: 1127677
Conc: 9.68 ng/ml

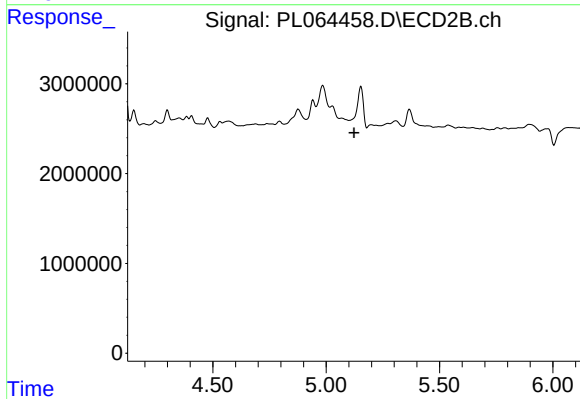

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.123 min
Response: 0
Conc: N.D.

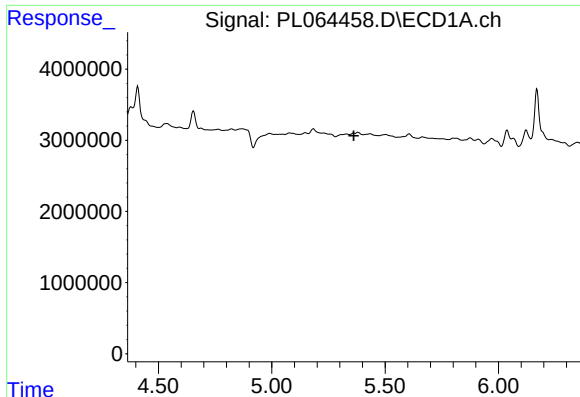

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.362 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

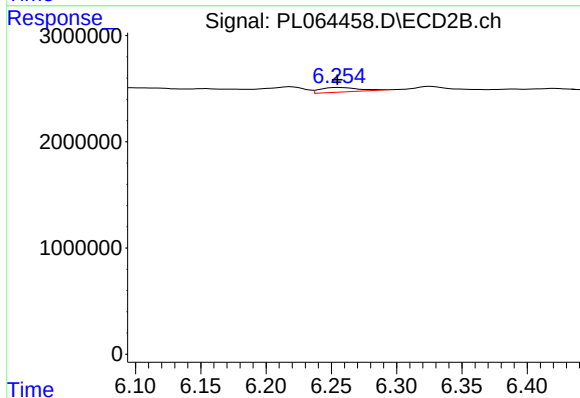


#25 Chlordane-3

R.T.: 6.256 min
Delta R.T.: 0.001 min
Response: 871877
Conc: 2.16 ng/ml

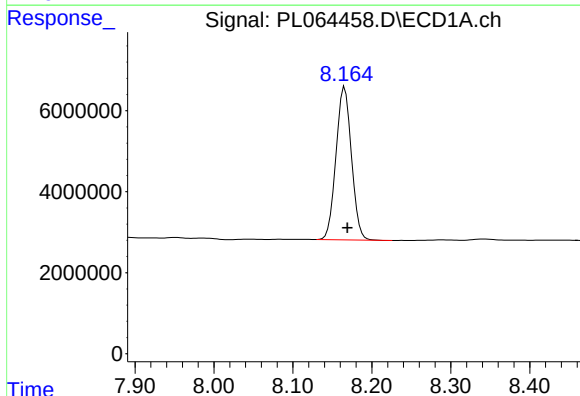

#28 Decachlorobiphenyl

R.T.: 8.166 min
Delta R.T.: -0.003 min
Response: 51263739
Conc: 16.80 ng/ml

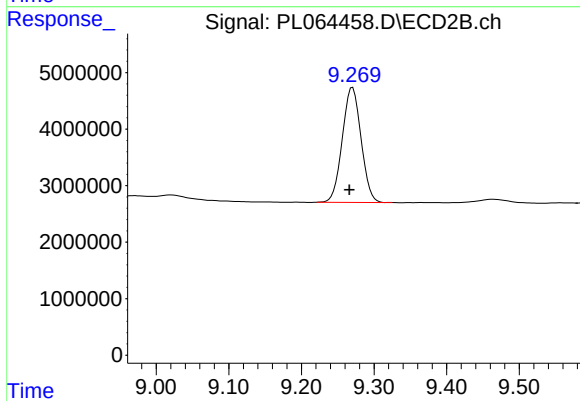

#28 Decachlorobiphenyl

R.T.: 9.270 min
Delta R.T.: 0.004 min
Response: 36575965
Conc: 15.41 ng/ml