

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012721\
 Data File : PL064453.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 27 Jan 2021 13:43
 Operator : AR\AJ
 Sample : M1228-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OK-01-012521

Manual Integrations
 APPROVED

Ankita
 1/29/2021 1:24:06 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Jan 27 15:55:52 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
 Quant Title : GC Extractables
 QLast Update : Mon Jan 18 13:25:12 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.433	4.108	41516313	29894254	13.846	11.694
28) SA Decachlor...	8.164	9.268	31151183	25215687	10.207	10.624
Target Compounds						
11) B alpha-Chl...	5.415	6.325	2545464	4970641	0.665m	1.633m#
12) B 4,4'-DDE	5.583	6.483	2326682	3736976	0.660	1.403 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL012721\
Data File : PL064453.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 27 Jan 2021 13:43
Operator : AR\AJ
Sample : M1228-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OK-01-012521


Manual Integrations
APPROVED

Ankita
1/29/2021 1:24:06 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Jan 27 15:55:52 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL011221.M
Quant Title : GC Extractables
QLast Update : Mon Jan 18 13:25:12 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

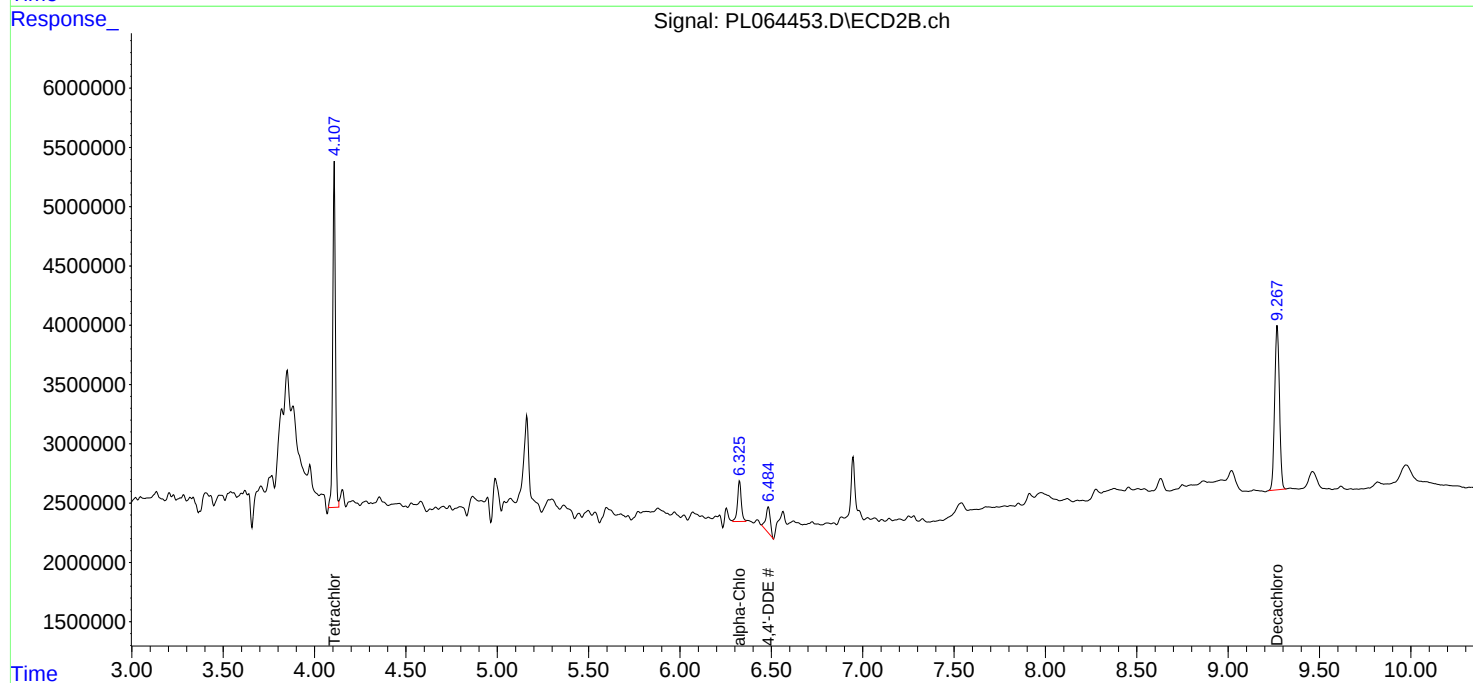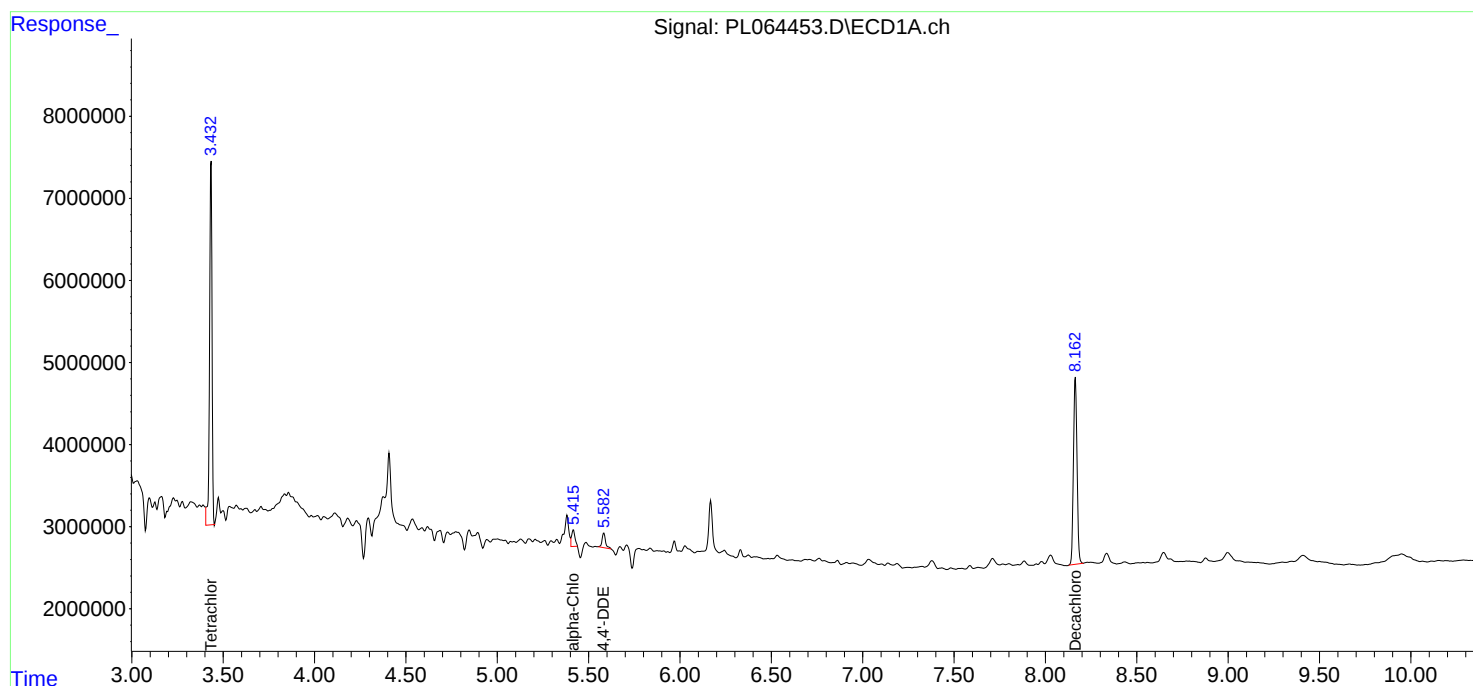

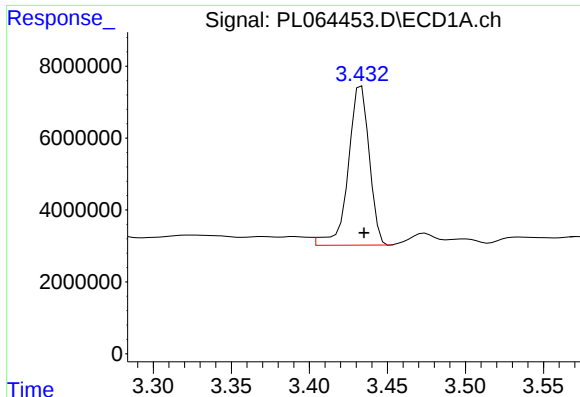


#1 Tetrachloro-m-xylene

R.T.: 3.433 min
Delta R.T.: -0.002 min
Response: 41516313
Conc: 13.85 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-012521


Manual Integrations
APPROVED

Ankita
1/29/2021 1:24:06 PM

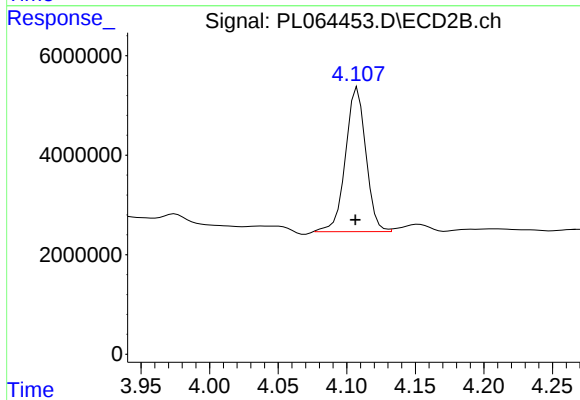


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.002 min
Response: 29894254
Conc: 11.69 ng/ml

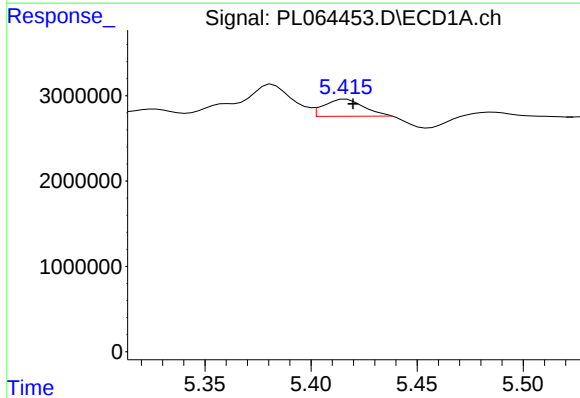


#11 alpha-Chlordane

R.T.: 5.415 min
Delta R.T.: -0.005 min
Response: 2545464
Conc: 0.67 ng/ml m

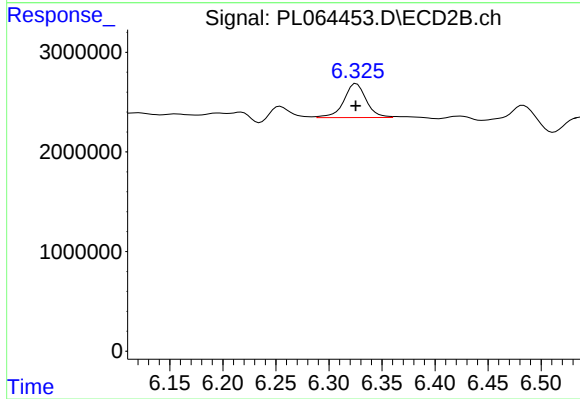

#11 alpha-Chlordane

R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 4970641
Conc: 1.63 ng/ml m

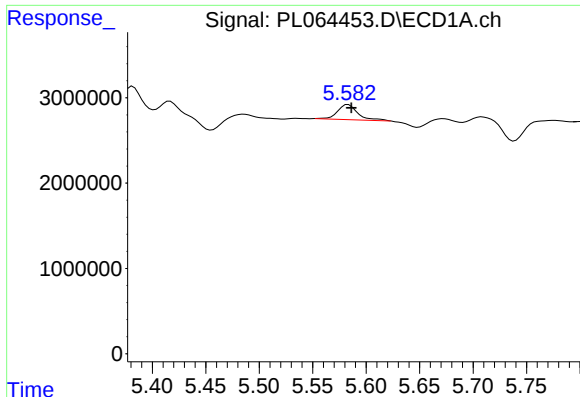


#12 4,4'-DDE

R.T.: 5.583 min
Delta R.T.: -0.003 min
Response: 2326682
Conc: 0.66 ng/ml

Instrument :
ECD_L
ClientSampleId :
OK-01-012521


Manual Integrations
APPROVED

Ankita
1/29/2021 1:24:06 PM

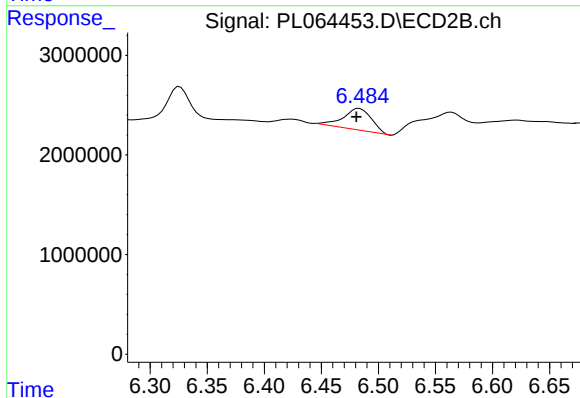


#12 4,4'-DDE

R.T.: 6.483 min
Delta R.T.: 0.003 min
Response: 3736976
Conc: 1.40 ng/ml

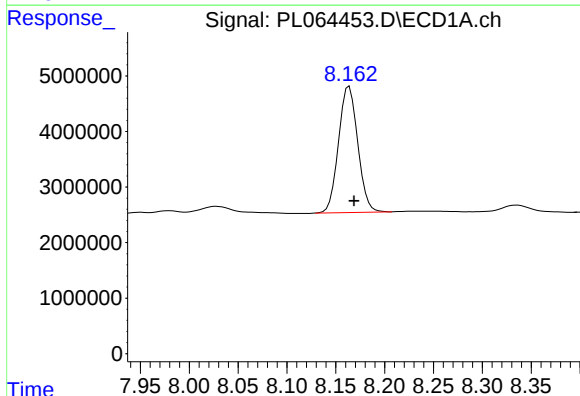

#28 Decachlorobiphenyl

R.T.: 8.164 min
Delta R.T.: -0.005 min
Response: 31151183
Conc: 10.21 ng/ml

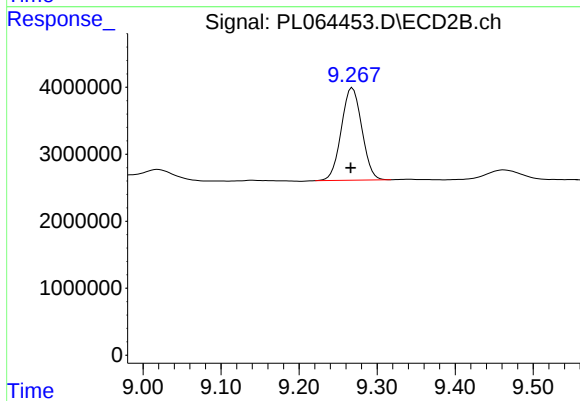

#28 Decachlorobiphenyl

R.T.: 9.268 min
Delta R.T.: 0.002 min
Response: 25215687
Conc: 10.62 ng/ml