

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL020421\  
 Data File : PL064617.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 04 Feb 2021 09:34  
 Operator : AR\AJ  
 Sample : PB134443BL  
 Misc :  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 ECD\_L  
 ClientSampleId :

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Feb 05 01:59:50 2021  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL012921.M  
 Quant Title : GC Extractables  
 QLast Update : Fri Jan 29 04:48:57 2021  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

|                             | Compound        | RT#1   | RT#2  | Resp#1   | Resp#2   | ng/ml  | ng/ml   |
|-----------------------------|-----------------|--------|-------|----------|----------|--------|---------|
| -----                       |                 |        |       |          |          |        |         |
| System Monitoring Compounds |                 |        |       |          |          |        |         |
| 1)                          | SA Tetrachlo... | 3.432  | 4.108 | 60188159 | 49475012 | 19.772 | 20.770  |
| 28)                         | SA Decachlor... | 8.164  | 9.271 | 62868896 | 45117988 | 19.950 | 22.037  |
| Target Compounds            |                 |        |       |          |          |        |         |
| 4)                          | MA Heptachlor   | 0.000  | 5.299 | 0        | 6533874  | N.D.   | 1.875 # |
| 6)                          | B beta-BHC      | 0.000  | 4.983 | 0        | 2748286  | N.D.   | 1.624 # |
| 14)                         | MA Endrin       | 5.970  | 0.000 | 6753194  | 0        | 1.846  | N.D. #  |
| 23)                         | Chlordane-1     | 4.320f | 0.000 | 1890544  | 0        | 17.199 | N.D. #  |
| -----                       |                 |        |       |          |          |        |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_L\Data\PL020421\  
Data File : PL064617.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 04 Feb 2021 09:34  
Operator : AR\AJ  
Sample : PB134443BL  
Misc :  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
ECD\_L  
ClientSampleId :

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Feb 05 01:59:50 2021  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_L\methods\PL012921.M  
Quant Title : GC Extractables  
QLast Update : Fri Jan 29 04:48:57 2021  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1  
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

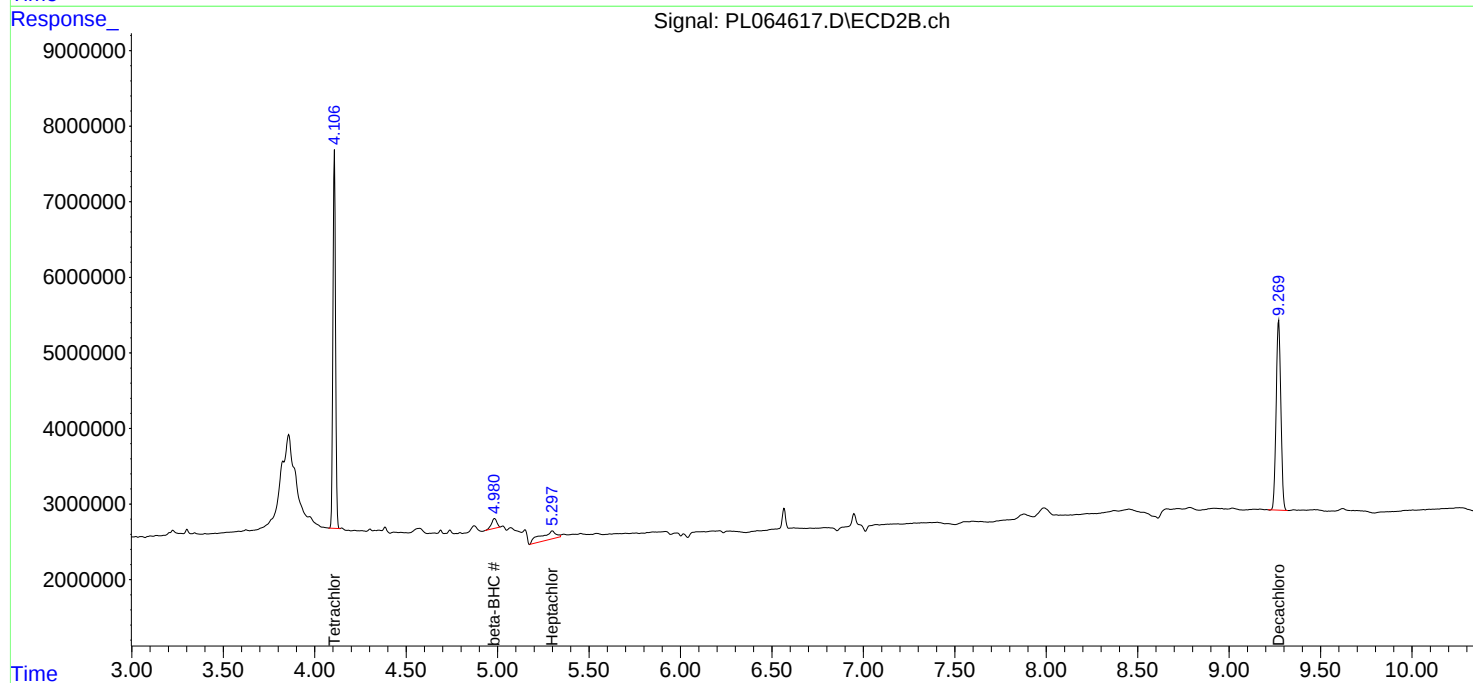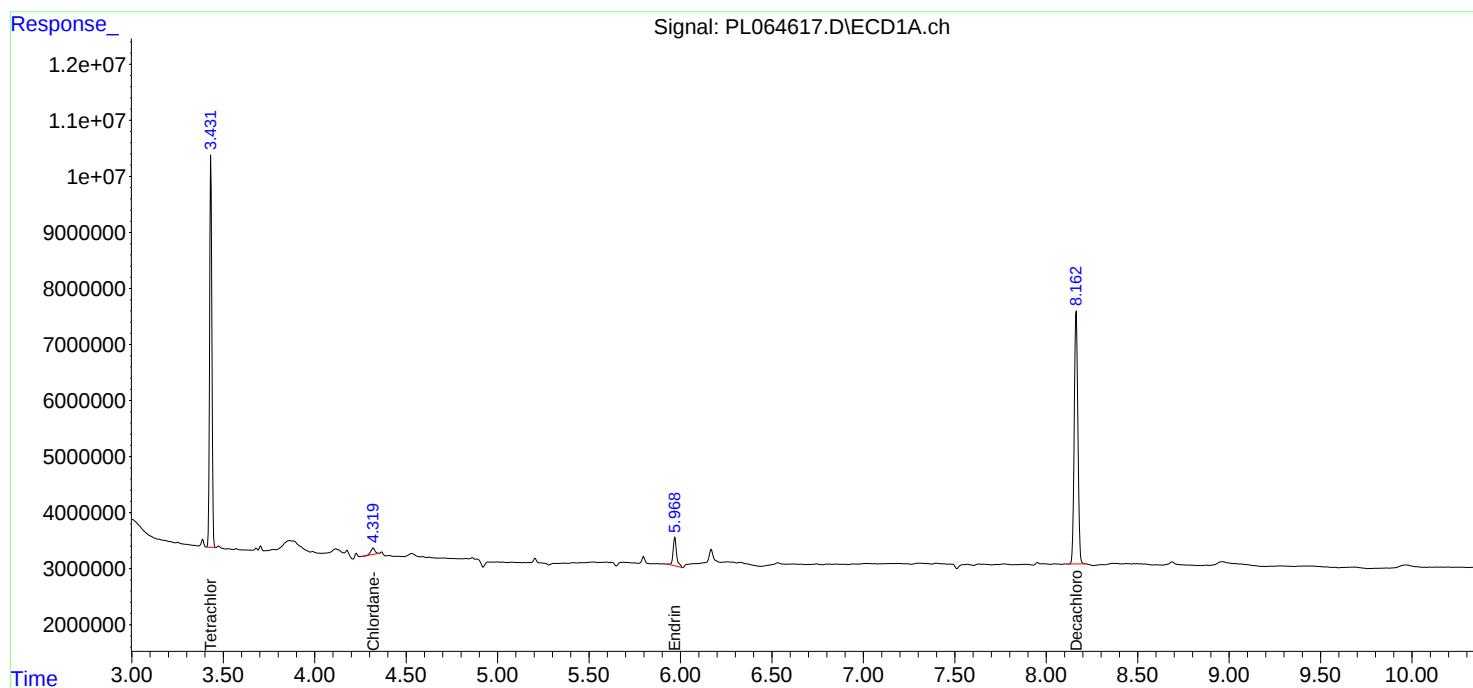


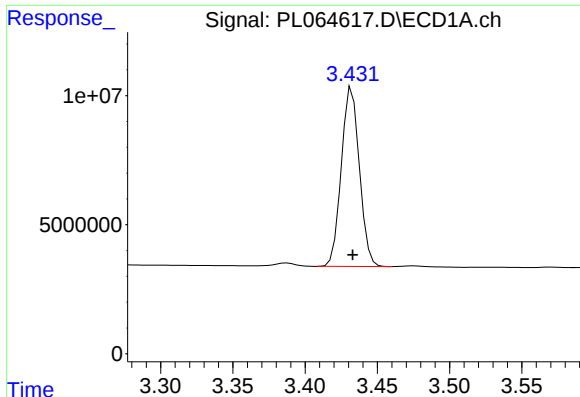

#1 Tetrachloro-m-xylene


R.T.: 3.432 min  
Delta R.T.: 0.000 min  
Response: 60188159  
Conc: 19.77 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

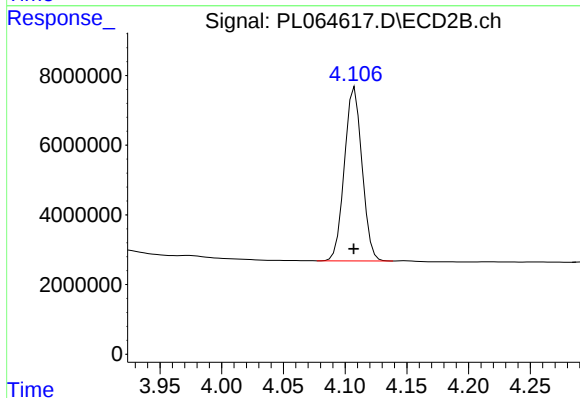


#1 Tetrachloro-m-xylene

R.T.: 4.108 min  
Delta R.T.: 0.000 min  
Response: 49475012  
Conc: 20.77 ng/ml

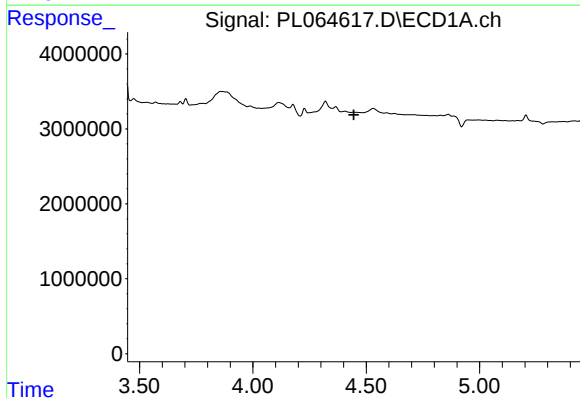


#4 Heptachlor

R.T.: 0.000 min  
Exp R.T. : 4.445 min  
Response: 0  
Conc: N.D.

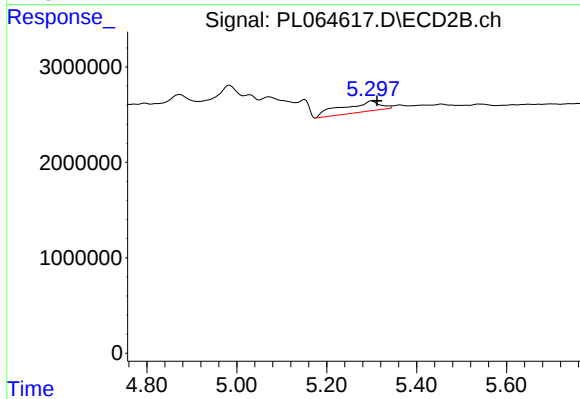

#4 Heptachlor


R.T.: 5.299 min  
Delta R.T.: -0.012 min  
Response: 6533874  
Conc: 1.87 ng/ml

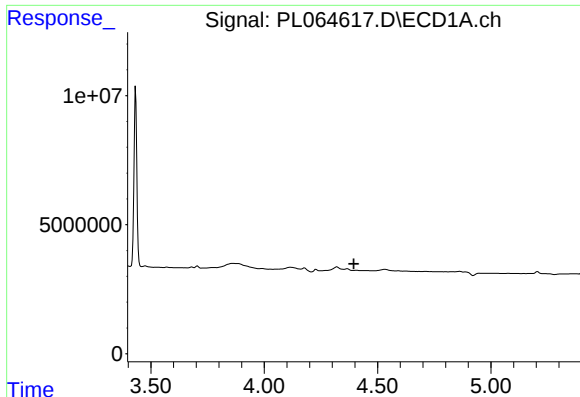

#6 beta-BHC


R.T.: 0.000 min  
Exp R.T.: 4.395 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_L  
ClientSampleId :

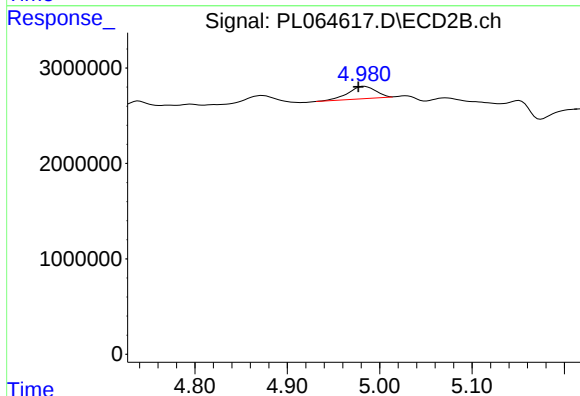


#6 beta-BHC

R.T.: 4.983 min  
Delta R.T.: 0.006 min  
Response: 2748286  
Conc: 1.62 ng/ml

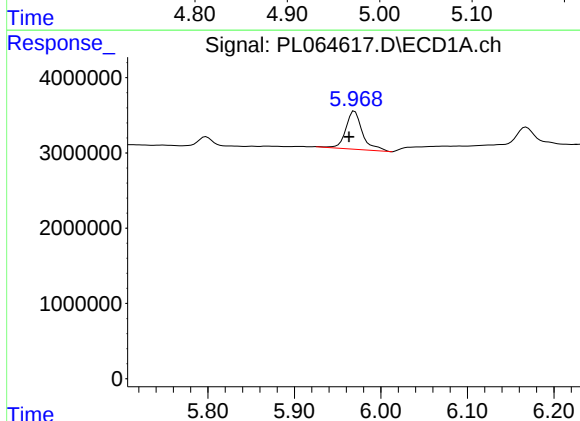


#14 Endrin

R.T.: 5.970 min  
Delta R.T.: 0.007 min  
Response: 6753194  
Conc: 1.85 ng/ml

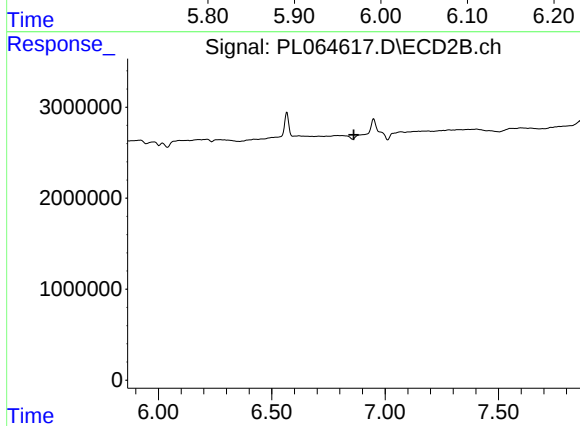

#14 Endrin


R.T.: 0.000 min  
Exp R.T.: 6.862 min  
Response: 0  
Conc: N.D.

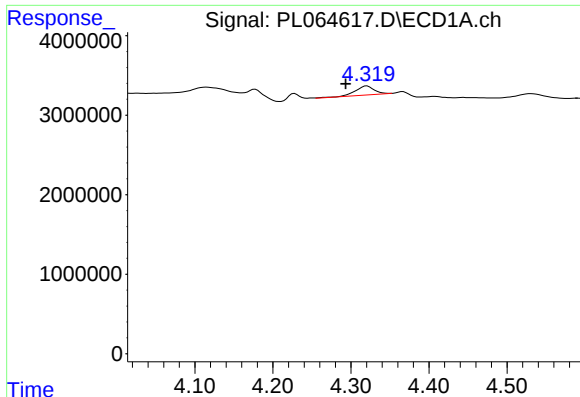

#23 Chlordane-1


R.T.: 4.320 min  
Delta R.T.: 0.027 min  
Response: 1890544  
Conc: 17.20 ng/ml

Instrument :  
ECD\_L  
ClientSampleId :

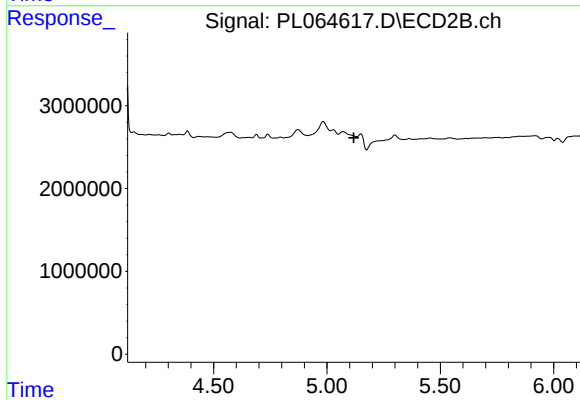


#23 Chlordane-1

R.T.: 0.000 min  
Exp R.T. : 5.119 min  
Response: 0  
Conc: N.D.

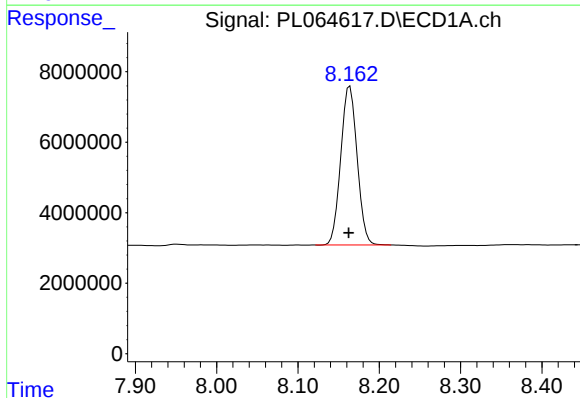

#28 Decachlorobiphenyl

R.T.: 8.164 min  
Delta R.T.: 0.001 min  
Response: 62868896  
Conc: 19.95 ng/ml

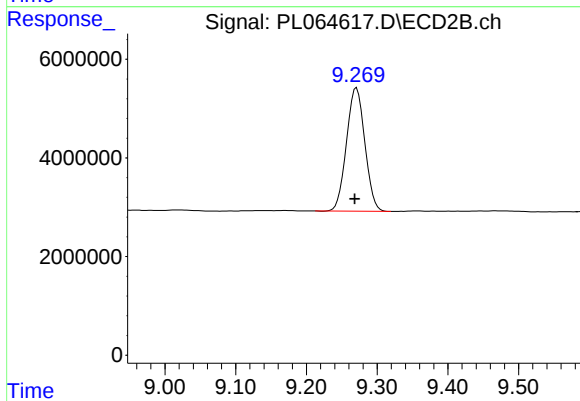

#28 Decachlorobiphenyl

R.T.: 9.271 min  
Delta R.T.: 0.002 min  
Response: 45117988  
Conc: 22.04 ng/ml