

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020421\
 Data File : PL064617.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2021 09:34
 Operator : AR\AJ
 Sample : PB134443BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB134443BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 01:59:50 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	4.108	60188159	49475012	19.772	20.770
28)	SA Decachlor...	8.164	9.271	62868896	45117988	19.950	22.037
Target Compounds							
4)	MA Heptachlor	0.000	5.299	0	6533874	N.D.	1.875 #
6)	B beta-BHC	0.000	4.983	0	2748286	N.D.	1.624 #
14)	MA Endrin	5.970	0.000	6753194	0	1.846	N.D. #
23)	Chlordane-1	4.320f	0.000	1890544	0	17.199	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020421\
Data File : PL064617.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2021 09:34
Operator : AR\AJ
Sample : PB134443BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB134443BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 01:59:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

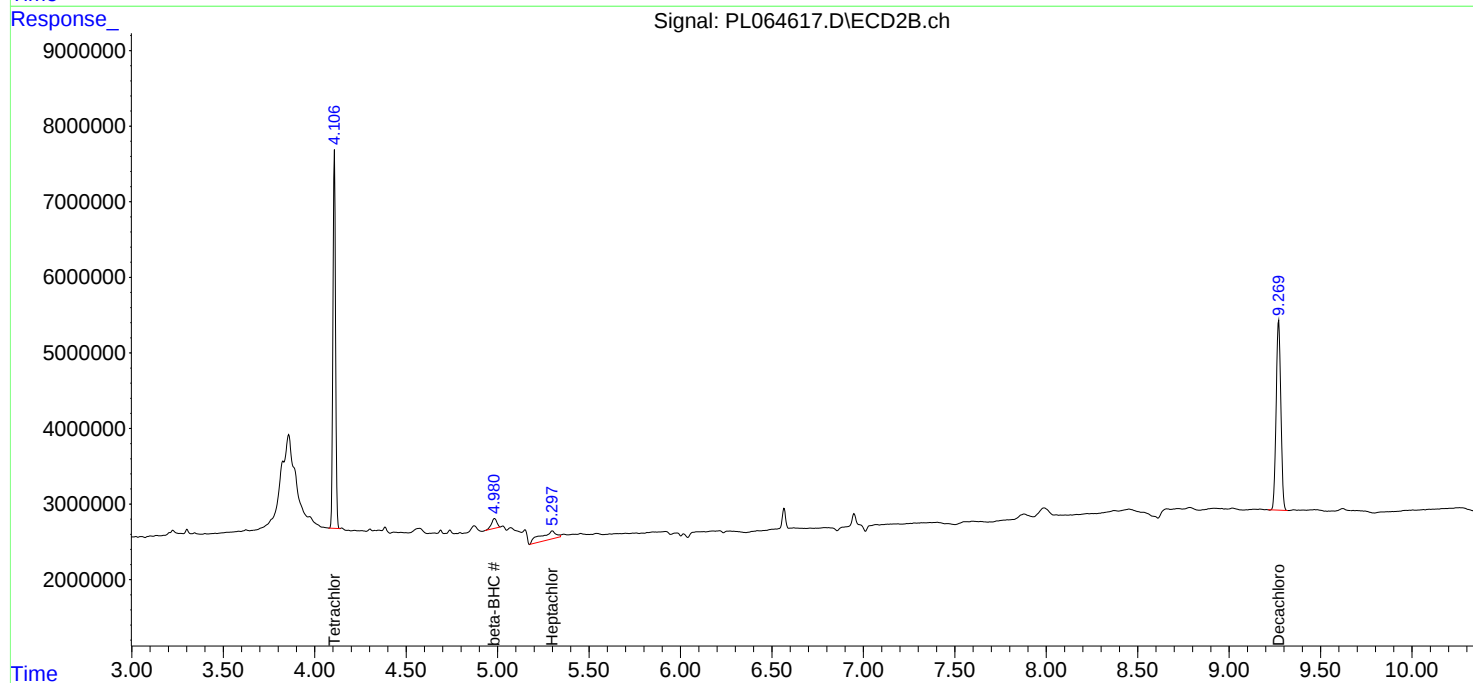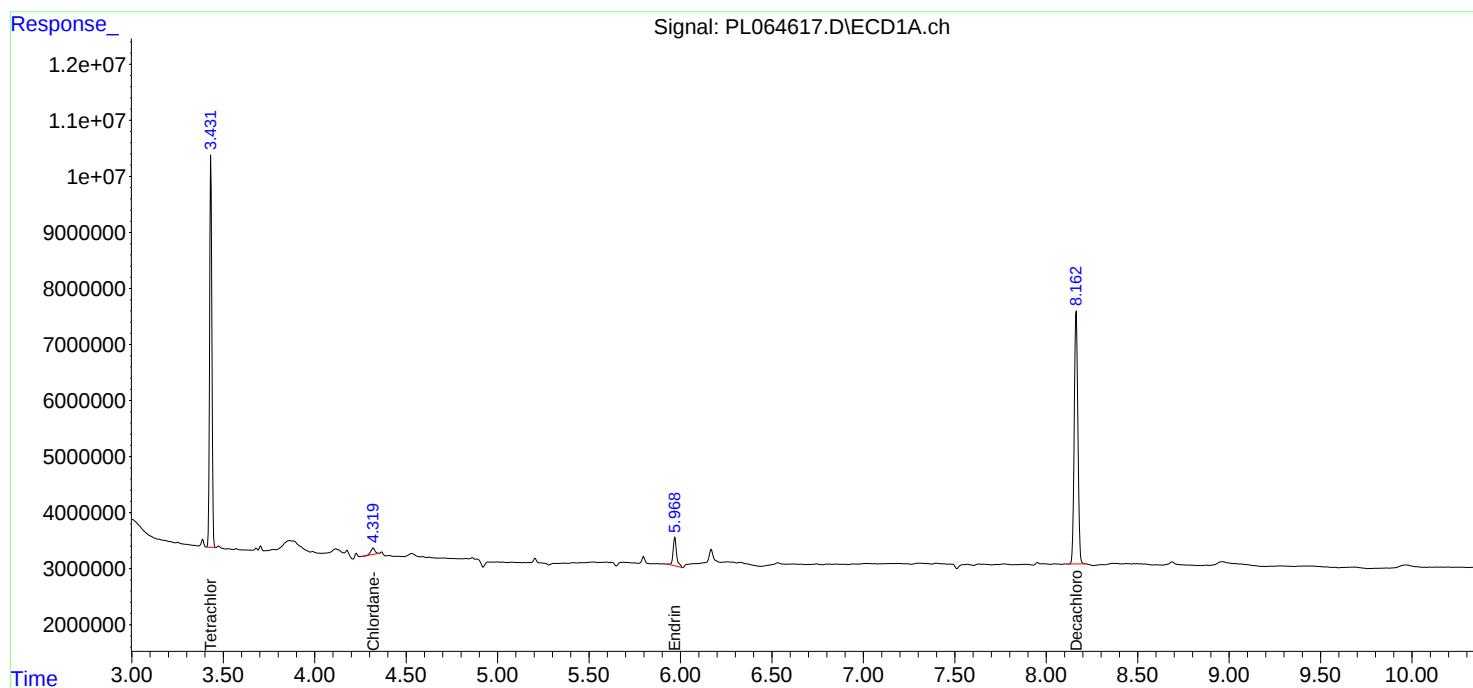


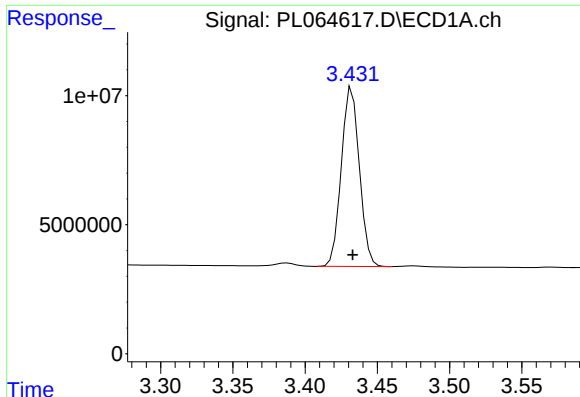

#1 Tetrachloro-m-xylene


R.T.: 3.432 min
Delta R.T.: 0.000 min
Response: 60188159
Conc: 19.77 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB134443BL

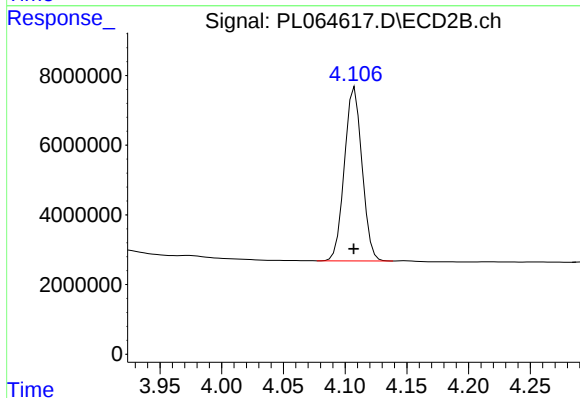


#1 Tetrachloro-m-xylene

R.T.: 4.108 min
Delta R.T.: 0.000 min
Response: 49475012
Conc: 20.77 ng/ml

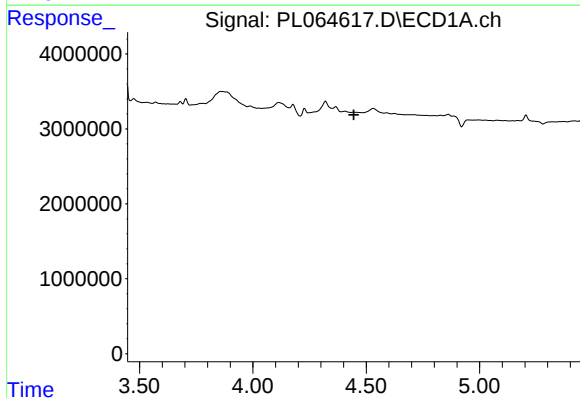


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.445 min
Response: 0
Conc: N.D.

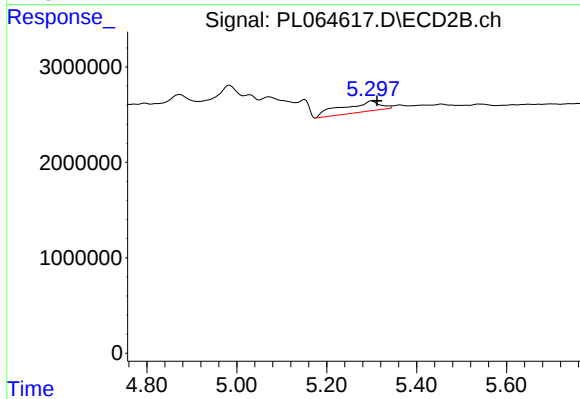

#4 Heptachlor


R.T.: 5.299 min
Delta R.T.: -0.012 min
Response: 6533874
Conc: 1.87 ng/ml

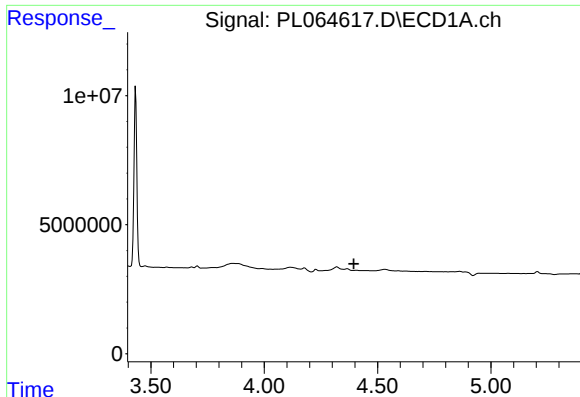

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
PB134443BL

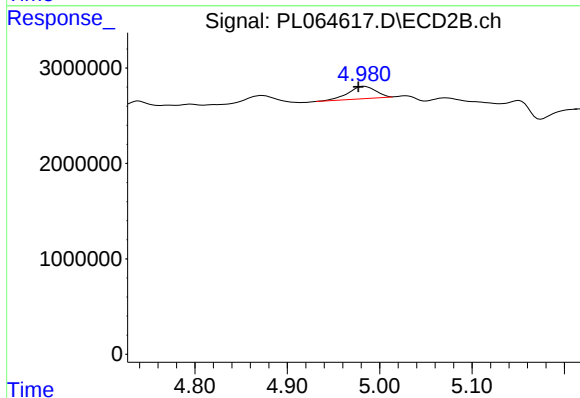


#6 beta-BHC

R.T.: 4.983 min
Delta R.T.: 0.006 min
Response: 2748286
Conc: 1.62 ng/ml

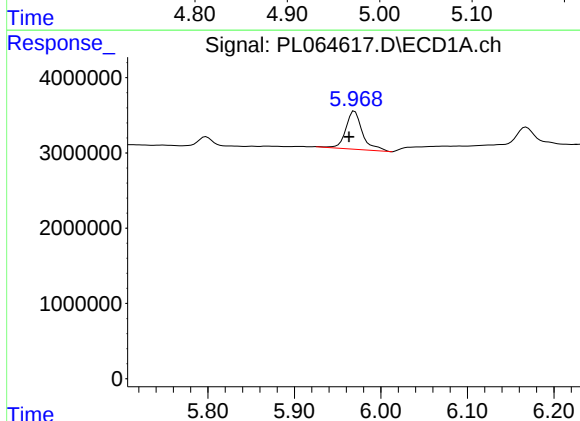


#14 Endrin

R.T.: 5.970 min
Delta R.T.: 0.007 min
Response: 6753194
Conc: 1.85 ng/ml

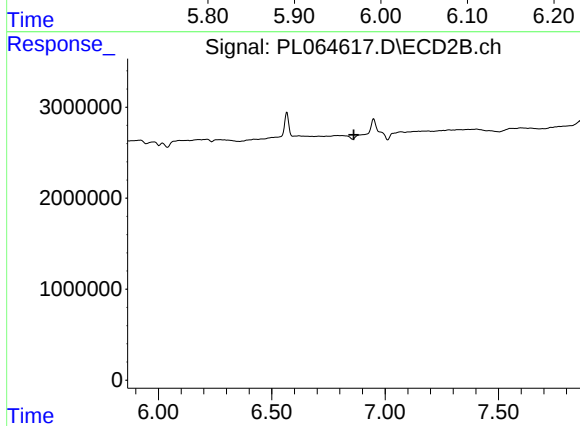

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.862 min
Response: 0
Conc: N.D.

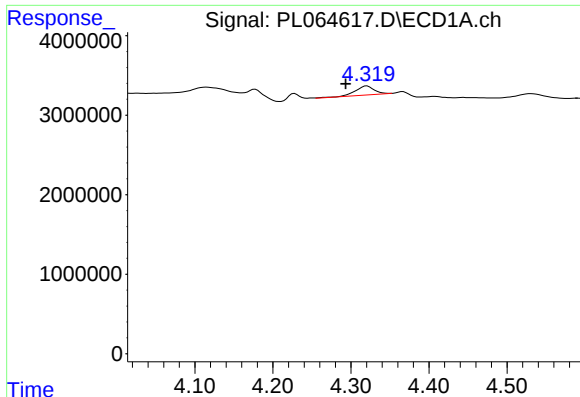

#23 Chlordane-1


R.T.: 4.320 min
Delta R.T.: 0.027 min
Response: 1890544
Conc: 17.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB134443BL

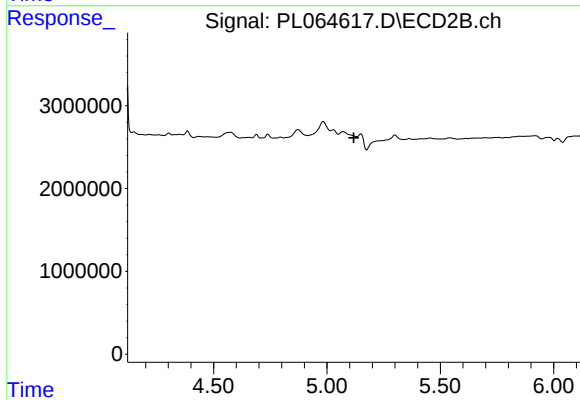


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.119 min
Response: 0
Conc: N.D.

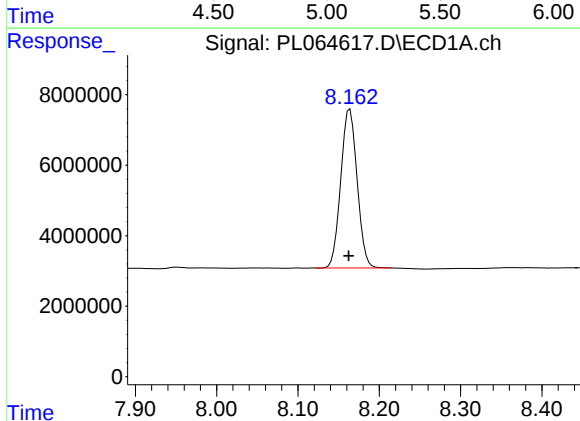

#28 Decachlorobiphenyl

R.T.: 8.164 min
Delta R.T.: 0.001 min
Response: 62868896
Conc: 19.95 ng/ml

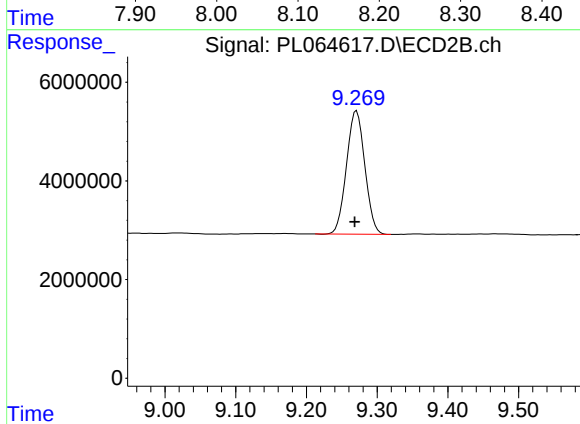

#28 Decachlorobiphenyl

R.T.: 9.271 min
Delta R.T.: 0.002 min
Response: 45117988
Conc: 22.04 ng/ml