

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020421\
 Data File : PL064618.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2021 09:49
 Operator : AR\AJ
 Sample : M1291-03
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OU421-007-0510

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 02:00:06 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	4.107	40174979	33261474	13.197	13.963
28)	SA Decachlor...	8.164	9.270	47297267	34451482	15.008	16.827
Target Compounds							
4)	MA Heptachlor	0.000	5.300	0	5103990	N.D.	1.464 #
6)	B beta-BHC	0.000	4.985	0	2897014	N.D.	1.712 #
19)	B Endosulfa...	6.617	0.000	2949291	0	0.811	N.D. #
20)	A Methoxychlor	6.861f	0.000	2151081	0	1.191	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020421\
Data File : PL064618.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2021 09:49
Operator : AR\AJ
Sample : M1291-03
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
OU421-007-0510

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 02:00:06 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

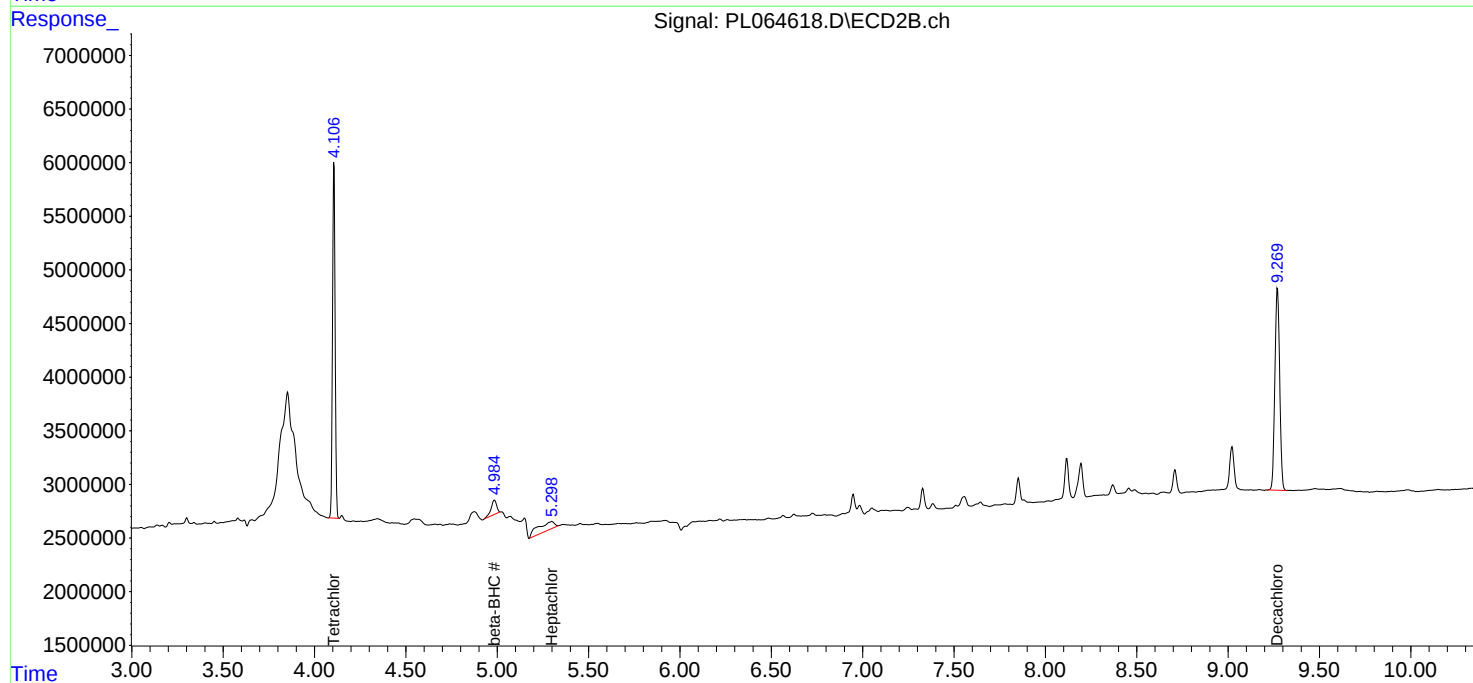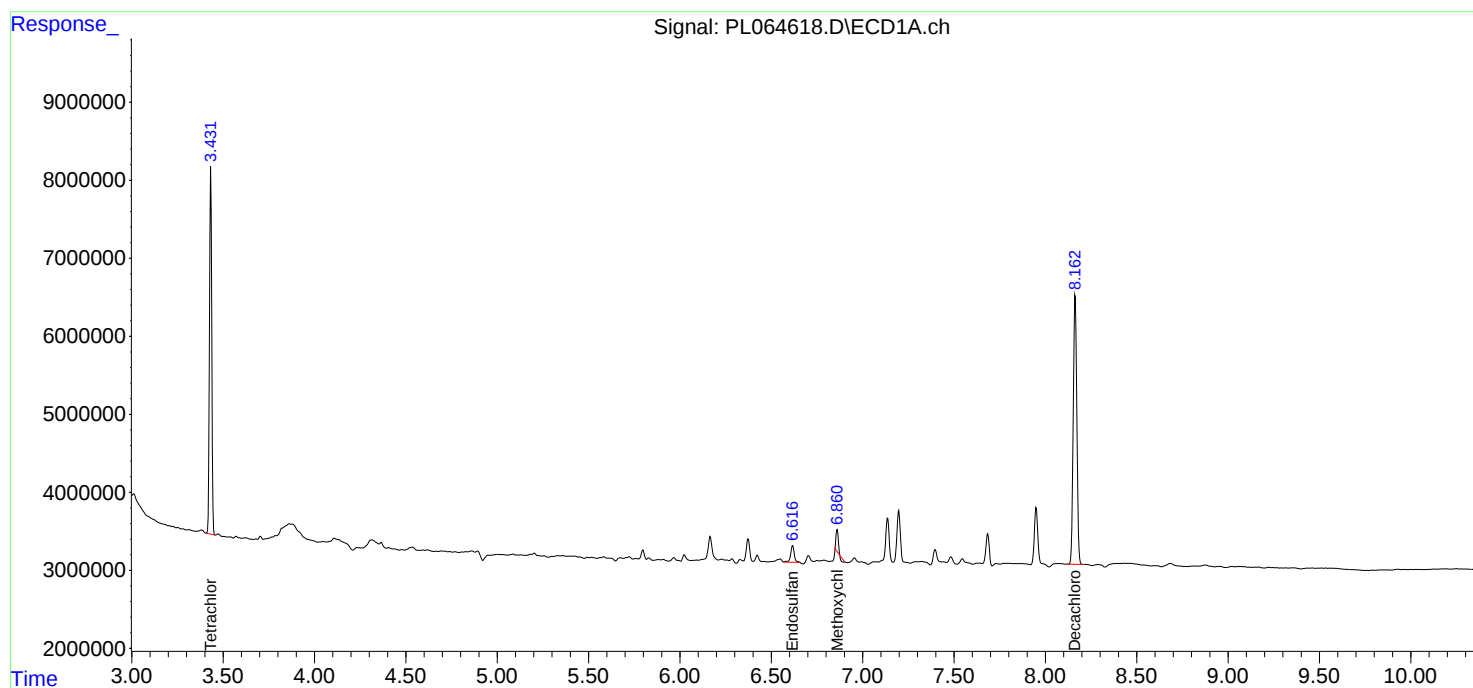


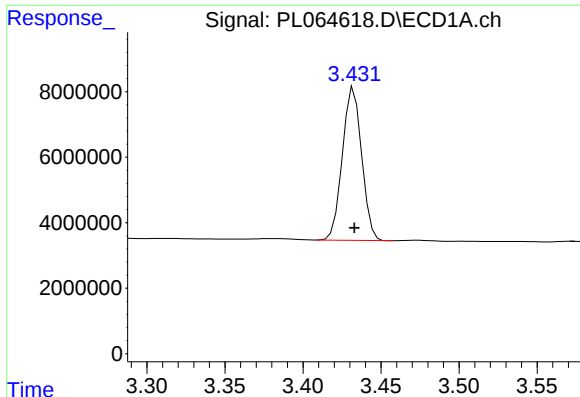

#1 Tetrachloro-m-xylene


R.T.: 3.433 min
Delta R.T.: 0.000 min
Response: 40174979
Conc: 13.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU421-007-0510

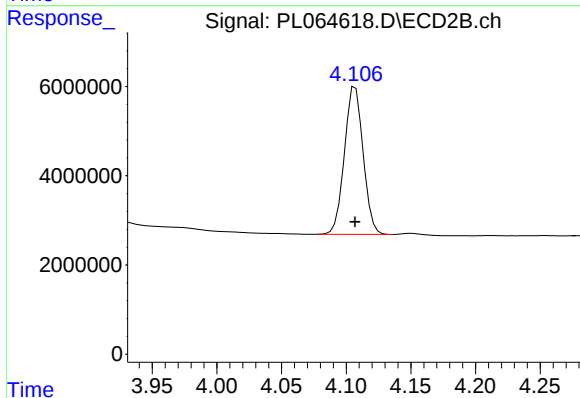


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 33261474
Conc: 13.96 ng/ml

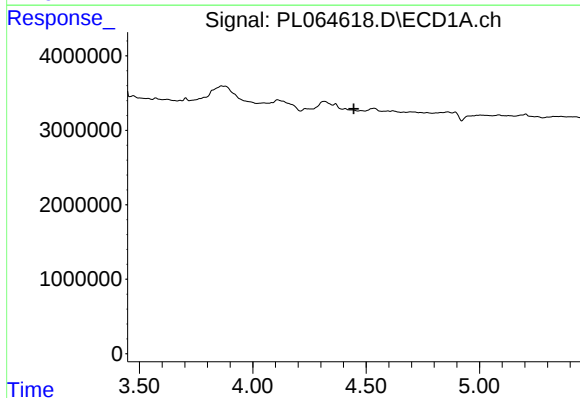


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.445 min
Response: 0
Conc: N.D.

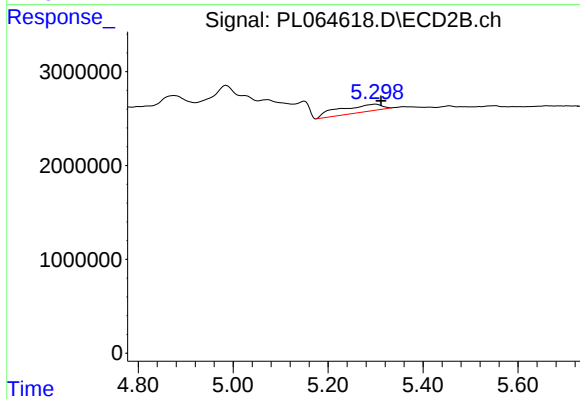

#4 Heptachlor


R.T.: 5.300 min
Delta R.T.: -0.011 min
Response: 5103990
Conc: 1.46 ng/ml

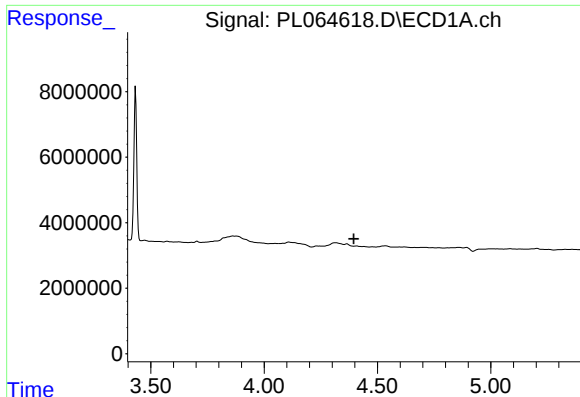

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
OU421-007-0510

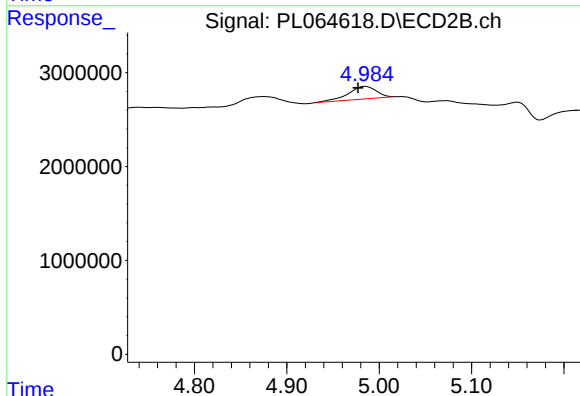


#6 beta-BHC

R.T.: 4.985 min
Delta R.T.: 0.008 min
Response: 2897014
Conc: 1.71 ng/ml

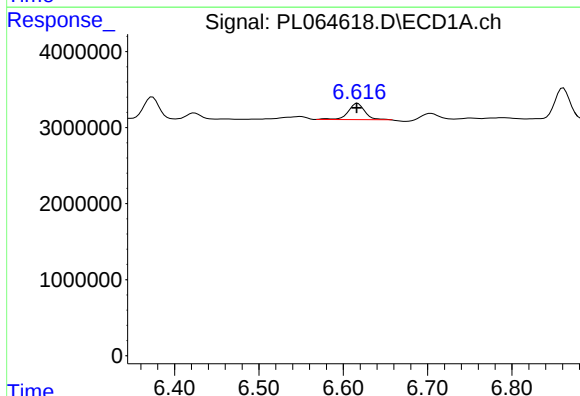


#19 Endosulfan Sulfate

R.T.: 6.617 min
Delta R.T.: 0.001 min
Response: 2949291
Conc: 0.81 ng/ml

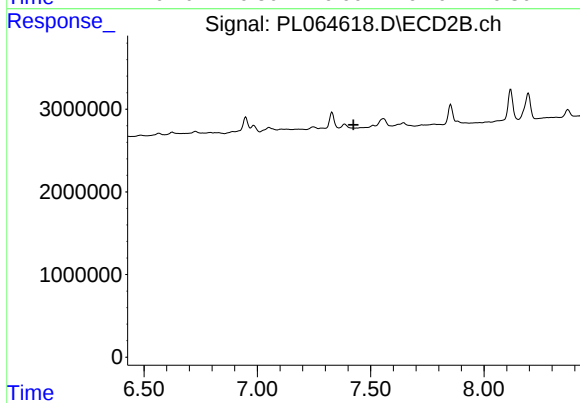

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T.: 7.425 min
Response: 0
Conc: N.D.

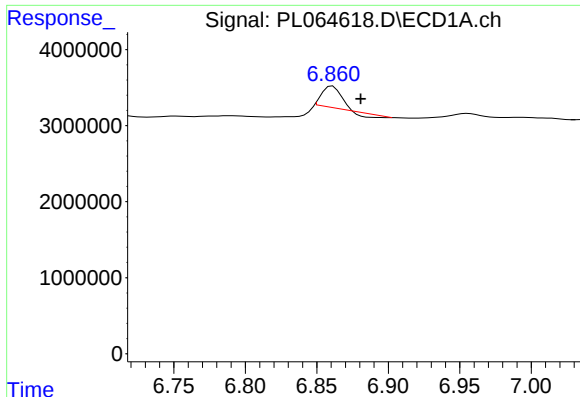

#20 Methoxychlor


R.T.: 6.861 min
Delta R.T.: -0.020 min
Response: 2151081
Conc: 1.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU421-007-0510

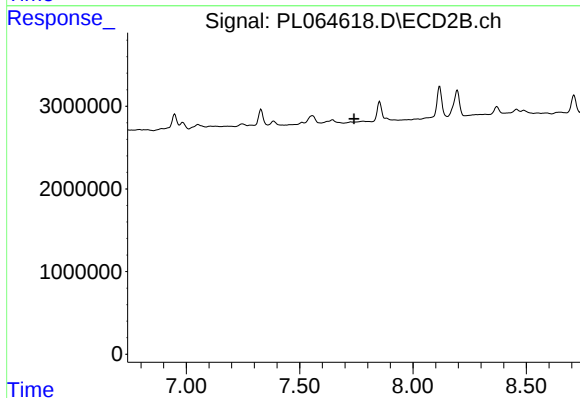


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T.: 7.740 min
Response: 0
Conc: N.D.

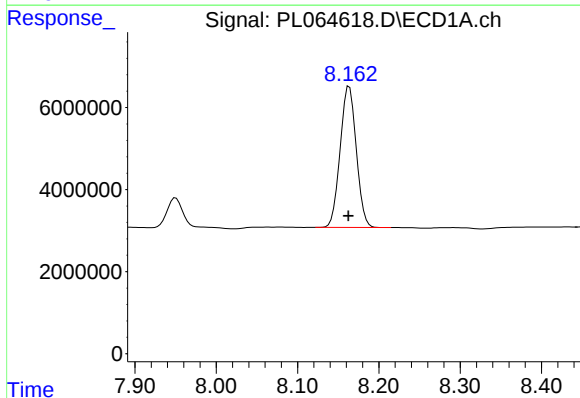

#28 Decachlorobiphenyl

R.T.: 8.164 min
Delta R.T.: 0.001 min
Response: 47297267
Conc: 15.01 ng/ml

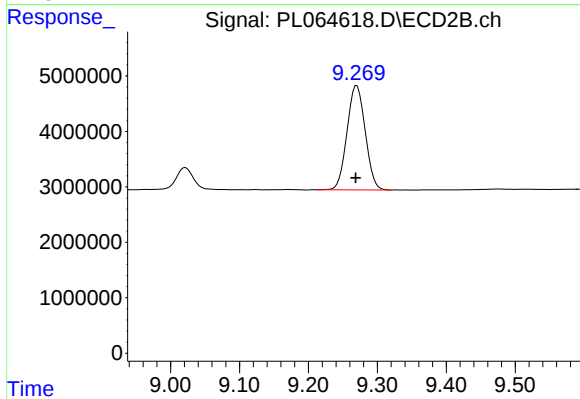

#28 Decachlorobiphenyl

R.T.: 9.270 min
Delta R.T.: 0.002 min
Response: 34451482
Conc: 16.83 ng/ml