

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020421\
 Data File : PL064635.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2021 16:53
 Operator : AR\AJ
 Sample : PB134435BL
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PB134435BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 02:06:04 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	4.107	59342120	49597182	19.494	20.821
28)	SA Decachlor...	8.161	9.270	61049615	46158750	19.372	22.545
Target Compounds							
4)	MA Heptachlor	0.000	5.302	0	22519816	N.D.	6.461 #
6)	B beta-BHC	4.367f	0.000	414997	0	0.215	N.D. #
10)	B gamma-Chl...	0.000	6.261	0	1899243	N.D.	0.653 #
23)	Chlordane-1	4.281	0.000	15125536	0	137.601	N.D. #
25)	Chlordane-3	0.000	6.261	0	1899243	N.D.	5.298 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020421\
Data File : PL064635.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2021 16:53
Operator : AR\AJ
Sample : PB134435BL
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PB134435BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 02:06:04 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

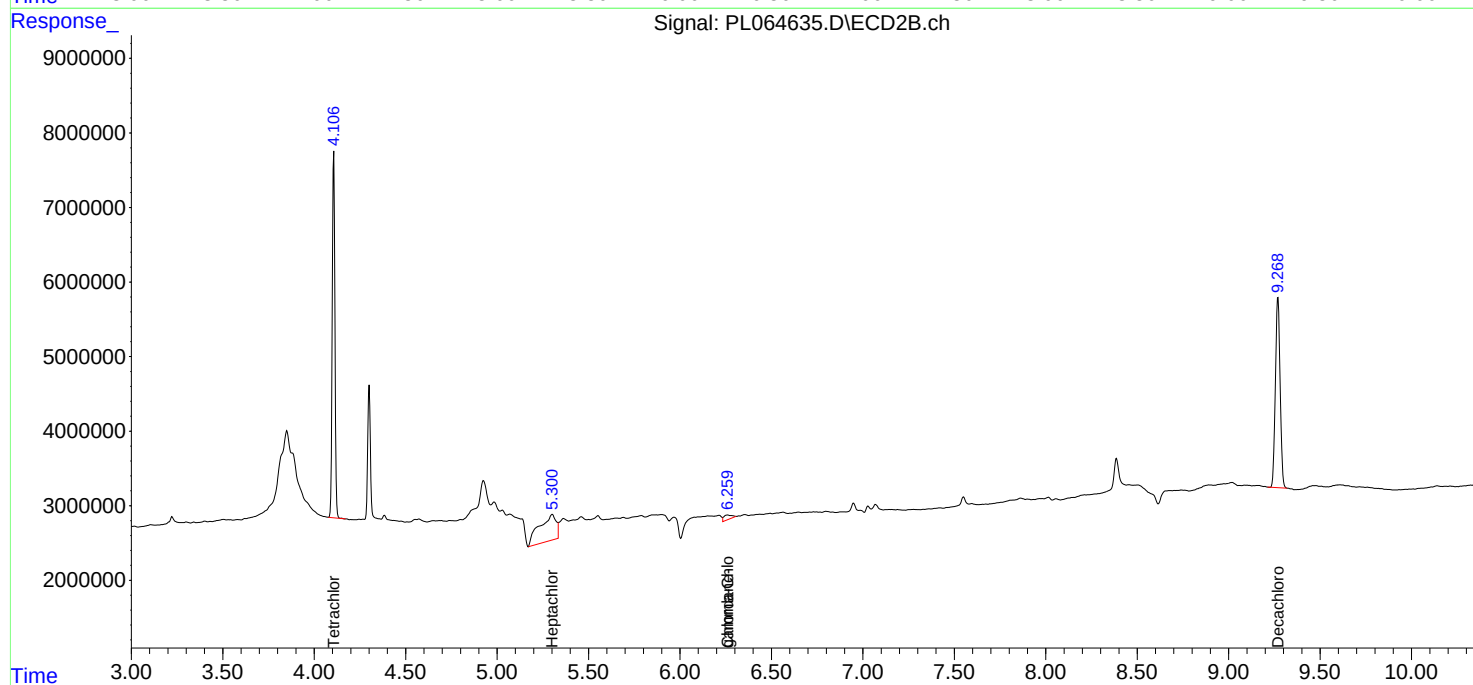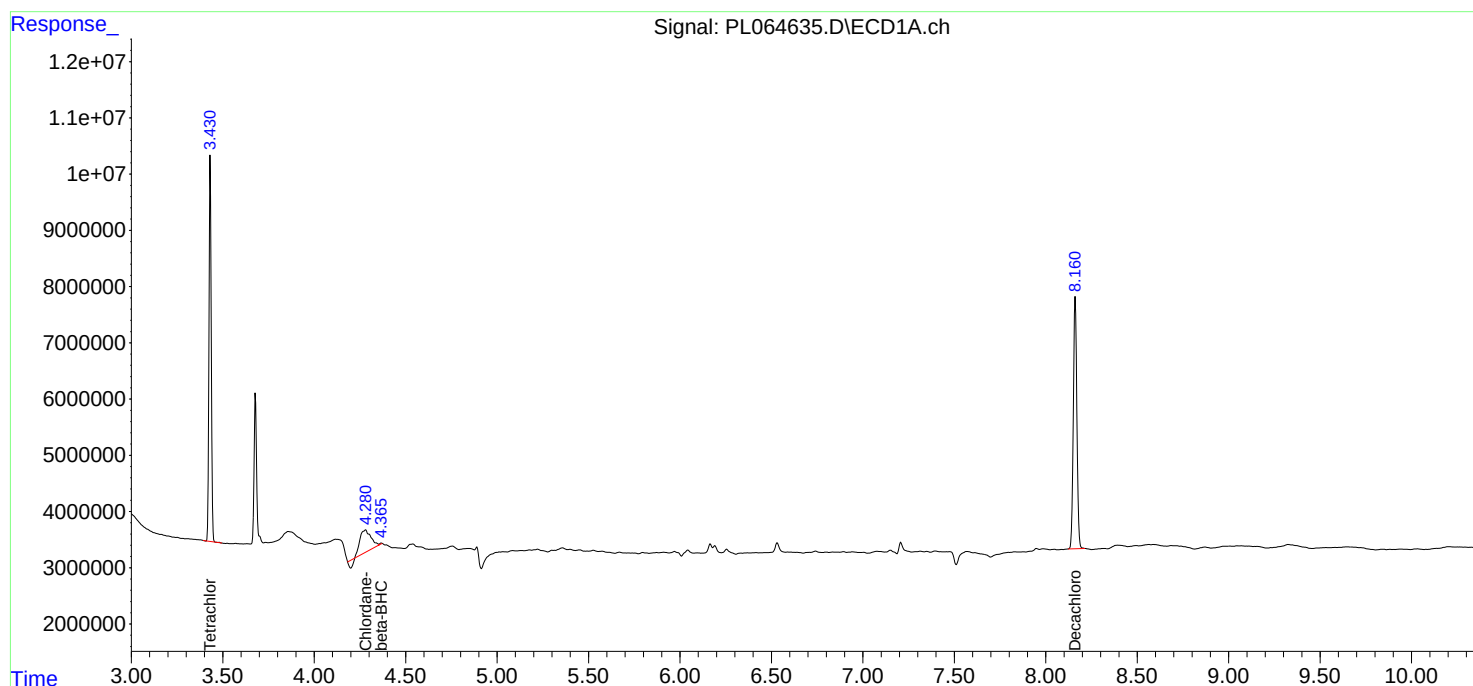


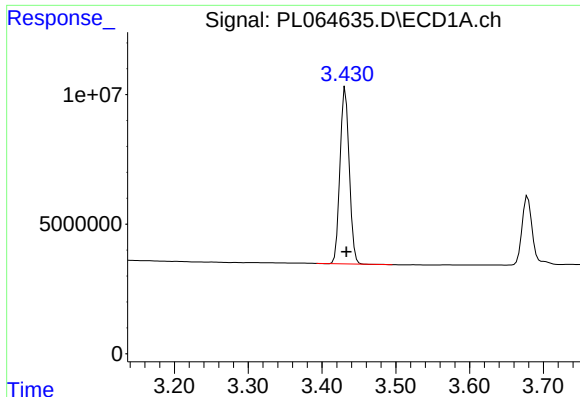

#1 Tetrachloro-m-xylene


R.T.: 3.432 min
Delta R.T.: -0.001 min
Response: 59342120
Conc: 19.49 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB134435BL

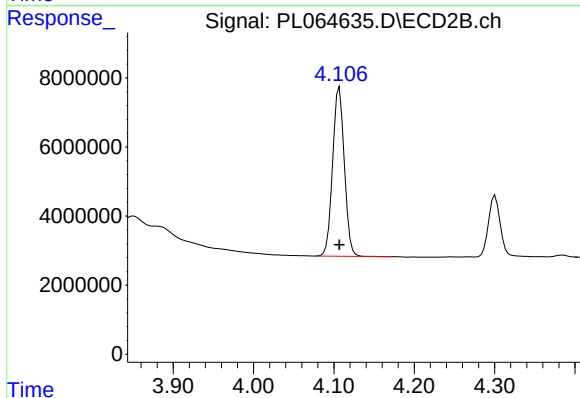


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 49597182
Conc: 20.82 ng/ml

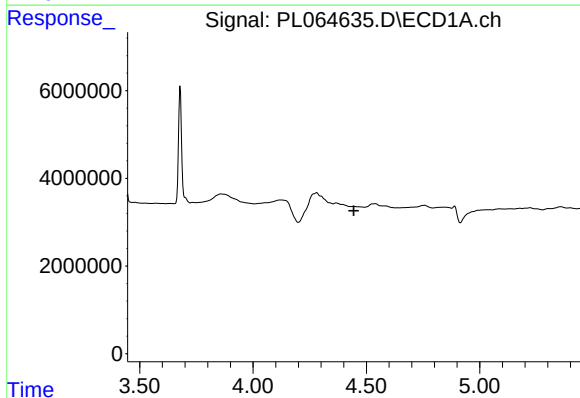


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.445 min
Response: 0
Conc: N.D.

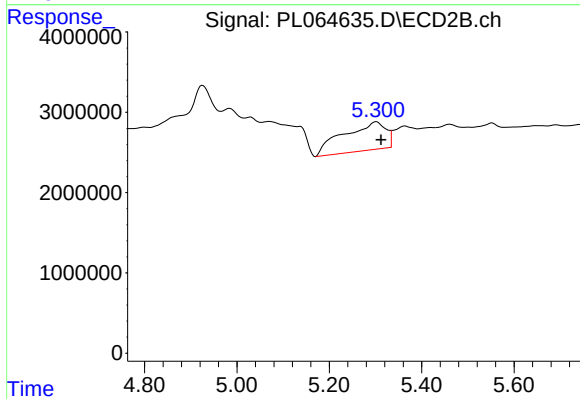

#4 Heptachlor


R.T.: 5.302 min
Delta R.T.: -0.010 min
Response: 22519816
Conc: 6.46 ng/ml

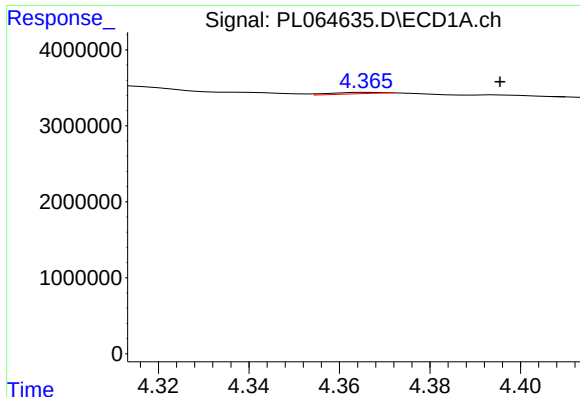

#6 beta-BHC


R.T.: 4.367 min
Delta R.T.: -0.029 min
Response: 414997
Conc: 0.21 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB134435BL

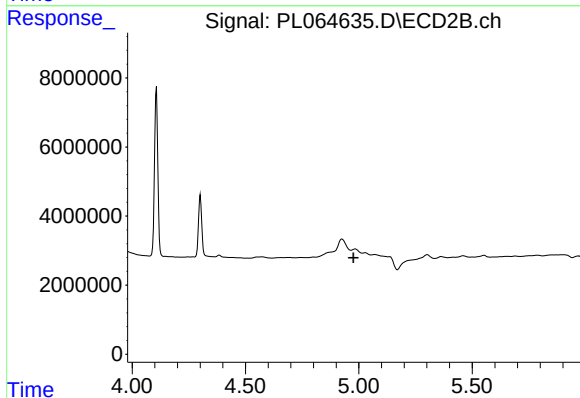


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.977 min
Response: 0
Conc: N.D.

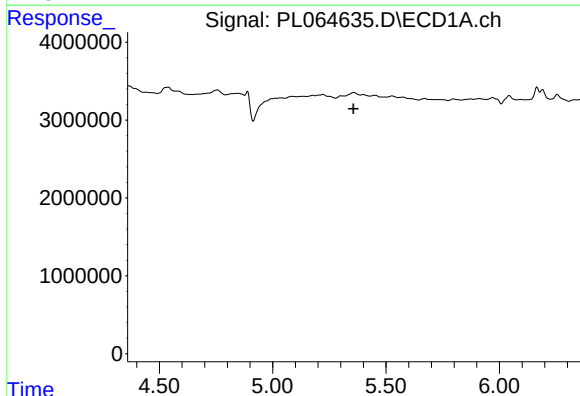


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.357 min
Response: 0
Conc: N.D.

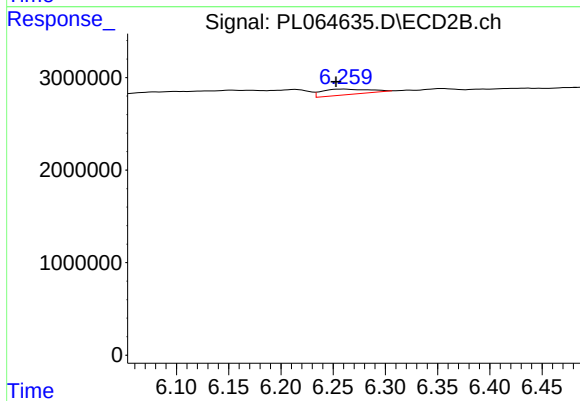

#10 gamma-Chlordane


R.T.: 6.261 min
Delta R.T.: 0.008 min
Response: 1899243
Conc: 0.65 ng/ml

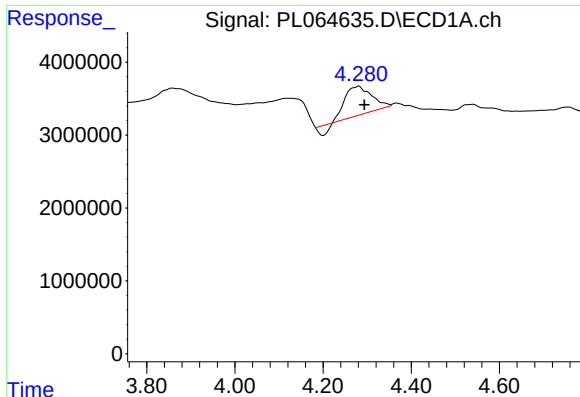

#23 Chlordane-1


R.T.: 4.281 min
Delta R.T.: -0.012 min
Response: 15125536
Conc: 137.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB134435BL

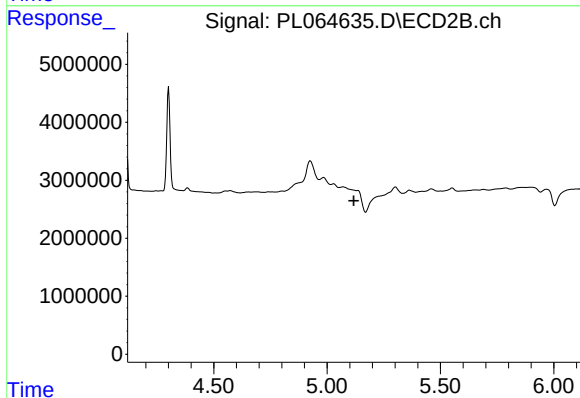


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.119 min
Response: 0
Conc: N.D.

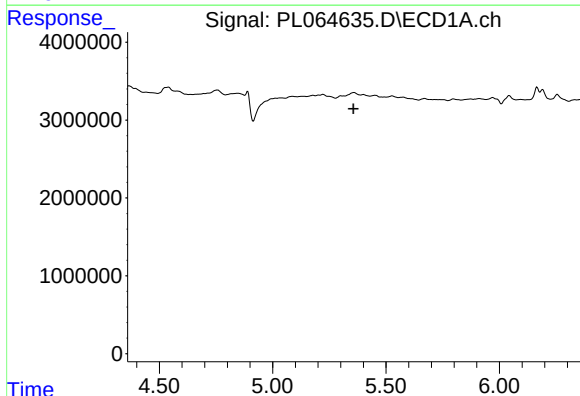


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.357 min
Response: 0
Conc: N.D.

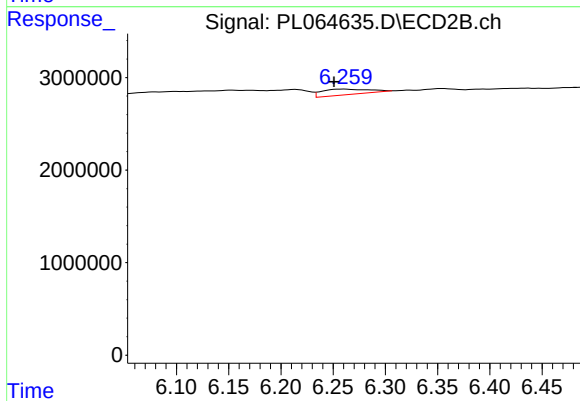

#25 Chlordane-3


R.T.: 6.261 min
Delta R.T.: 0.010 min
Response: 1899243
Conc: 5.30 ng/ml

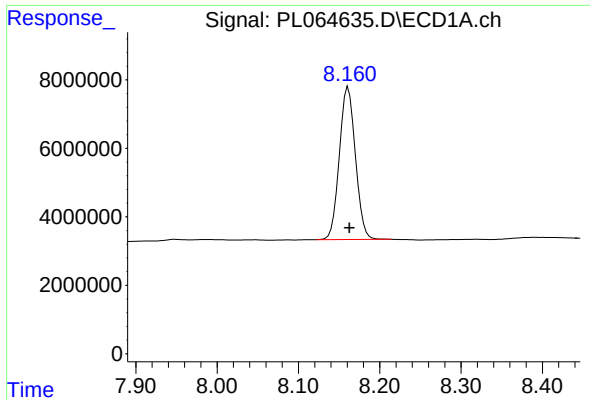

#28 Decachlorobiphenyl

R.T.: 8.161 min
Delta R.T.: -0.001 min
Response: 61049615
Conc: 19.37 ng/ml

Instrument :
ECD_L
ClientSampleId :
PB134435BL

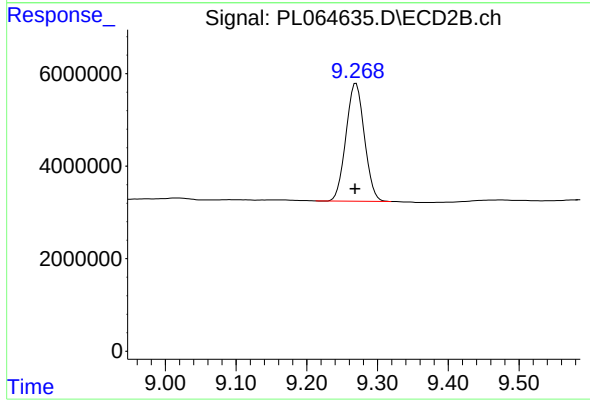

#28 Decachlorobiphenyl

R.T.: 9.270 min
Delta R.T.: 0.001 min
Response: 46158750
Conc: 22.55 ng/ml