

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020421\
 Data File : PL064637.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2021 17:22
 Operator : AR\AJ
 Sample : PB134435TB
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 02:06:44 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	4.107	58126794	48975057	19.095	20.560
28)	SA Decachlor...	8.162	9.269	60414050	46662421	19.171	22.791
Target Compounds							
4)	MA Heptachlor	0.000	5.300	0	14270859	N.D.	4.095 #
10)	B gamma-Chl...	0.000	6.256	0	788301	N.D.	0.271 #
14)	MA Endrin	0.000	6.889f	0	17363057	N.D.	7.564 #
23)	Chlordane-1	4.282	0.000	12524174	0	113.936	N.D. #
25)	Chlordane-3	0.000	6.256	0	788301	N.D.	2.199 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020421\
Data File : PL064637.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2021 17:22
Operator : AR\AJ
Sample : PB134435TB
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 02:06:44 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

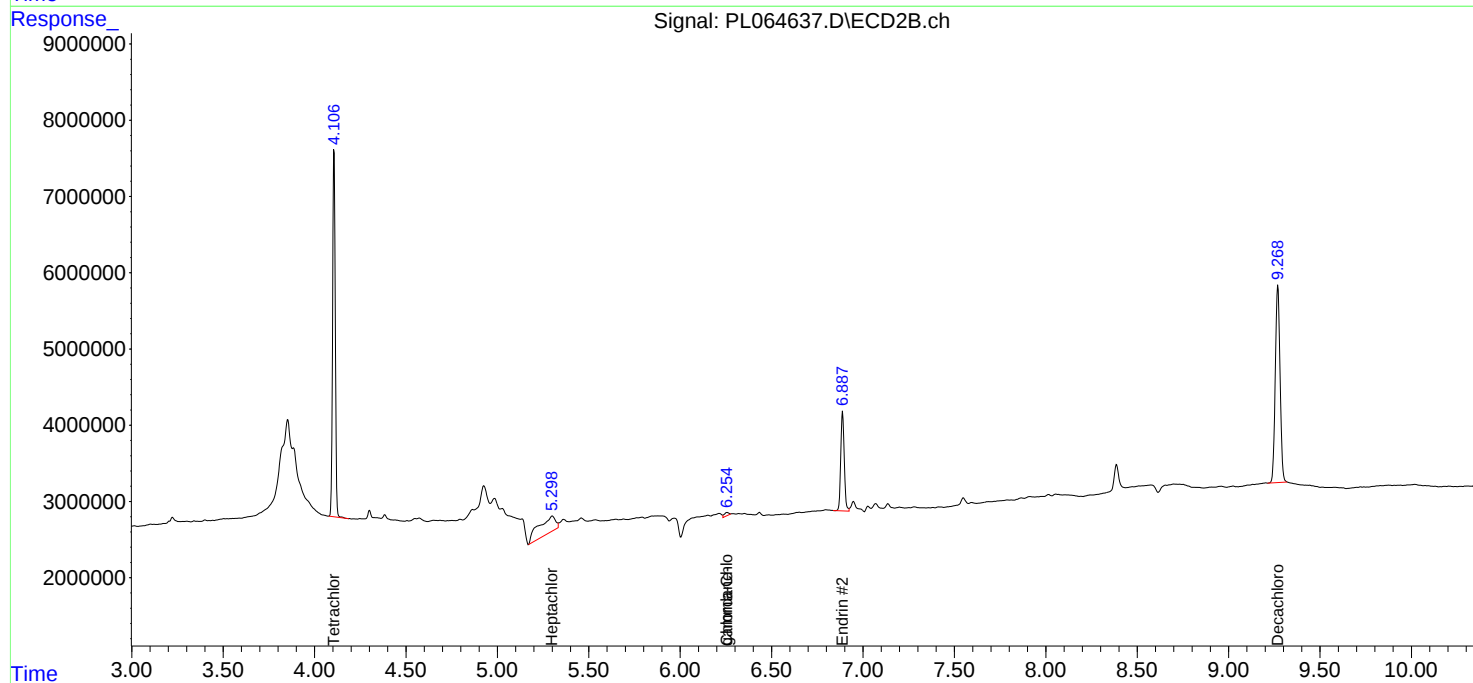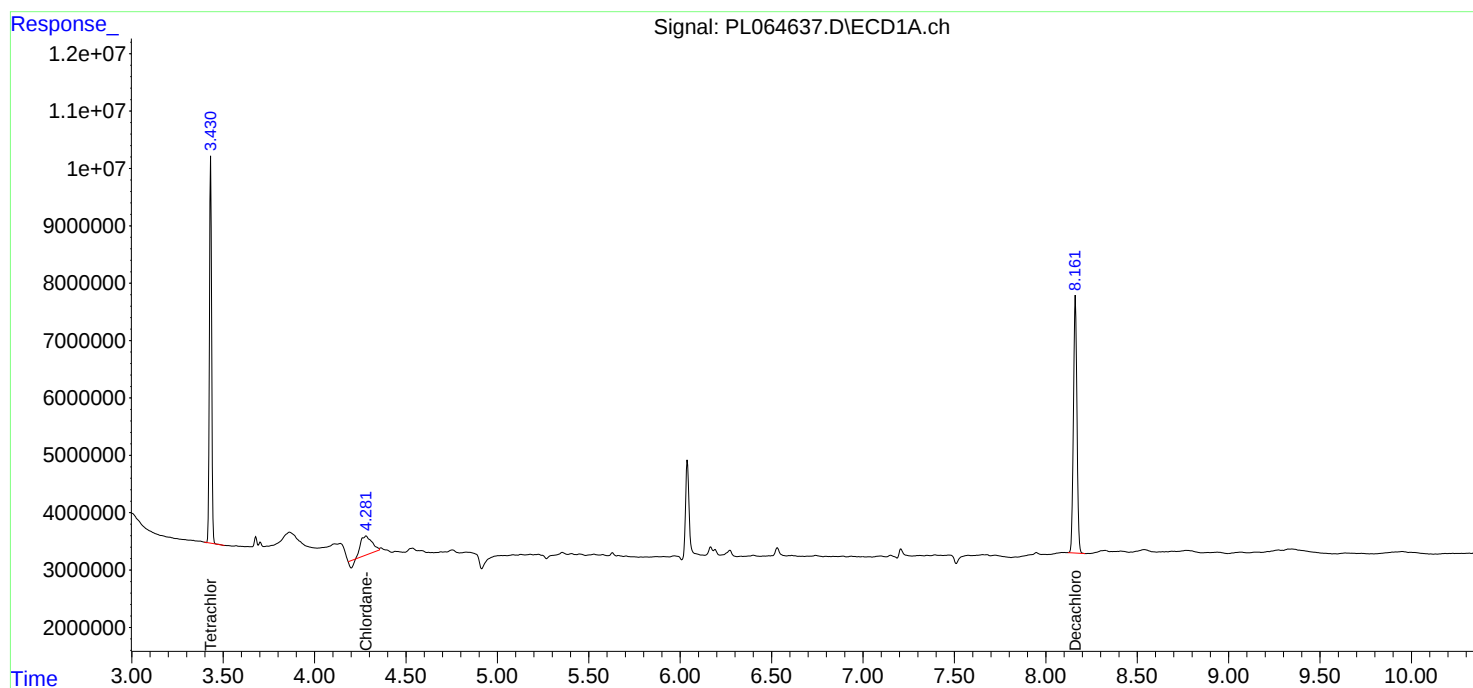


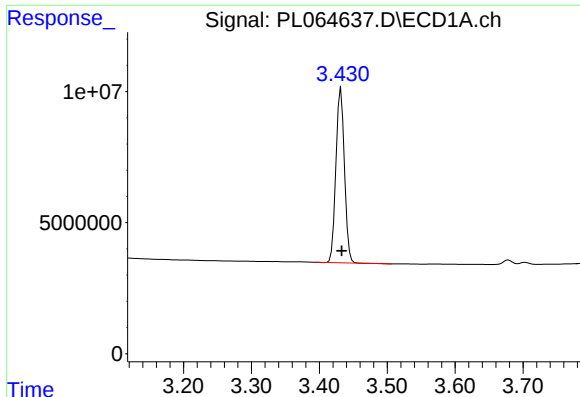

#1 Tetrachloro-m-xylene


R.T.: 3.432 min
Delta R.T.: -0.001 min
Response: 58126794
Conc: 19.09 ng/ml

Instrument :
ECD_L
ClientSampleId :

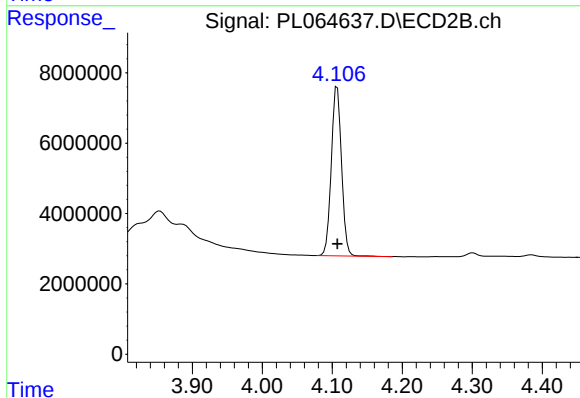


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 48975057
Conc: 20.56 ng/ml

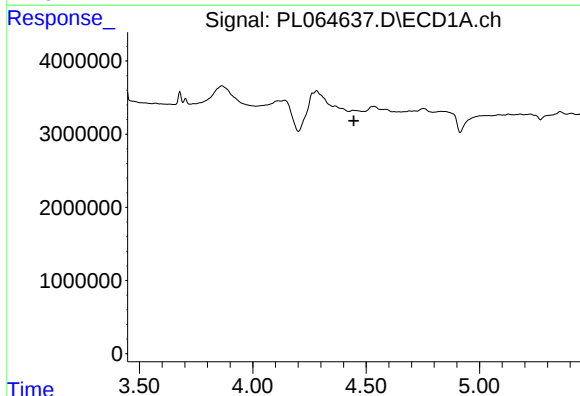


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.445 min
Response: 0
Conc: N.D.

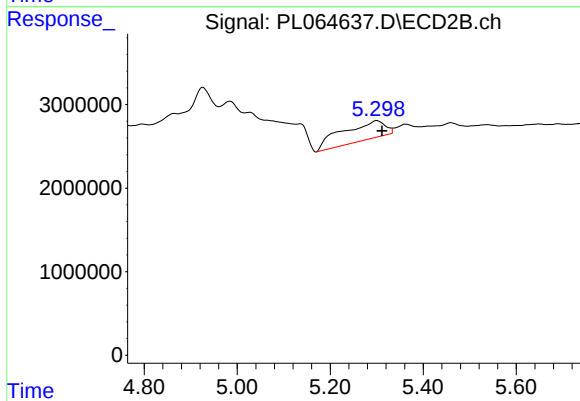

#4 Heptachlor


R.T.: 5.300 min
Delta R.T.: -0.011 min
Response: 14270859
Conc: 4.09 ng/ml

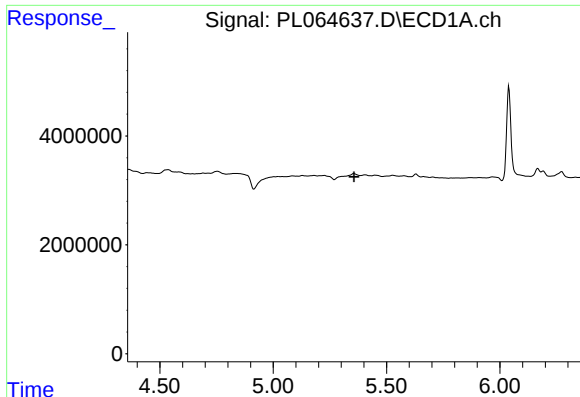

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.357 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

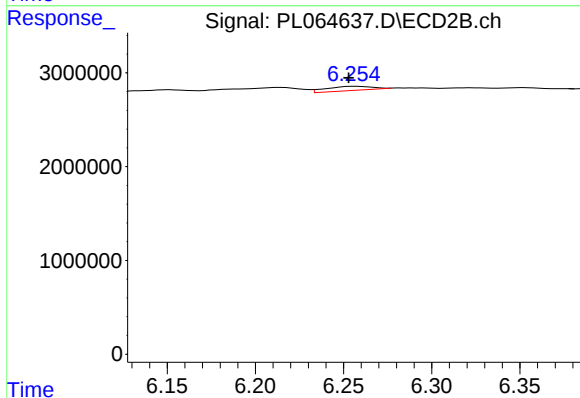


#10 gamma-Chlordane

R.T.: 6.256 min
Delta R.T.: 0.003 min
Response: 788301
Conc: 0.27 ng/ml

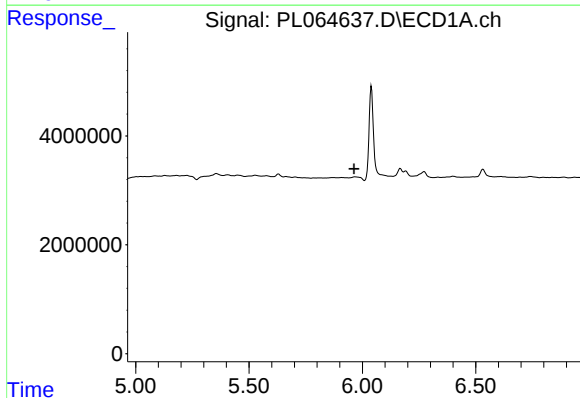


#14 Endrin

R.T.: 0.000 min
Exp R.T.: 5.963 min
Response: 0
Conc: N.D.

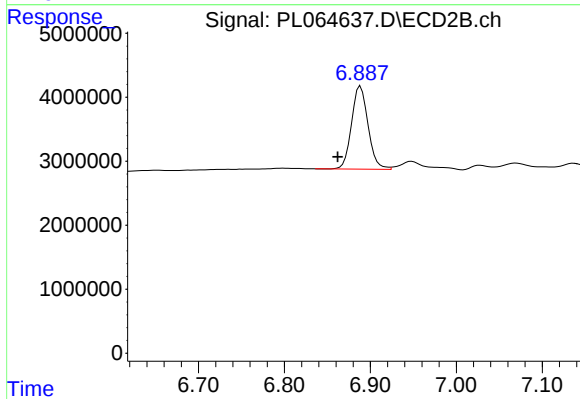

#14 Endrin


R.T.: 6.889 min
Delta R.T.: 0.027 min
Response: 17363057
Conc: 7.56 ng/ml

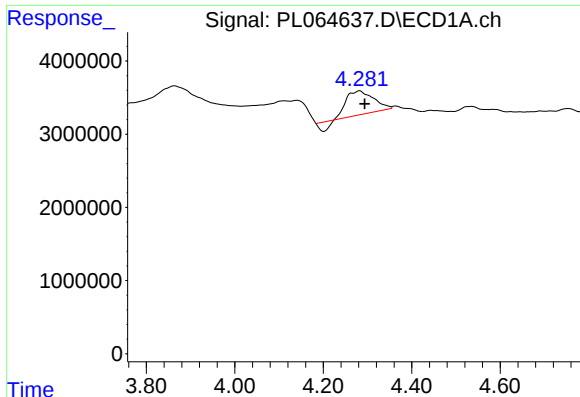

#23 Chlordane-1


R.T.: 4.282 min
Delta R.T.: -0.011 min
Response: 12524174
Conc: 113.94 ng/ml

Instrument :
ECD_L
ClientSampleId :

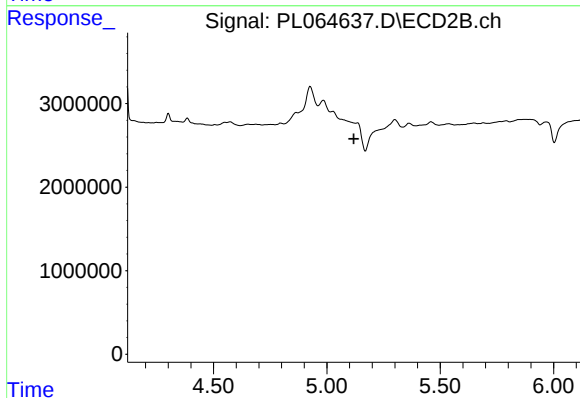


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.119 min
Response: 0
Conc: N.D.

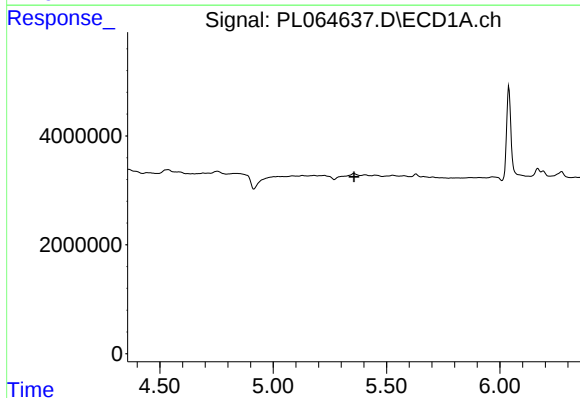


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.357 min
Response: 0
Conc: N.D.

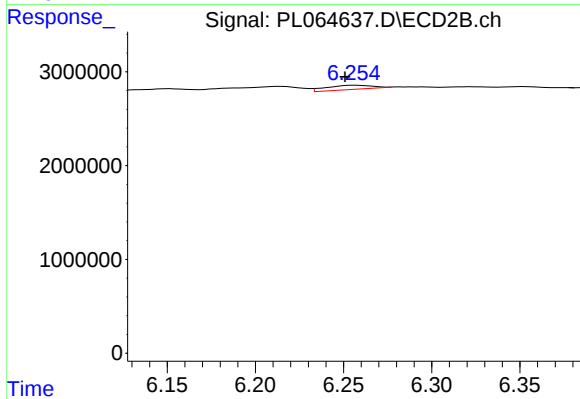

#25 Chlordane-3


R.T.: 6.256 min
Delta R.T.: 0.005 min
Response: 788301
Conc: 2.20 ng/ml

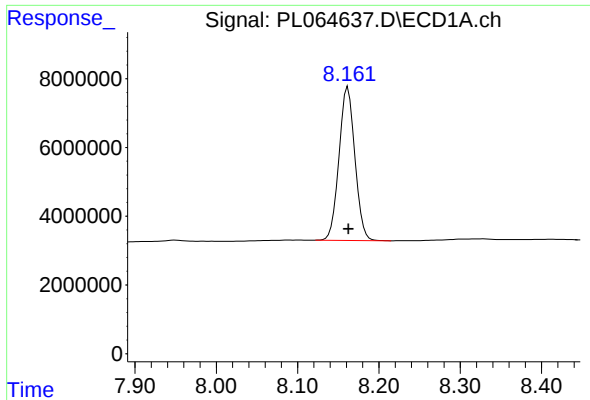

#28 Decachlorobiphenyl

R.T.: 8.162 min
Delta R.T.: 0.000 min
Response: 60414050
Conc: 19.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

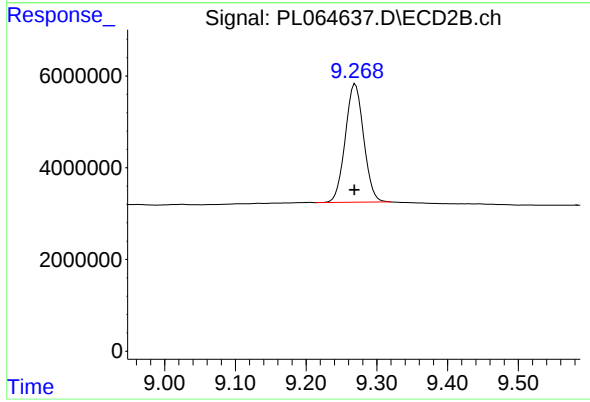

#28 Decachlorobiphenyl

R.T.: 9.269 min
Delta R.T.: 0.001 min
Response: 46662421
Conc: 22.79 ng/ml