

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020421\
 Data File : PL064641.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2021 18:19
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 02:08:02 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.432	4.107	60824289	50826236	19.981	21.337
28)	SA Decachlor...	8.164	9.271	61792358	47165206	19.608	23.037
Target Compounds							
4)	MA Heptachlor	0.000	5.303	0	11399814	N.D.	3.271 #
6)	B beta-BHC	0.000	4.984	0	2030040	N.D.	1.200 #
7)	B delta-BHC	0.000	5.220f	0	6149154	N.D.	1.996 #
9)	A Endosulfan I	0.000	6.380	0	1096410	N.D.	0.412 #
10)	B gamma-Chl...	0.000	6.257	0	2625940	N.D.	0.903 #
11)	B alpha-Chl...	0.000	6.325	0	1987417	N.D.	0.675 #
23)	Chlordane-1	4.283	0.000	12917500	0	117.514	N.D. #
25)	Chlordane-3	0.000	6.257	0	2625940	N.D.	7.325 #
26)	Chlordane-4	0.000	6.325	0	1987417	N.D.	4.519 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020421\
Data File : PL064641.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2021 18:19
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 02:08:02 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

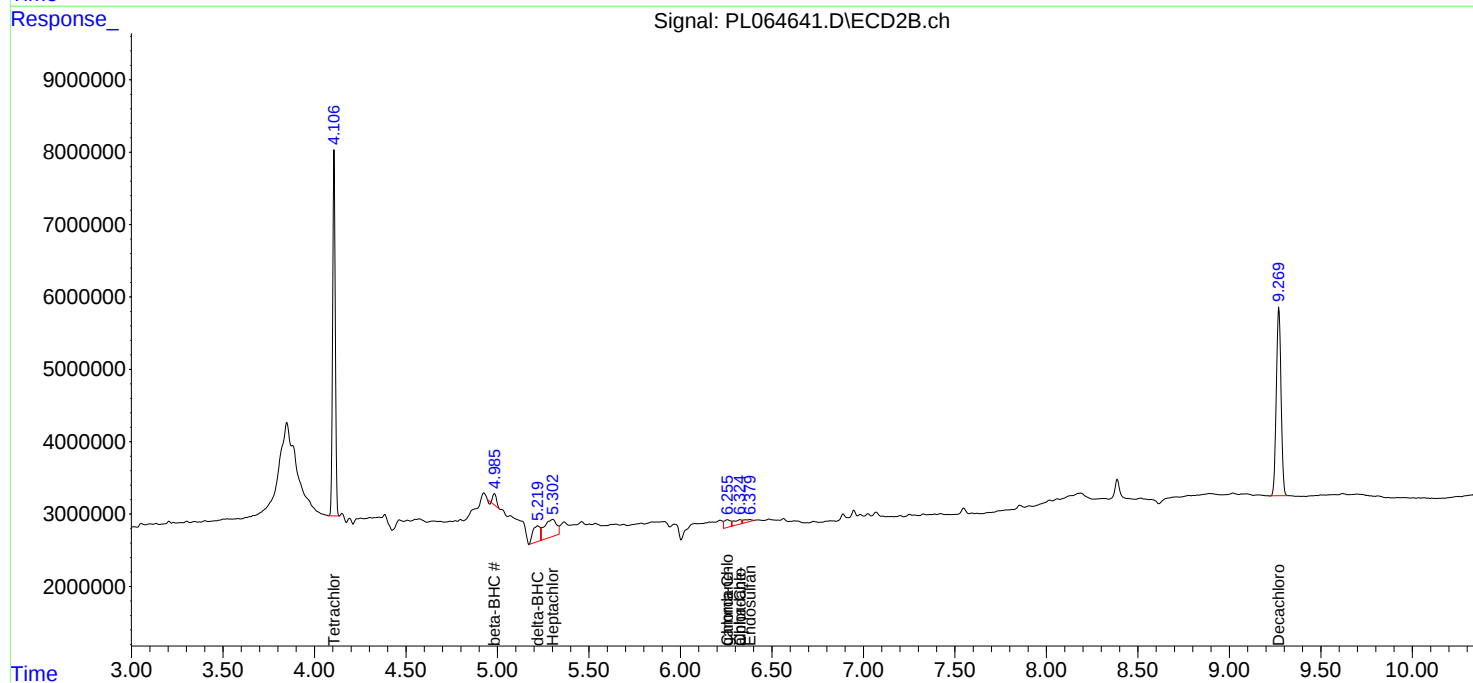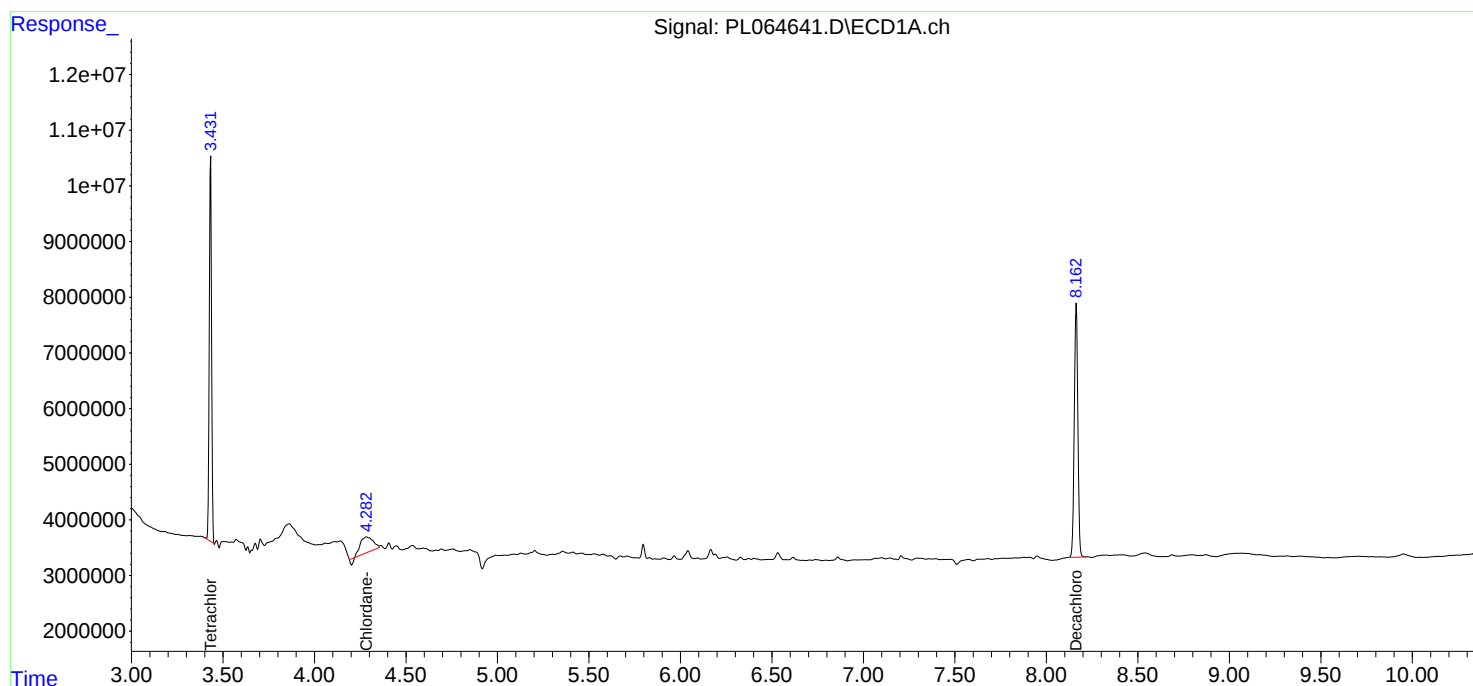


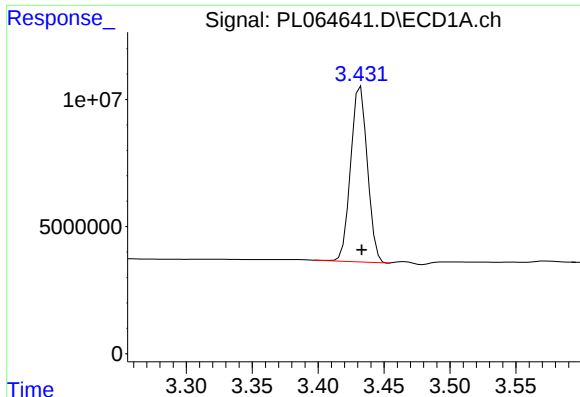

#1 Tetrachloro-m-xylene


R.T.: 3.432 min
Delta R.T.: 0.000 min
Response: 60824289
Conc: 19.98 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

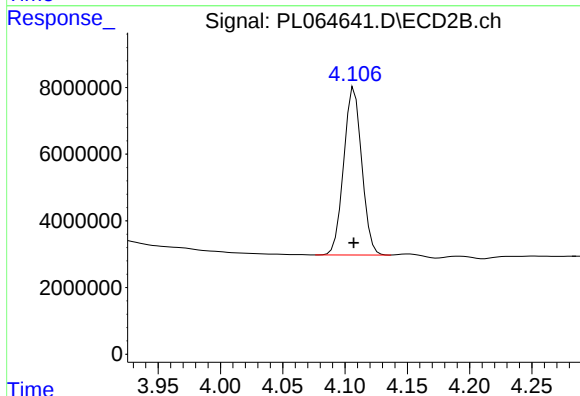


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 50826236
Conc: 21.34 ng/ml

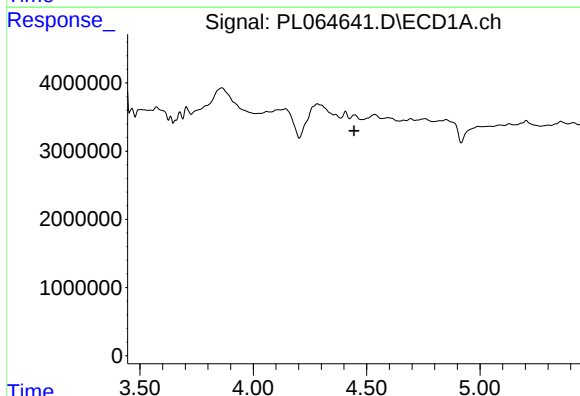


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 4.445 min
Response: 0
Conc: N.D.

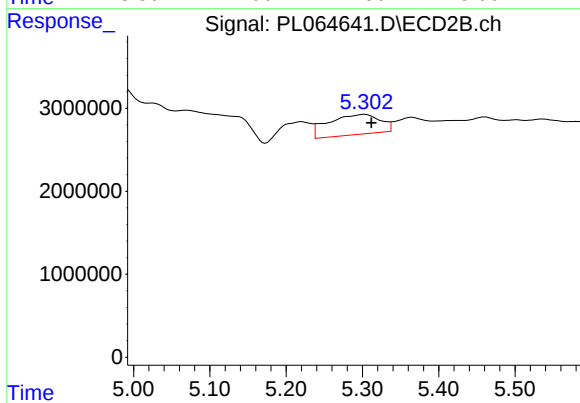

#4 Heptachlor


R.T.: 5.303 min
Delta R.T.: -0.009 min
Response: 11399814
Conc: 3.27 ng/ml

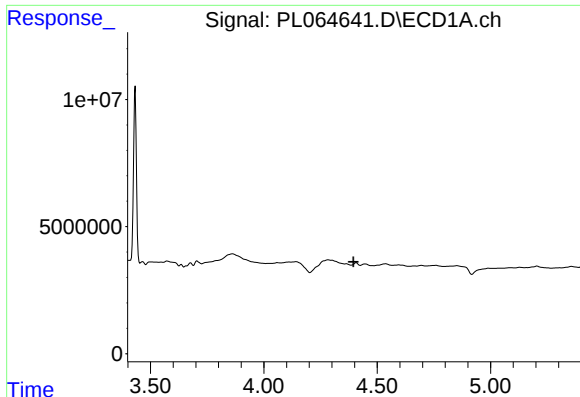

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.395 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

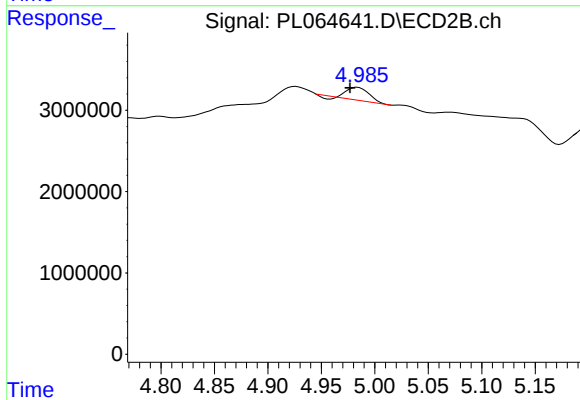


#6 beta-BHC

R.T.: 4.984 min
Delta R.T.: 0.007 min
Response: 2030040
Conc: 1.20 ng/ml

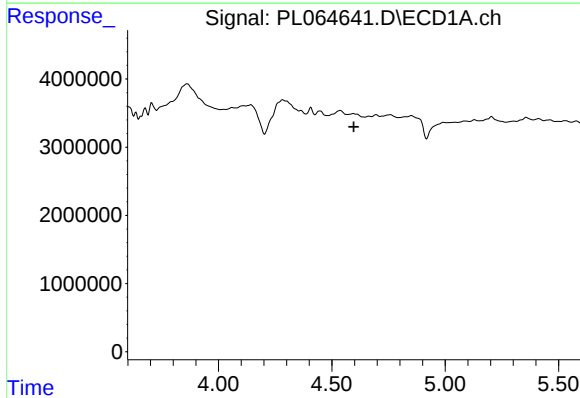


#7 delta-BHC

R.T.: 0.000 min
Exp R.T.: 4.597 min
Response: 0
Conc: N.D.

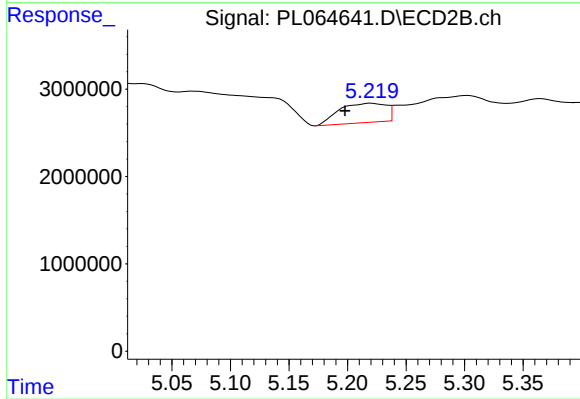

#7 delta-BHC


R.T.: 5.220 min
Delta R.T.: 0.022 min
Response: 6149154
Conc: 2.00 ng/ml

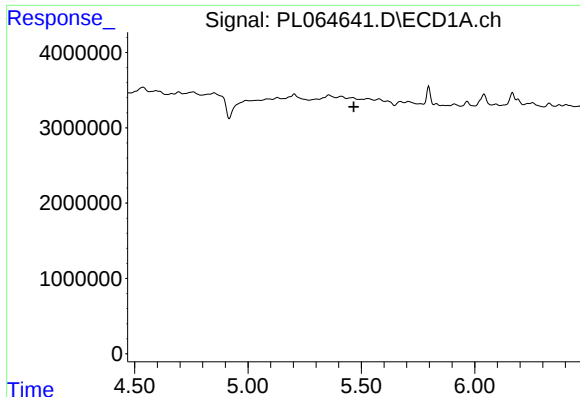

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.467 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

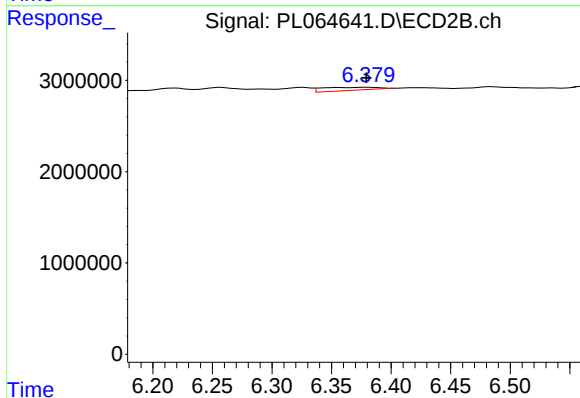


#9 Endosulfan I

R.T.: 6.380 min
Delta R.T.: 0.000 min
Response: 1096410
Conc: 0.41 ng/ml

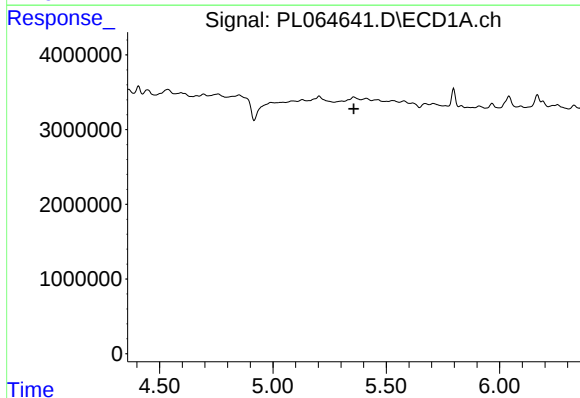


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.357 min
Response: 0
Conc: N.D.

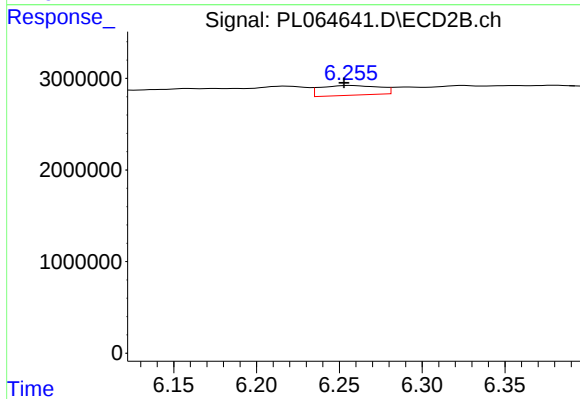

#10 gamma-Chlordane


R.T.: 6.257 min
Delta R.T.: 0.004 min
Response: 2625940
Conc: 0.90 ng/ml

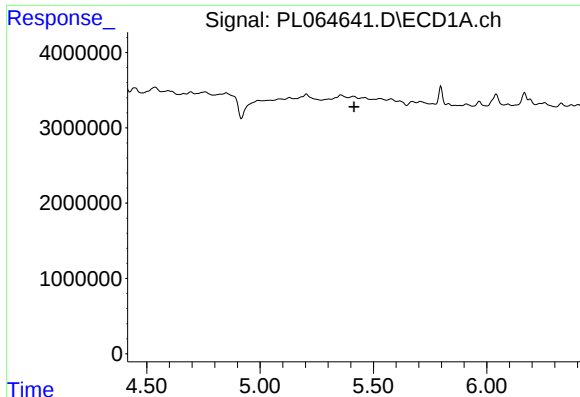

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.415 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

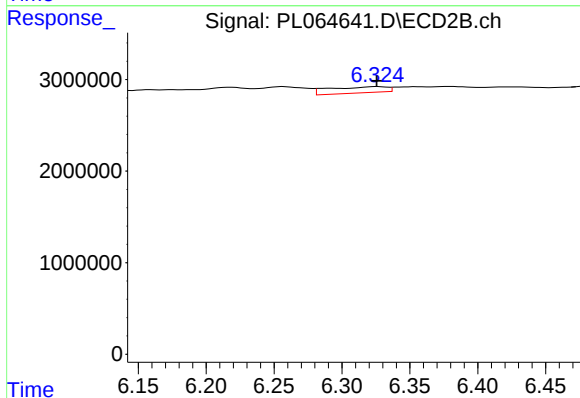


#11 alpha-Chlordane

R.T.: 6.325 min
Delta R.T.: 0.000 min
Response: 1987417
Conc: 0.68 ng/ml

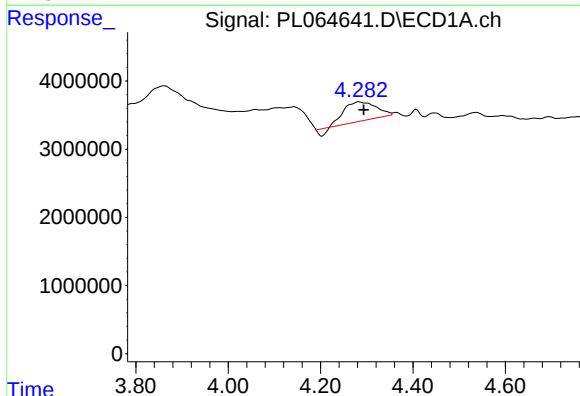


#23 Chlordane-1

R.T.: 4.283 min
Delta R.T.: -0.010 min
Response: 12917500
Conc: 117.51 ng/ml

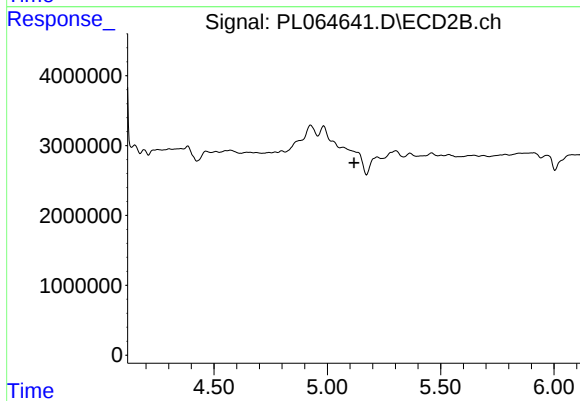

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T.: 5.119 min
Response: 0
Conc: N.D.

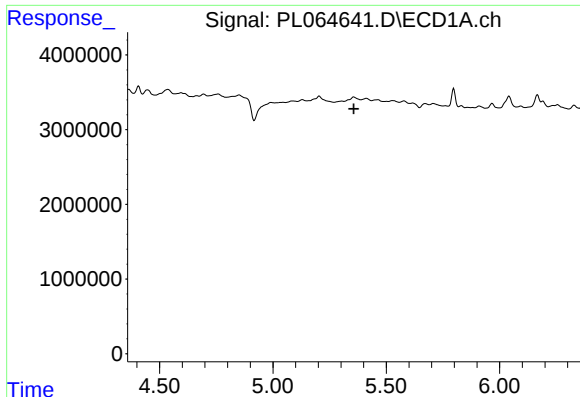

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T.: 5.357 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
I.BLK

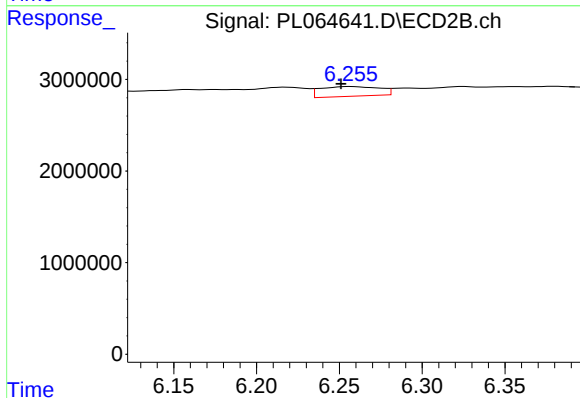


#25 Chlordane-3

R.T.: 6.257 min
Delta R.T.: 0.006 min
Response: 2625940
Conc: 7.33 ng/ml

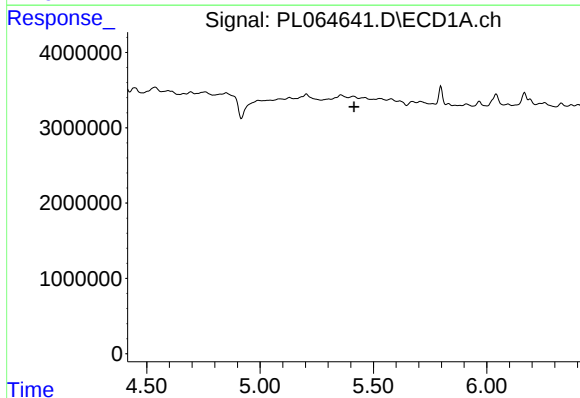


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T.: 5.414 min
Response: 0
Conc: N.D.

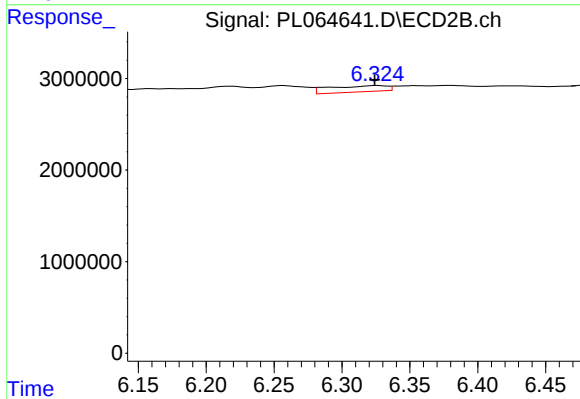

#26 Chlordane-4


R.T.: 6.325 min
Delta R.T.: 0.001 min
Response: 1987417
Conc: 4.52 ng/ml

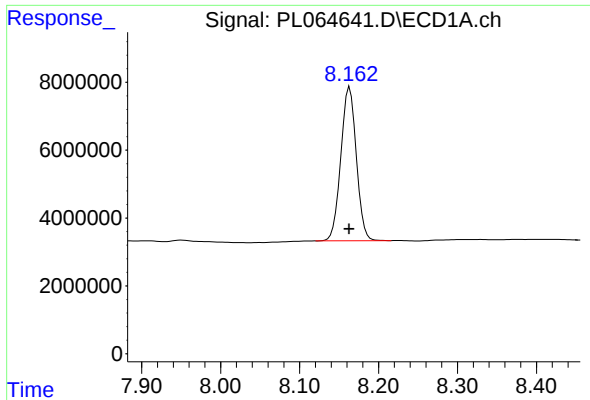

#28 Decachlorobiphenyl

R.T.: 8.164 min
Delta R.T.: 0.000 min
Response: 61792358
Conc: 19.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
I.BLK

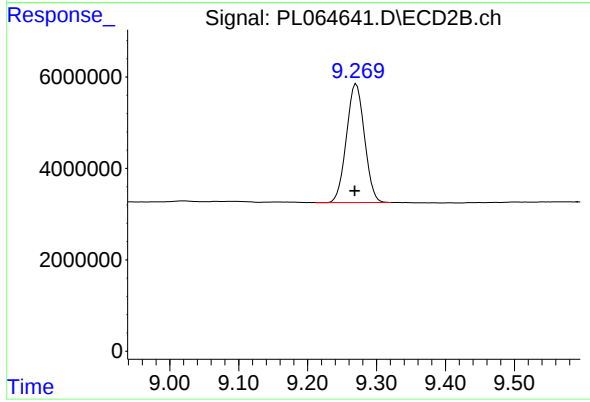

#28 Decachlorobiphenyl

R.T.: 9.271 min
Delta R.T.: 0.002 min
Response: 47165206
Conc: 23.04 ng/ml