

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020421\
 Data File : PL064619.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2021 10:03
 Operator : AR\AJ
 Sample : M1292-08RE
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OU421-003-1015RE

Manual Integrations
 APPROVED

Ankita
 2/8/2021 8:28:08 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 02:00:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.433	4.107	71876031	59775837	23.611	25.094
28)	SA Decachlor...	8.164	9.271	96081309	73434533	30.489	35.867
Target Compounds							
12)	B 4,4'-DDE	5.581	6.484	5236845	3805458	1.389m	1.470
17)	MA 4,4'-DDT	6.334	7.282	6690771	3521792	2.180	1.715

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020421\
Data File : PL064619.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2021 10:03
Operator : AR\AJ
Sample : M1292-08RE
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OU421-003-1015RE


Manual Integrations
APPROVED

Ankita
2/8/2021 8:28:08 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 02:00:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

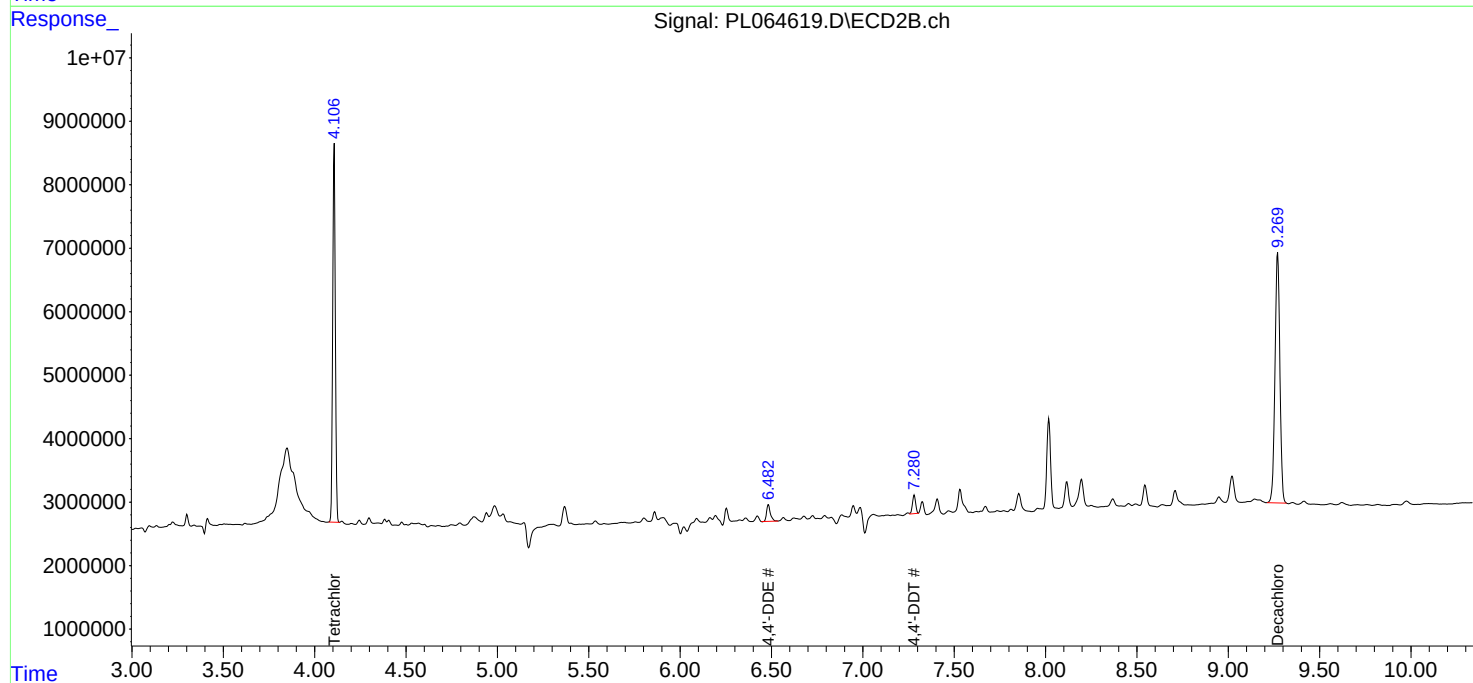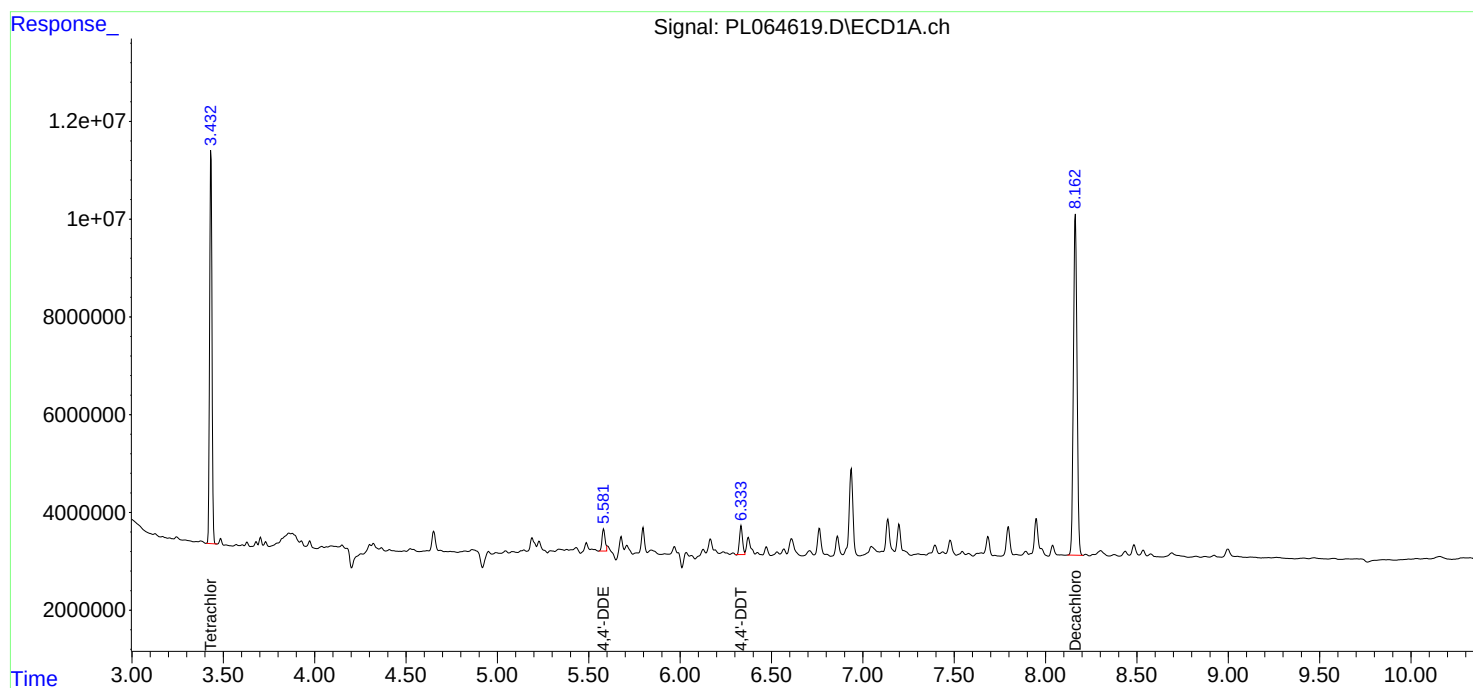

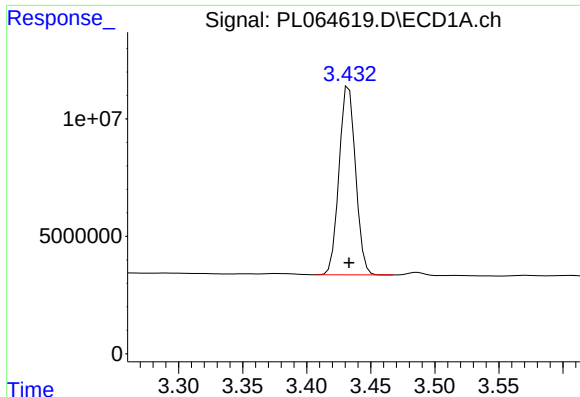


#1 Tetrachloro-m-xylene

R.T.: 3.433 min
Delta R.T.: 0.000 min
Response: 71876031
Conc: 23.61 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU421-003-1015RE


Manual Integrations
APPROVED

Ankita
2/8/2021 8:28:08 AM

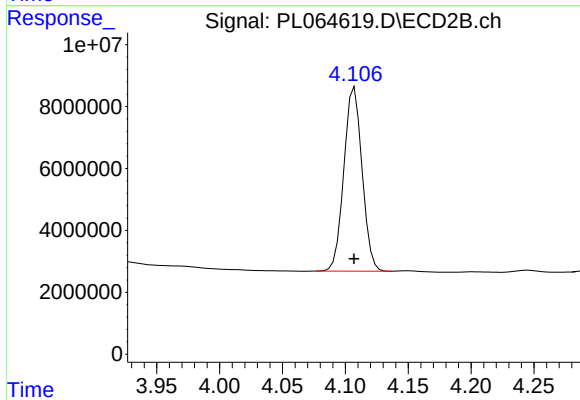


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 59775837
Conc: 25.09 ng/ml

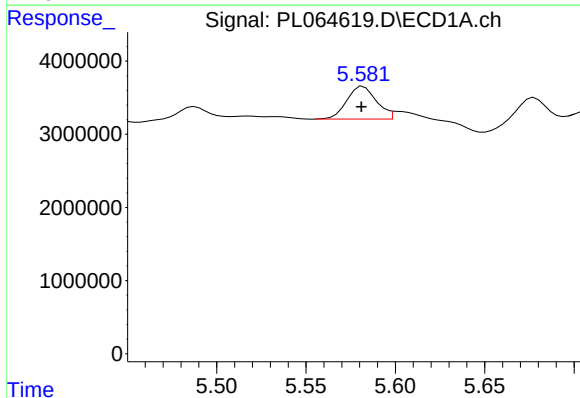


#12 4,4'-DDE

R.T.: 5.581 min
Delta R.T.: 0.000 min
Response: 5236845
Conc: 1.39 ng/ml m

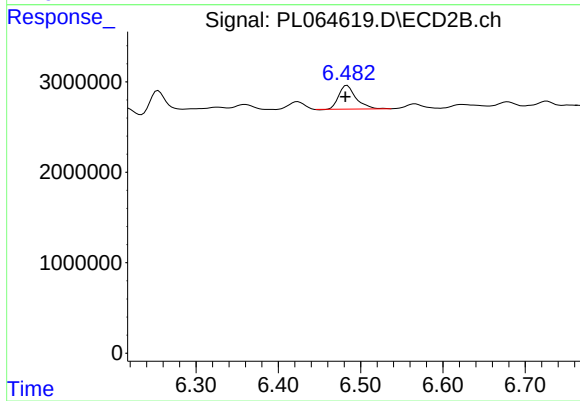

#12 4,4'-DDE

R.T.: 6.484 min
Delta R.T.: 0.002 min
Response: 3805458
Conc: 1.47 ng/ml

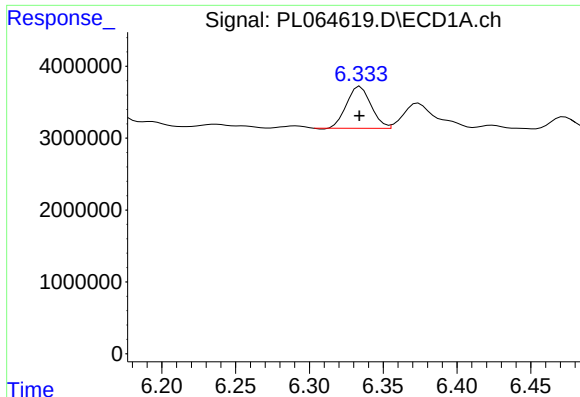


#17 4,4'-DDT

R.T.: 6.334 min
Delta R.T.: 0.000 min
Response: 6690771
Conc: 2.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU421-003-1015RE


Manual Integrations
APPROVED

Ankita
2/8/2021 8:28:08 AM

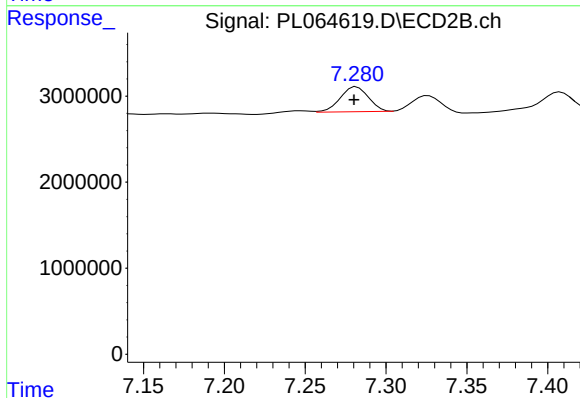


#17 4,4'-DDT

R.T.: 7.282 min
Delta R.T.: 0.002 min
Response: 3521792
Conc: 1.71 ng/ml

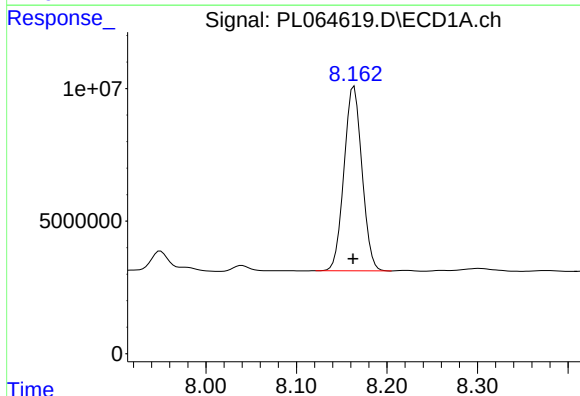

#28 Decachlorobiphenyl

R.T.: 8.164 min
Delta R.T.: 0.001 min
Response: 96081309
Conc: 30.49 ng/ml

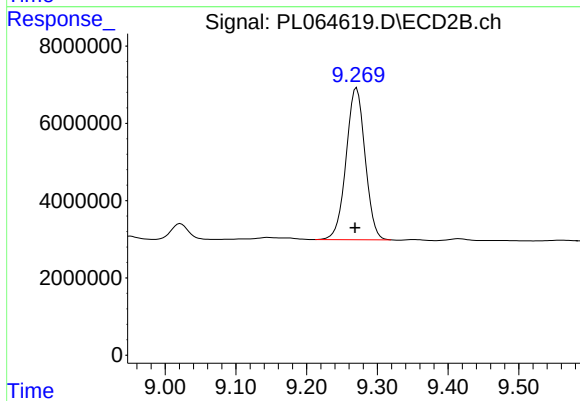

#28 Decachlorobiphenyl

R.T.: 9.271 min
Delta R.T.: 0.002 min
Response: 73434533
Conc: 35.87 ng/ml