

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020421\
 Data File : PL064634.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 04 Feb 2021 14:13
 Operator : AR\AJ
 Sample : M1291-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 OU421-007-0002

Manual Integrations
 APPROVED

Ankita
 2/8/2021 8:28:24 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 05 02:05:42 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
 Quant Title : GC Extractables
 QLast Update : Fri Jan 29 04:48:57 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.431	4.107	38642816	31743792	12.694m	13.326
28) SA Decachlor...	8.163	9.270	53808709	48728692	17.075	23.800 #
Target Compounds						
12) B 4,4'-DDE	5.582	6.484	70834063	61120372	18.791	23.605 #
17) MA 4,4'-DDT	6.333	7.283	103.9E6	60813223	33.859	29.607

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL020421\
Data File : PL064634.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 04 Feb 2021 14:13
Operator : AR\AJ
Sample : M1291-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
OU421-007-0002


Manual Integrations
APPROVED

Ankita
2/8/2021 8:28:24 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 05 02:05:42 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL012921.M
Quant Title : GC Extractables
QLast Update : Fri Jan 29 04:48:57 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

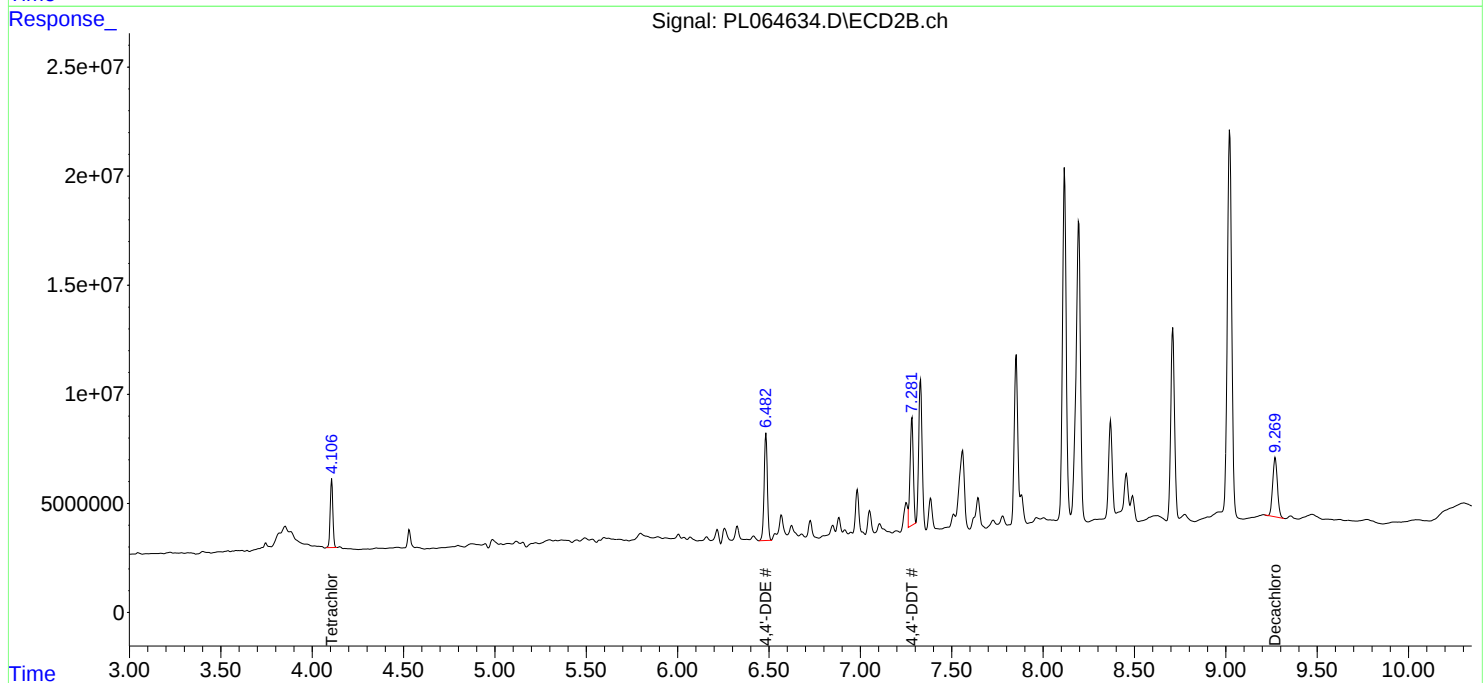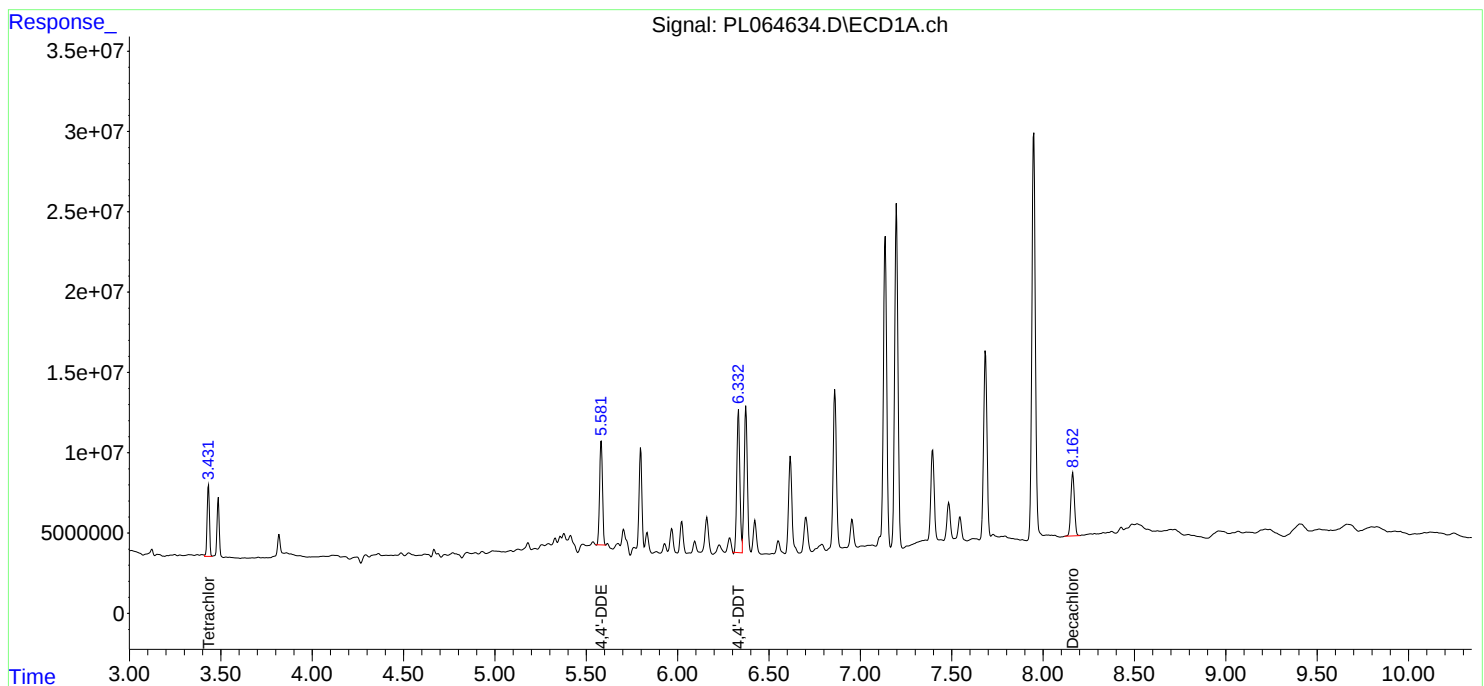

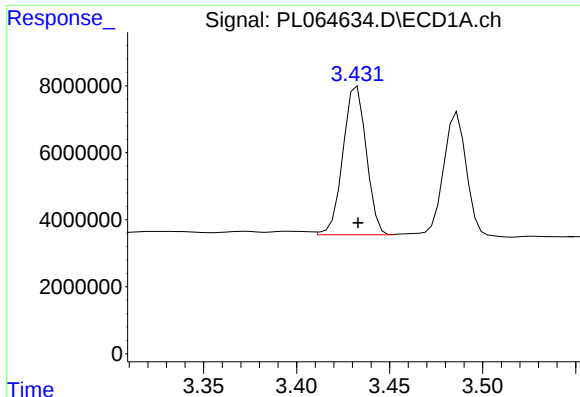


#1 Tetrachloro-m-xylene

R.T.: 3.431 min
Delta R.T.: -0.002 min
Response: 38642816
Conc: 12.69 ng/ml m

Instrument :
ECD_L
ClientSampleId :
OU421-007-0002


Manual Integrations
APPROVED

Ankita
2/8/2021 8:28:24 AM

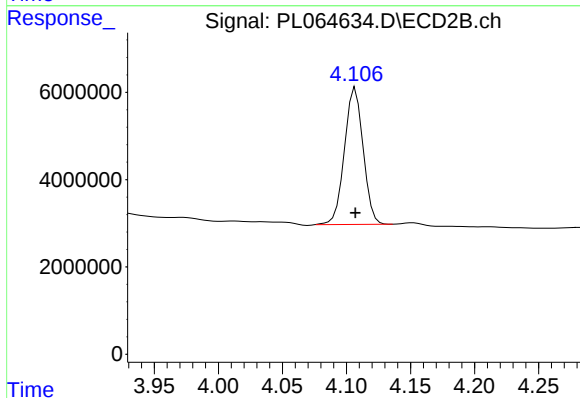


#1 Tetrachloro-m-xylene

R.T.: 4.107 min
Delta R.T.: 0.000 min
Response: 31743792
Conc: 13.33 ng/ml

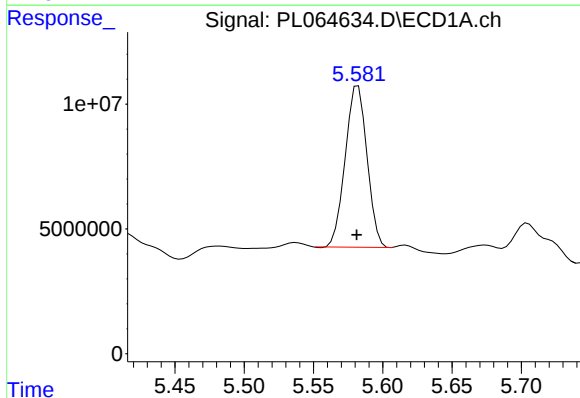


#12 4,4'-DDE

R.T.: 5.582 min
Delta R.T.: 0.001 min
Response: 70834063
Conc: 18.79 ng/ml

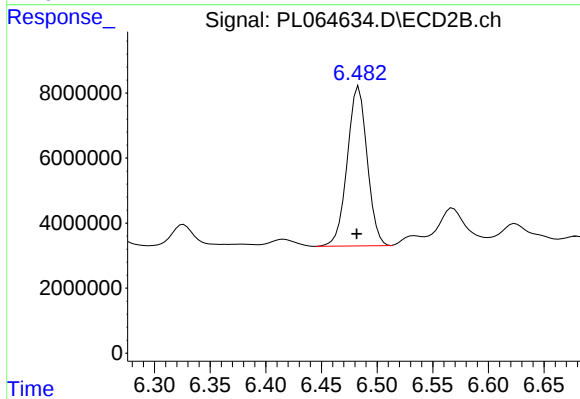

#12 4,4'-DDE

R.T.: 6.484 min
Delta R.T.: 0.002 min
Response: 61120372
Conc: 23.60 ng/ml

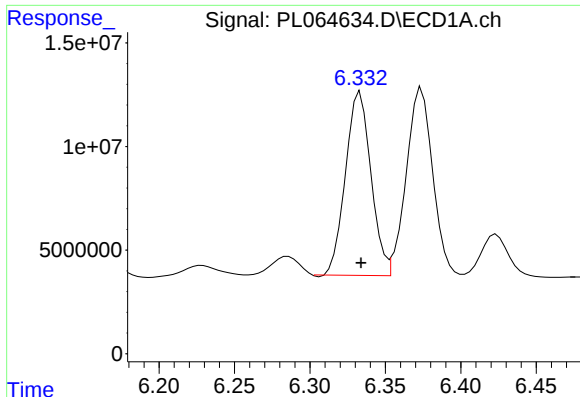


#17 4,4'-DDT

R.T.: 6.333 min
Delta R.T.: 0.000 min
Response: 103913125
Conc: 33.86 ng/ml

Instrument :
ECD_L
ClientSampleId :
OU421-007-0002


Manual Integrations
APPROVED

Ankita
2/8/2021 8:28:24 AM

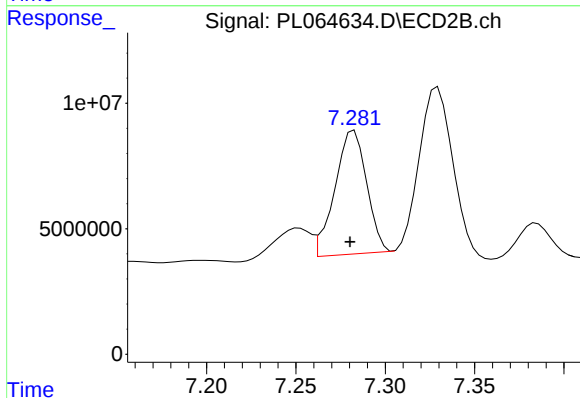


#17 4,4'-DDT

R.T.: 7.283 min
Delta R.T.: 0.002 min
Response: 60813223
Conc: 29.61 ng/ml

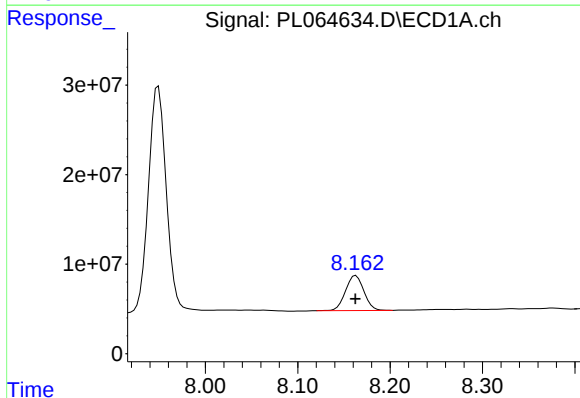

#28 Decachlorobiphenyl

R.T.: 8.163 min
Delta R.T.: 0.000 min
Response: 53808709
Conc: 17.07 ng/ml

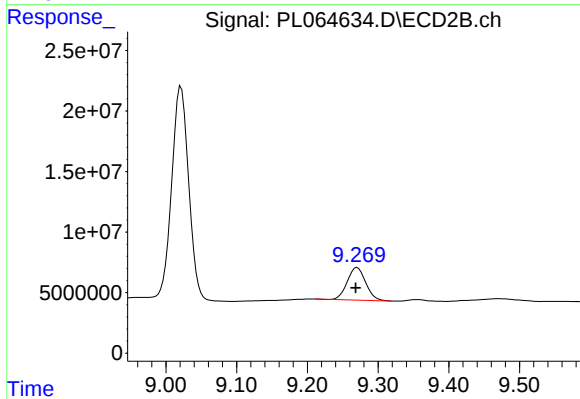

#28 Decachlorobiphenyl

R.T.: 9.270 min
Delta R.T.: 0.002 min
Response: 48728692
Conc: 23.80 ng/ml