

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021819\
 Data File : PL044891.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2019 15:11
 Operator : AJ\SJ
 Sample : K1513-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FLOORS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 01:16:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.365	3.984	52022357	17655843	7.311	7.516
28)	SA Decachlor...	8.051	9.044	127.1E6	36623525	17.424	16.535
Target Compounds							
8)	B Heptachlo...	0.000	5.847	0	1913210	N.D.	0.765 #
12)	B 4,4'-DDE	5.487	6.321	5228681	3858634	0.603	1.616 #
13)	MA Dieldrin	0.000	6.462	0	1967086	N.D.	0.762 #
16)	A 4,4'-DDD	0.000	6.817	0	4999959	N.D.	2.604 #
17)	MA 4,4'-DDT	6.229	7.082f	17559152	1225137	2.449	0.624 #
18)	B Endrin al...	6.321	0.000	7702320	0	1.099	N.D. #
19)	B Endosulfa...	6.512	7.215f	15477122	484049	2.130	0.229 #
20)	A Methoxychlor	6.758f	0.000	29013176	0	7.230	N.D. #
21)	B Endrin ke...	7.029f	0.000	8473178	0	1.018	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021819\
Data File : PL044891.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2019 15:11
Operator : AJ\SJ
Sample : K1513-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :
FLOORS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 01:16:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

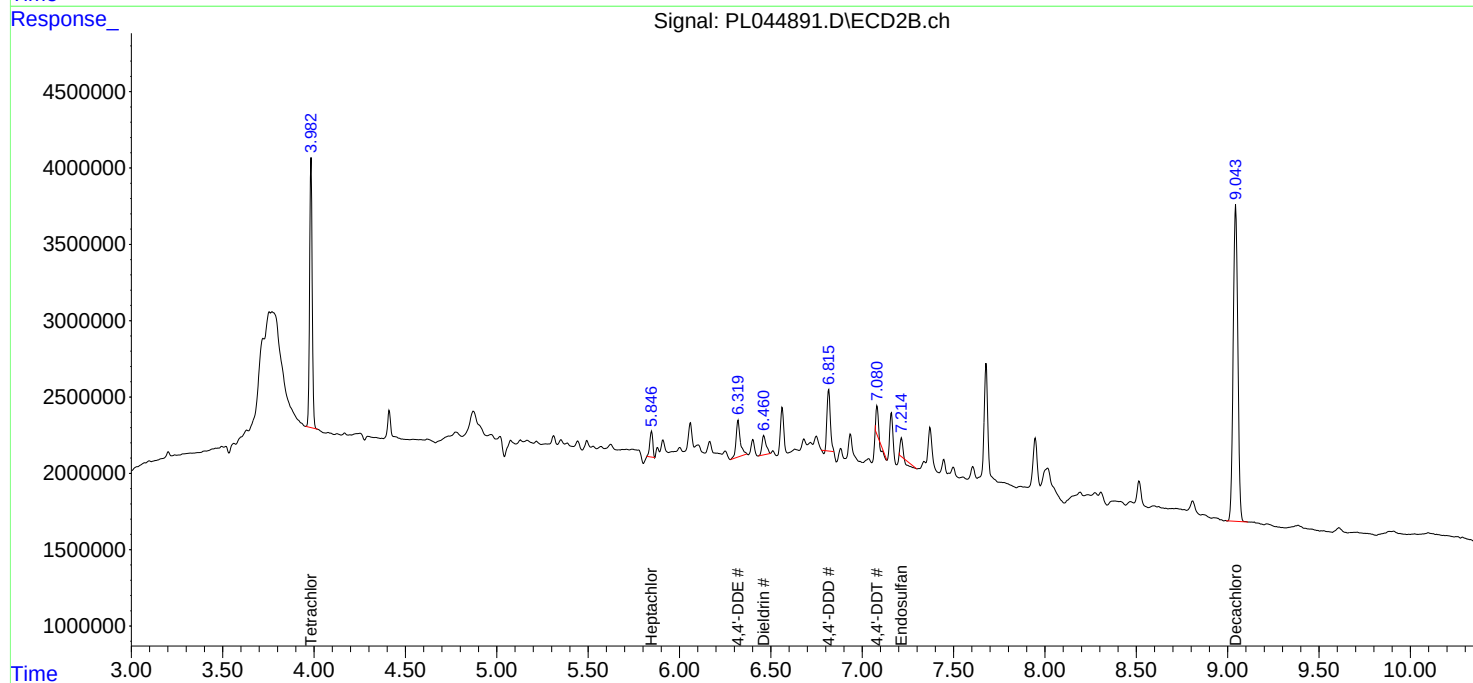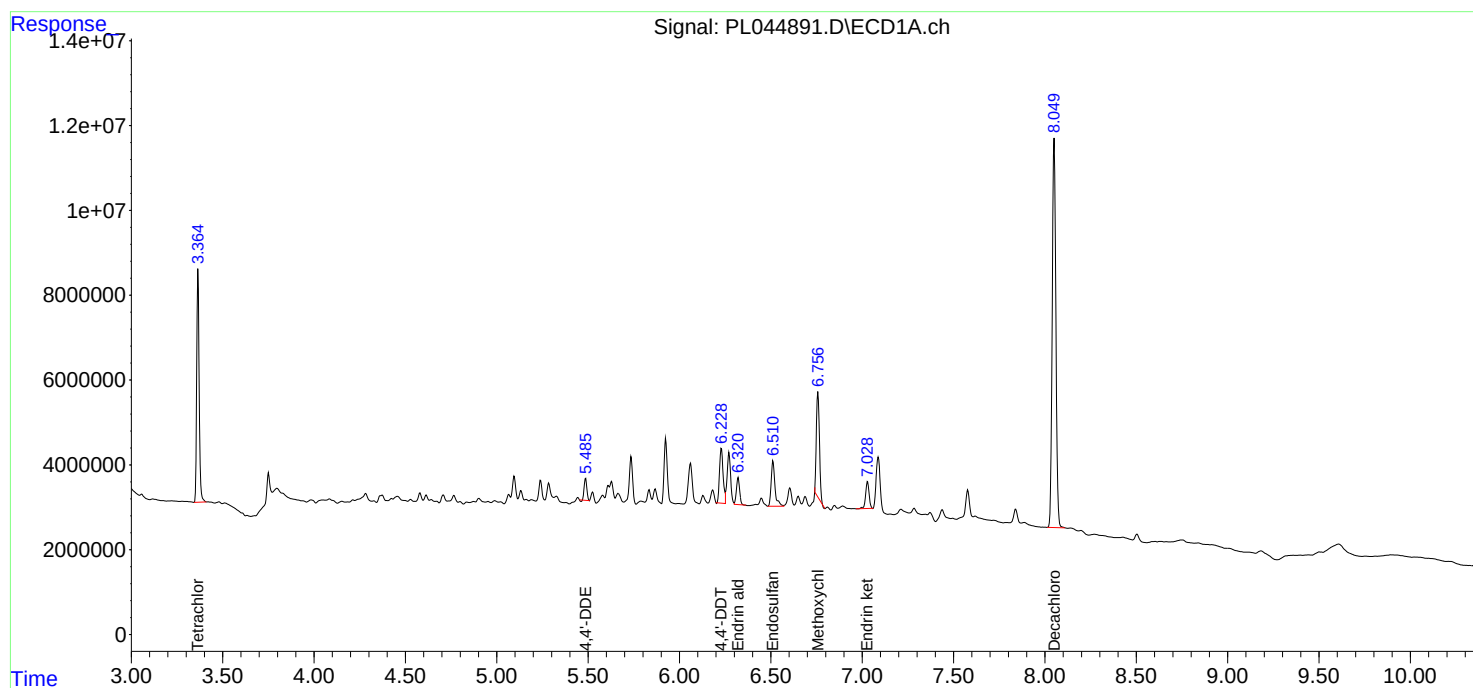


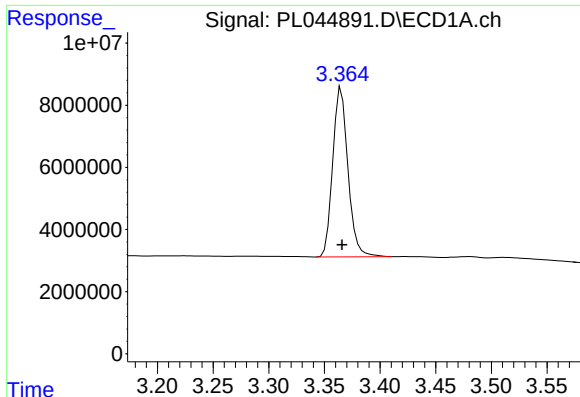

#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: 0.000 min
Response: 52022357
Conc: 7.31 ng/ml

Instrument :
ECD_L
ClientSampleId :
FLOORS

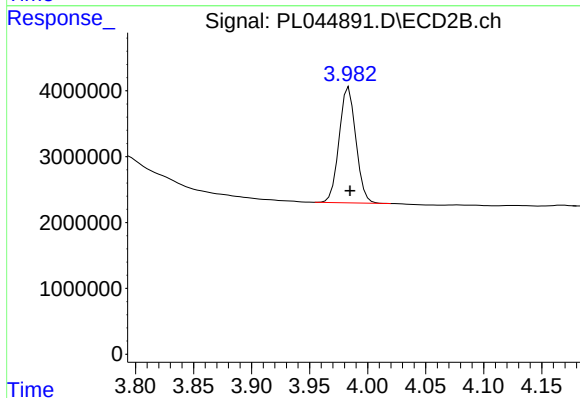


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: -0.001 min
Response: 17655843
Conc: 7.52 ng/ml

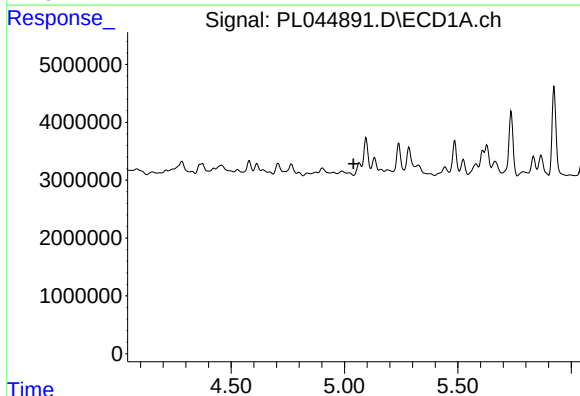


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.040 min
Response: 0
Conc: N.D.

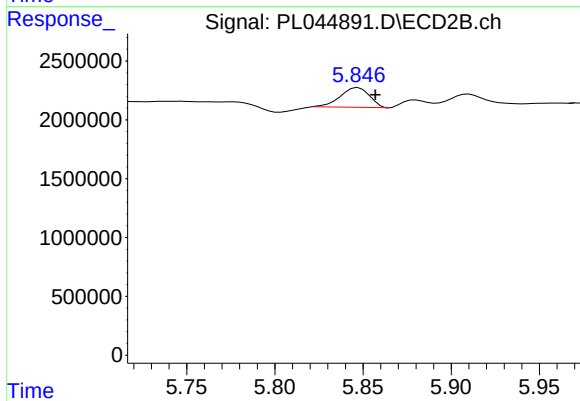

#8 Heptachlor epoxide


R.T.: 5.847 min
Delta R.T.: -0.010 min
Response: 1913210
Conc: 0.77 ng/ml

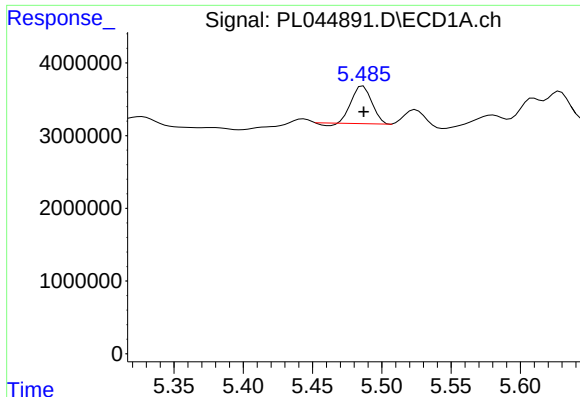

#12 4,4'-DDE


R.T.: 5.487 min
Delta R.T.: 0.000 min
Response: 5228681
Conc: 0.60 ng/ml

Instrument :
ECD_L
ClientSampleId :
FLOORS

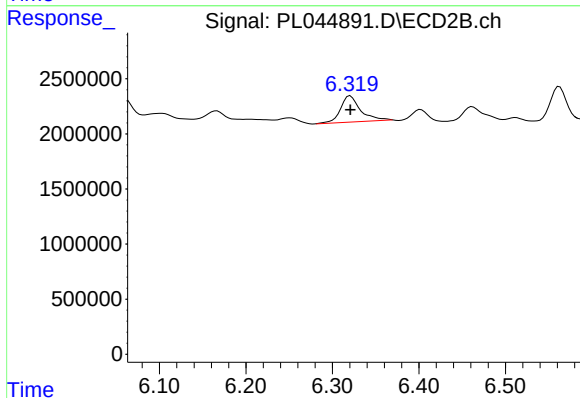


#12 4,4'-DDE

R.T.: 6.321 min
Delta R.T.: 0.000 min
Response: 3858634
Conc: 1.62 ng/ml

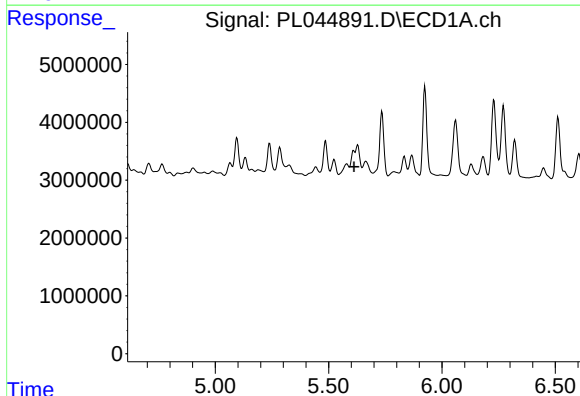


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 5.612 min
Response: 0
Conc: N.D.

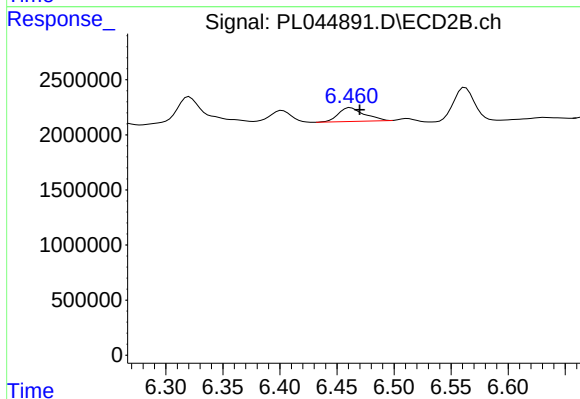

#13 Dieldrin


R.T.: 6.462 min
Delta R.T.: -0.008 min
Response: 1967086
Conc: 0.76 ng/ml

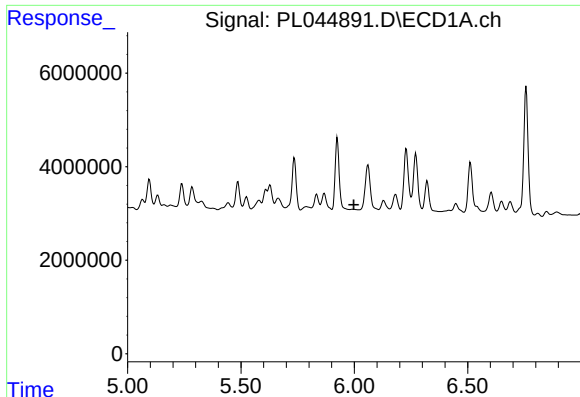

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 5.998 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :
FLOORS

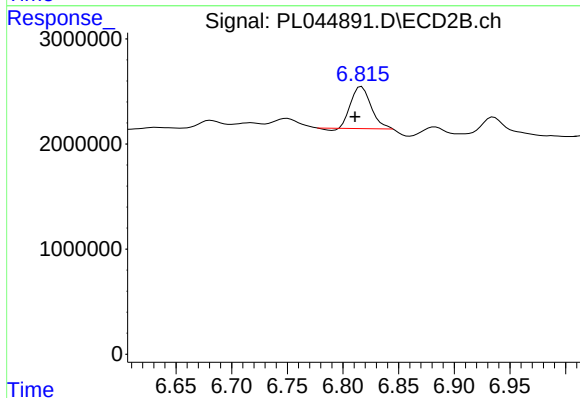


#16 4,4'-DDD

R.T.: 6.817 min
Delta R.T.: 0.006 min
Response: 4999959
Conc: 2.60 ng/ml

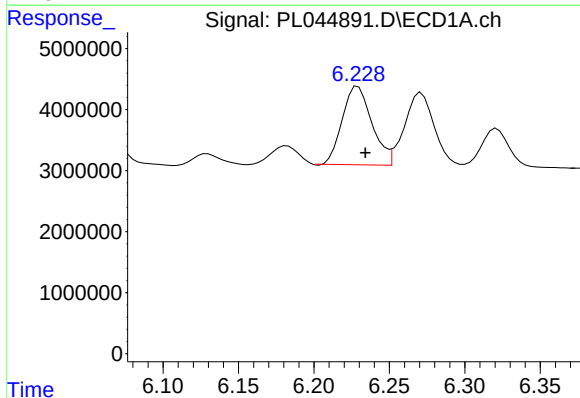


#17 4,4'-DDT

R.T.: 6.229 min
Delta R.T.: -0.005 min
Response: 17559152
Conc: 2.45 ng/ml

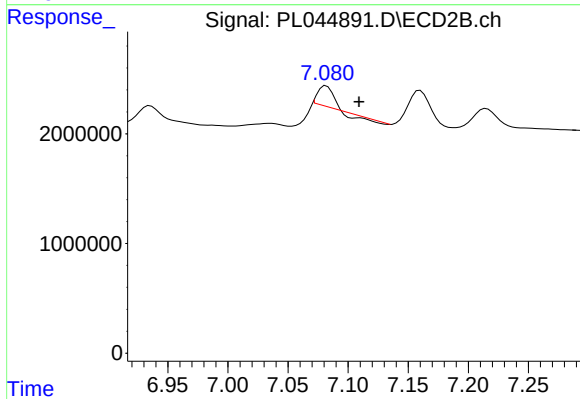

#17 4,4'-DDT


R.T.: 7.082 min
Delta R.T.: -0.027 min
Response: 1225137
Conc: 0.62 ng/ml

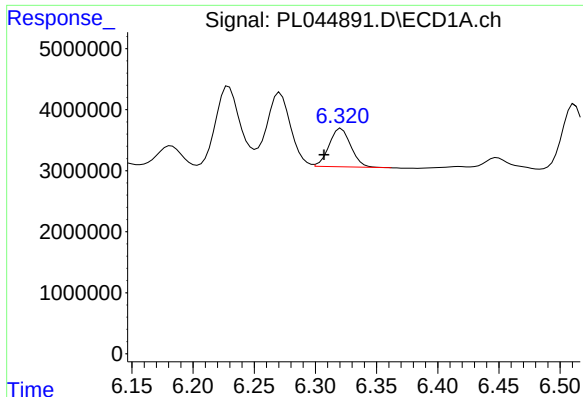

#18 Endrin aldehyde


R.T.: 6.321 min
Delta R.T.: 0.014 min
Response: 7702320
Conc: 1.10 ng/ml

Instrument :
ECD_L
ClientSampleId :
FLOORS

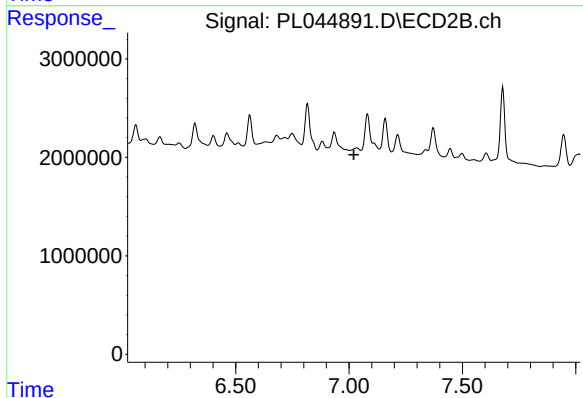


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T.: 7.021 min
Response: 0
Conc: N.D.

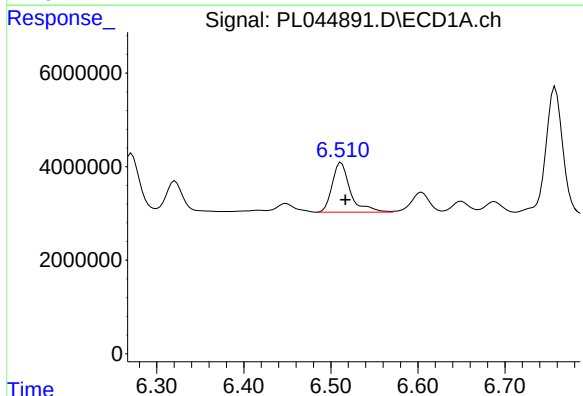


#19 Endosulfan Sulfate

R.T.: 6.512 min
Delta R.T.: -0.005 min
Response: 15477122
Conc: 2.13 ng/ml

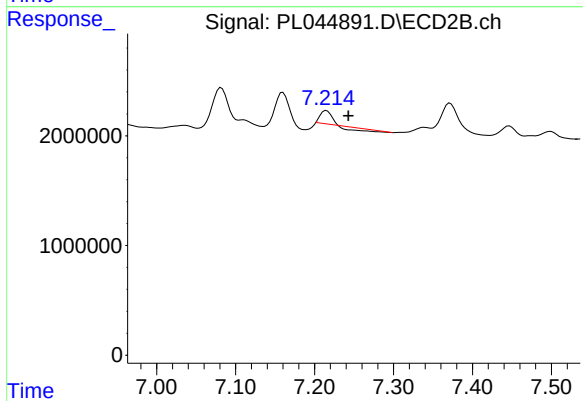

#19 Endosulfan Sulfate


R.T.: 7.215 min
Delta R.T.: -0.028 min
Response: 484049
Conc: 0.23 ng/ml

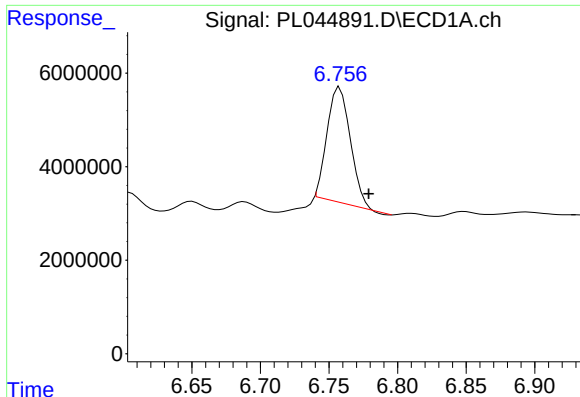

#20 Methoxychlor


R.T.: 6.758 min
Delta R.T.: -0.021 min
Response: 29013176
Conc: 7.23 ng/ml

Instrument :
ECD_L
ClientSampleId :
FLOORS

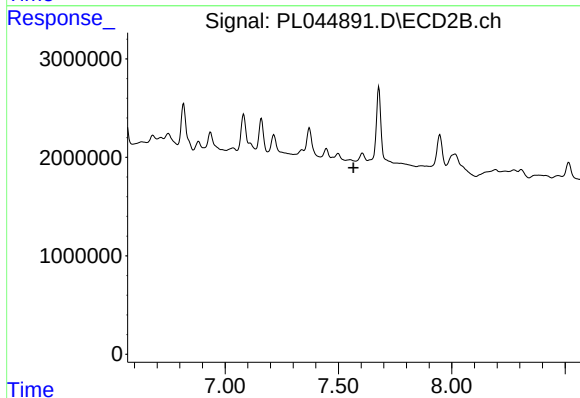


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.567 min
Response: 0
Conc: N.D.

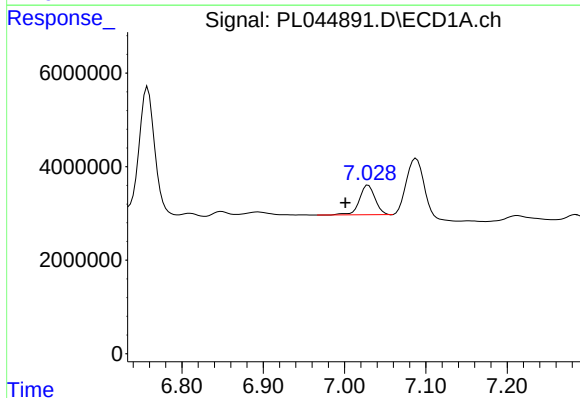


#21 Endrin ketone

R.T.: 7.029 min
Delta R.T.: 0.028 min
Response: 8473178
Conc: 1.02 ng/ml

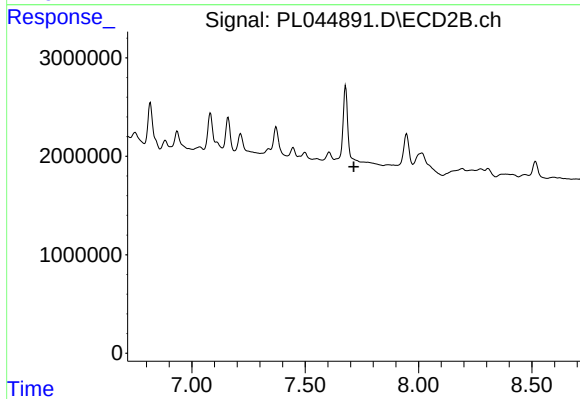

#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 7.714 min
Response: 0
Conc: N.D.

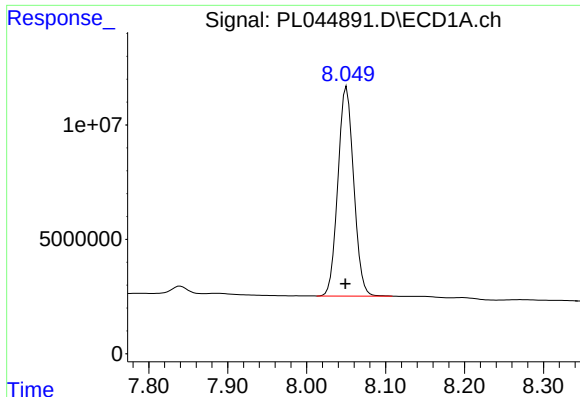

#28 Decachlorobiphenyl


R.T.: 8.051 min

Delta R.T.: 0.002 min

Response: 127079813

Conc: 17.42 ng/ml

Instrument :
ECD_L
ClientSampleId :
FLOORS

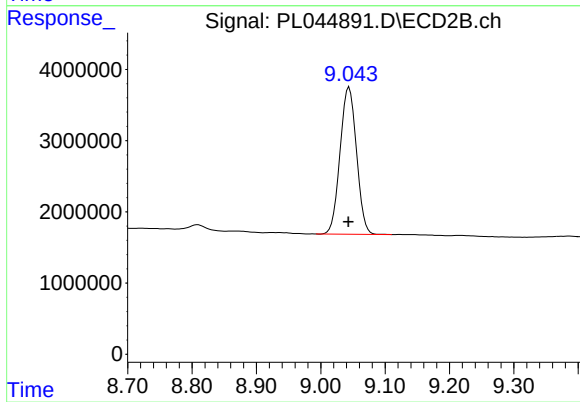

#28 Decachlorobiphenyl

R.T.: 9.044 min

Delta R.T.: 0.001 min

Response: 36623525

Conc: 16.54 ng/ml