

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021819\
Data File : PL044894.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2019 15:53
Operator : AJ\SJ
Sample : K1514-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-BPM-004-CLEARBROOK-PILE-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 01:17:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.365	3.983	141.0E6	45846713	19.815	19.516
28)	SA Decachlor...	8.050	9.043	148.2E6	43478011	20.316	19.630

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021819\
Data File : PL044894.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2019 15:53
Operator : AJ\SJ
Sample : K1514-01
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
FK-BPM-004-CLEARBROOK-PILE-1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 01:17:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

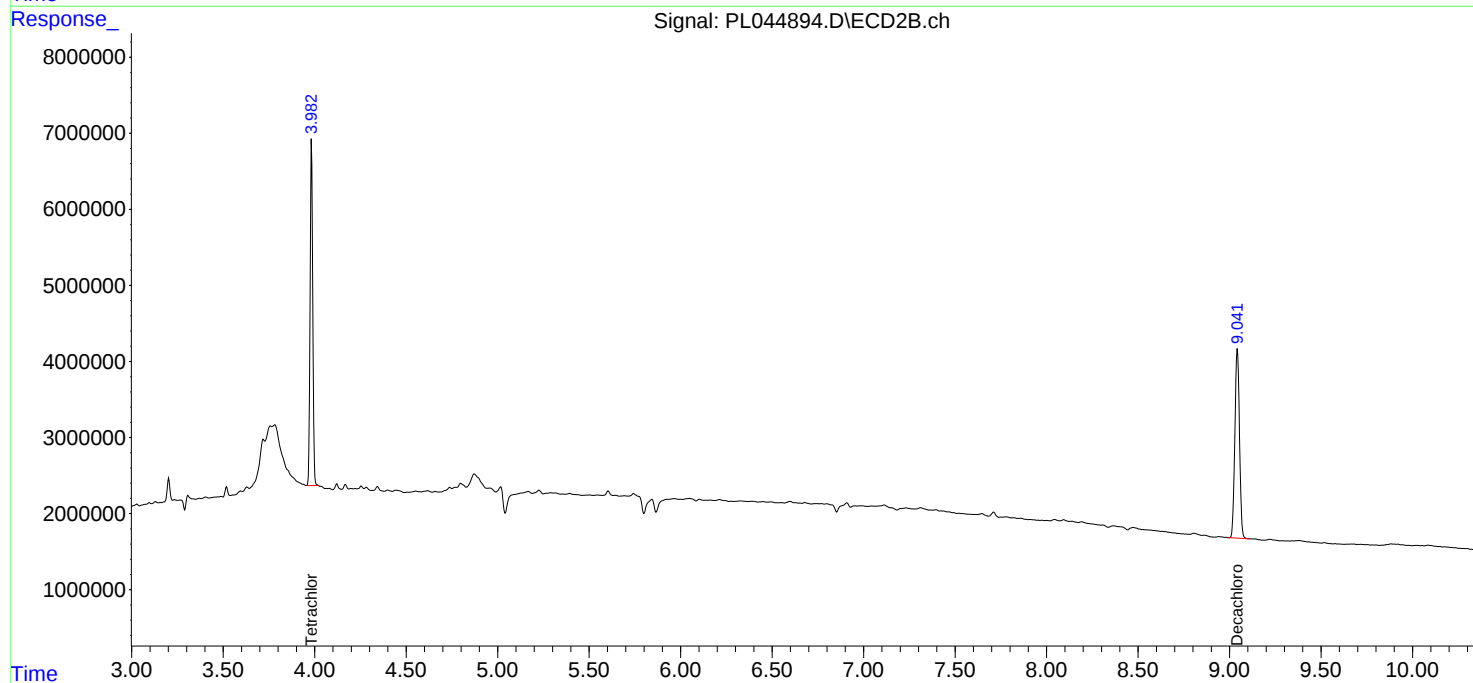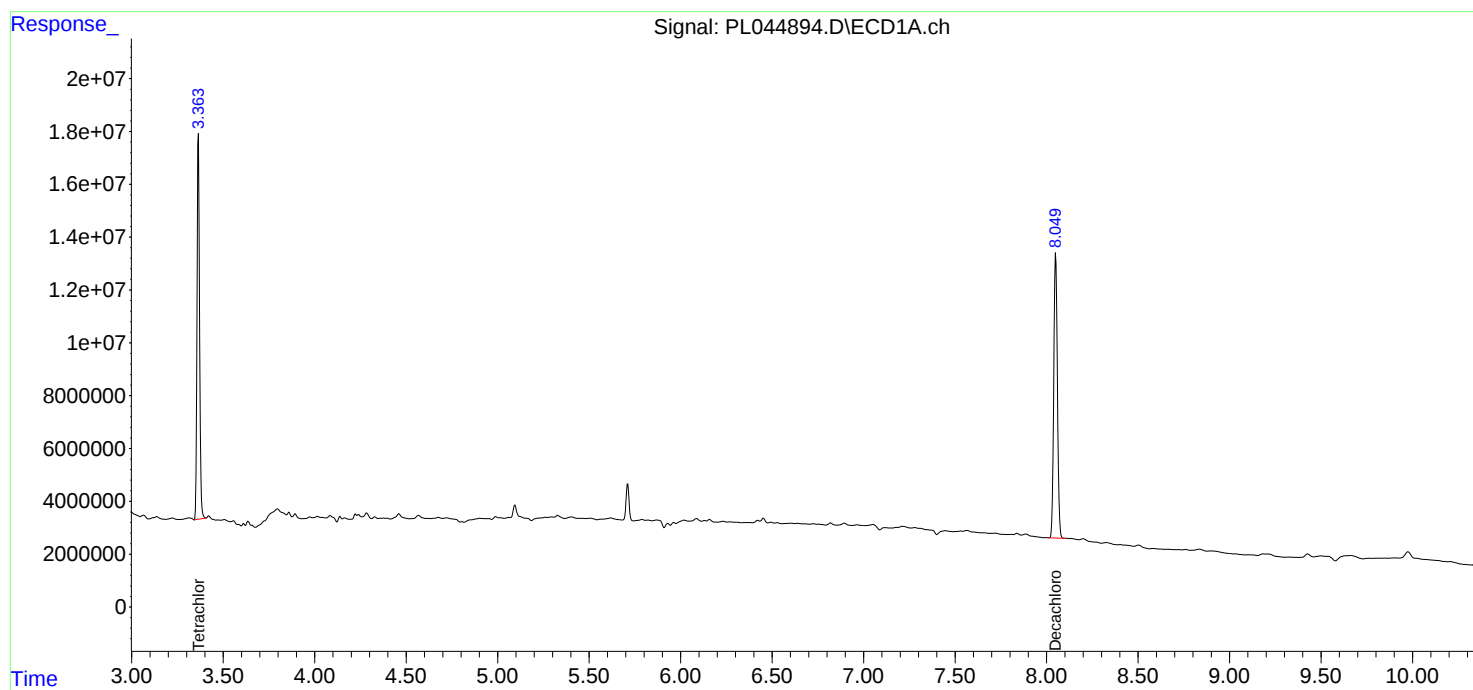


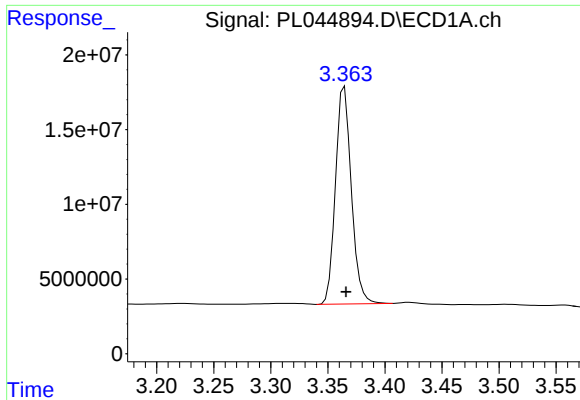

#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: -0.001 min
Response: 140999106
Conc: 19.81 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-BPM-004-CLEARBROOK-PILE-1

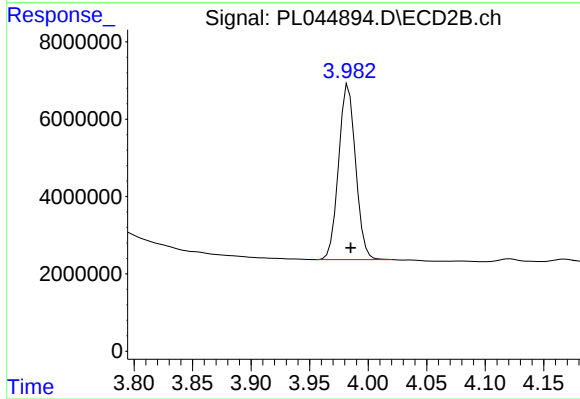


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: -0.002 min
Response: 45846713
Conc: 19.52 ng/ml

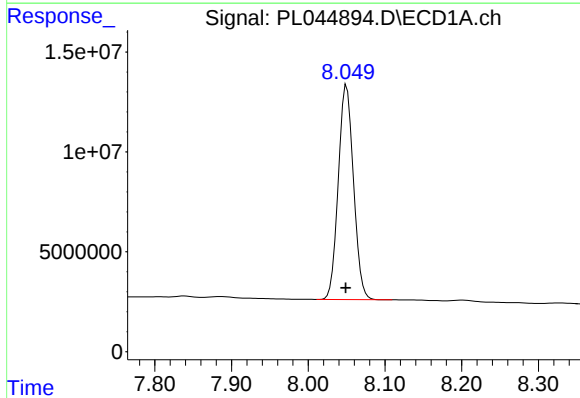

#28 Decachlorobiphenyl

R.T.: 8.050 min
Delta R.T.: 0.001 min
Response: 148177302
Conc: 20.32 ng/ml

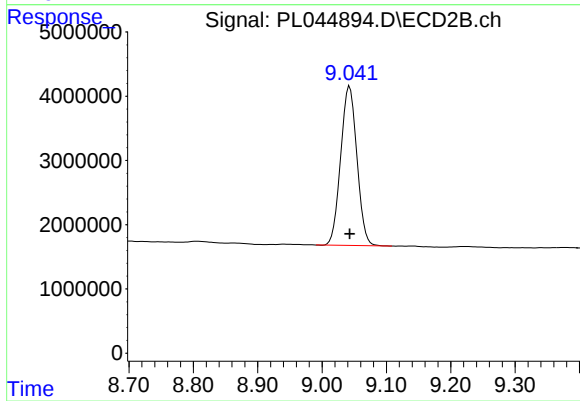

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.000 min
Response: 43478011
Conc: 19.63 ng/ml