

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021819\
 Data File : PL044910.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2019 19:39
 Operator : AJ\SJ
 Sample : K1508-12
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 M-13-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 01:20:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.365	3.983	143.6E6	46821554	20.184	19.931
28)	SA Decachlor...	8.049	9.041	149.2E6	43767458	20.458	19.761
Target Compounds							
7)	B delta-BHC	0.000	5.018f	0	826261	N.D.	0.452 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021819\
Data File : PL044910.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2019 19:39
Operator : AJ\SJ
Sample : K1508-12
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
M-13-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 01:20:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

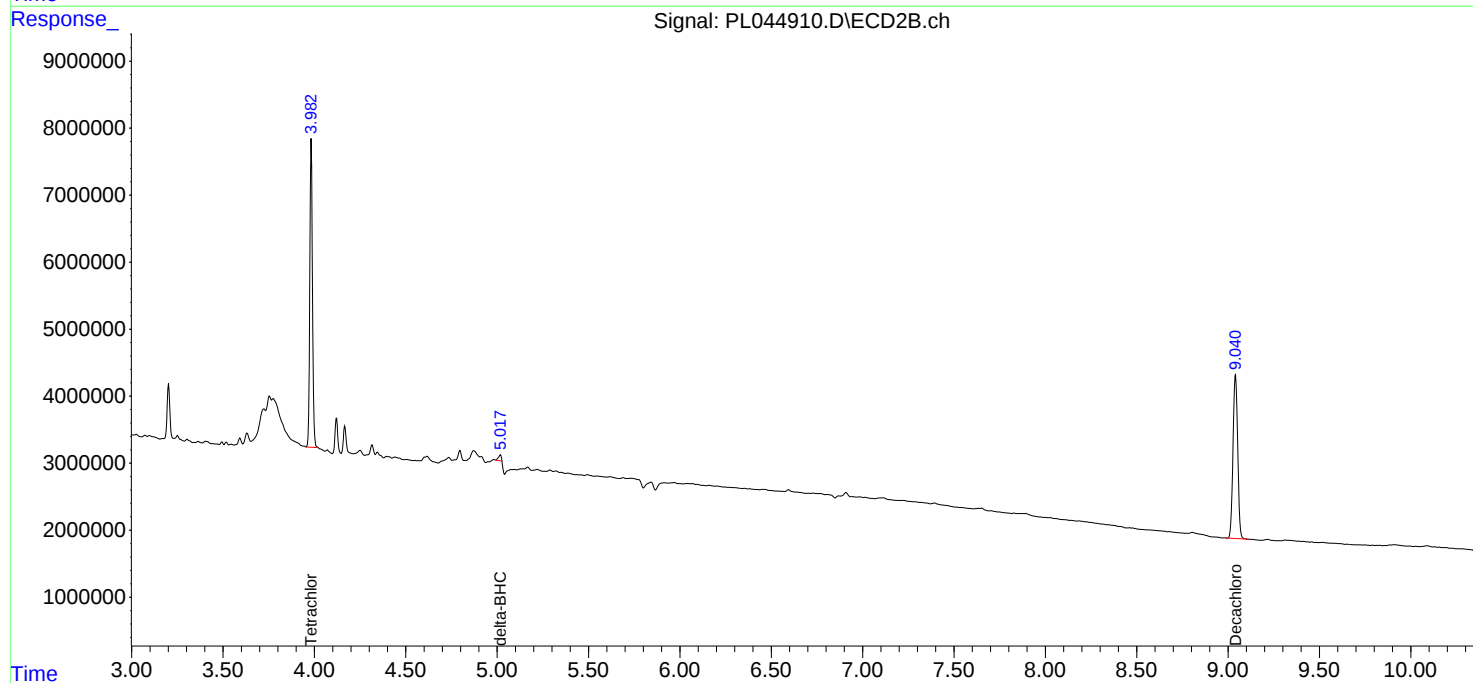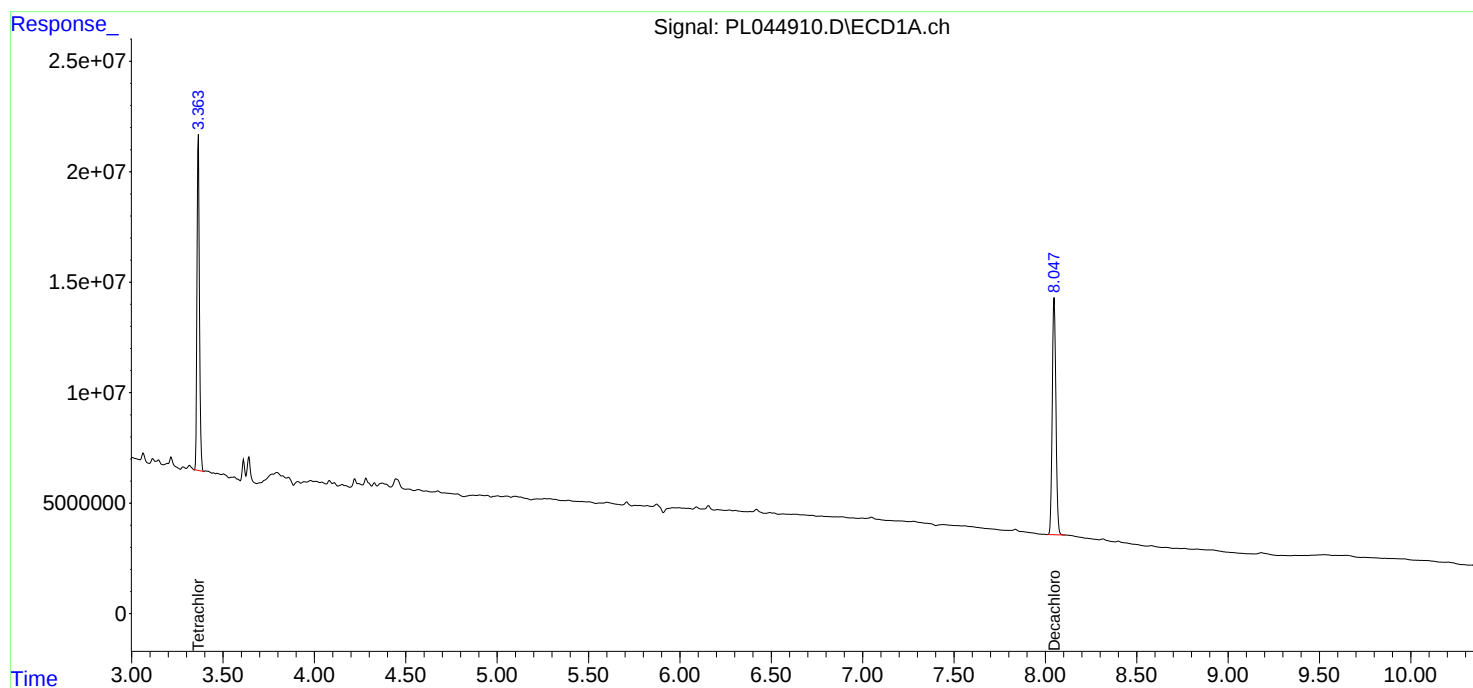


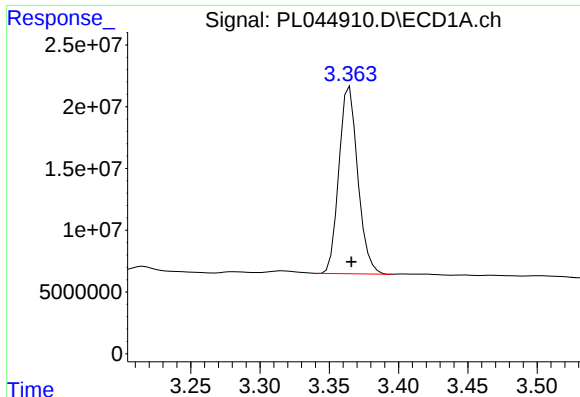

#1 Tetrachloro-m-xylene


R.T.: 3.365 min
Delta R.T.: -0.001 min
Response: 143624666
Conc: 20.18 ng/ml

Instrument :
ECD_L
ClientSampleId :
M-13-S

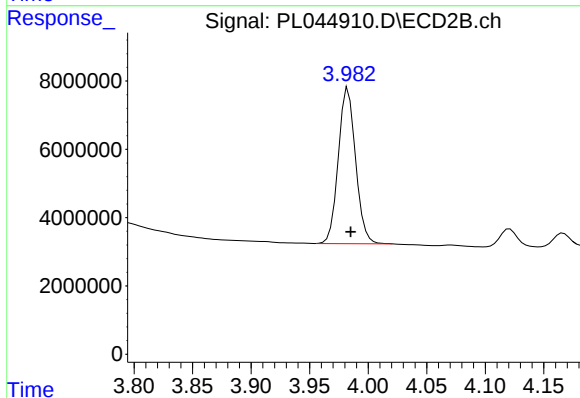


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: -0.002 min
Response: 46821554
Conc: 19.93 ng/ml

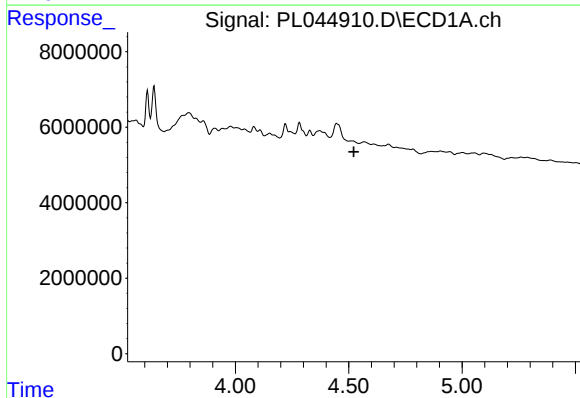


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.522 min
Response: 0
Conc: N.D.

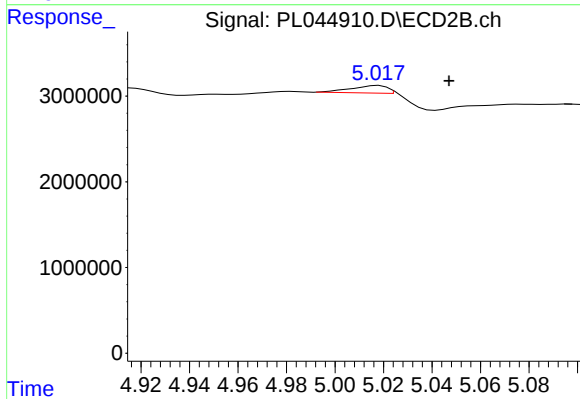

#7 delta-BHC


R.T.: 5.018 min
Delta R.T.: -0.029 min
Response: 826261
Conc: 0.45 ng/ml

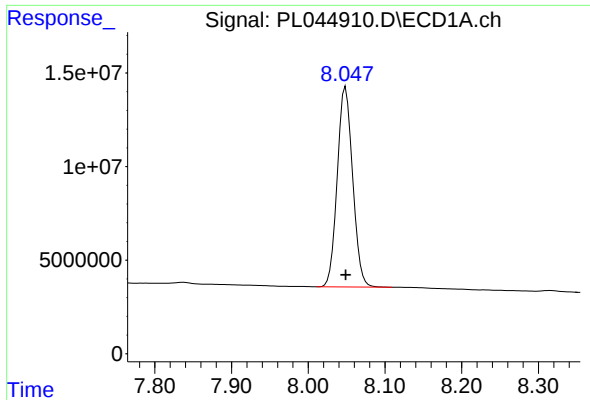

#28 Decachlorobiphenyl

R.T.: 8.049 min
Delta R.T.: 0.000 min
Response: 149214024
Conc: 20.46 ng/ml

Instrument :
ECD_L
ClientSampleId :
M-13-S

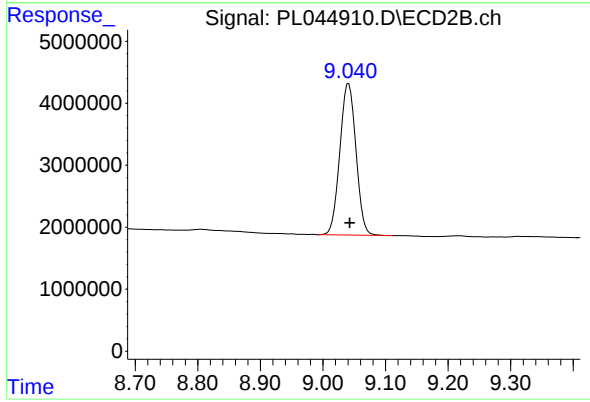

#28 Decachlorobiphenyl

R.T.: 9.041 min
Delta R.T.: -0.002 min
Response: 43767458
Conc: 19.76 ng/ml