

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021819\
 Data File : PL044888.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2019 14:29
 Operator : AJ\SJ
 Sample : K1510-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-GF-02-030-A

Manual Integrations
 APPROVED

Sohil
 2/19/2019 2:22:57 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 01:16:06 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.365	3.983	77958131	26197611	10.956	11.152
28) SA Decachlor...	8.051	9.043	110.9E6	32950300	15.206	14.877
Target Compounds						
4) MA Heptachlor	4.361	5.165	5616881	2215330	0.545	0.727 #
11) B alpha-Chl...	5.319	6.164	7782654	3915490	0.814m	1.413 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021819\
Data File : PL044888.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2019 14:29
Operator : AJ\SJ
Sample : K1510-01
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FK-GF-02-030-A


Manual Integrations
APPROVED

Sohil
2/19/2019 2:22:57 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 01:16:06 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

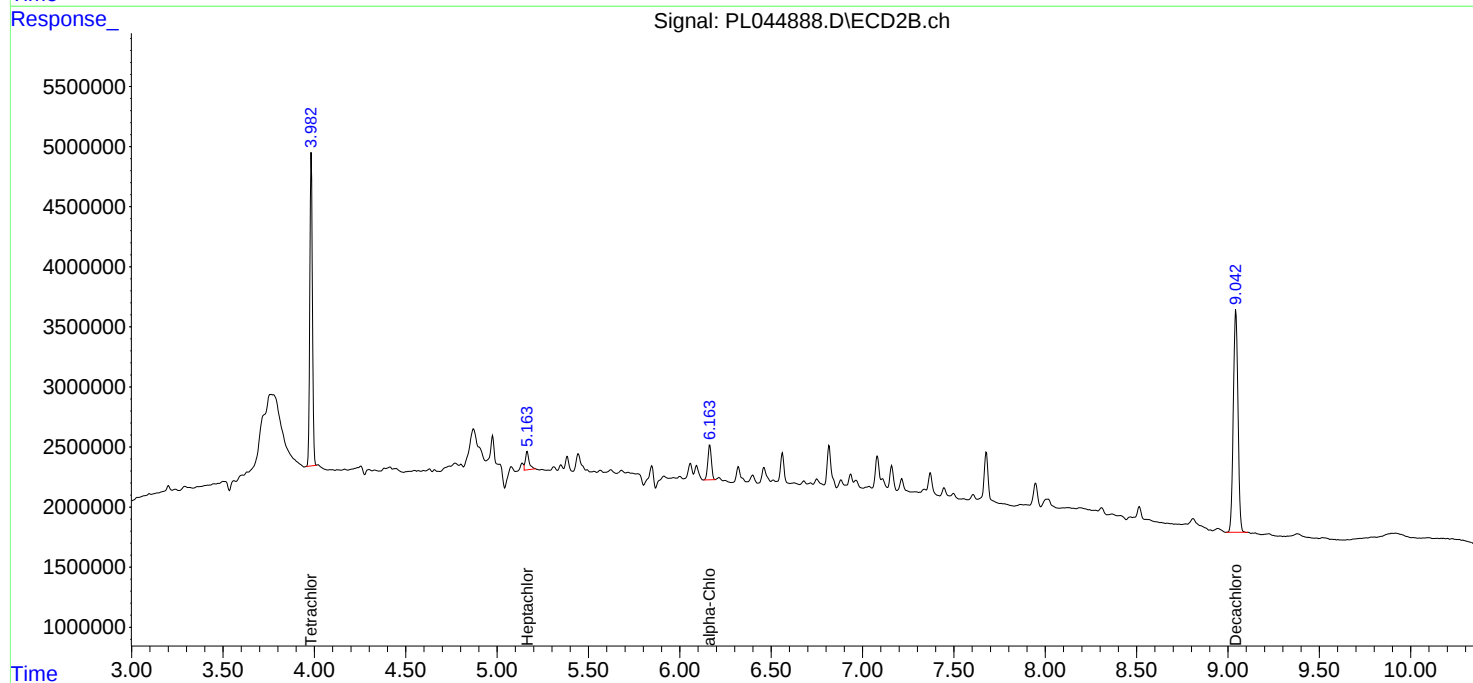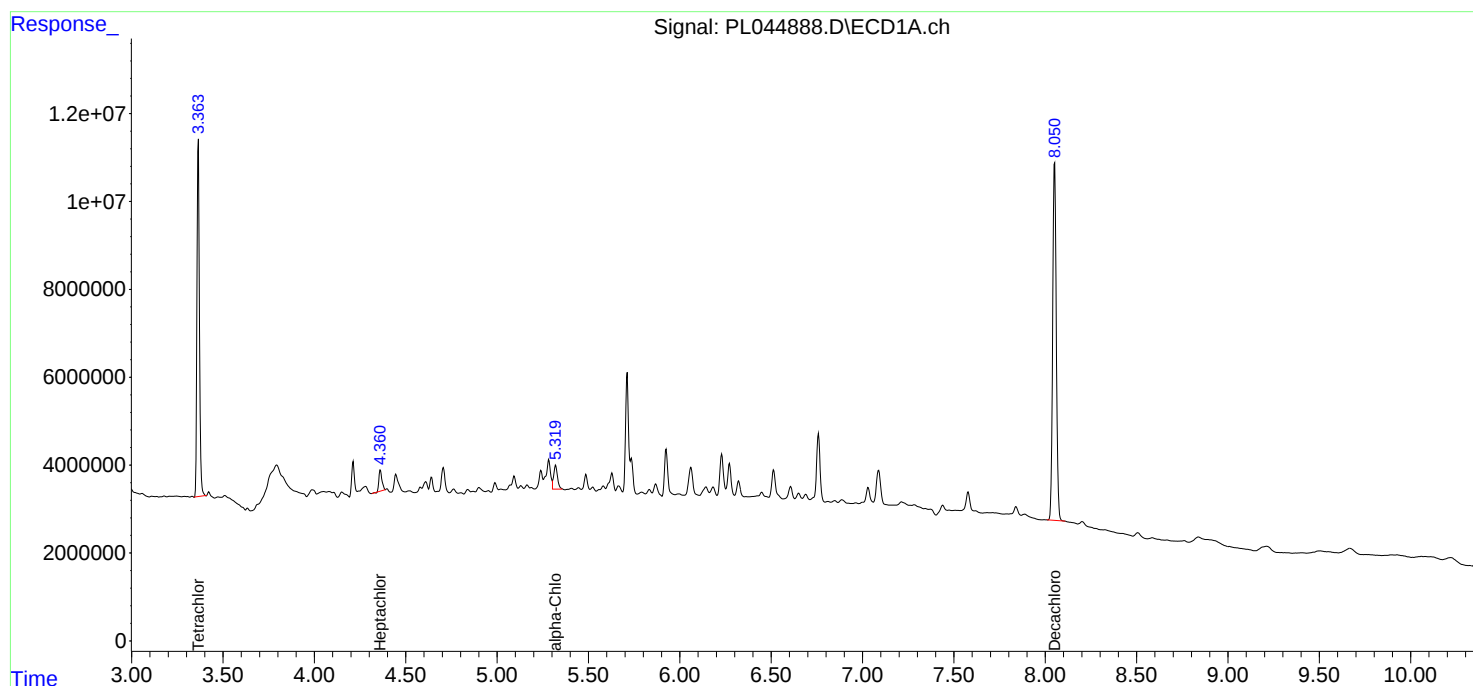

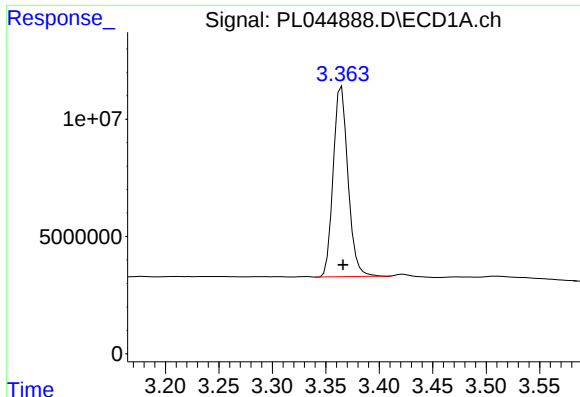


#1 Tetrachloro-m-xylene

R.T.: 3.365 min
Delta R.T.: -0.001 min
Response: 77958131
Conc: 10.96 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-GF-02-030-A


Manual Integrations
APPROVED

Sohil
2/19/2019 2:22:57 PM

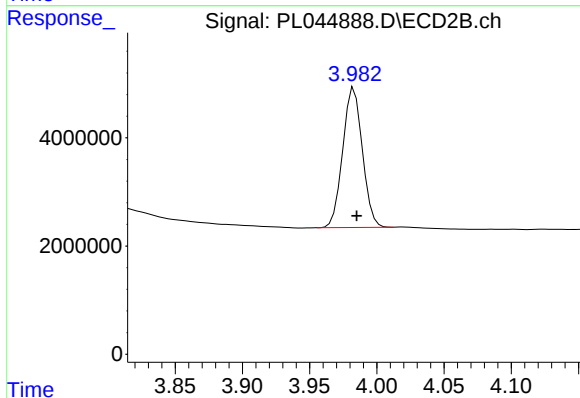


#1 Tetrachloro-m-xylene

R.T.: 3.983 min
Delta R.T.: -0.002 min
Response: 26197611
Conc: 11.15 ng/ml

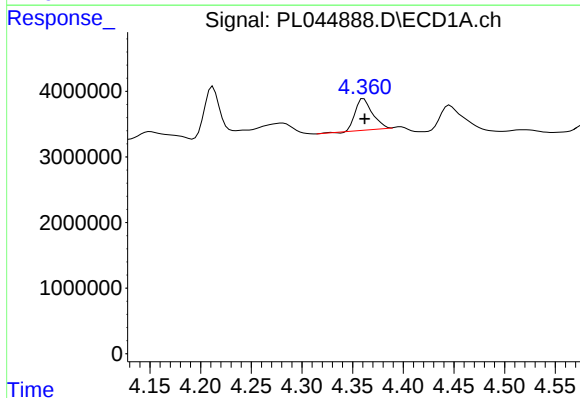


#4 Heptachlor

R.T.: 4.361 min
Delta R.T.: -0.001 min
Response: 5616881
Conc: 0.55 ng/ml

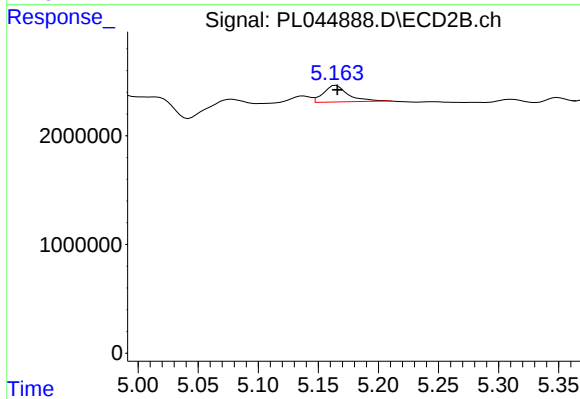

#4 Heptachlor

R.T.: 5.165 min
Delta R.T.: -0.001 min
Response: 2215330
Conc: 0.73 ng/ml

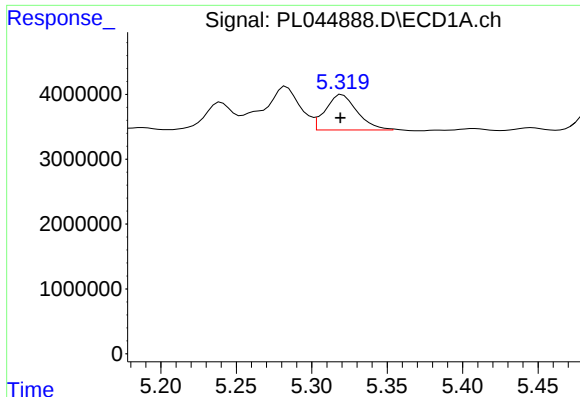


#11 alpha-Chlordane

R.T.: 5.319 min
Delta R.T.: 0.000 min
Response: 7782654
Conc: 0.81 ng/ml m

Instrument :
ECD_L
ClientSampleId :
FK-GF-02-030-A


Manual Integrations
APPROVED

Sohil
2/19/2019 2:22:57 PM

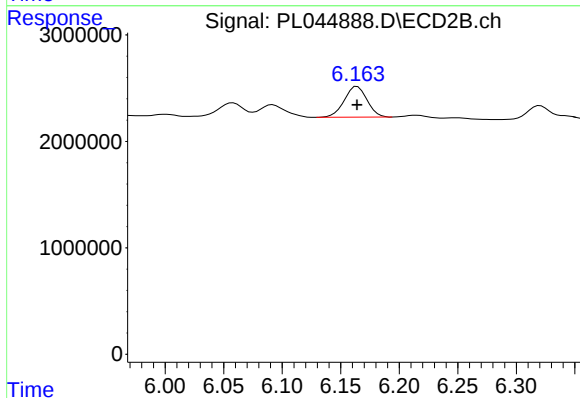


#11 alpha-Chlordane

R.T.: 6.164 min
Delta R.T.: 0.000 min
Response: 3915490
Conc: 1.41 ng/ml

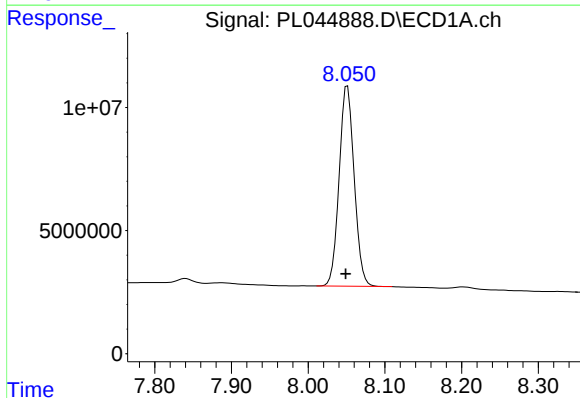

#28 Decachlorobiphenyl

R.T.: 8.051 min
Delta R.T.: 0.002 min
Response: 110904589
Conc: 15.21 ng/ml

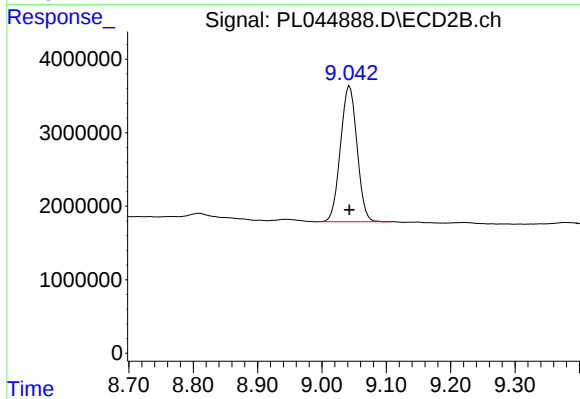

#28 Decachlorobiphenyl

R.T.: 9.043 min
Delta R.T.: 0.000 min
Response: 32950300
Conc: 14.88 ng/ml