

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021819\
 Data File : PL044889.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Feb 2019 14:43
 Operator : AJ\SJ
 Sample : K1510-03
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 FK-GF-02-030-B

Manual Integrations
 APPROVED

Sohil
 2/19/2019 2:22:59 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 19 01:16:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
 Quant Title : GC Extractables
 QLast Update : Thu Feb 07 01:39:50 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.365	3.984	81158083	27104744	11.405	11.538
28) SA Decachlor...	8.051	9.044	116.7E6	34615798	15.995	15.629
Target Compounds						
4) MA Heptachlor	4.361	5.166	10810104	3880377	1.049	1.274
11) B alpha-Chl...	5.318	6.165	10859546	6644888	1.136m	2.398 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL021819\
Data File : PL044889.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Feb 2019 14:43
Operator : AJ\SJ
Sample : K1510-03
Misc :
ALS Vial : 8 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
FK-GF-02-030-B


Manual Integrations
APPROVED

Sohil
2/19/2019 2:22:59 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 19 01:16:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020619.M
Quant Title : GC Extractables
QLast Update : Thu Feb 07 01:39:50 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x0.25µm

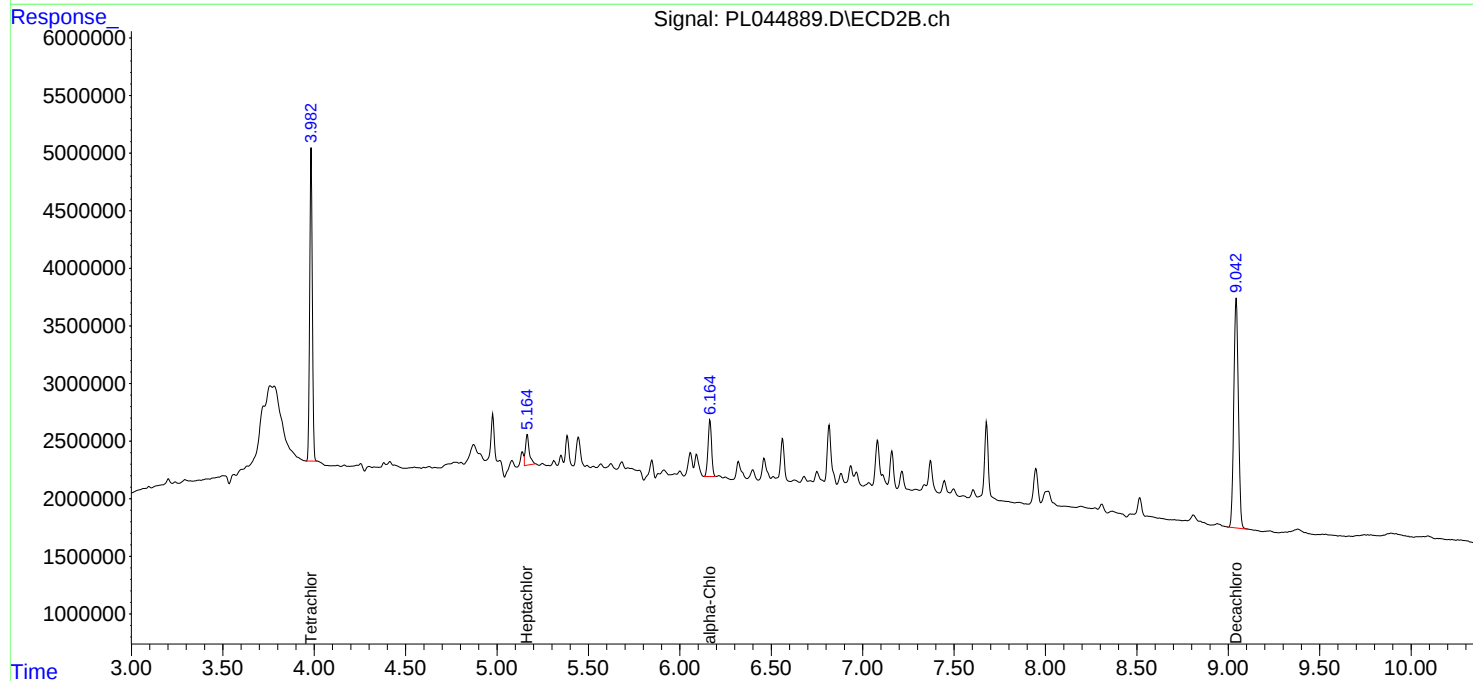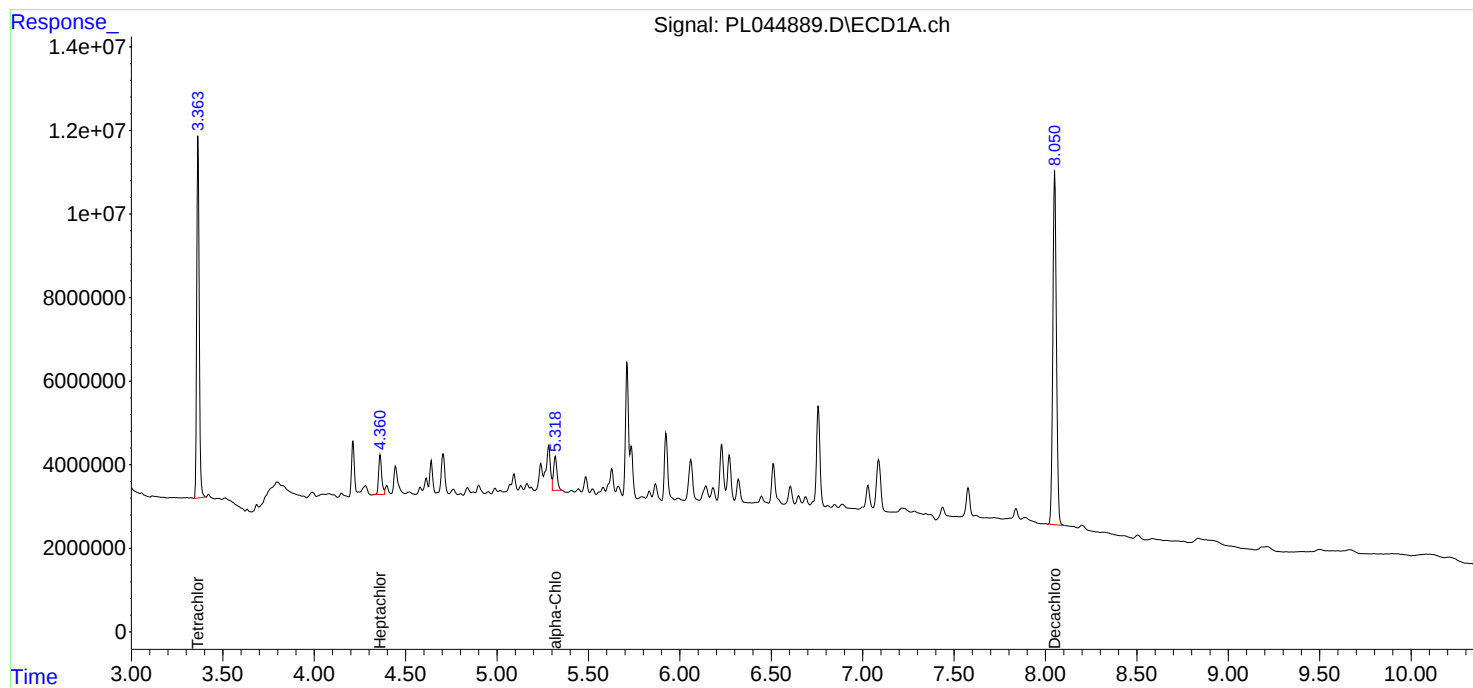

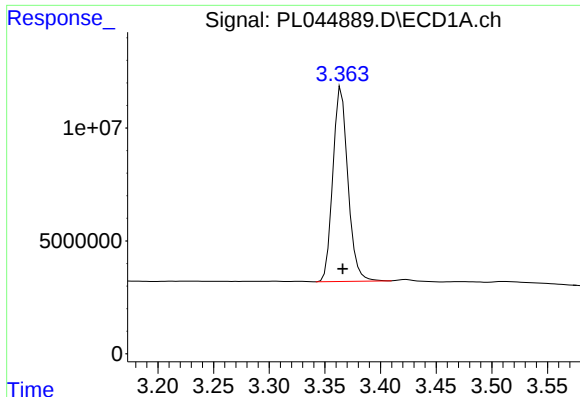


#1 Tetrachloro-m-xylene

R.T.: 3.365 min
Delta R.T.: -0.001 min
Response: 81158083
Conc: 11.41 ng/ml

Instrument :
ECD_L
ClientSampleId :
FK-GF-02-030-B


Manual Integrations
APPROVED

Sohil
2/19/2019 2:22:59 PM

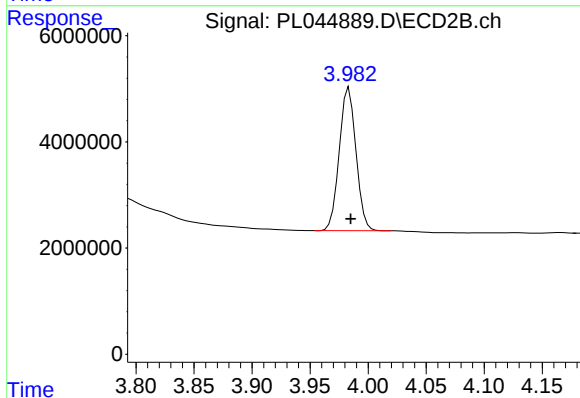


#1 Tetrachloro-m-xylene

R.T.: 3.984 min
Delta R.T.: -0.001 min
Response: 27104744
Conc: 11.54 ng/ml

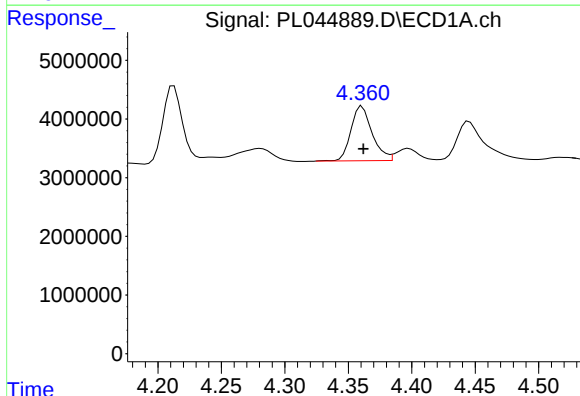


#4 Heptachlor

R.T.: 4.361 min
Delta R.T.: -0.001 min
Response: 10810104
Conc: 1.05 ng/ml

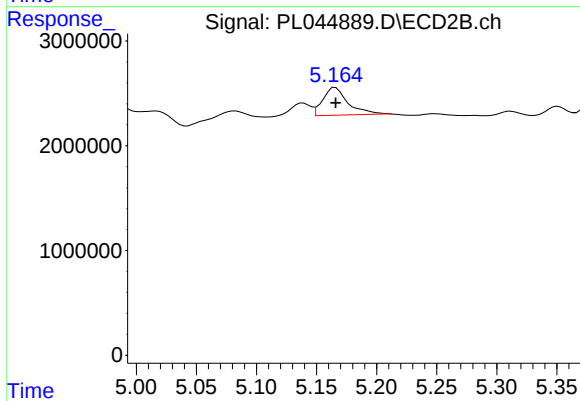

#4 Heptachlor

R.T.: 5.166 min
Delta R.T.: 0.000 min
Response: 3880377
Conc: 1.27 ng/ml

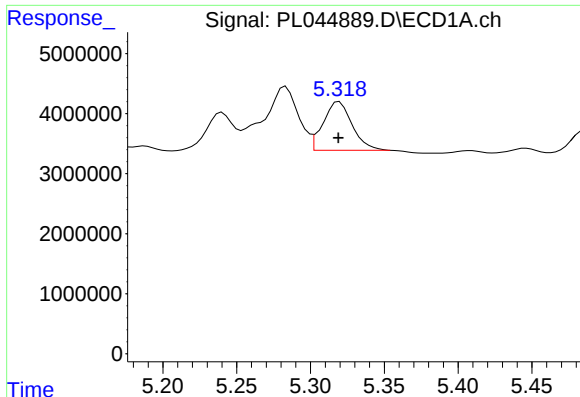


#11 alpha-Chlordane

R.T.: 5.318 min
Delta R.T.: 0.000 min
Response: 10859546
Conc: 1.14 ng/ml m

Instrument :
ECD_L
ClientSampleId :
FK-GF-02-030-B


Manual Integrations
APPROVED

Sohil
2/19/2019 2:22:59 PM

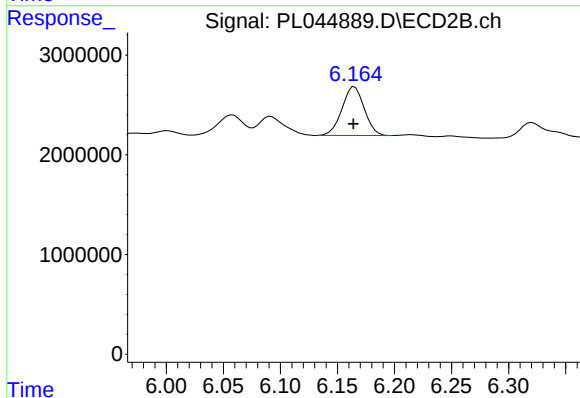


#11 alpha-Chlordane

R.T.: 6.165 min
Delta R.T.: 0.001 min
Response: 6644888
Conc: 2.40 ng/ml

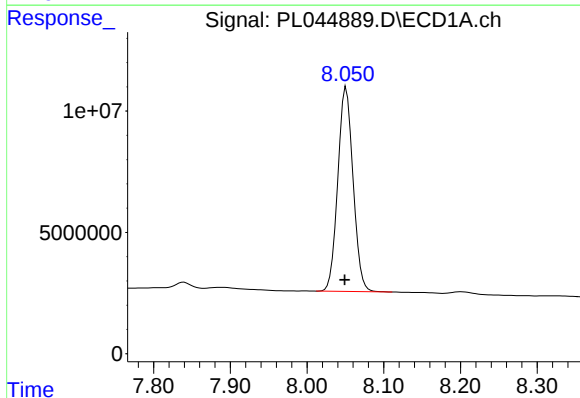

#28 Decachlorobiphenyl

R.T.: 8.051 min
Delta R.T.: 0.002 min
Response: 116661080
Conc: 16.00 ng/ml

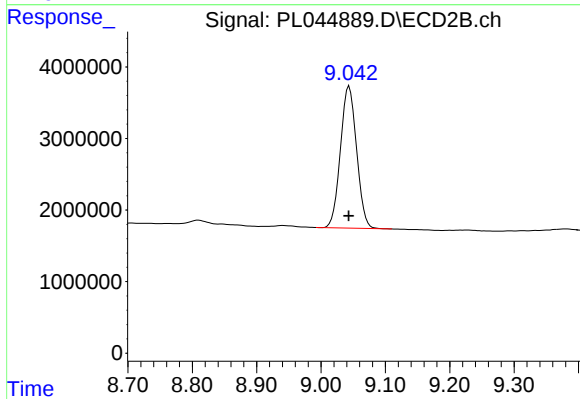

#28 Decachlorobiphenyl

R.T.: 9.044 min
Delta R.T.: 0.000 min
Response: 34615798
Conc: 15.63 ng/ml