

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022721\
 Data File : PL064974.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2021 13:59
 Operator : AR\AJ
 Sample : M1477-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 17:02:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.428	4.098	57506706	50554149	20.440	23.403
28)	SA Decachlor...	8.150	9.254	58155611	51048416	25.861	26.876
Target Compounds							
3)	MA gamma-BHC...	4.147	0.000	2007236	0	0.464	N.D. #
6)	B beta-BHC	4.406	0.000	2049539	0	1.199	N.D. #
7)	B delta-BHC	4.588	0.000	496596	0	0.123	N.D. #
9)	A Endosulfan I	5.482f	0.000	3227458	0	1.006	N.D. #
12)	B 4,4'-DDE	5.593f	0.000	3901892	0	1.247	N.D. #
13)	MA Dieldrin	5.704	0.000	5613163	0	1.711	N.D. #
17)	MA 4,4'-DDT	0.000	7.266	0	4887296	N.D.	3.205 #
23)	Chlordane-1	4.291	0.000	4402034	0	38.724	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022721\
Data File : PL064974.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2021 13:59
Operator : AR\AJ
Sample : M1477-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 17:02:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

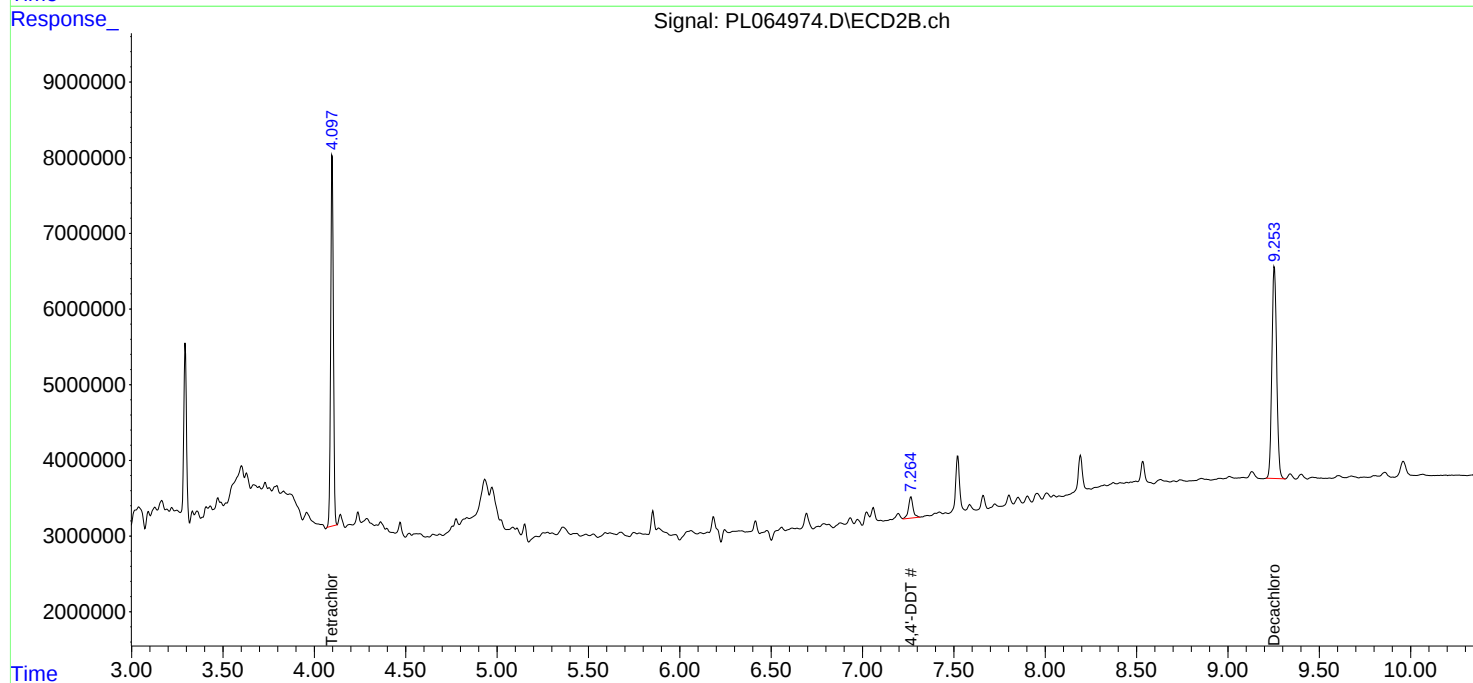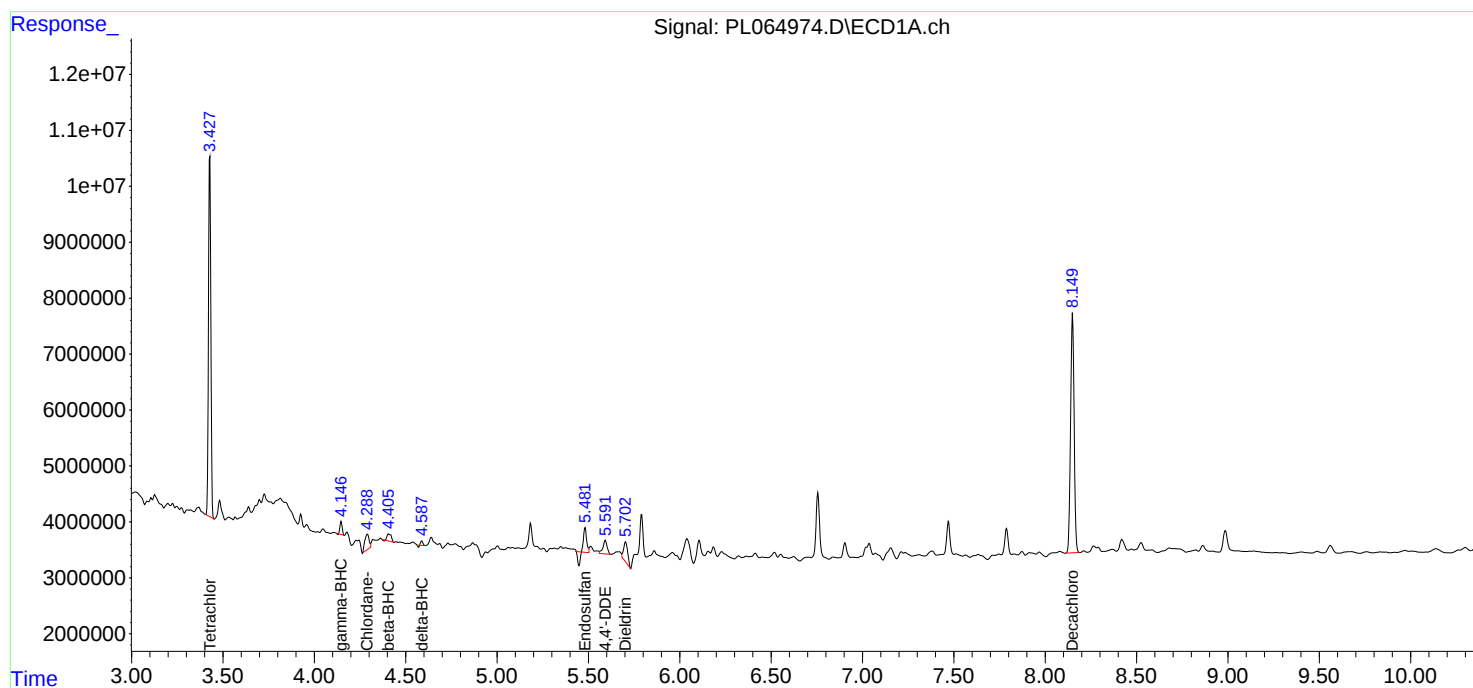


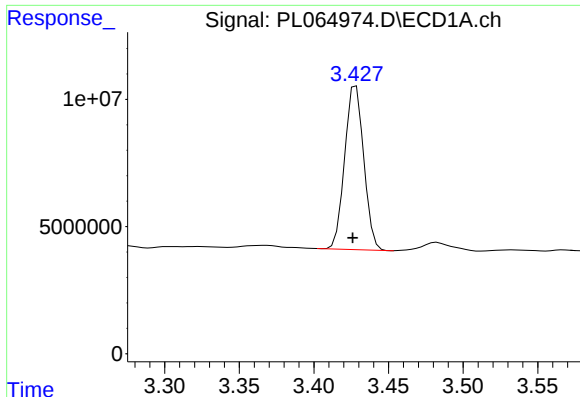

#1 Tetrachloro-m-xylene


R.T.: 3.428 min
Delta R.T.: 0.002 min
Response: 57506706
Conc: 20.44 ng/ml

Instrument :
ECD_L
ClientSampleId :

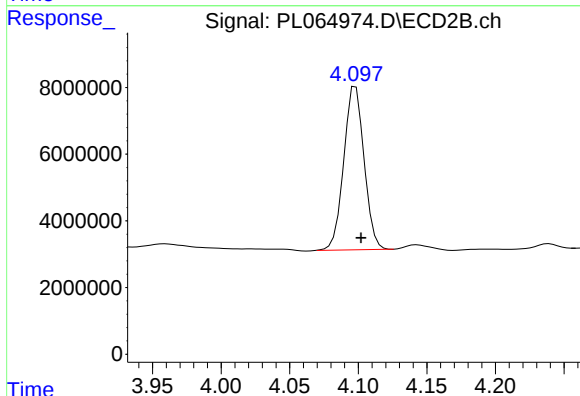


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: -0.004 min
Response: 50554149
Conc: 23.40 ng/ml

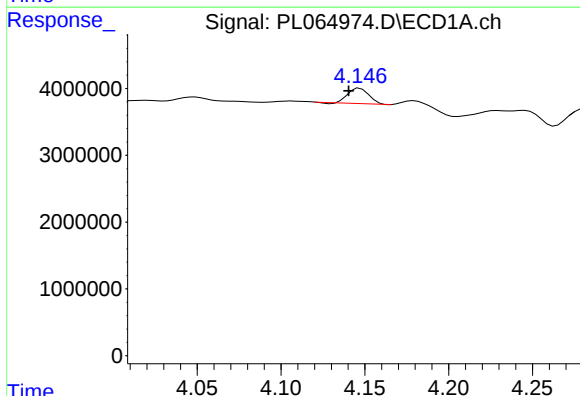


#3 gamma-BHC (Lindane)

R.T.: 4.147 min
Delta R.T.: 0.007 min
Response: 2007236
Conc: 0.46 ng/ml

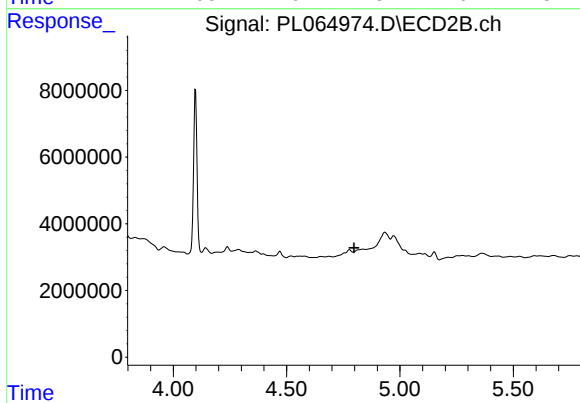

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.797 min
Response: 0
Conc: N.D.

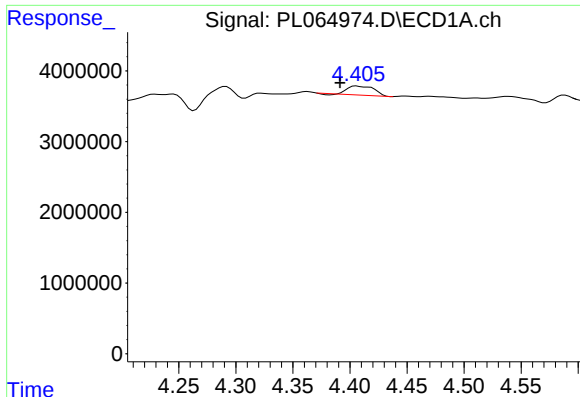

#6 beta-BHC


R.T.: 4.406 min
Delta R.T.: 0.014 min
Response: 2049539
Conc: 1.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

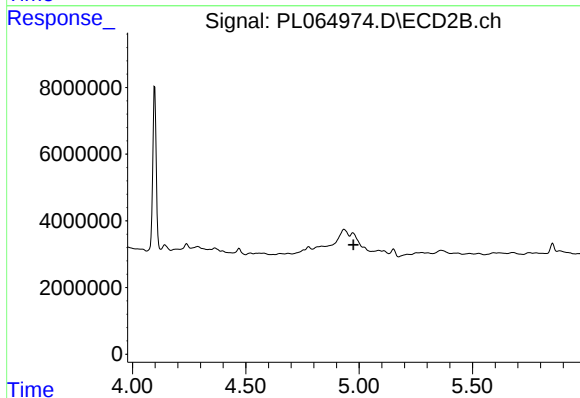


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.976 min
Response: 0
Conc: N.D.

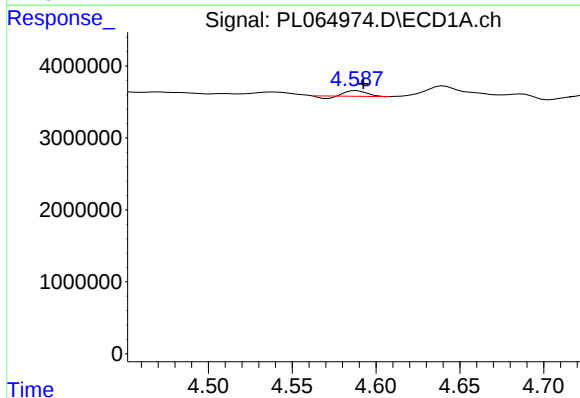


#7 delta-BHC

R.T.: 4.588 min
Delta R.T.: -0.004 min
Response: 496596
Conc: 0.12 ng/ml

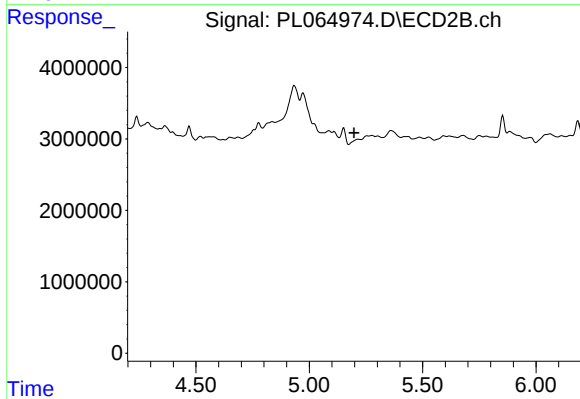

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 5.198 min
Response: 0
Conc: N.D.

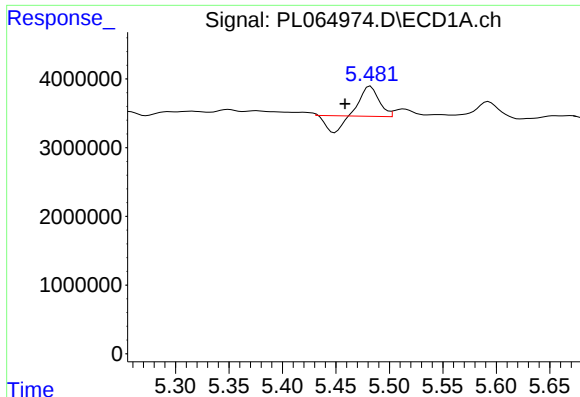

#9 Endosulfan I


R.T.: 5.482 min
Delta R.T.: 0.024 min
Response: 3227458
Conc: 1.01 ng/ml

Instrument :
ECD_L
ClientSampleId :

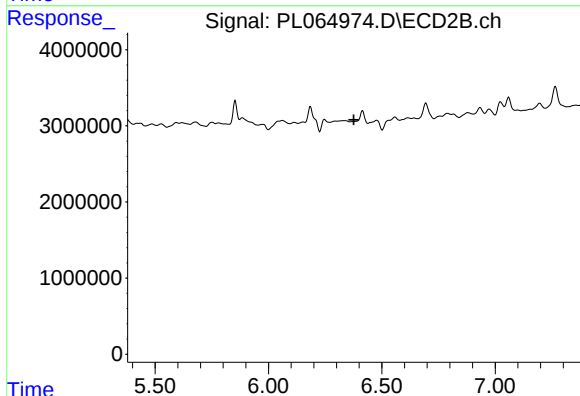


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.376 min
Response: 0
Conc: N.D.

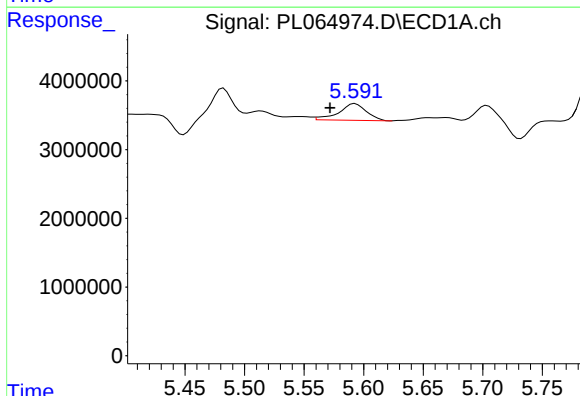


#12 4,4'-DDE

R.T.: 5.593 min
Delta R.T.: 0.021 min
Response: 3901892
Conc: 1.25 ng/ml

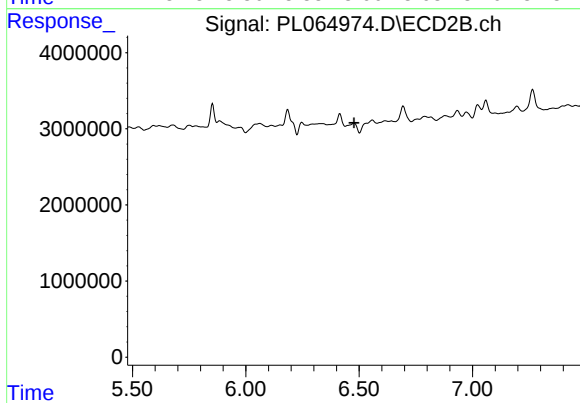

#12 4,4'-DDE


R.T.: 0.000 min
Exp R.T. : 6.478 min
Response: 0
Conc: N.D.

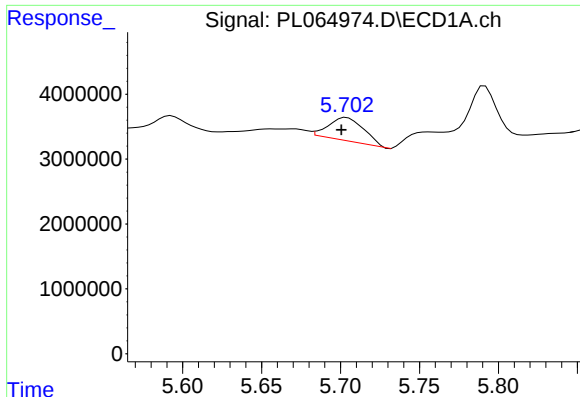

#13 Dieldrin


R.T.: 5.704 min
Delta R.T.: 0.003 min
Response: 5613163
Conc: 1.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

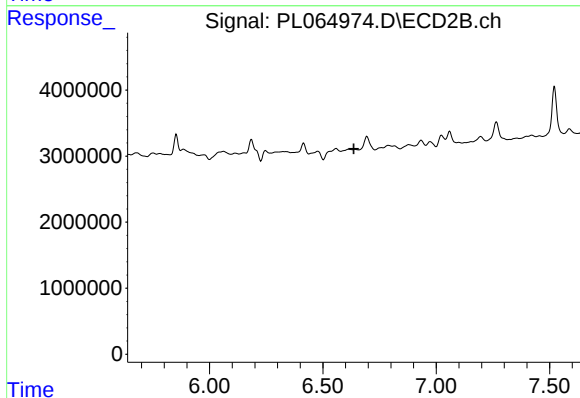


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.637 min
Response: 0
Conc: N.D.

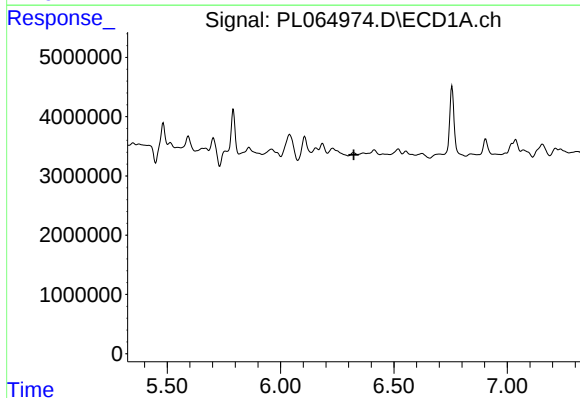


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.324 min
Response: 0
Conc: N.D.

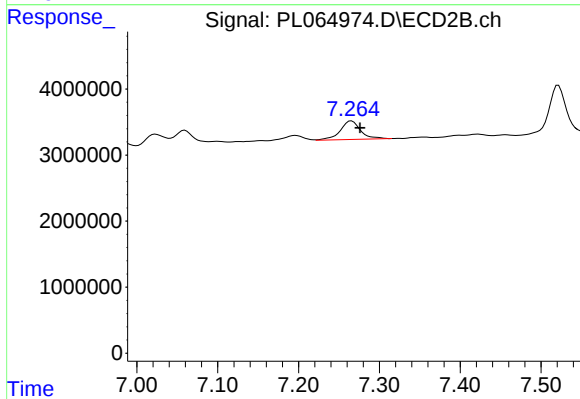

#17 4,4'-DDT


R.T.: 7.266 min
Delta R.T.: -0.011 min
Response: 4887296
Conc: 3.21 ng/ml

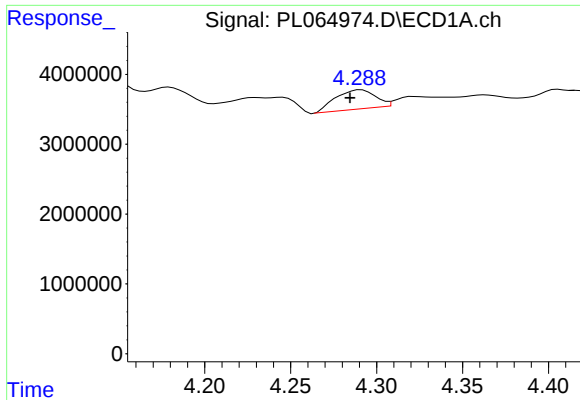

#23 Chlordane-1


R.T.: 4.291 min
Delta R.T.: 0.007 min
Response: 4402034
Conc: 38.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

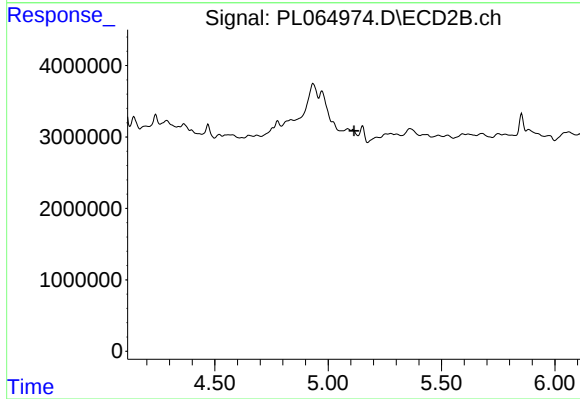


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

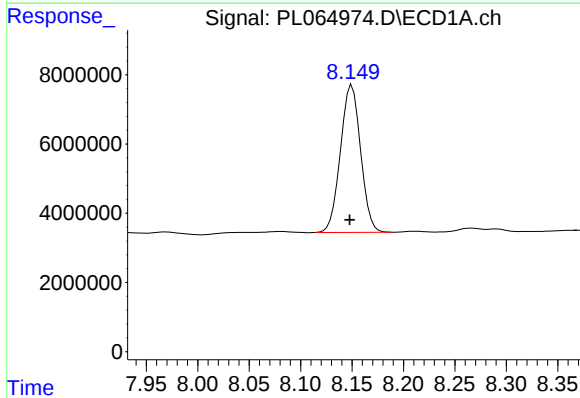

#28 Decachlorobiphenyl

R.T.: 8.150 min
Delta R.T.: 0.002 min
Response: 58155611
Conc: 25.86 ng/ml

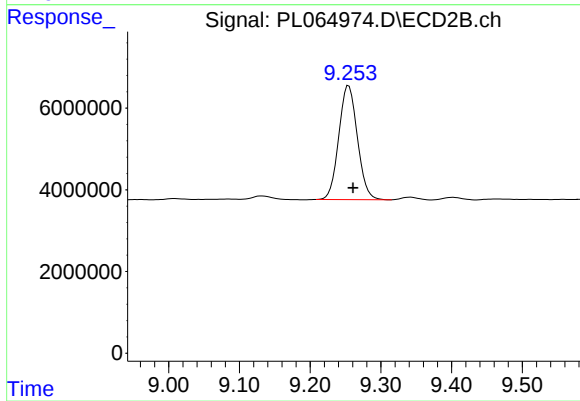

#28 Decachlorobiphenyl

R.T.: 9.254 min
Delta R.T.: -0.006 min
Response: 51048416
Conc: 26.88 ng/ml