

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022721\
 Data File : PL064975.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2021 14:13
 Operator : AR\AJ
 Sample : M1491-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 17:02:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.096	37123229	31769432	13.195	14.707
28)	SA Decachlor...	8.141	9.252	35984012	34197107	16.001	18.004
Target Compounds							
5)	MB Aldrin	4.654f	0.000	1577726	0	0.424	N.D. #
6)	B beta-BHC	0.000	4.971	0	9018748	N.D.	3.404 #
10)	B gamma-Chl...	5.364f	0.000	3939237	0	1.123	N.D. #
12)	B 4,4'-DDE	5.565	0.000	6571021	0	2.100	N.D. #
16)	A 4,4'-DDD	0.000	6.970	0	2644159	N.D.	1.525 #
17)	MA 4,4'-DDT	6.312	0.000	2972644	0	1.318	N.D. #
19)	B Endosulfa...	6.598	0.000	1595274	0	0.563	N.D. #
23)	Chlordane-1	4.292	0.000	2641699	0	23.239	N.D. #
25)	Chlordane-3	5.364f	0.000	3939237	0	11.987	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022721\
Data File : PL064975.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2021 14:13
Operator : AR\AJ
Sample : M1491-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 17:02:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

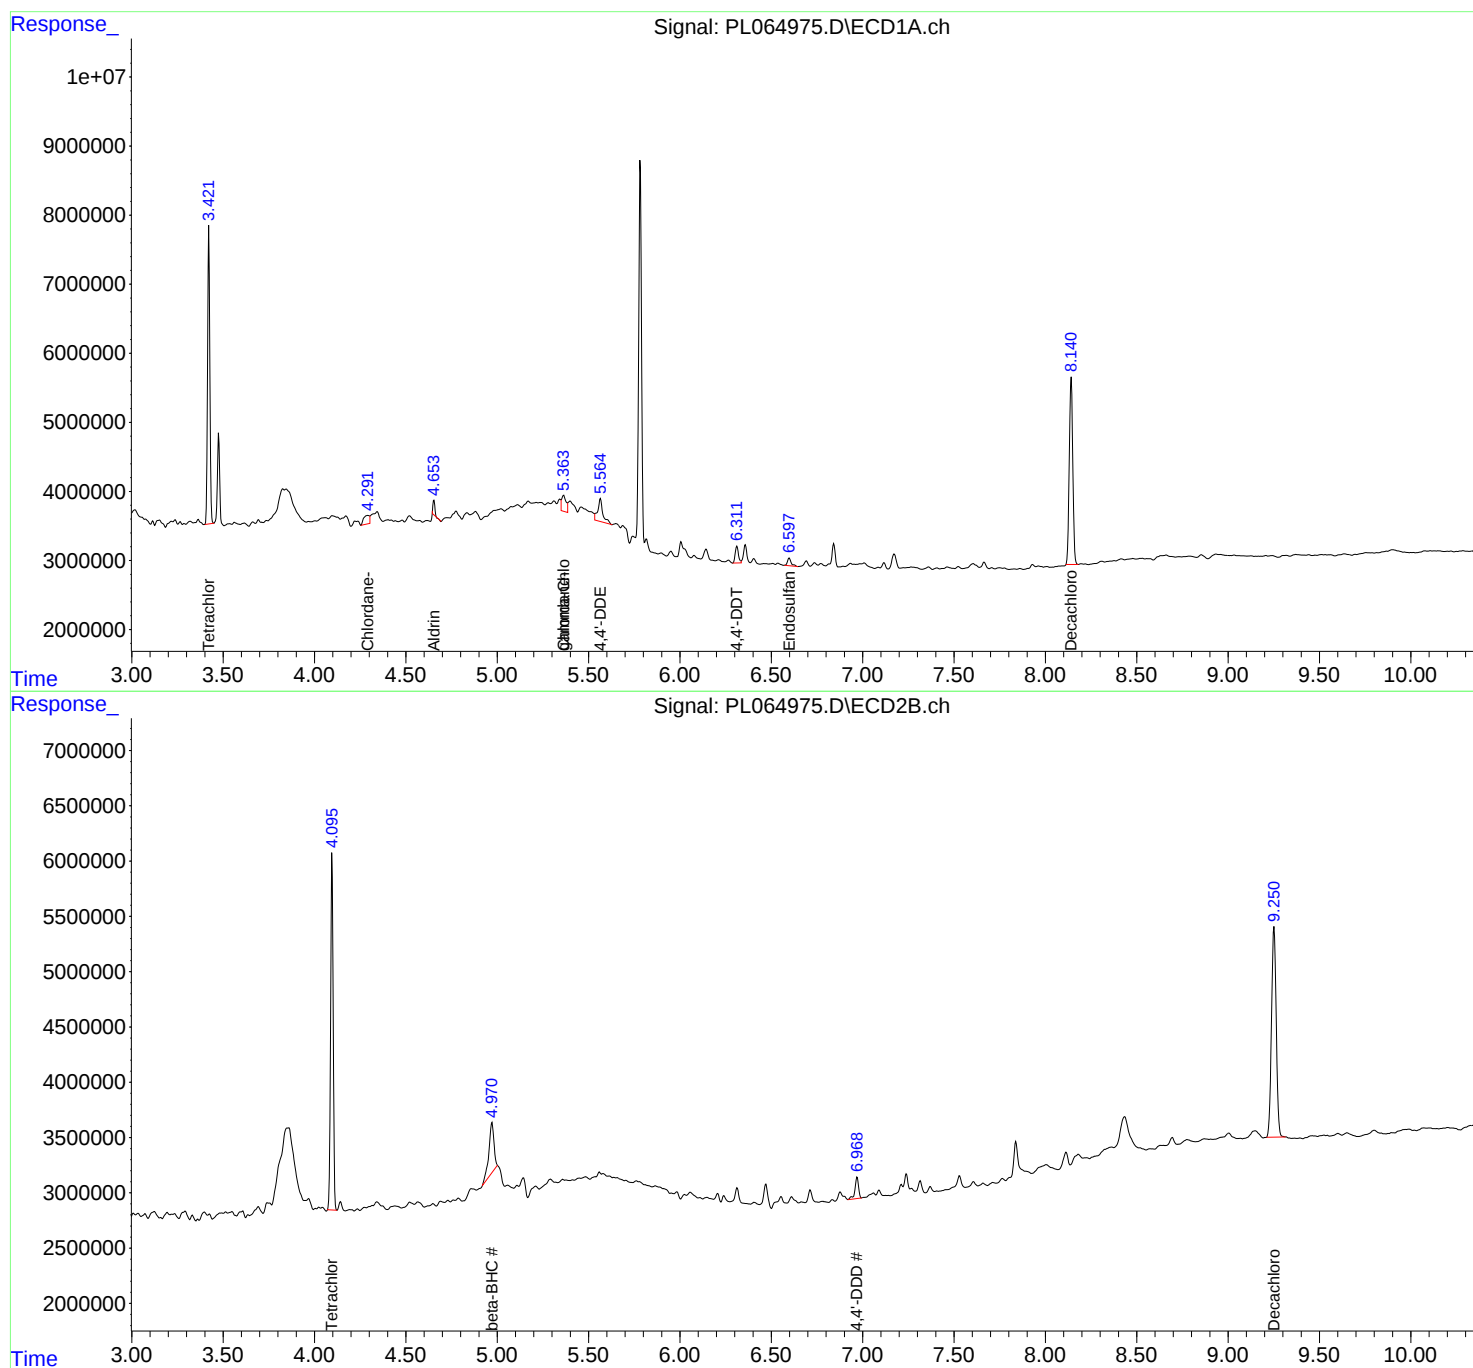


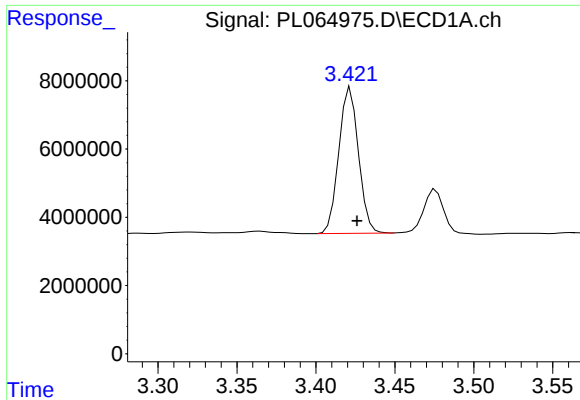

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: -0.004 min
Response: 37123229
Conc: 13.19 ng/ml

Instrument :
ECD_L
ClientSampleId :

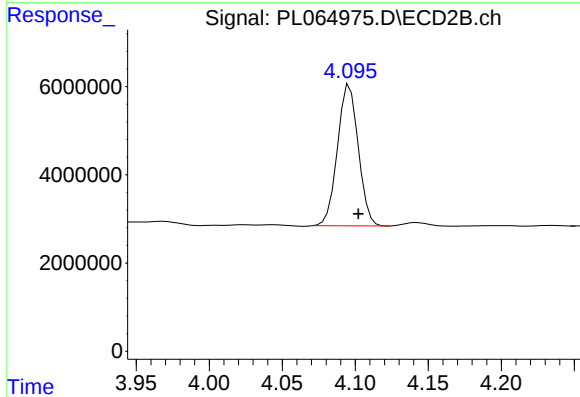


#1 Tetrachloro-m-xylene

R.T.: 4.096 min
Delta R.T.: -0.006 min
Response: 31769432
Conc: 14.71 ng/ml

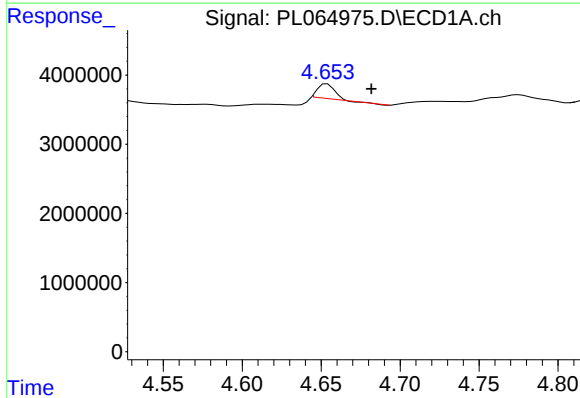


#5 Aldrin

R.T.: 4.654 min
Delta R.T.: -0.028 min
Response: 1577726
Conc: 0.42 ng/ml

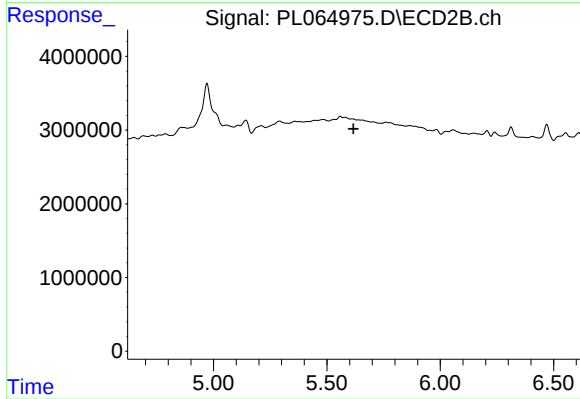

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.618 min
Response: 0
Conc: N.D.

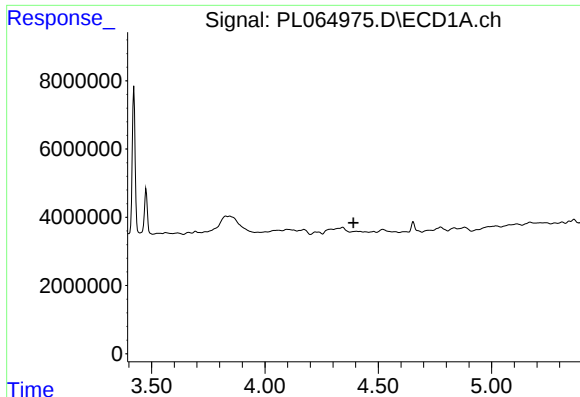

#6 beta-BHC


R.T.: 0.000 min
Exp R.T.: 4.391 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

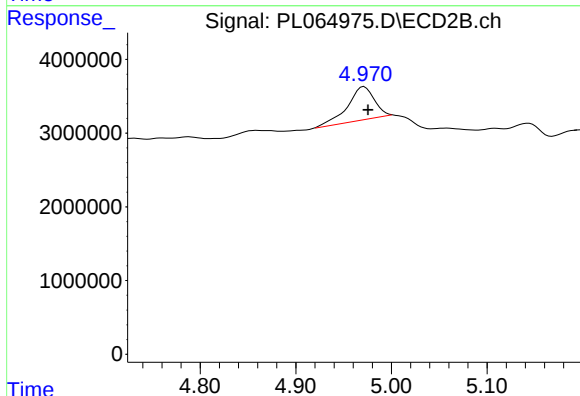


#6 beta-BHC

R.T.: 4.971 min
Delta R.T.: -0.004 min
Response: 9018748
Conc: 3.40 ng/ml

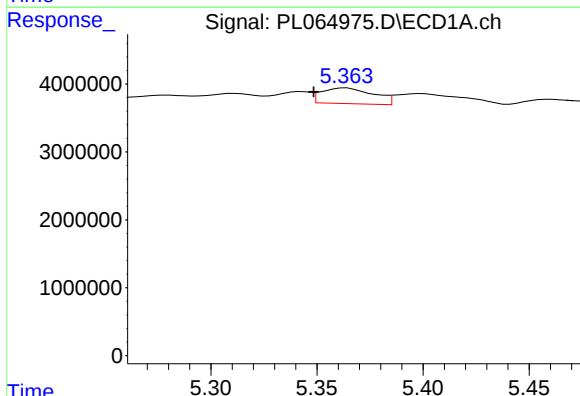


#10 gamma-Chlordane

R.T.: 5.364 min
Delta R.T.: 0.015 min
Response: 3939237
Conc: 1.12 ng/ml

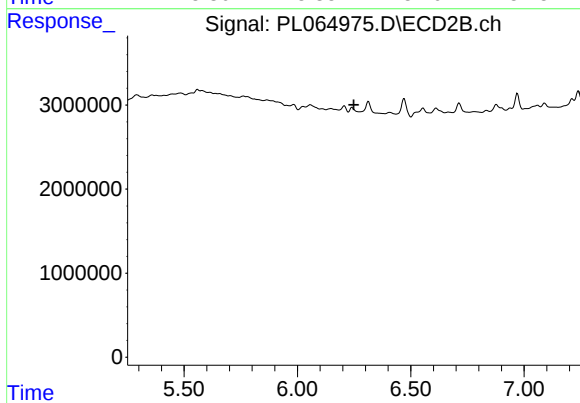

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 6.249 min
Response: 0
Conc: N.D.

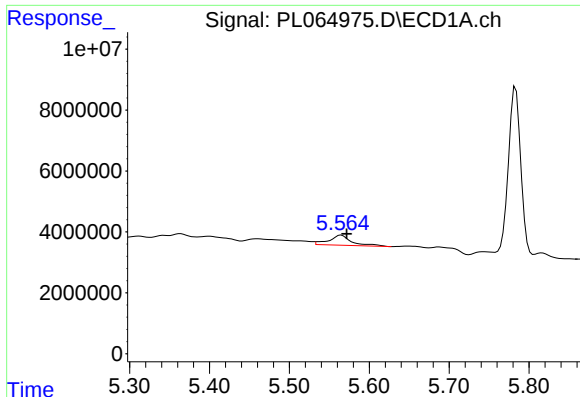

#12 4,4'-DDE


R.T.: 5.565 min
Delta R.T.: -0.007 min
Response: 6571021
Conc: 2.10 ng/ml

Instrument :
ECD_L
ClientSampleId :

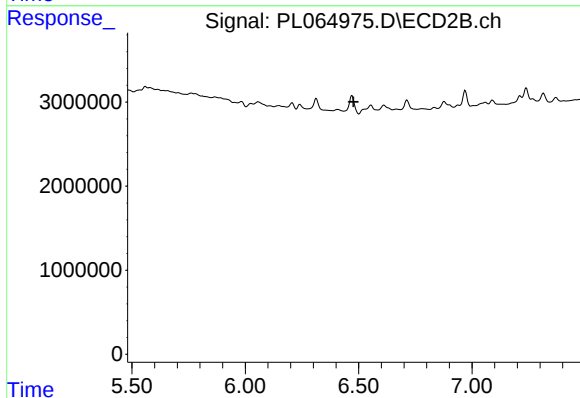


#12 4,4'-DDE

R.T.: 0.000 min
Exp R.T. : 6.478 min
Response: 0
Conc: N.D.

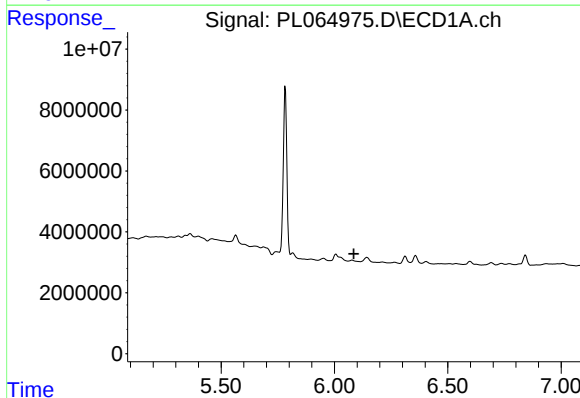


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.085 min
Response: 0
Conc: N.D.

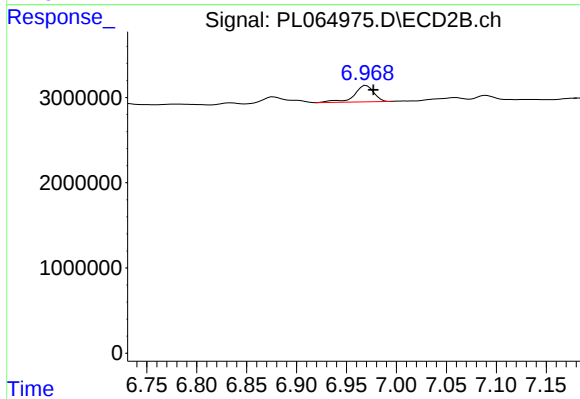

#16 4,4'-DDD


R.T.: 6.970 min
Delta R.T.: -0.007 min
Response: 2644159
Conc: 1.53 ng/ml

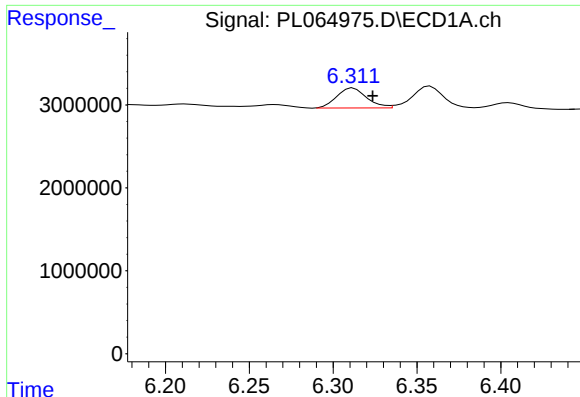

#17 4,4'-DDT


R.T.: 6.312 min
Delta R.T.: -0.012 min
Response: 2972644
Conc: 1.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

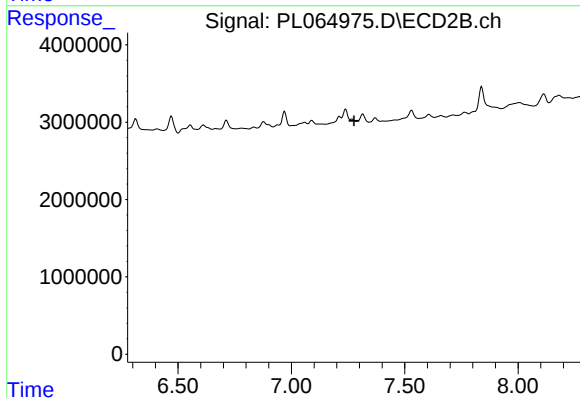


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 7.276 min
Response: 0
Conc: N.D.

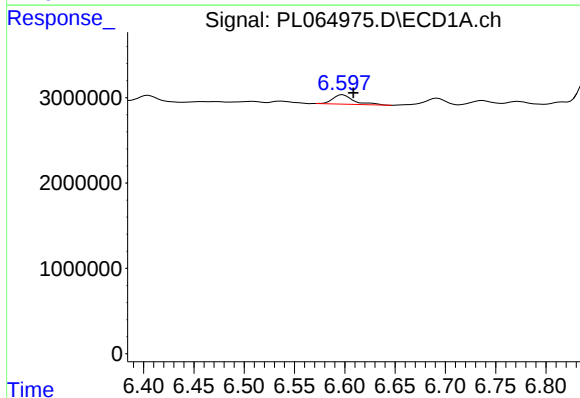


#19 Endosulfan Sulfate

R.T.: 6.598 min
Delta R.T.: -0.011 min
Response: 1595274
Conc: 0.56 ng/ml

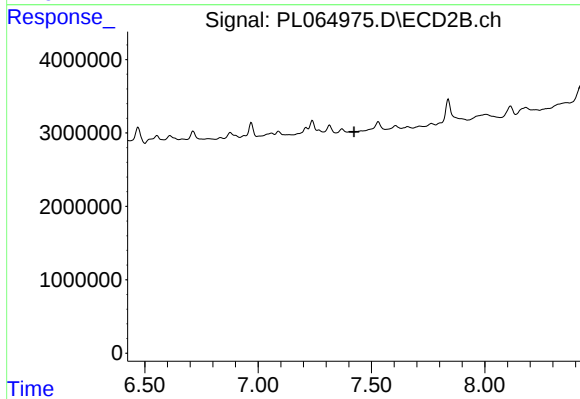

#19 Endosulfan Sulfate


R.T.: 0.000 min
Exp R.T. : 7.424 min
Response: 0
Conc: N.D.

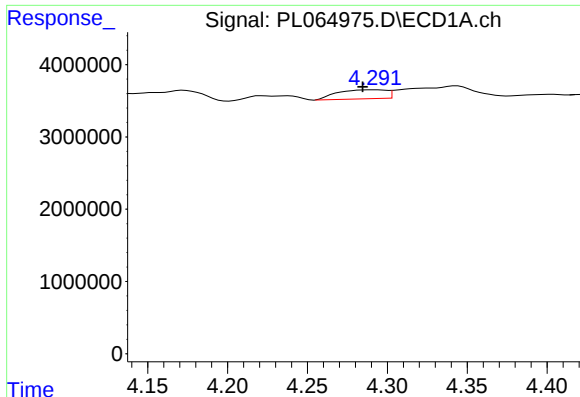

#23 Chlordane-1


R.T.: 4.292 min
Delta R.T.: 0.008 min
Response: 2641699
Conc: 23.24 ng/ml

Instrument :
ECD_L
ClientSampleId :

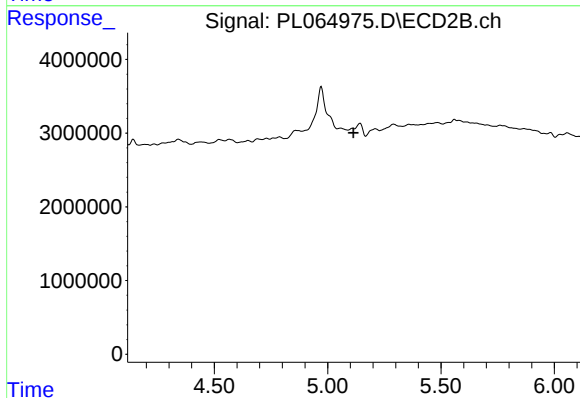


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

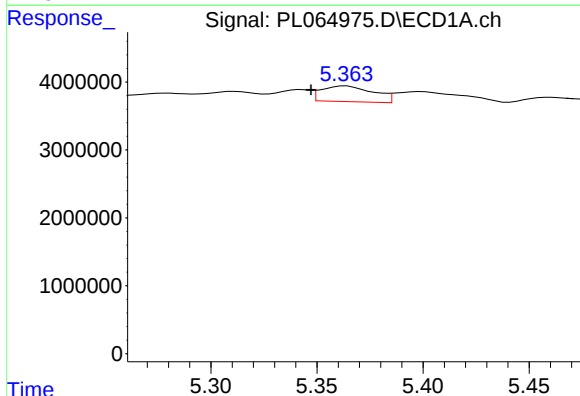


#25 Chlordane-3

R.T.: 5.364 min
Delta R.T.: 0.017 min
Response: 3939237
Conc: 11.99 ng/ml

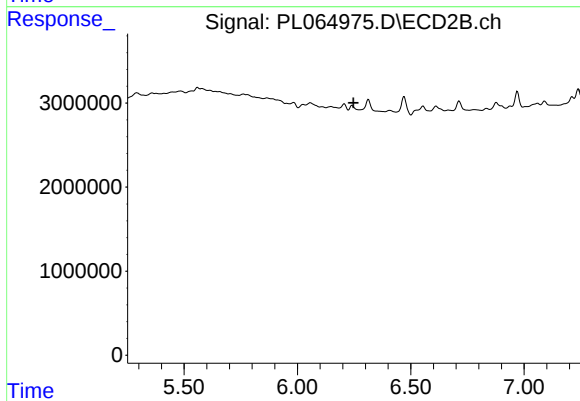

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 6.248 min
Response: 0
Conc: N.D.

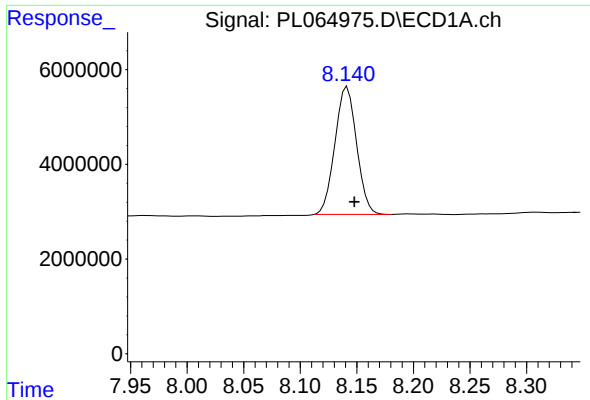

#28 Decachlorobiphenyl

R.T.: 8.141 min
Delta R.T.: -0.006 min
Response: 35984012
Conc: 16.00 ng/ml

Instrument :
ECD_L
ClientSampleId :

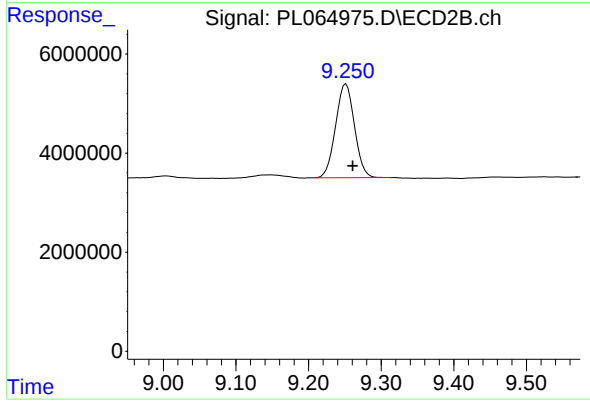

#28 Decachlorobiphenyl

R.T.: 9.252 min
Delta R.T.: -0.009 min
Response: 34197107
Conc: 18.00 ng/ml