

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022721\
 Data File : PL064984.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2021 16:21
 Operator : AR\AJ
 Sample : M1475-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 17:04:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.096	63020401	50759416	22.399	23.498
28)	SA Decachlor...	8.139	9.250	56609561	46106841	25.173	24.275
Target Compounds							
2)	A alpha-BHC	3.852	0.000	3146068	0	0.678	N.D. #
4)	MA Heptachlor	4.420f	0.000	4990707	0	1.217	N.D. #
6)	B beta-BHC	4.392	4.966	1452426	5712945	0.850	0.674
9)	A Endosulfan I	0.000	6.403f	0	3459858	N.D.	1.650 #
10)	B gamma-Chl...	0.000	6.249	0	2704498	N.D.	1.170 #
13)	MA Dieldrin	5.692	0.000	2559057	0	0.780	N.D. #
20)	A Methoxychlor	0.000	7.764f	0	6628139	N.D.	7.332 #
23)	Chlordane-1	4.288	0.000	2444720	0	21.506	N.D. #
25)	Chlordane-3	0.000	6.249	0	2704498	N.D.	8.845 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022721\
Data File : PL064984.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2021 16:21
Operator : AR\AJ
Sample : M1475-02
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 17:04:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

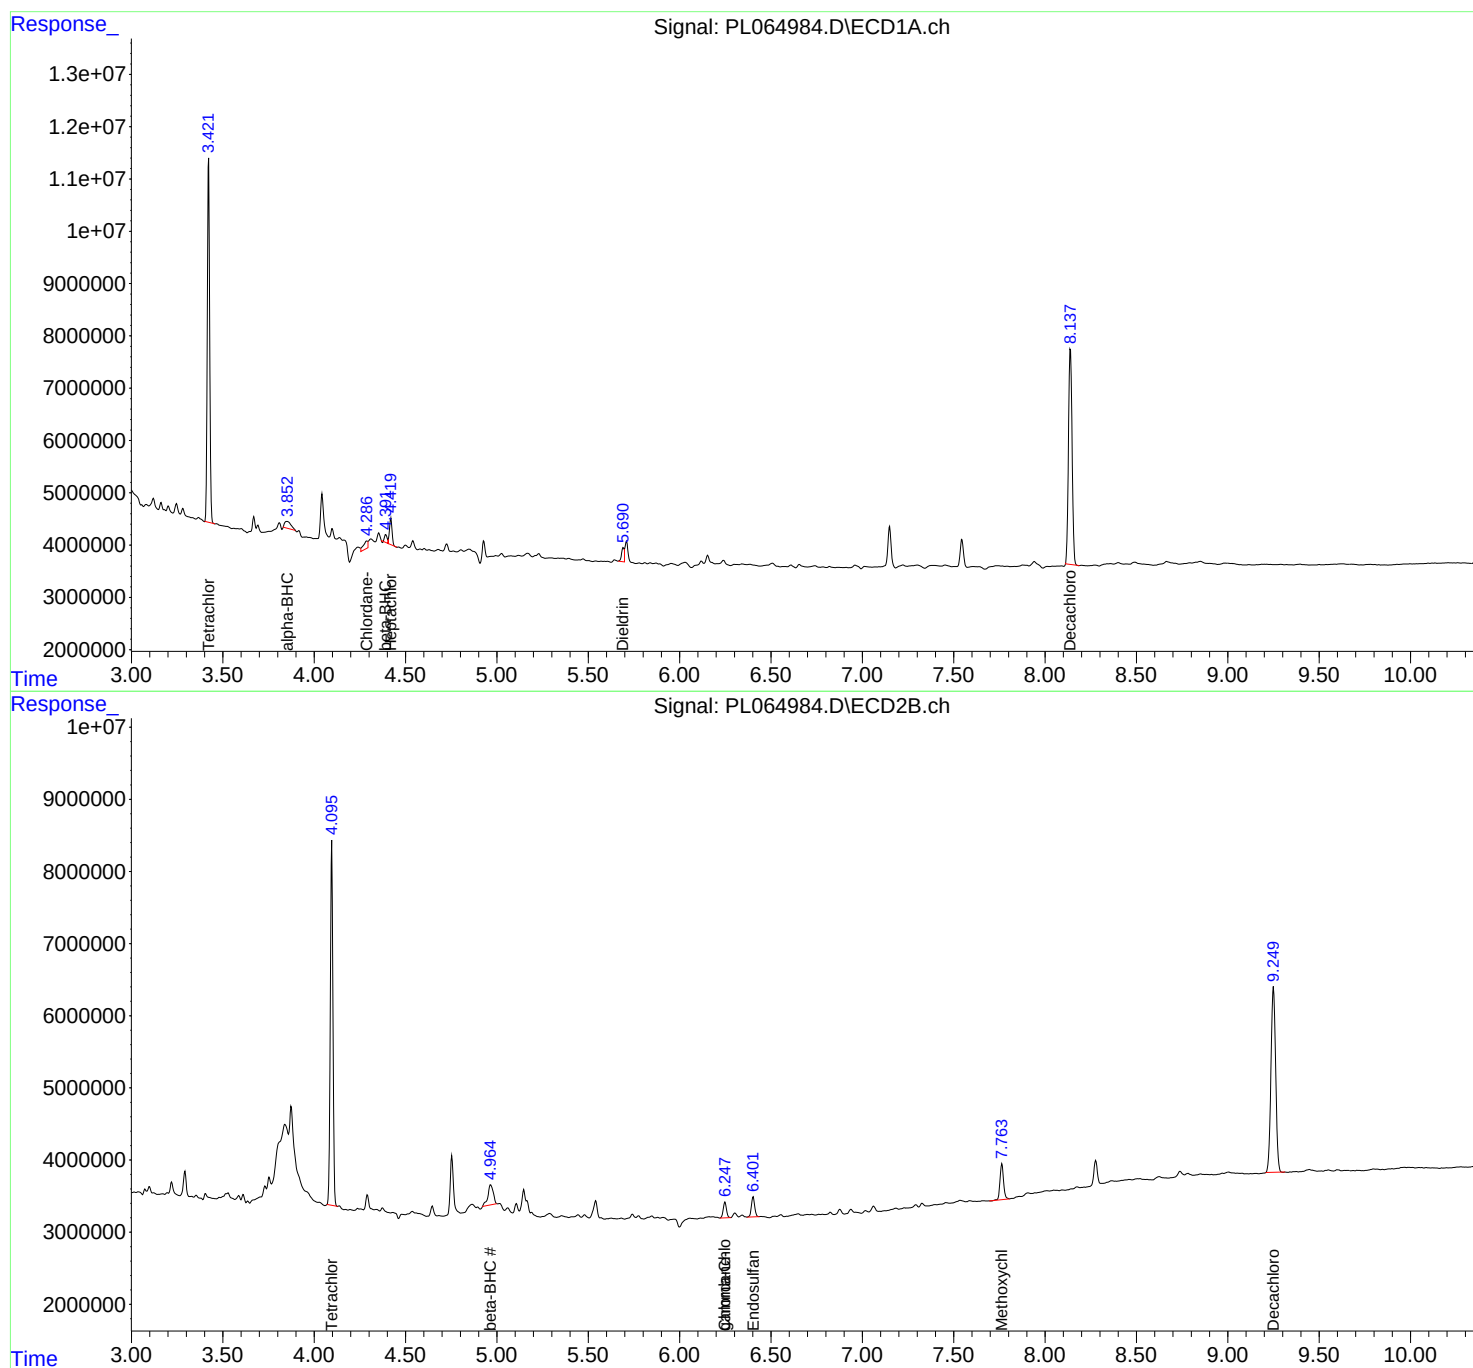


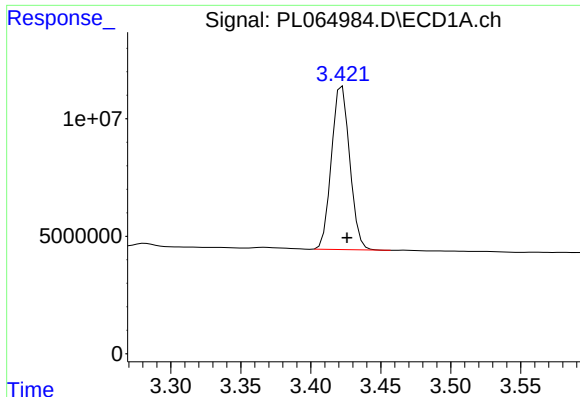

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: -0.004 min
Response: 63020401
Conc: 22.40 ng/ml

Instrument :
ECD_L
ClientSampleId :

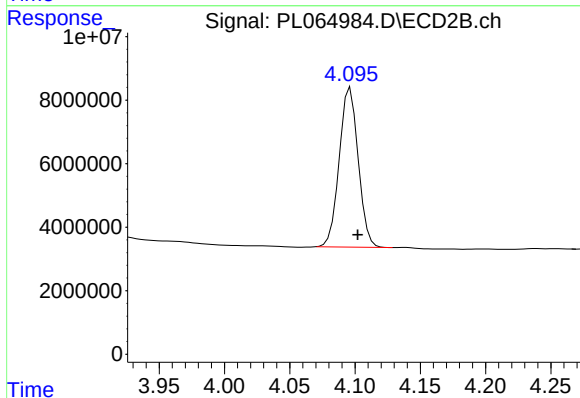


#1 Tetrachloro-m-xylene

R.T.: 4.096 min
Delta R.T.: -0.006 min
Response: 50759416
Conc: 23.50 ng/ml

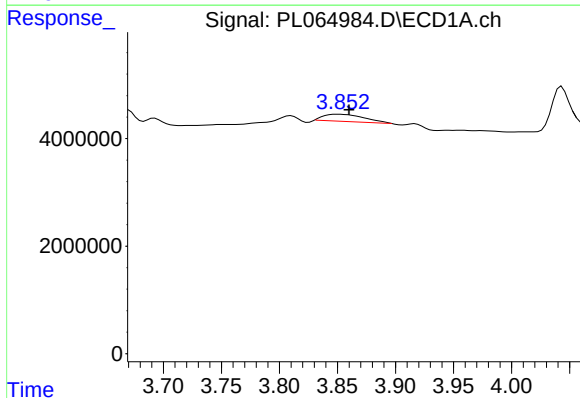


#2 alpha-BHC

R.T.: 3.852 min
Delta R.T.: -0.008 min
Response: 3146068
Conc: 0.68 ng/ml

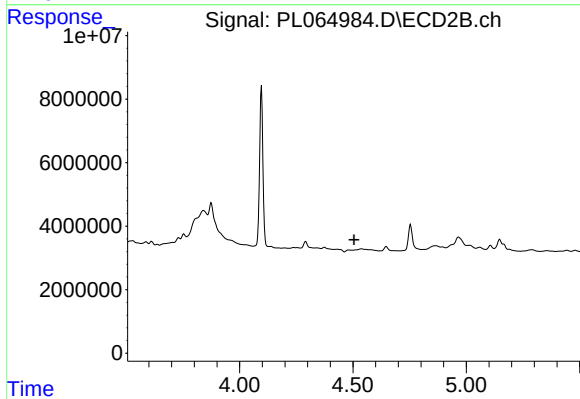

#2 alpha-BHC


R.T.: 0.000 min
Exp R.T.: 4.505 min
Response: 0
Conc: N.D.

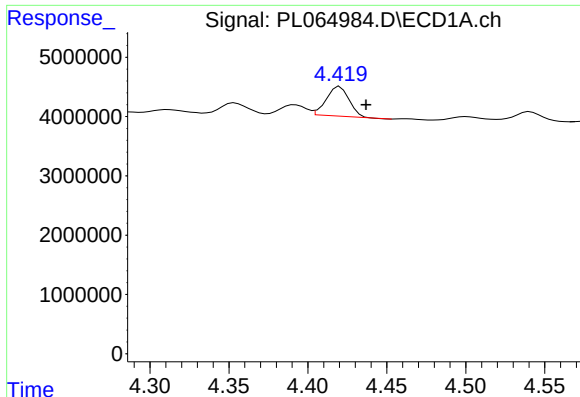

#4 Heptachlor


R.T.: 4.420 min
Delta R.T.: -0.016 min
Response: 4990707
Conc: 1.22 ng/ml

Instrument :
ECD_L
ClientSampleId :

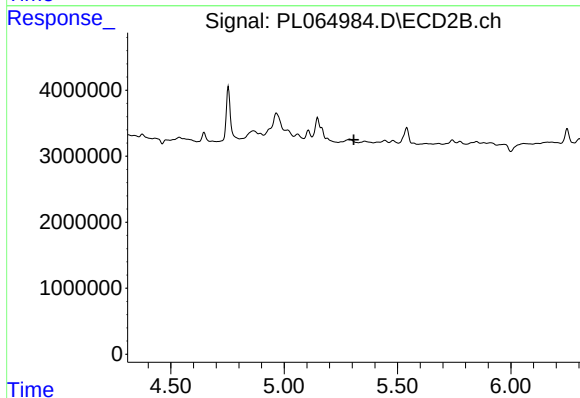


#4 Heptachlor

R.T.: 0.000 min
Exp R.T. : 5.307 min
Response: 0
Conc: N.D.

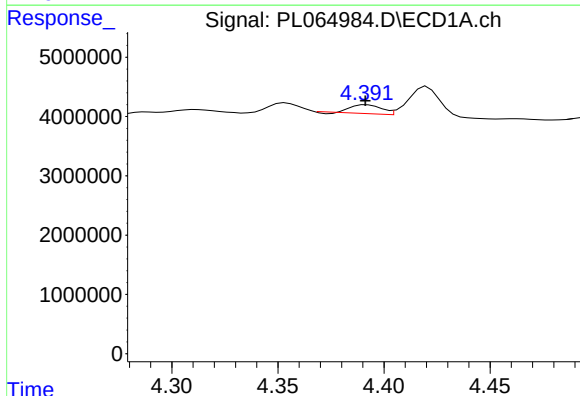


#6 beta-BHC

R.T.: 4.392 min
Delta R.T.: 0.000 min
Response: 1452426
Conc: 0.85 ng/ml

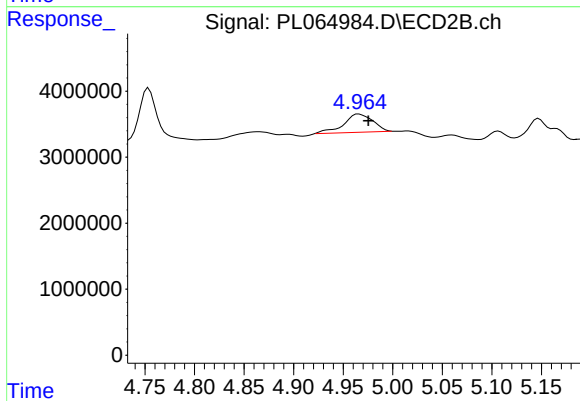

#6 beta-BHC


R.T.: 4.966 min
Delta R.T.: -0.010 min
Response: 5712945
Conc: 0.67 ng/ml

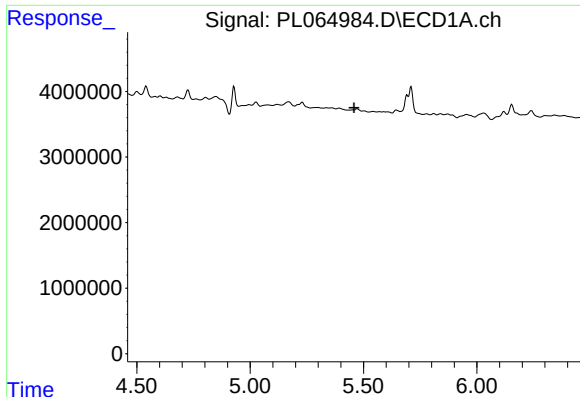

#9 Endosulfan I


R.T.: 0.000 min
Exp R.T.: 5.459 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

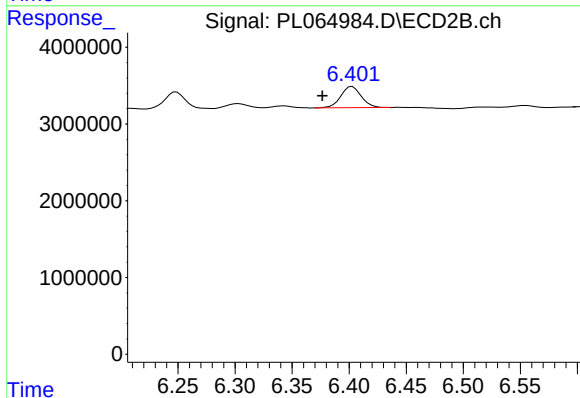


#9 Endosulfan I

R.T.: 6.403 min
Delta R.T.: 0.026 min
Response: 3459858
Conc: 1.65 ng/ml

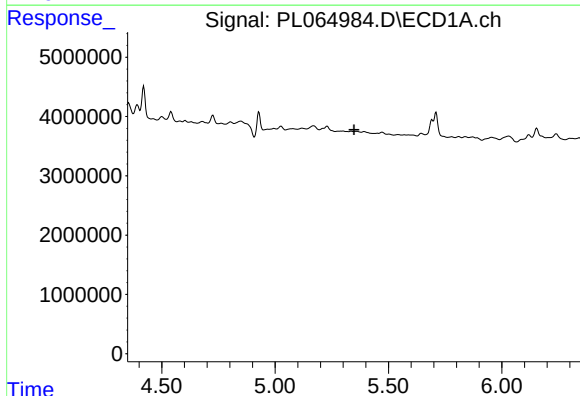


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T.: 5.349 min
Response: 0
Conc: N.D.

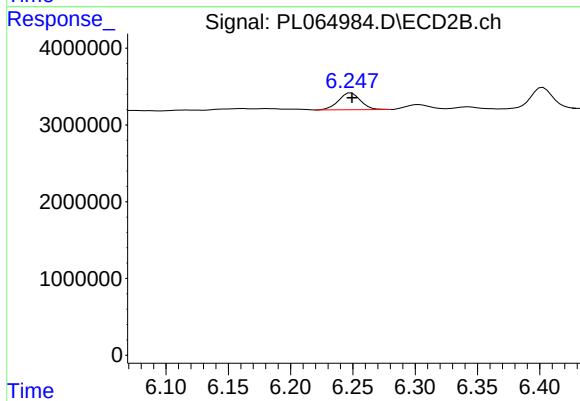

#10 gamma-Chlordane


R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 2704498
Conc: 1.17 ng/ml

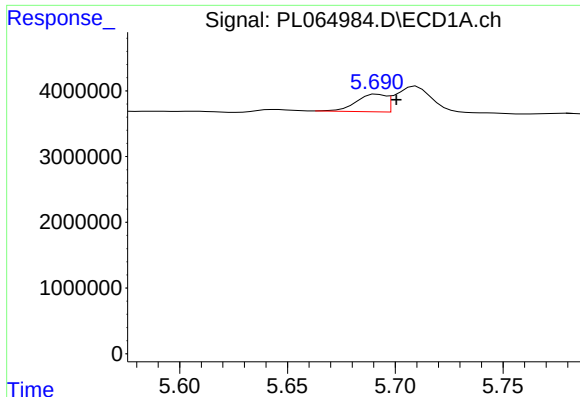

#13 Dieldrin


R.T.: 5.692 min
Delta R.T.: -0.009 min
Response: 2559057
Conc: 0.78 ng/ml

Instrument :
ECD_L
ClientSampleId :

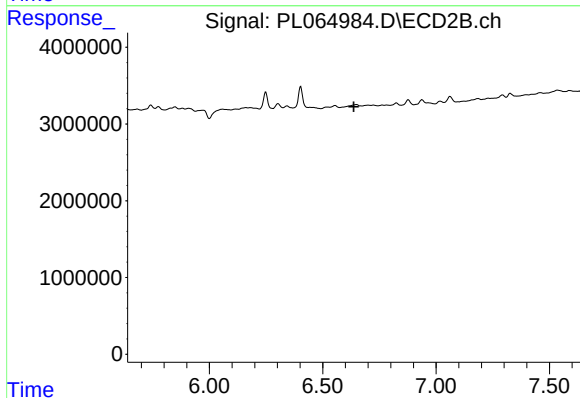


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 6.637 min
Response: 0
Conc: N.D.

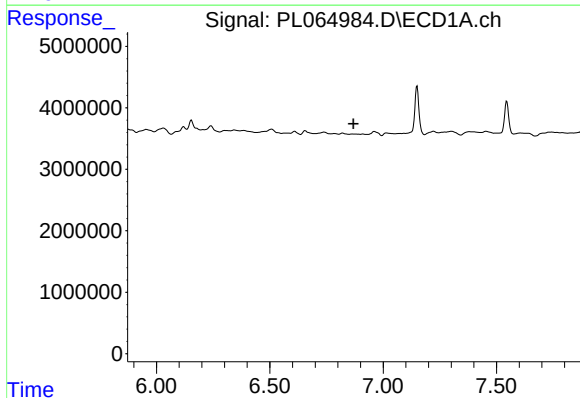


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 6.869 min
Response: 0
Conc: N.D.

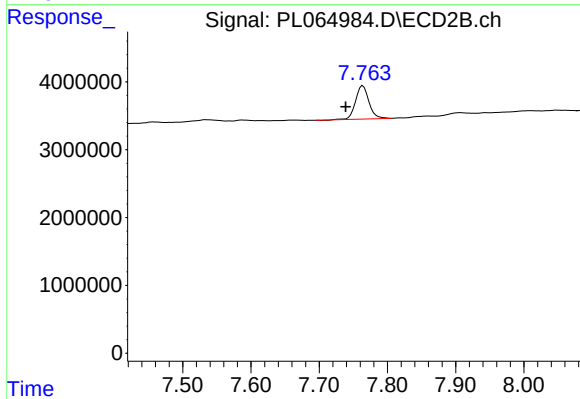

#20 Methoxychlor


R.T.: 7.764 min
Delta R.T.: 0.025 min
Response: 6628139
Conc: 7.33 ng/ml

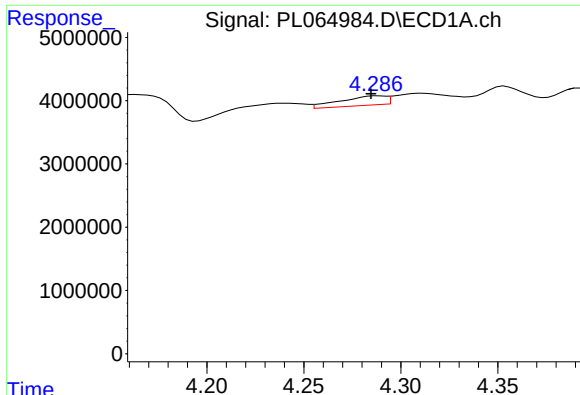

#23 Chlordane-1


R.T.: 4.288 min
Delta R.T.: 0.004 min
Response: 2444720
Conc: 21.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

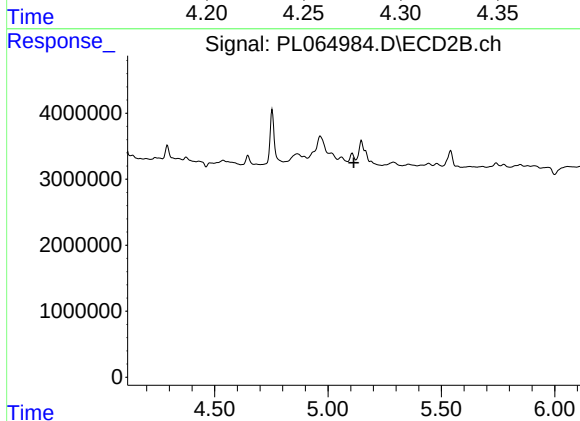


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

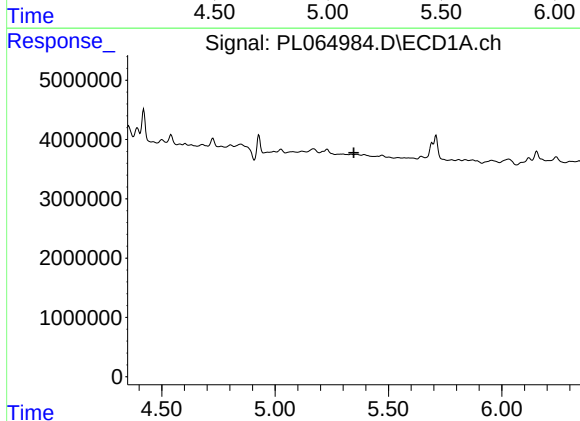


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.347 min
Response: 0
Conc: N.D.

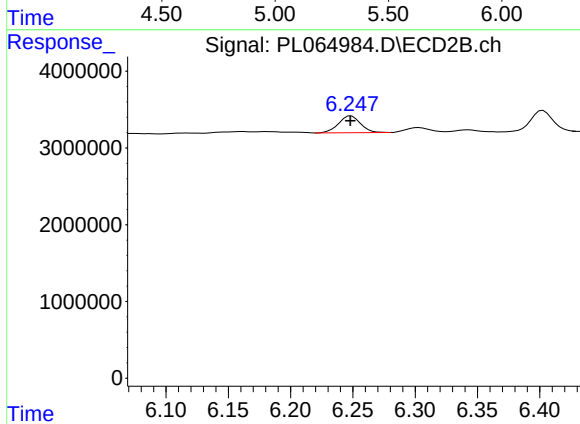

#25 Chlordane-3


R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 2704498
Conc: 8.85 ng/ml

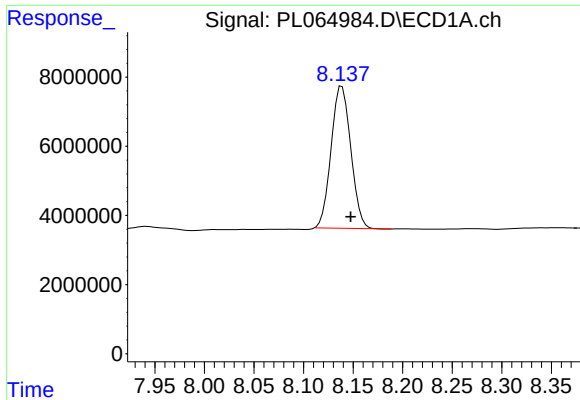

#28 Decachlorobiphenyl

R.T.: 8.139 min
Delta R.T.: -0.009 min
Response: 56609561
Conc: 25.17 ng/ml

Instrument :
ECD_L
ClientSampleId :

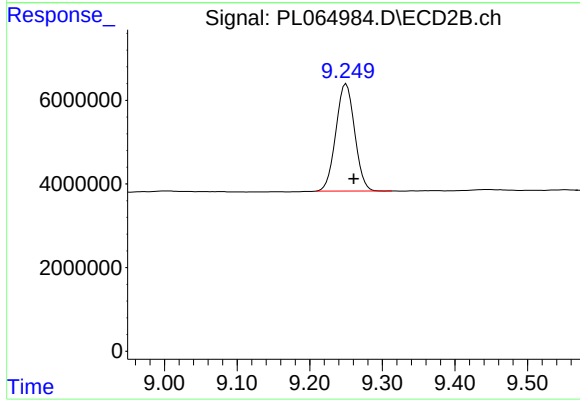

#28 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.010 min
Response: 46106841
Conc: 24.27 ng/ml