

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022721\
 Data File : PL064987.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2021 17:04
 Operator : AR\AJ
 Sample : M1476-02
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 17:25:53 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.097	55487390	48841669	19.722	22.610
28)	SA Decachlor...	8.140	9.250	56989392	48407686	25.342	25.486
Target Compounds							
6)	B beta-BHC	0.000	4.970	0	5079492	N.D.	0.151 #
10)	B gamma-Chl...	0.000	6.249	0	7645097	N.D.	3.308 #
13)	MA Dieldrin	5.691	0.000	9799298	0	2.987	N.D. #
20)	A Methoxychlor	0.000	7.764f	0	7051700	N.D.	7.801 #
25)	Chlordane-3	0.000	6.249	0	7645097	N.D.	25.004 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022721\
Data File : PL064987.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2021 17:04
Operator : AR\AJ
Sample : M1476-02
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 17:25:53 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

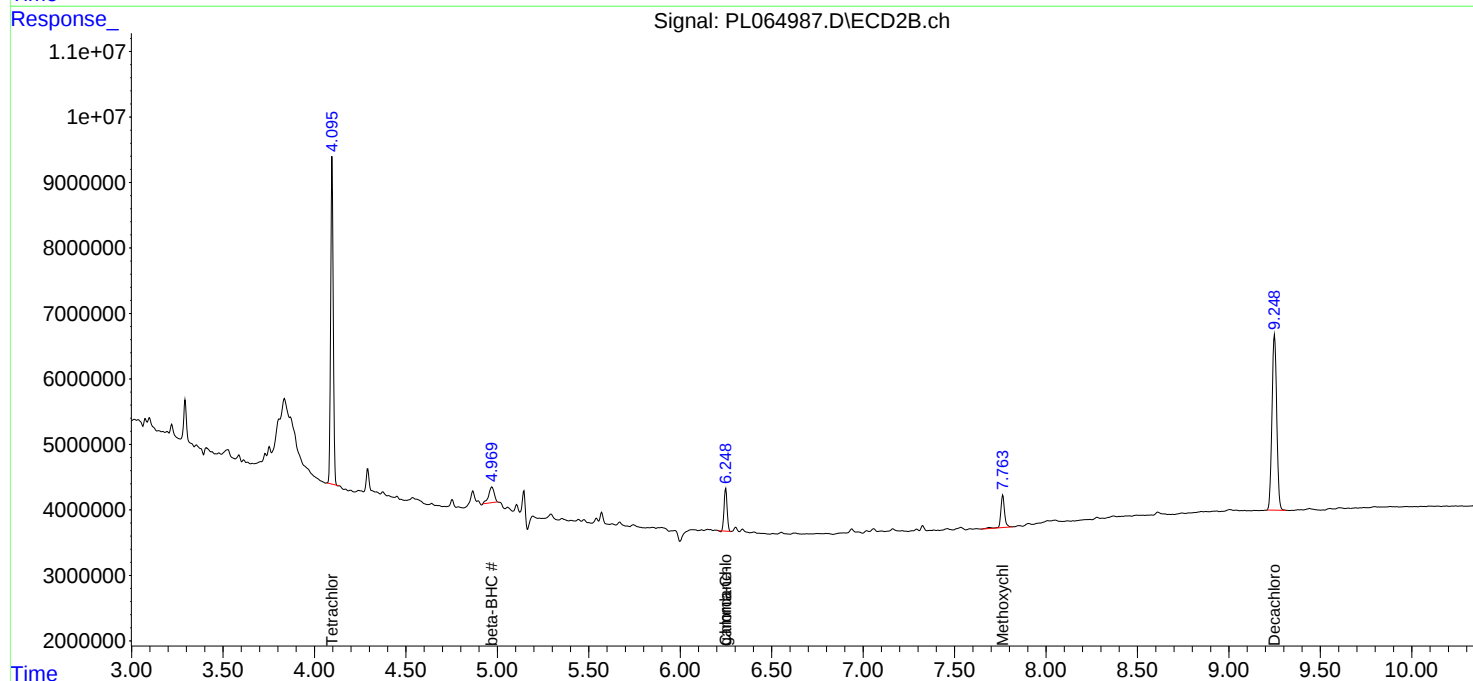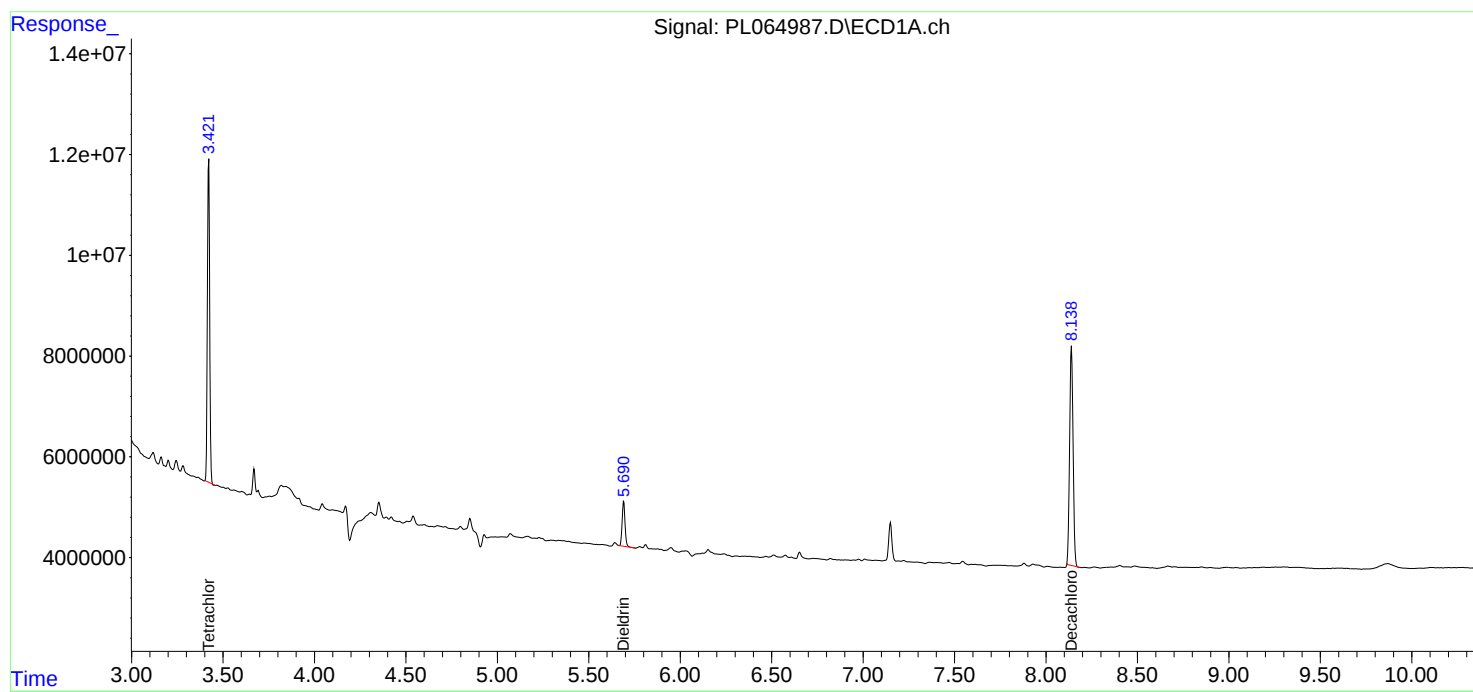


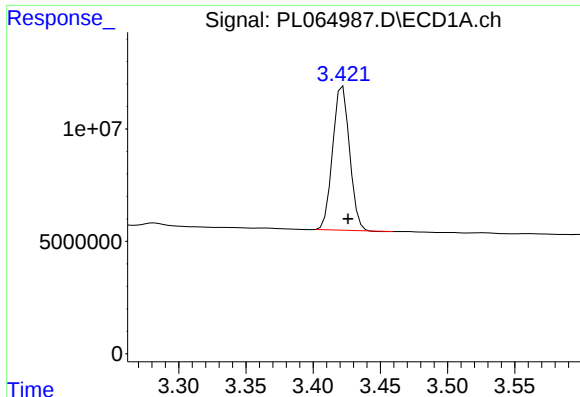

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: -0.004 min
Response: 55487390
Conc: 19.72 ng/ml

Instrument :
ECD_L
ClientSampleId :

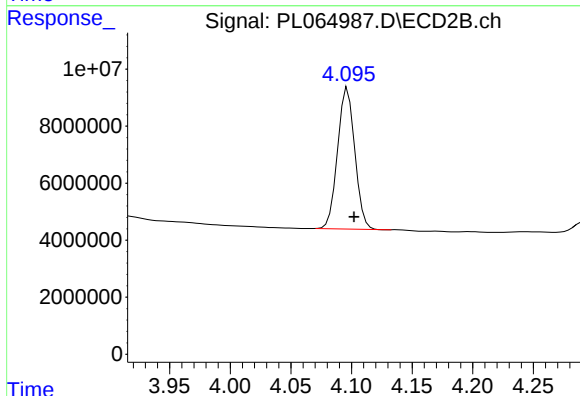


#1 Tetrachloro-m-xylene

R.T.: 4.097 min
Delta R.T.: -0.005 min
Response: 48841669
Conc: 22.61 ng/ml

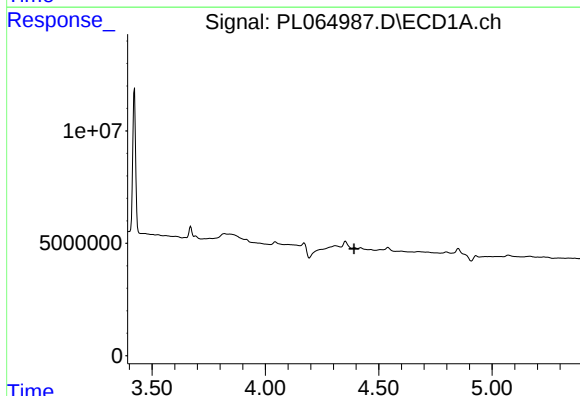


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.391 min
Response: 0
Conc: N.D.

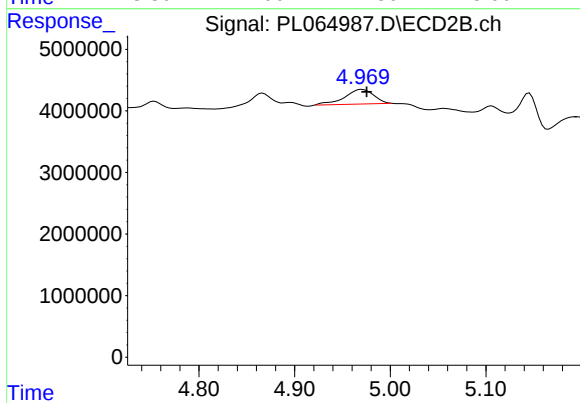

#6 beta-BHC


R.T.: 4.970 min
Delta R.T.: -0.005 min
Response: 5079492
Conc: 0.15 ng/ml

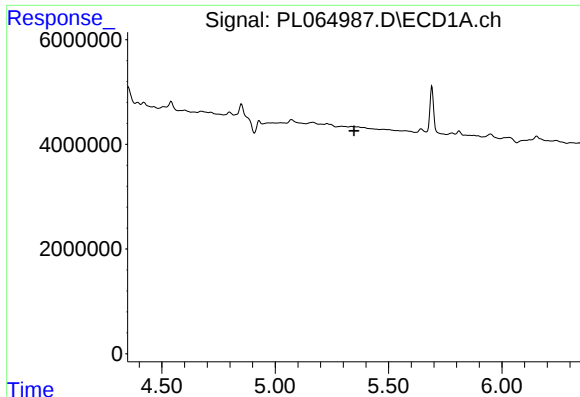

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T.: 5.349 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

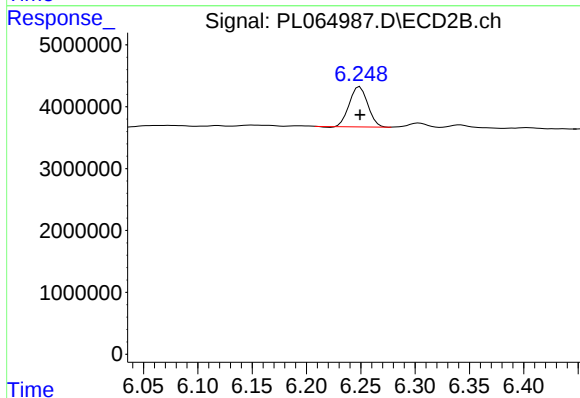


#10 gamma-Chlordane

R.T.: 6.249 min
Delta R.T.: 0.000 min
Response: 7645097
Conc: 3.31 ng/ml

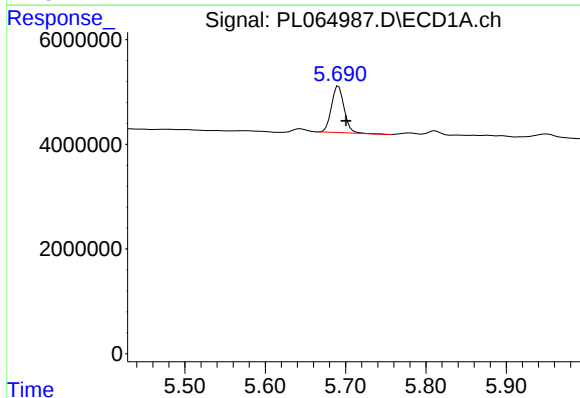


#13 Dieldrin

R.T.: 5.691 min
Delta R.T.: -0.009 min
Response: 9799298
Conc: 2.99 ng/ml

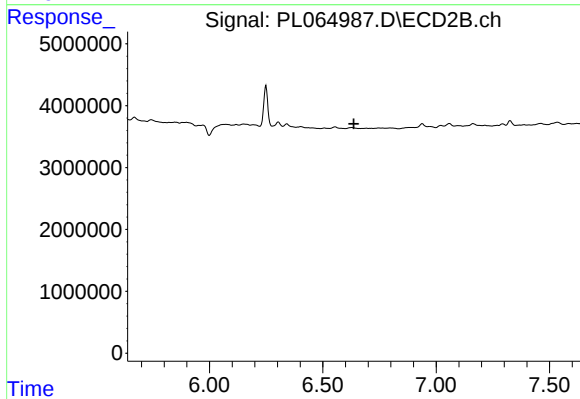

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 6.637 min
Response: 0
Conc: N.D.

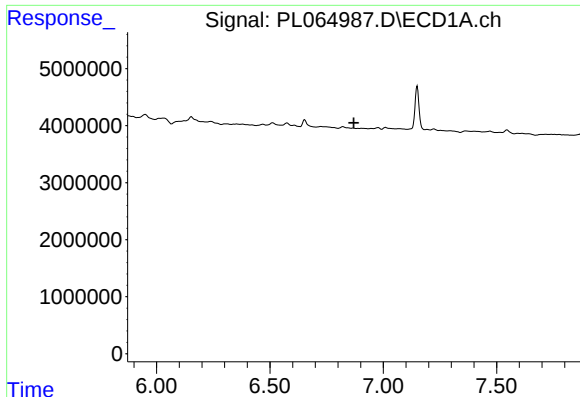

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T.: 6.869 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

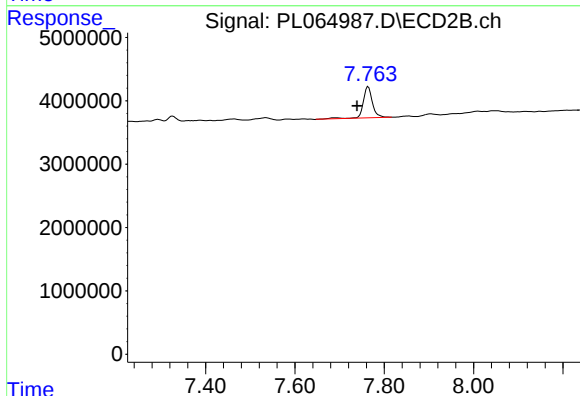


#20 Methoxychlor

R.T.: 7.764 min
Delta R.T.: 0.025 min
Response: 7051700
Conc: 7.80 ng/ml

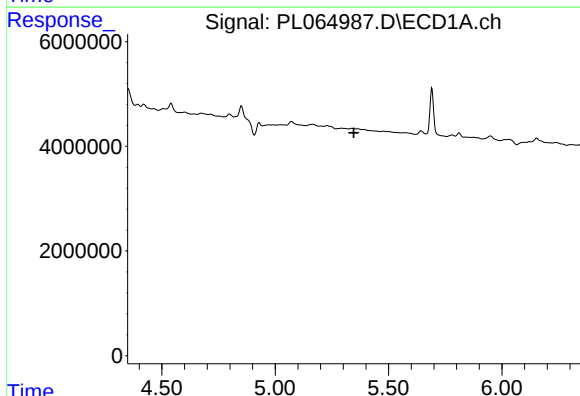


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T.: 5.347 min
Response: 0
Conc: N.D.

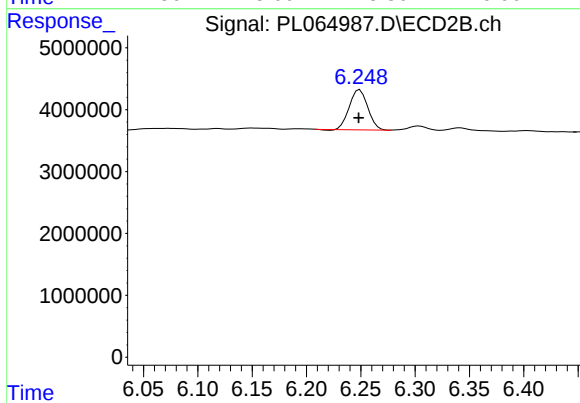

#25 Chlordane-3


R.T.: 6.249 min
Delta R.T.: 0.001 min
Response: 7645097
Conc: 25.00 ng/ml

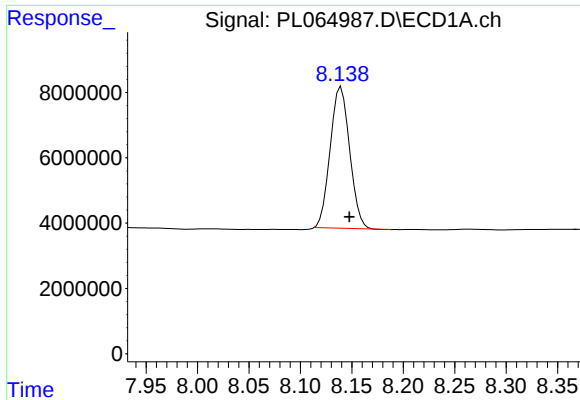

#28 Decachlorobiphenyl

R.T.: 8.140 min
Delta R.T.: -0.008 min
Response: 56989392
Conc: 25.34 ng/ml

Instrument :
ECD_L
ClientSampleId :

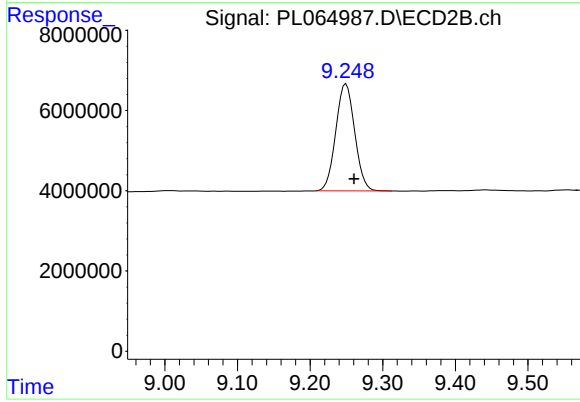

#28 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.011 min
Response: 48407686
Conc: 25.49 ng/ml