

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022721\
 Data File : PL064988.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2021 17:18
 Operator : AR\AJ
 Sample : M1503-05
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 17:58:15 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.097	54223018	49250366	19.272	22.799
28)	SA Decachlor...	8.139	9.251	54431183	47766468	24.205	25.148
Target Compounds							
10)	B gamma-Chl...	0.000	6.245	0	1277960	N.D.	0.553 #
16)	A 4,4'-DDD	6.096	0.000	2345961	0	0.926	N.D. #
17)	MA 4,4'-DDT	0.000	7.263	0	4119765	N.D.	2.702 #
23)	Chlordane-1	4.284	0.000	1742044	0	15.325	N.D. #
25)	Chlordane-3	0.000	6.245	0	1277960	N.D.	4.180 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022721\
Data File : PL064988.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2021 17:18
Operator : AR\AJ
Sample : M1503-05
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 17:58:15 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

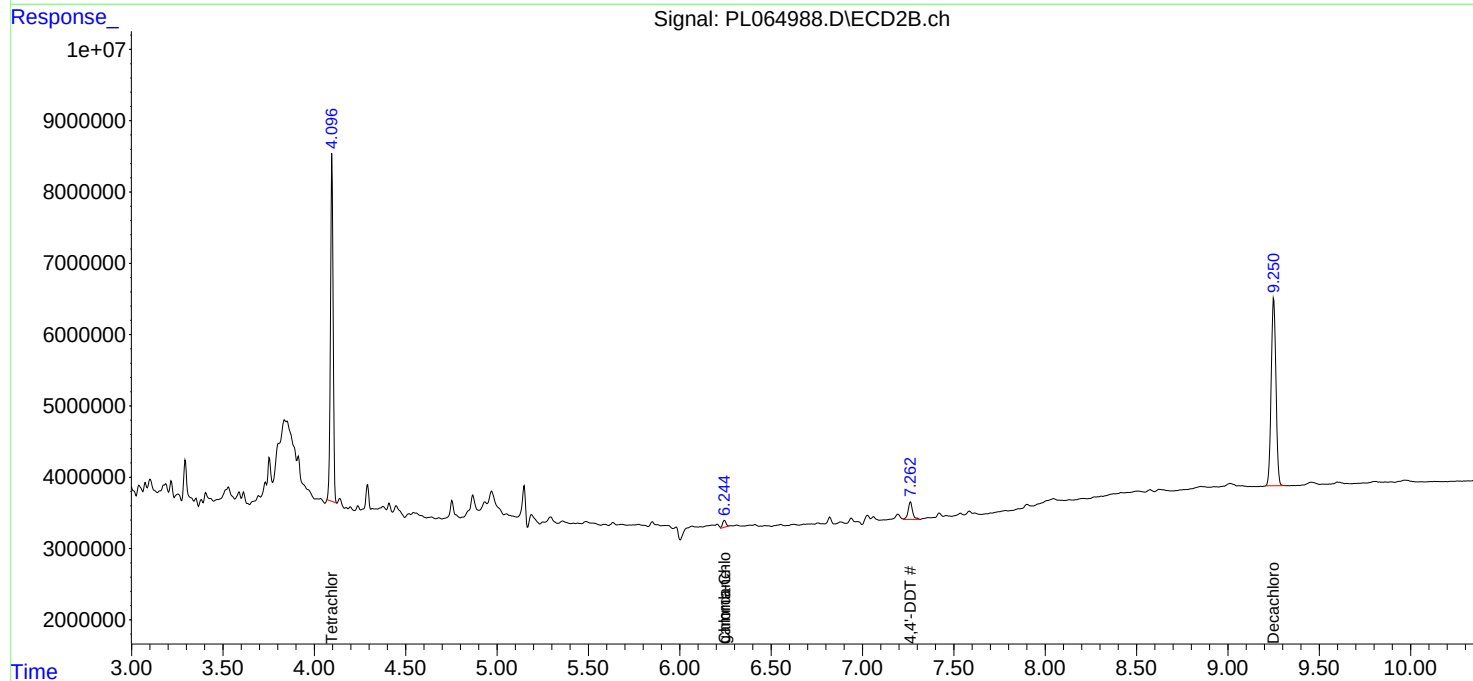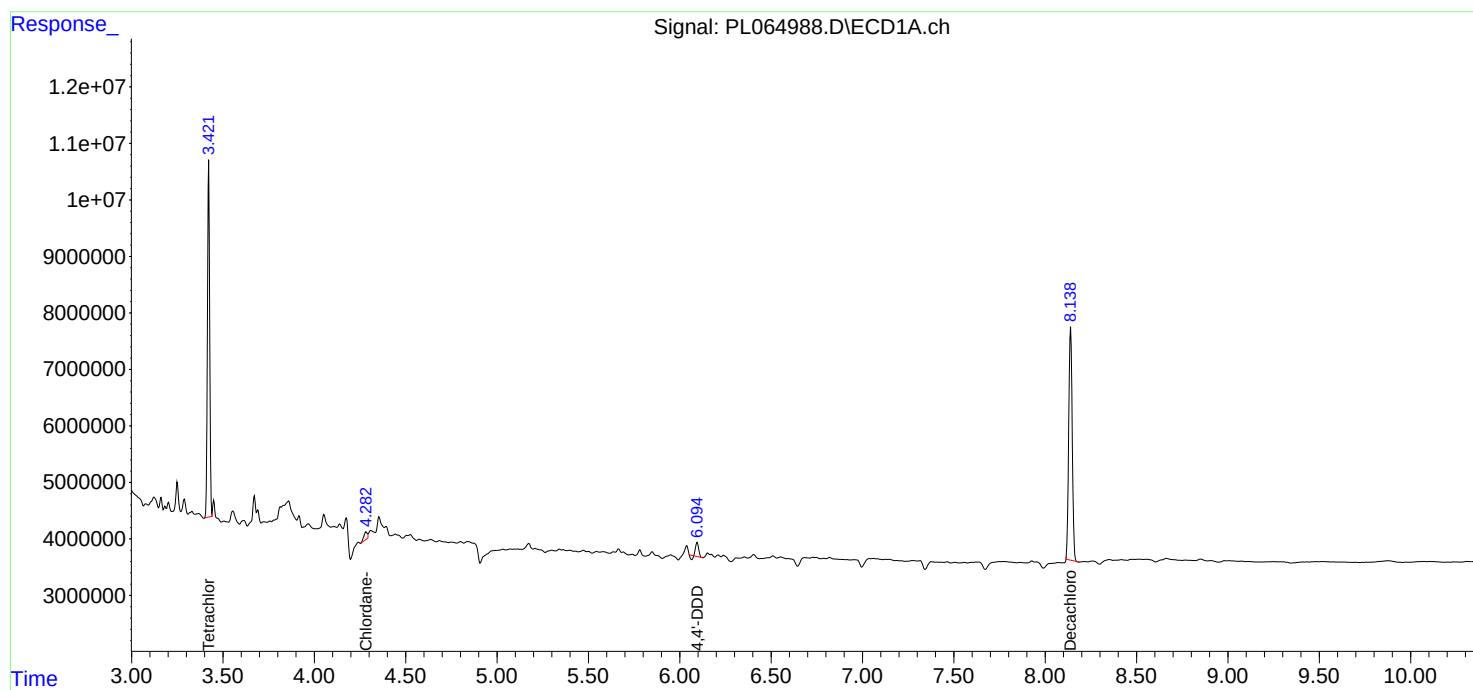


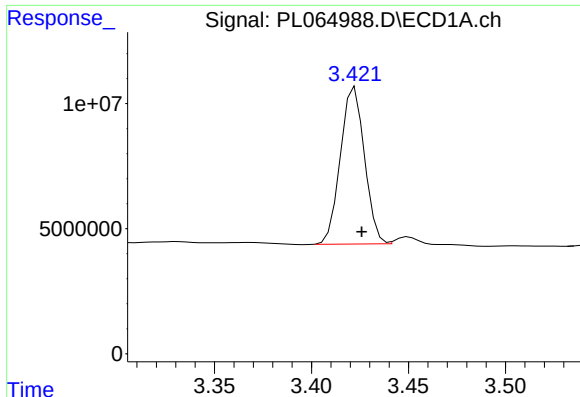

#1 Tetrachloro-m-xylene


R.T.: 3.422 min
Delta R.T.: -0.004 min
Response: 54223018
Conc: 19.27 ng/ml

Instrument :
ECD_L
ClientSampleId :

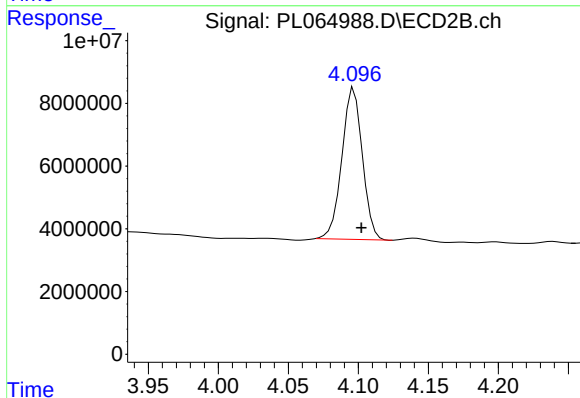


#1 Tetrachloro-m-xylene

R.T.: 4.097 min
Delta R.T.: -0.005 min
Response: 49250366
Conc: 22.80 ng/ml

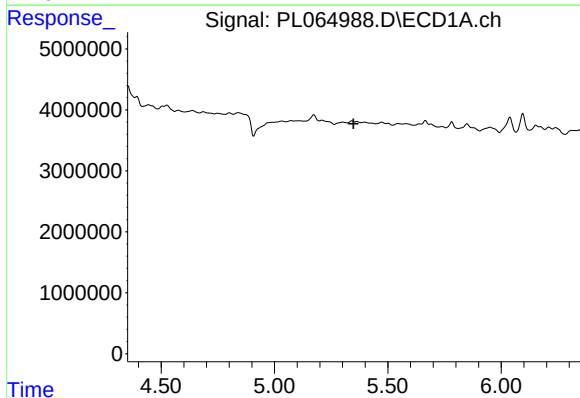


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.349 min
Response: 0
Conc: N.D.

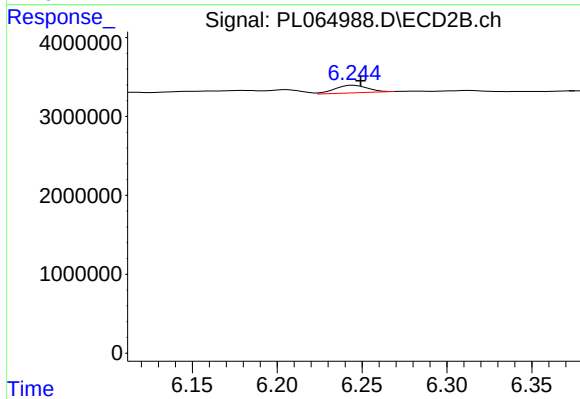

#10 gamma-Chlordane


R.T.: 6.245 min
Delta R.T.: -0.004 min
Response: 1277960
Conc: 0.55 ng/ml

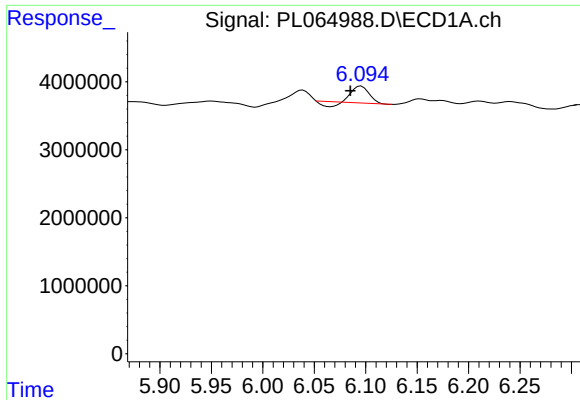

#16 4,4'-DDD


R.T.: 6.096 min
Delta R.T.: 0.010 min
Response: 2345961
Conc: 0.93 ng/ml

Instrument :
ECD_L
ClientSampleId :

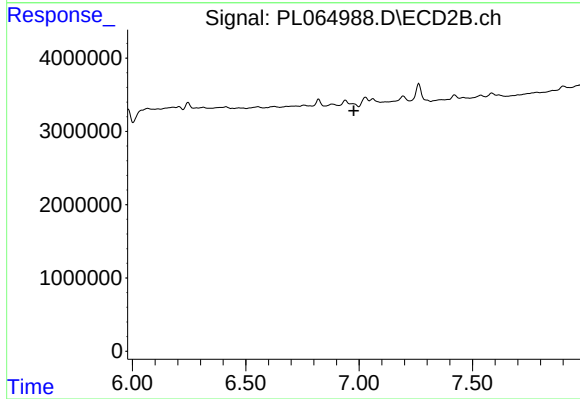


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.977 min
Response: 0
Conc: N.D.

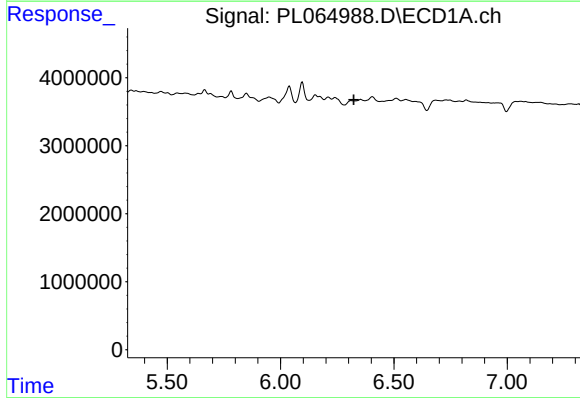


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.324 min
Response: 0
Conc: N.D.

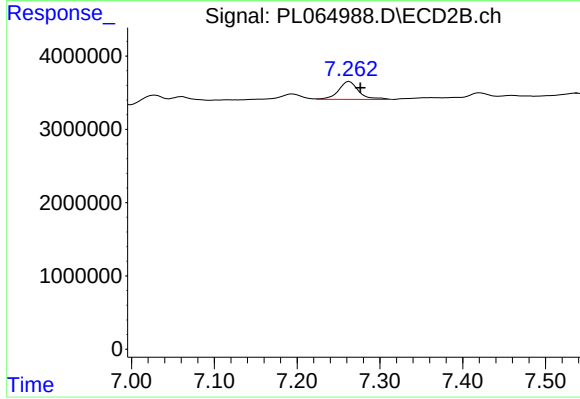

#17 4,4'-DDT


R.T.: 7.263 min
Delta R.T.: -0.013 min
Response: 4119765
Conc: 2.70 ng/ml

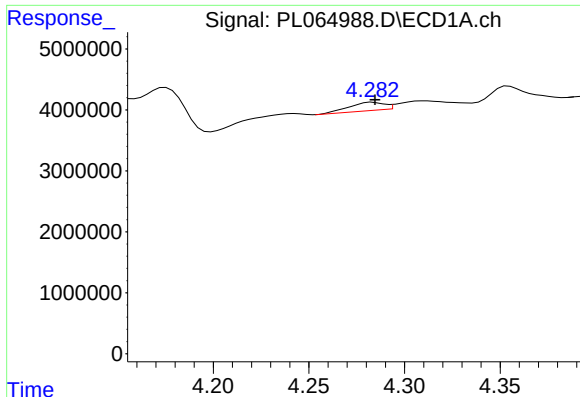

#23 Chlordane-1


R.T.: 4.284 min
Delta R.T.: -0.001 min
Response: 1742044
Conc: 15.32 ng/ml

Instrument :
ECD_L
ClientSampleId :

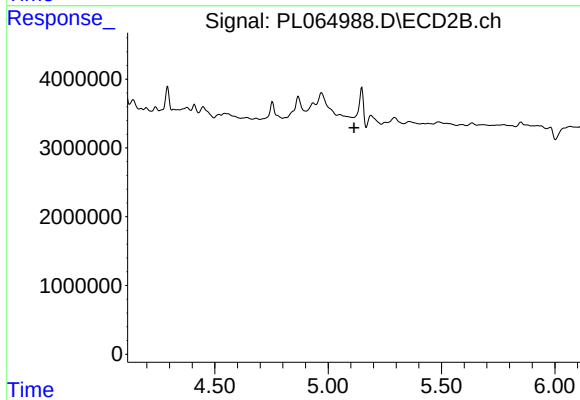


#23 Chlordane-1

R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

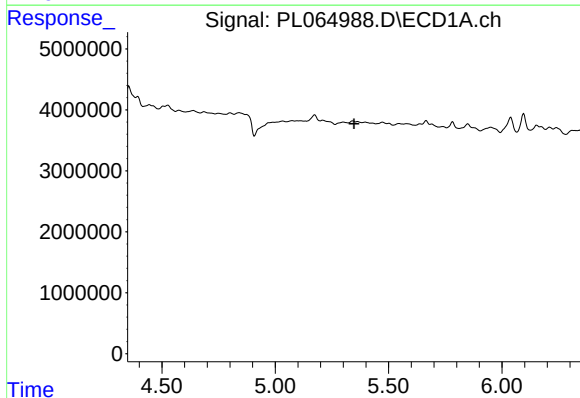


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 5.347 min
Response: 0
Conc: N.D.

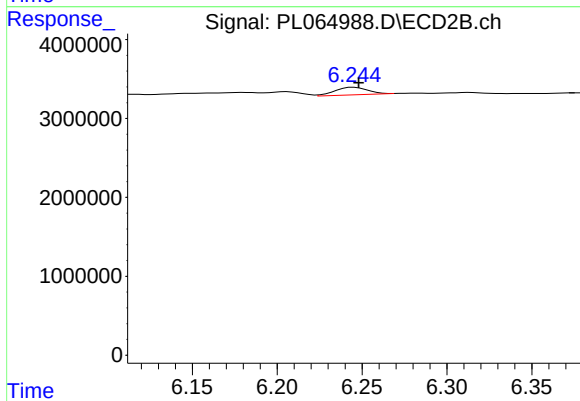

#25 Chlordane-3


R.T.: 6.245 min
Delta R.T.: -0.003 min
Response: 1277960
Conc: 4.18 ng/ml

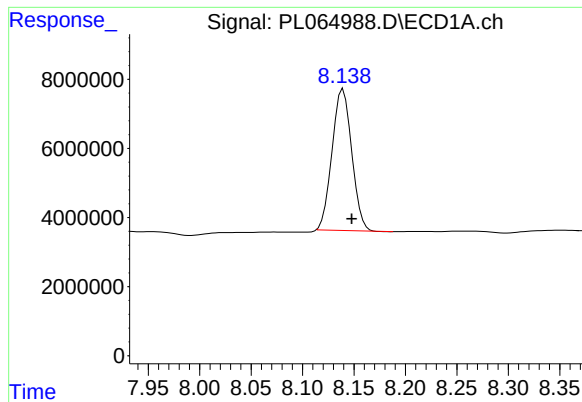

#28 Decachlorobiphenyl

R.T.: 8.139 min
Delta R.T.: -0.008 min
Response: 54431183
Conc: 24.20 ng/ml

Instrument :
ECD_L
ClientSampleId :

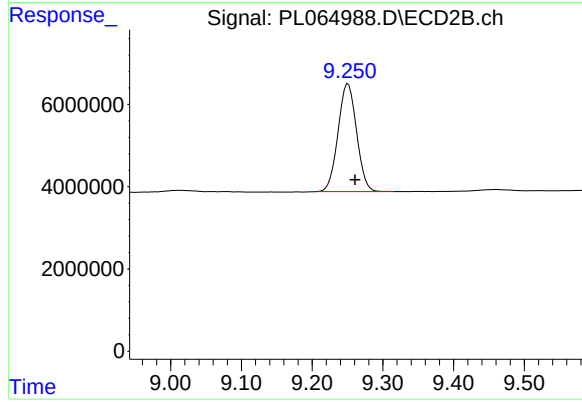

#28 Decachlorobiphenyl

R.T.: 9.251 min
Delta R.T.: -0.010 min
Response: 47766468
Conc: 25.15 ng/ml