

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022721\
 Data File : PL064975.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2021 14:13
 Operator : AR\AJ
 Sample : M1491-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SA-01-022521

Manual Integrations
 APPROVED

Ankita
 3/1/2021 9:25:55 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 17:02:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.096	37123229	31769432	13.195	14.707
28)	SA Decachlor...	8.141	9.252	35984012	34197107	16.001	18.004
Target Compounds							
12)	B 4,4'-DDE	5.564	6.469	3188936	3099379	1.019m	1.528m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022721\
Data File : PL064975.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2021 14:13
Operator : AR\AJ
Sample : M1491-01
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SA-01-022521


Manual Integrations
APPROVED

Ankita
3/1/2021 9:25:55 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 17:02:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

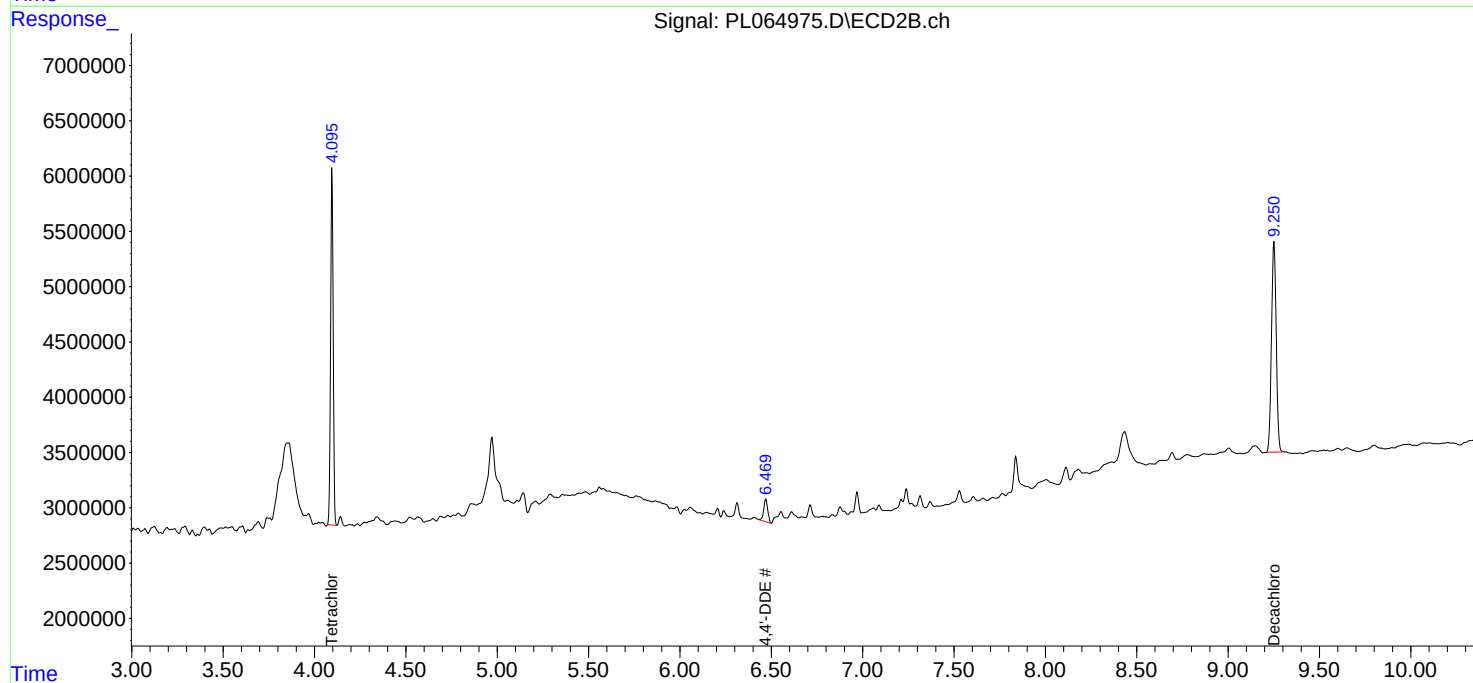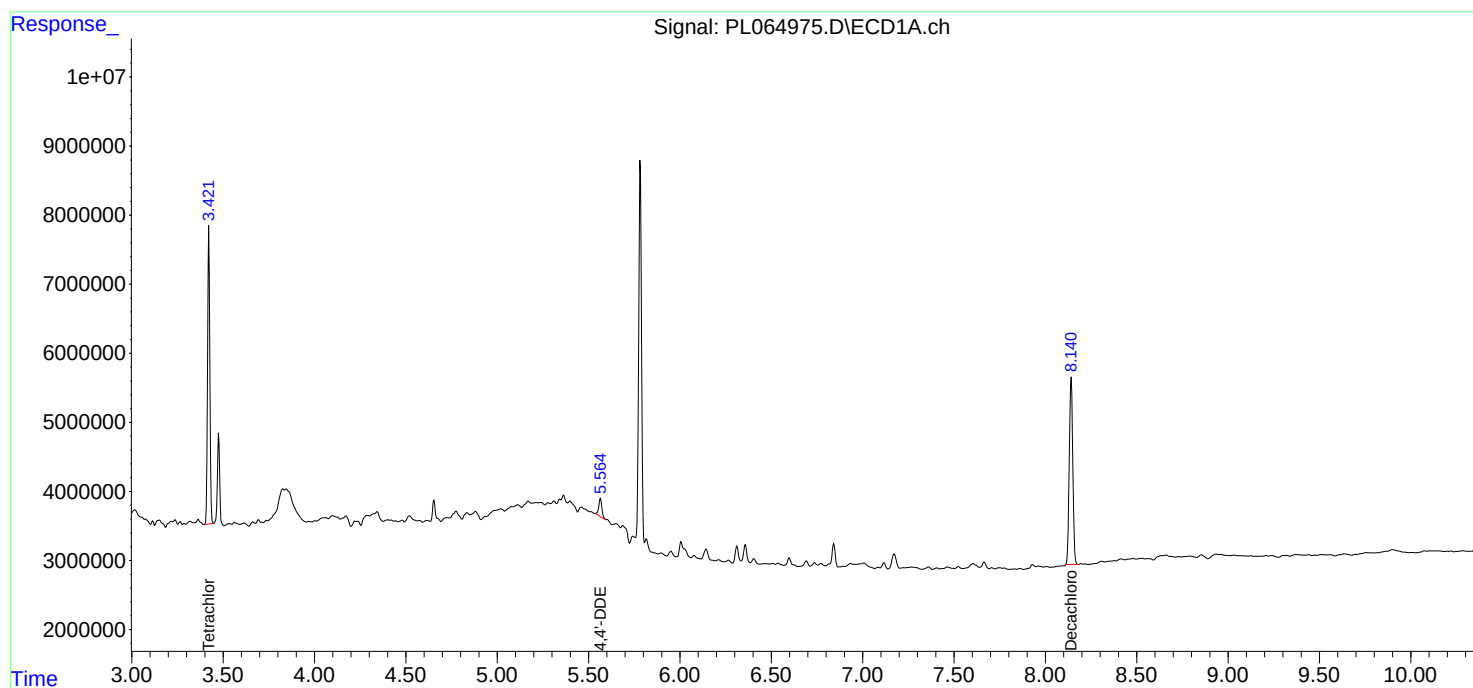

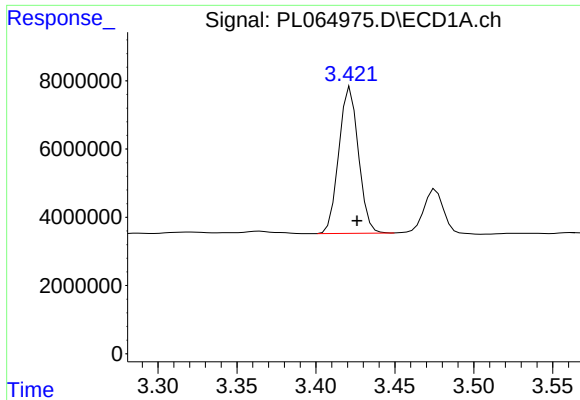


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: -0.004 min
Response: 37123229
Conc: 13.19 ng/ml

Instrument :
ECD_L
ClientSampleId :
SA-01-022521


Manual Integrations
APPROVED

Ankita
3/1/2021 9:25:55 AM

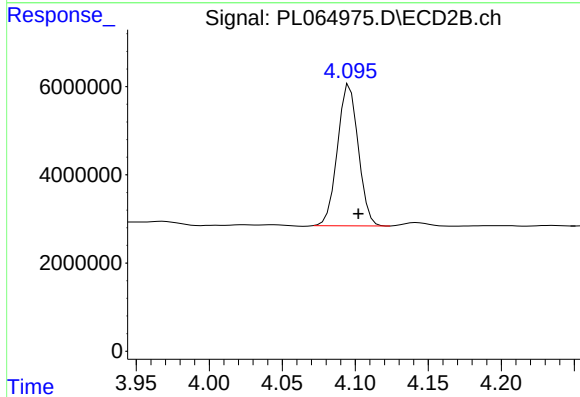


#1 Tetrachloro-m-xylene

R.T.: 4.096 min
Delta R.T.: -0.006 min
Response: 31769432
Conc: 14.71 ng/ml

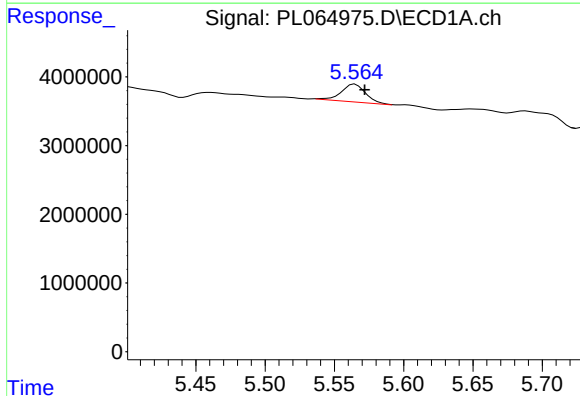


#12 4,4'-DDE

R.T.: 5.564 min
Delta R.T.: -0.008 min
Response: 3188936
Conc: 1.02 ng/ml m

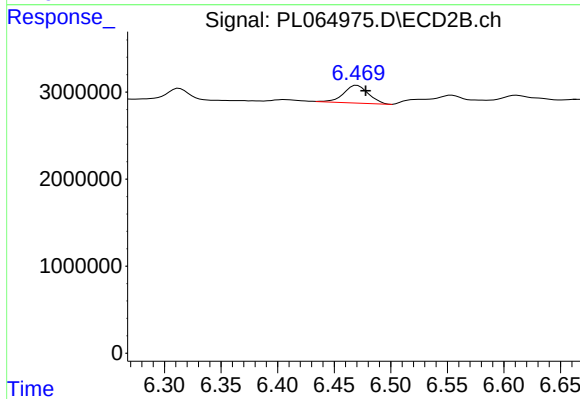

#12 4,4'-DDE

R.T.: 6.469 min
Delta R.T.: -0.009 min
Response: 3099379
Conc: 1.53 ng/ml m

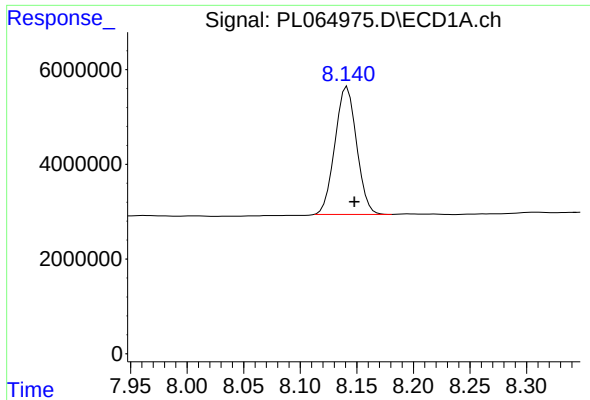


#28 Decachlorobiphenyl

R.T.: 8.141 min
Delta R.T.: -0.006 min
Response: 35984012
Conc: 16.00 ng/ml

Instrument :
ECD_L
ClientSampleId :
SA-01-022521

Manual Integrations
APPROVED

Ankita
3/1/2021 9:25:55 AM

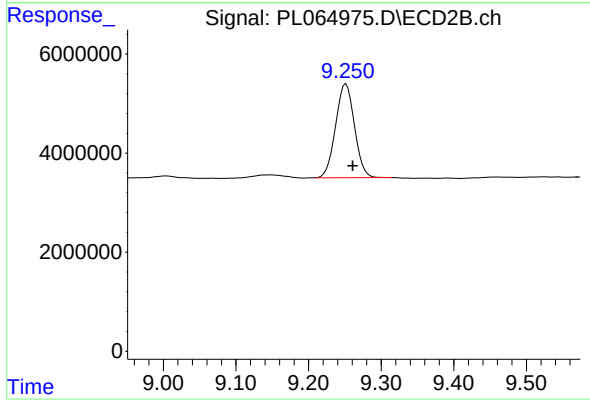

#28 Decachlorobiphenyl

R.T.: 9.252 min
Delta R.T.: -0.009 min
Response: 34197107
Conc: 18.00 ng/ml