

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022721\
 Data File : PL064980.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2021 15:24
 Operator : AR\AJ
 Sample : M1503-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SEDGWICK-AVE

Manual Integrations
 APPROVED

Ankita
 3/1/2021 9:26:04 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 17:04:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.095	34158493	31445575	12.141	14.557m
28)	SA Decachlor...	8.138	9.250	37531039	29485992	16.689m	15.524

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022721\
Data File : PL064980.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2021 15:24
Operator : AR\AJ
Sample : M1503-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SEDGWICK-AVE


Manual Integrations
APPROVED

Ankita
3/1/2021 9:26:04 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 17:04:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

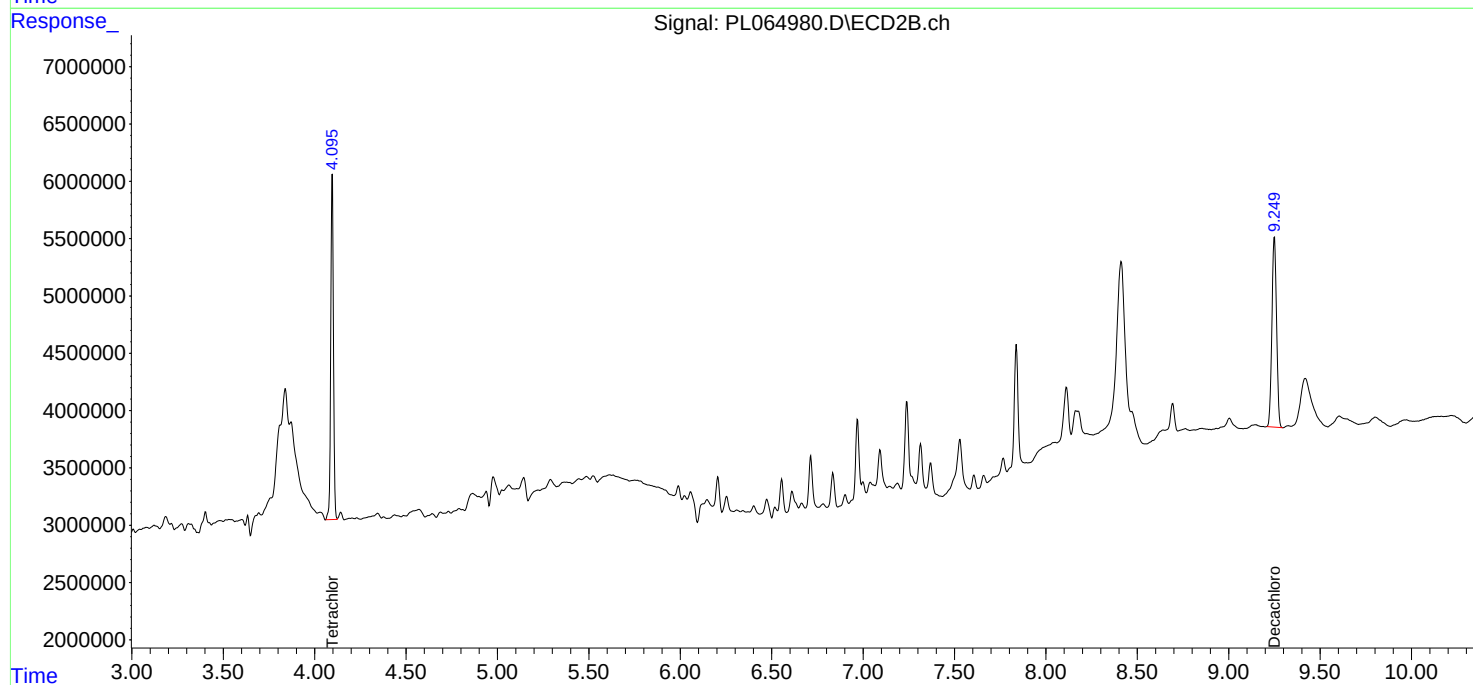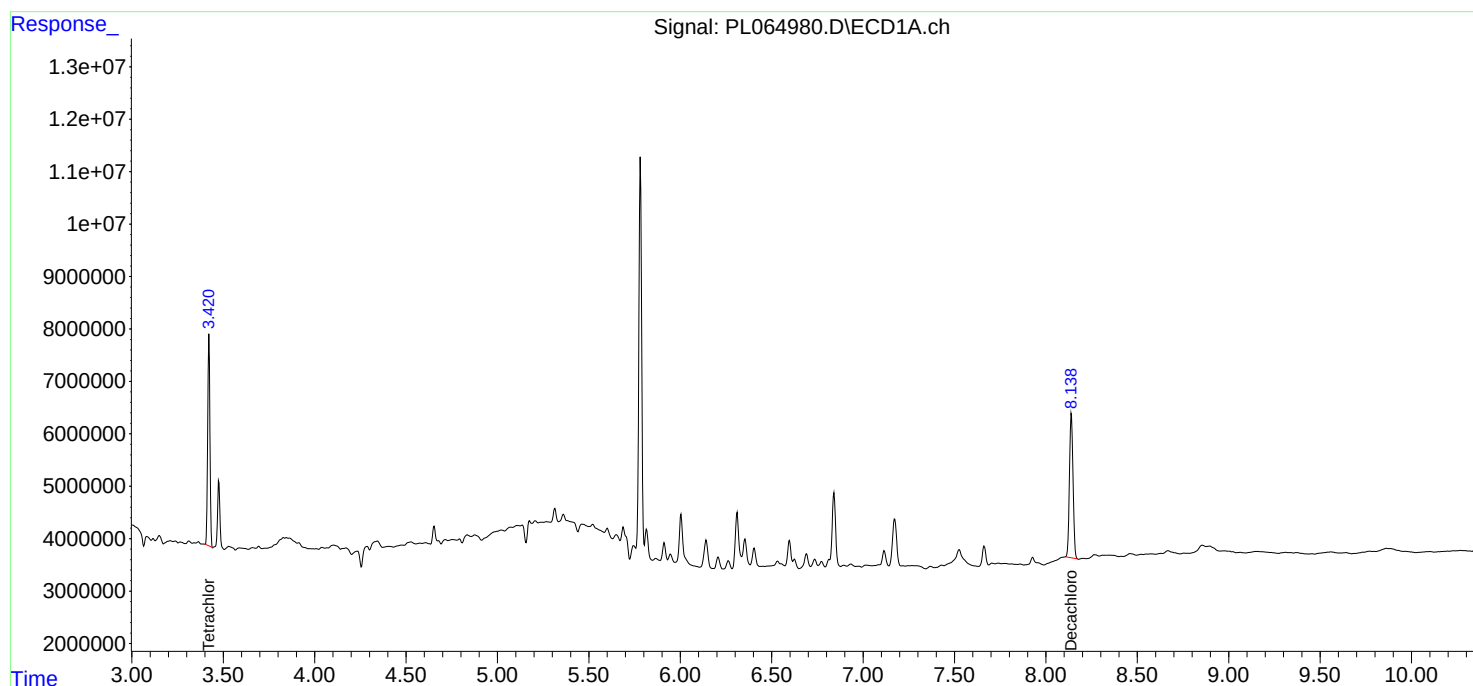

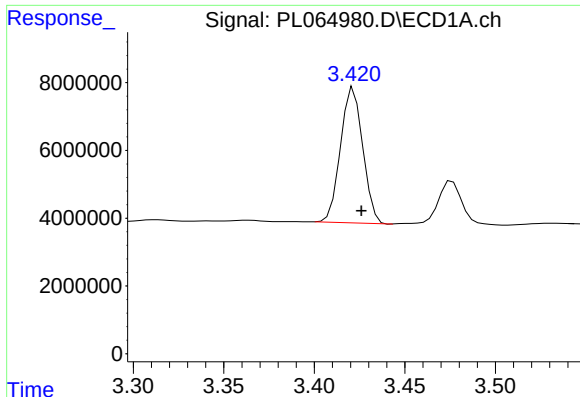


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: -0.004 min
Response: 34158493
Conc: 12.14 ng/ml

Instrument :
ECD_L
ClientSampleId :
SEDGWICK-AVE


Manual Integrations
APPROVED

Ankita
3/1/2021 9:26:04 AM

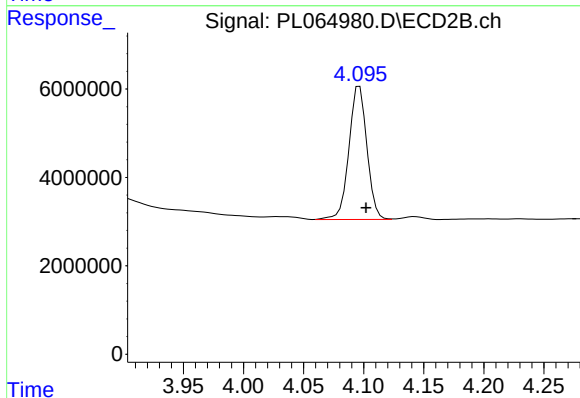


#1 Tetrachloro-m-xylene

R.T.: 4.095 min
Delta R.T.: -0.007 min
Response: 31445575
Conc: 14.56 ng/ml m

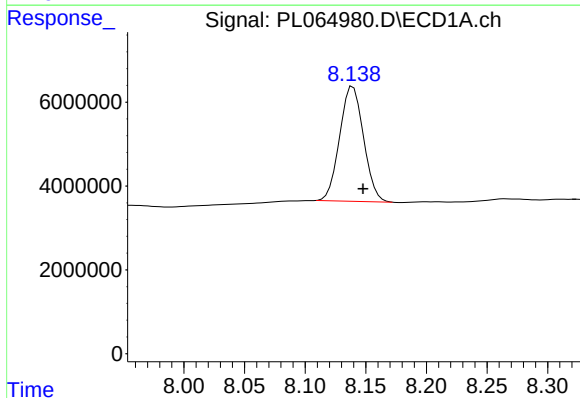

#28 Decachlorobiphenyl

R.T.: 8.138 min
Delta R.T.: -0.010 min
Response: 37531039
Conc: 16.69 ng/ml m

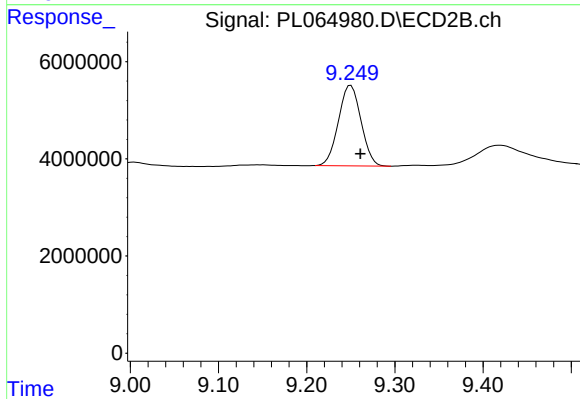

#28 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.011 min
Response: 29485992
Conc: 15.52 ng/ml