

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022721\
 Data File : PL064984.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 26 Feb 2021 16:21
 Operator : AR\AJ
 Sample : M1475-02
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 WA-CON

Manual Integrations
 APPROVED

Ankita
 3/1/2021 9:26:05 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Feb 26 17:04:49 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.096	63020401	50759416	22.399	23.498
28)	SA Decachlor...	8.137	9.250	57851395	46106841	25.725m	24.275

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL022721\
Data File : PL064984.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 26 Feb 2021 16:21
Operator : AR\AJ
Sample : M1475-02
Misc :
ALS Vial : 18 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
WA-CON


Manual Integrations
APPROVED

Ankita
3/1/2021 9:26:05 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Feb 26 17:04:49 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

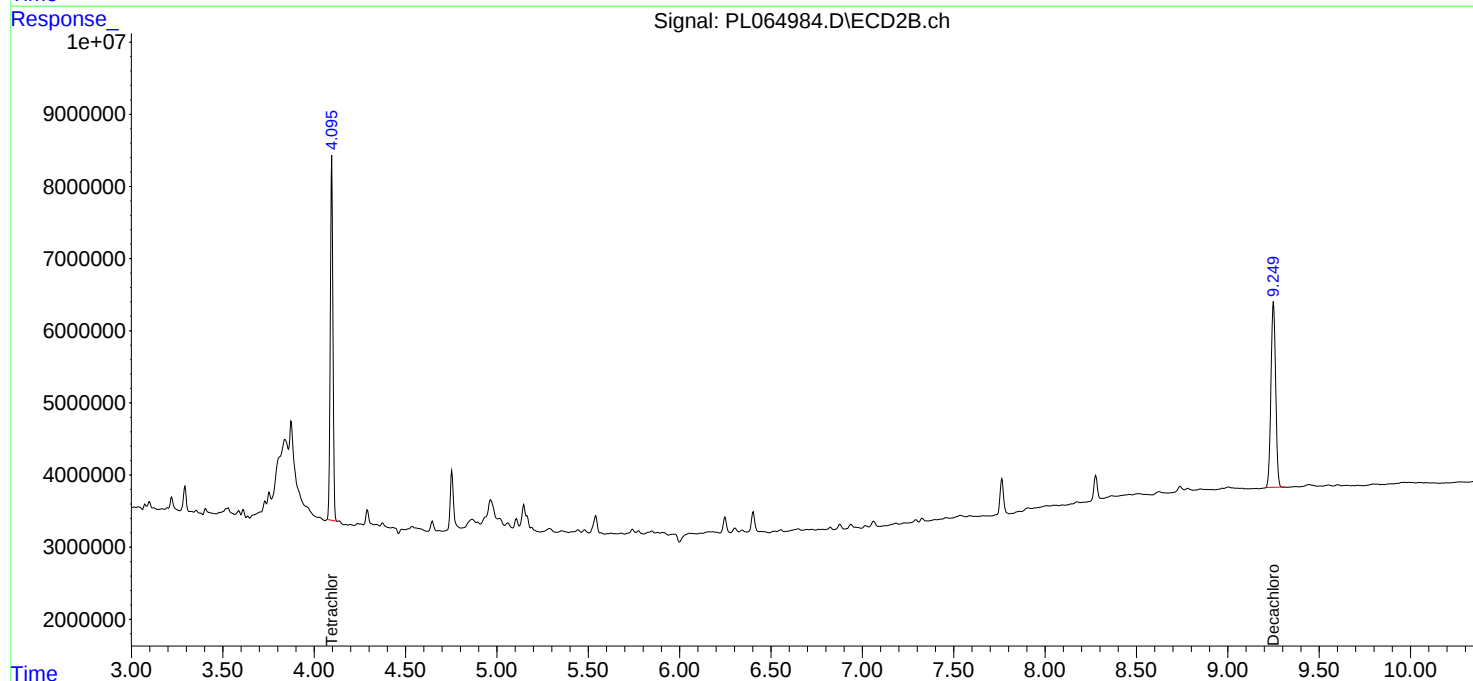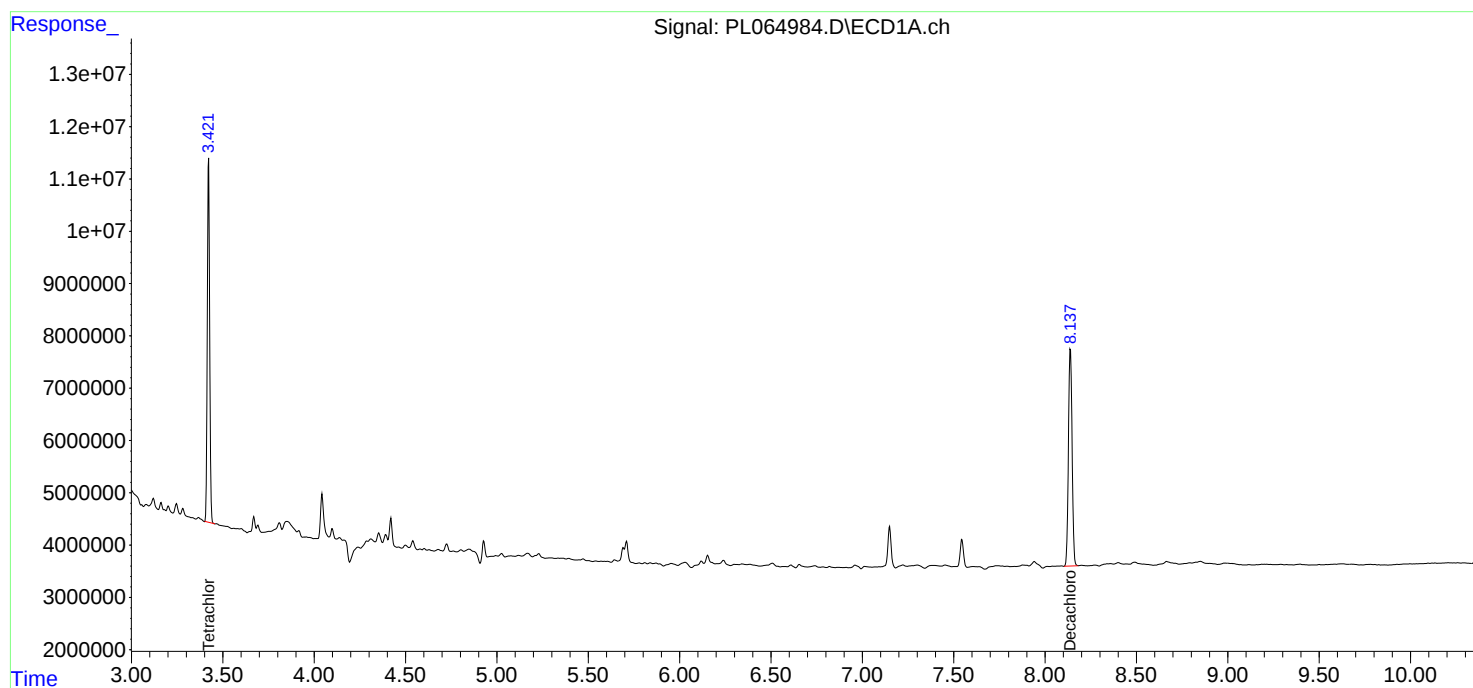

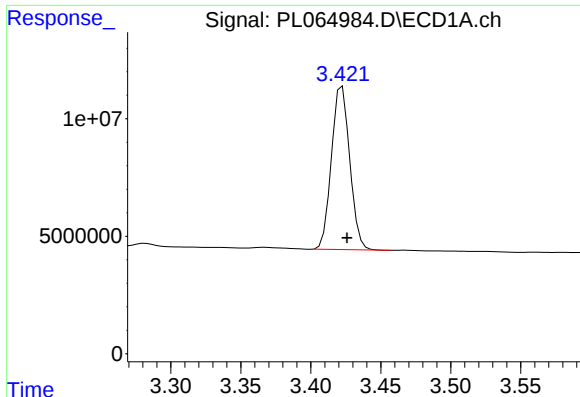


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: -0.004 min
Response: 63020401
Conc: 22.40 ng/ml

Instrument :
ECD_L
ClientSampleId :
WA-CON


Manual Integrations
APPROVED

Ankita
3/1/2021 9:26:05 AM

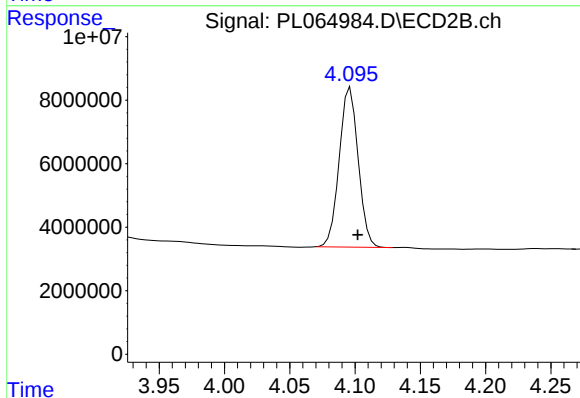


#1 Tetrachloro-m-xylene

R.T.: 4.096 min
Delta R.T.: -0.006 min
Response: 50759416
Conc: 23.50 ng/ml

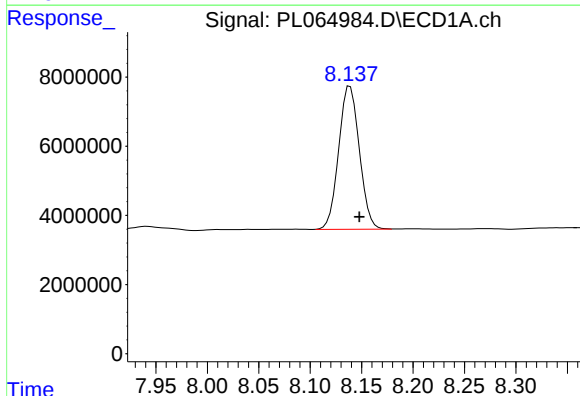

#28 Decachlorobiphenyl

R.T.: 8.137 min
Delta R.T.: -0.011 min
Response: 57851395
Conc: 25.73 ng/ml m

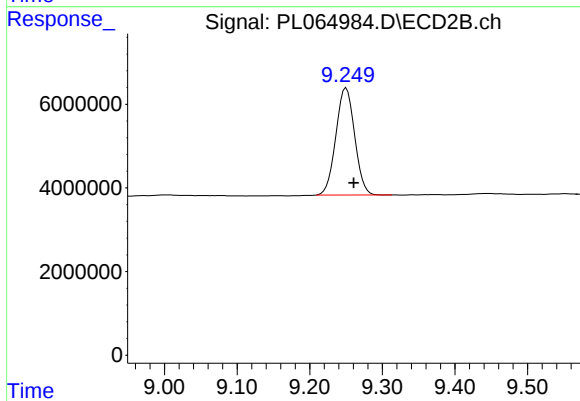

#28 Decachlorobiphenyl

R.T.: 9.250 min
Delta R.T.: -0.010 min
Response: 46106841
Conc: 24.27 ng/ml