

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030222\
 Data File : PL073103.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 02 Mar 2022 21:59
 Operator : AR\AJ
 Sample : PB143039TB
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 03 00:46:30 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
 Quant Title : GC Extractables
 QLast Update : Mon Feb 28 02:28:04 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.647	5.491	6315115	29585250	19.707	20.387
2)	SA Decachlor...	10.427	11.330	10177244	34081451	21.743	21.604
Target Compounds							
6)	B beta-BHC	0.000	6.674	0	669613	N.D.	0.743 #
7)	B delta-BHC	6.424	6.934	7992	642553	0.018	0.340 #
9)	A Endosulfan I	7.478f	8.327	3447	50087	0.008	0.031 #
10)	B gamma-Chl...	7.390f	0.000	8997	0	0.019	N.D. #
11)	B alpha-Chl...	7.421f	0.000	21737	0	0.045	N.D. #
13)	MA Dieldrin	7.782	0.000	18152	0	0.041	N.D. #
14)	MA Endrin	8.099f	0.000	26428	0	0.067	N.D. #
15)	B Endosulfa...	0.000	9.048f	0	371651	N.D.	0.269 #
16)	A 4,4'-DDD	8.248	0.000	3555	0	0.010	N.D. #
20)	A Methoxychlor	9.093	0.000	16535	0	0.066	N.D. #
22)	Mirex	9.537f	0.000	5932	0	0.011	N.D. #
24)	Chlordane-2	6.673	0.000	9311	0	0.470	N.D. #
25)	Chlordane-3	7.390f	0.000	8997	0	0.182	N.D. #
26)	Chlordane-4	7.421f	0.000	21737	0	0.411	N.D. #
27)	Chlordane-5	0.000	9.136	0	30117	N.D.	0.560 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030222\
Data File : PL073103.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 02 Mar 2022 21:59
Operator : AR\AJ
Sample : PB143039TB
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 03 00:46:30 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL022622.M
Quant Title : GC Extractables
QLast Update : Mon Feb 28 02:28:04 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

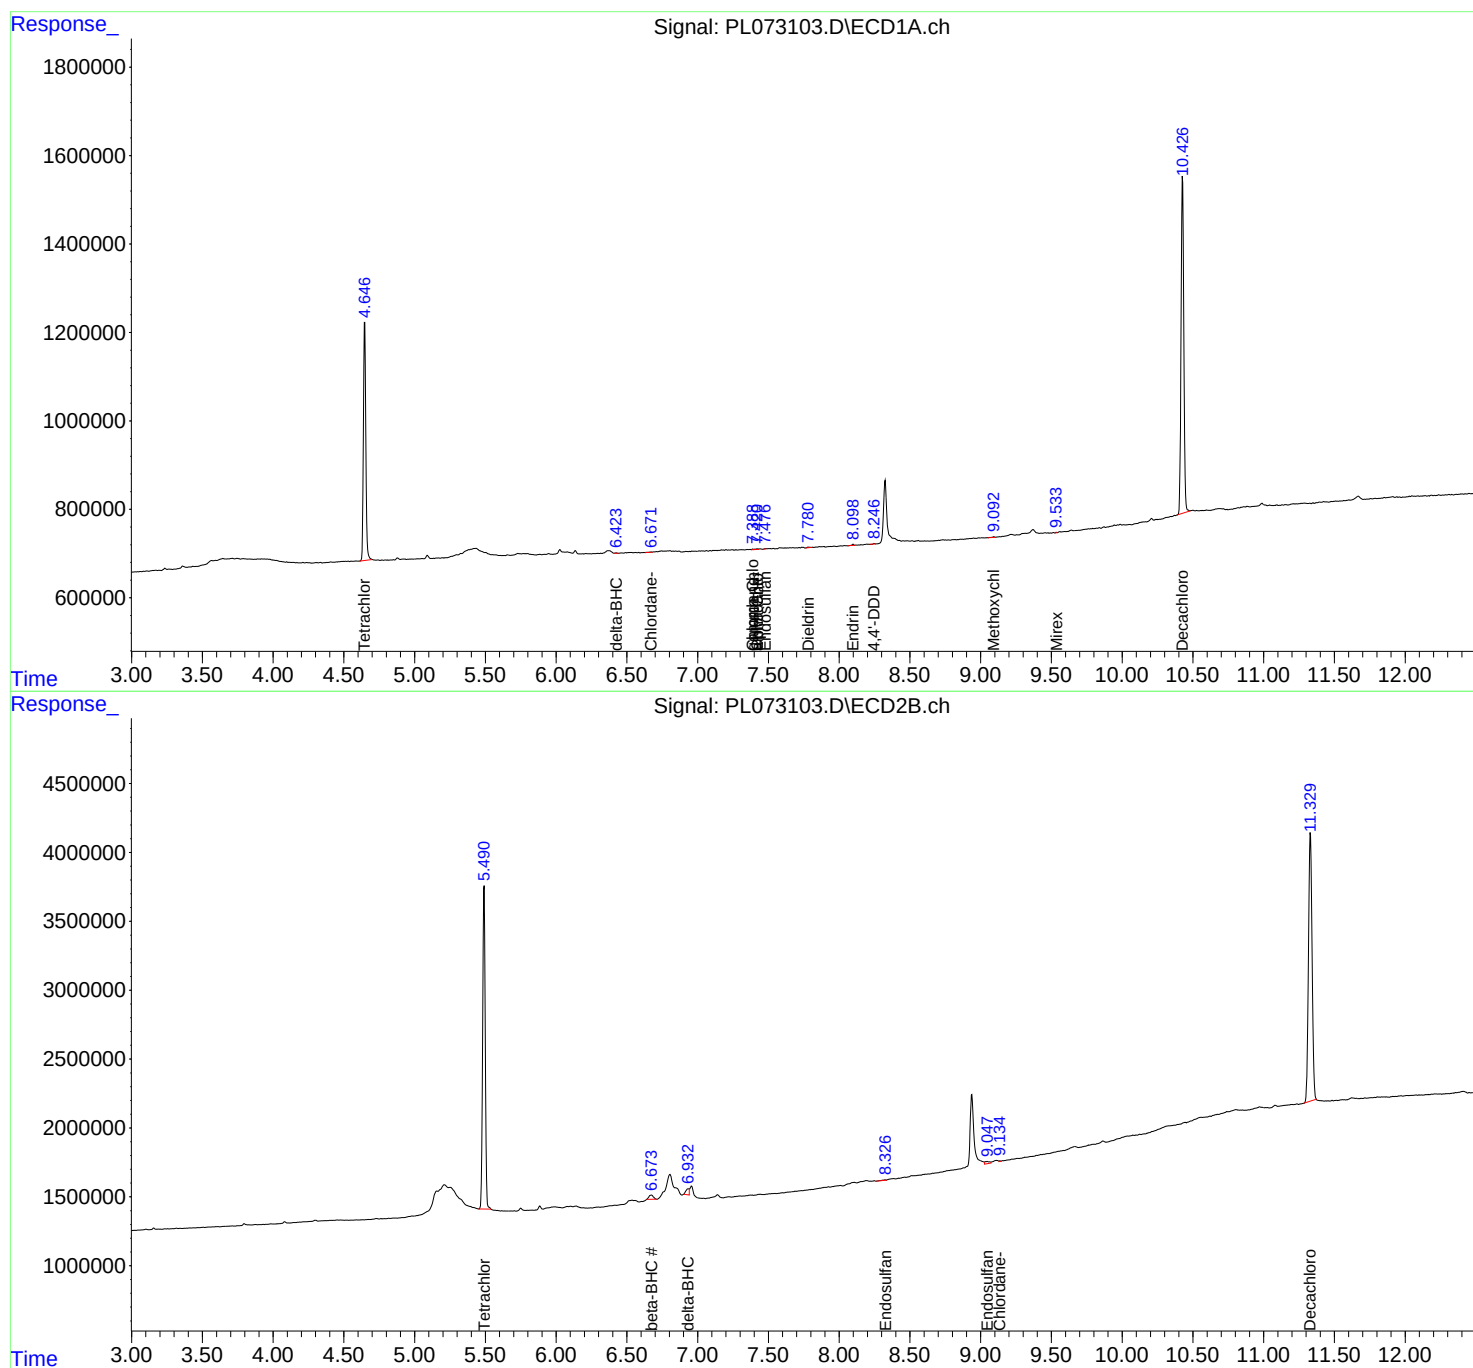


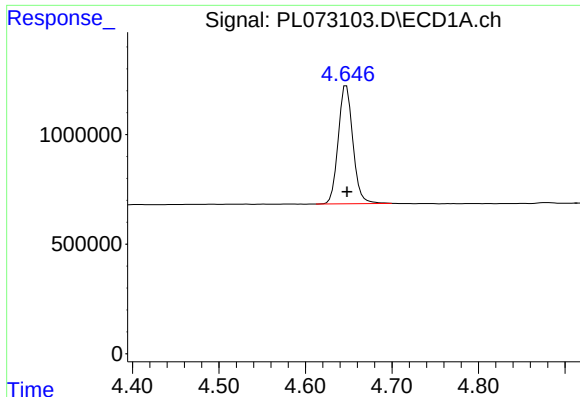

#1 Tetrachloro-m-xylene


R.T.: 4.647 min
Delta R.T.: 0.000 min
Response: 6315115
Conc: 19.71 ng/ml

Instrument :
ECD_L
ClientSampleId :

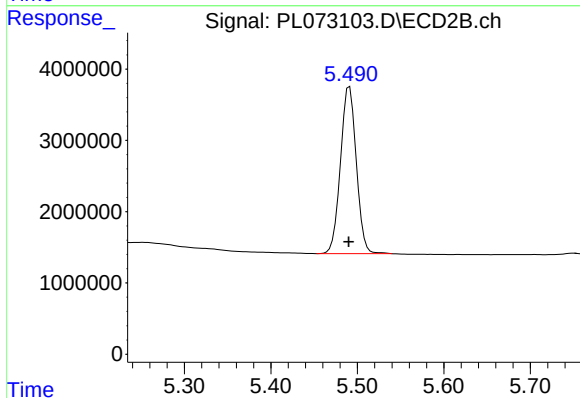


#1 Tetrachloro-m-xylene

R.T.: 5.491 min
Delta R.T.: 0.000 min
Response: 29585250
Conc: 20.39 ng/ml

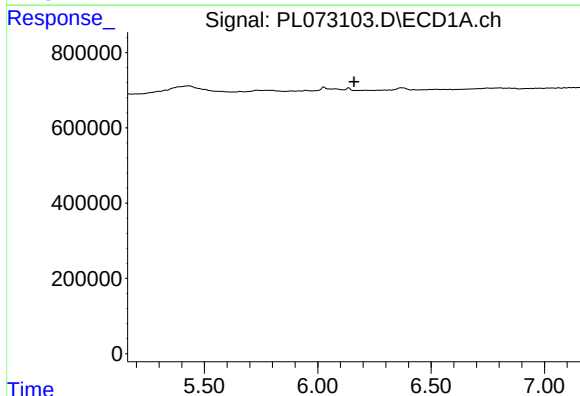


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 6.160 min
Response: 0
Conc: N.D.

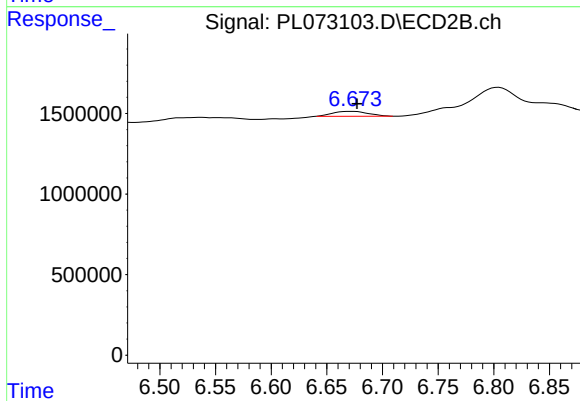

#6 beta-BHC


R.T.: 6.674 min
Delta R.T.: -0.003 min
Response: 669613
Conc: 0.74 ng/ml

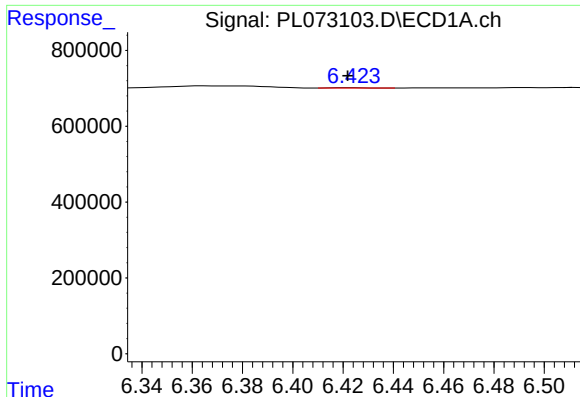

#7 delta-BHC


R.T.: 6.424 min
Delta R.T.: 0.002 min
Response: 7992
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

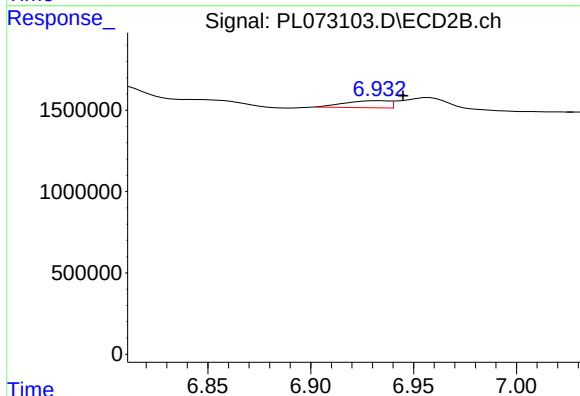


#7 delta-BHC

R.T.: 6.934 min
Delta R.T.: -0.011 min
Response: 642553
Conc: 0.34 ng/ml

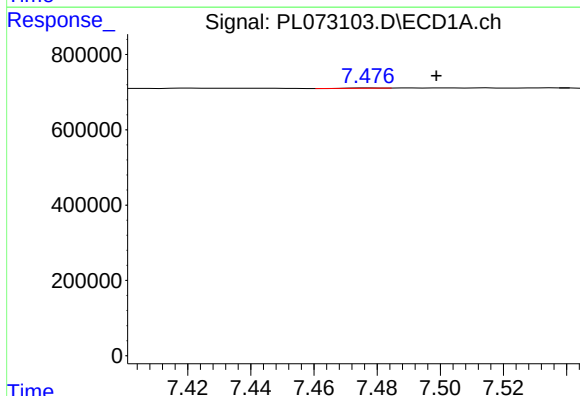


#9 Endosulfan I

R.T.: 7.478 min
Delta R.T.: -0.021 min
Response: 3447
Conc: 0.01 ng/ml

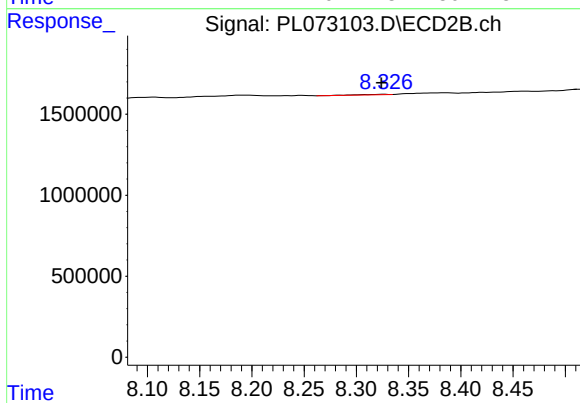

#9 Endosulfan I


R.T.: 8.327 min
Delta R.T.: 0.003 min
Response: 50087
Conc: 0.03 ng/ml

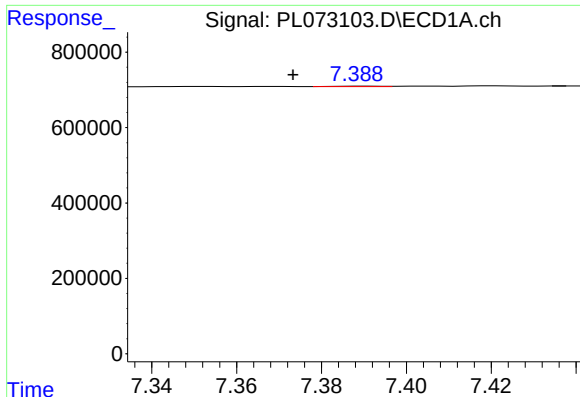

#10 gamma-Chlordane


R.T.: 7.390 min
Delta R.T.: 0.016 min
Response: 8997
Conc: 0.02 ng/ml

Instrument :
ECD_L
ClientSampleId :

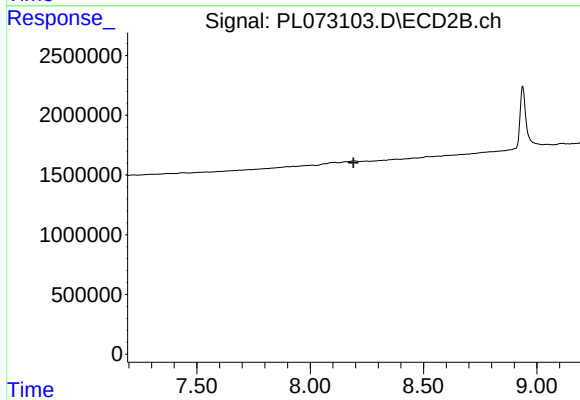


#10 gamma-Chlordane

R.T.: 0.000 min
Exp R.T. : 8.192 min
Response: 0
Conc: N.D.

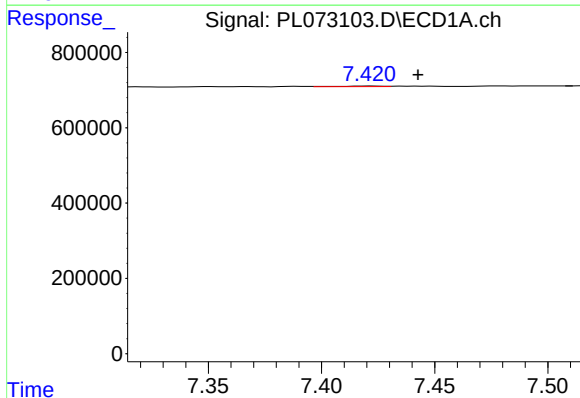


#11 alpha-Chlordane

R.T.: 7.421 min
Delta R.T.: -0.022 min
Response: 21737
Conc: 0.05 ng/ml

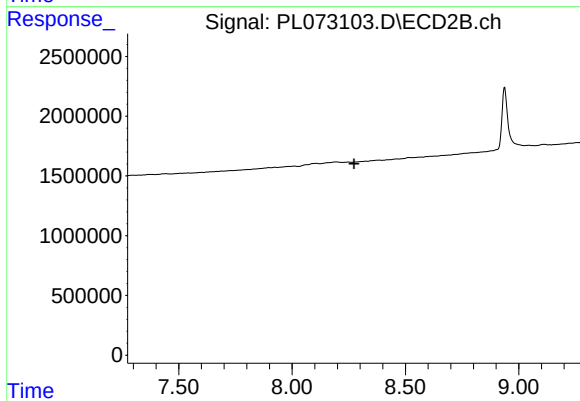

#11 alpha-Chlordane


R.T.: 0.000 min
Exp R.T. : 8.274 min
Response: 0
Conc: N.D.

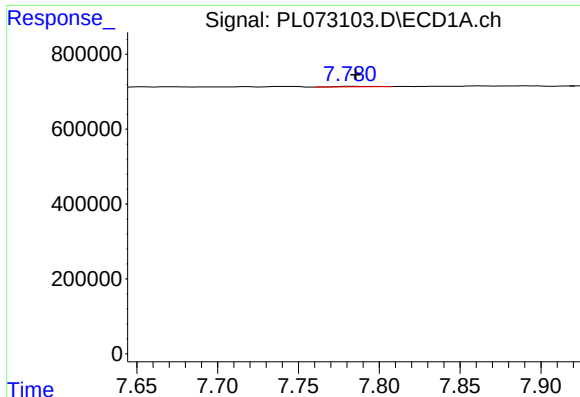

#13 Dieldrin


R.T.: 7.782 min
Delta R.T.: -0.004 min
Response: 18152
Conc: 0.04 ng/ml

Instrument :
ECD_L
ClientSampleId :

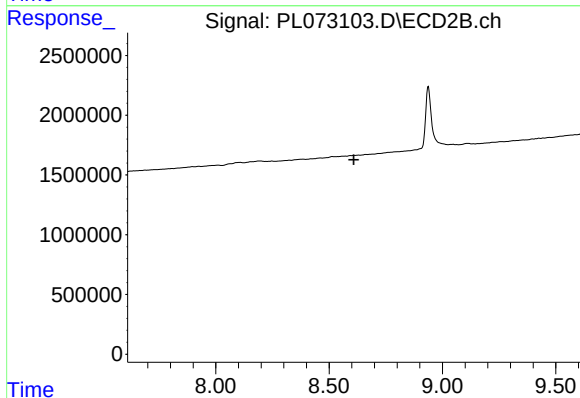


#13 Dieldrin

R.T.: 0.000 min
Exp R.T. : 8.609 min
Response: 0
Conc: N.D.

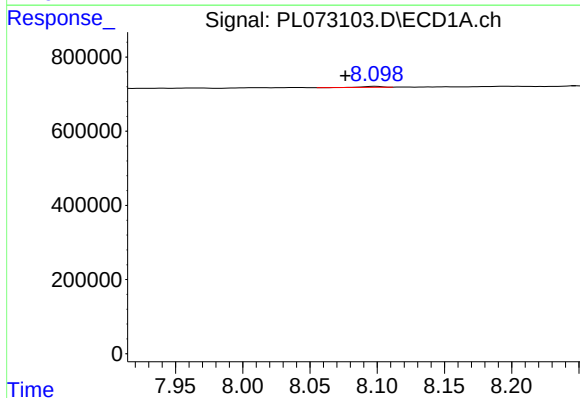


#14 Endrin

R.T.: 8.099 min
Delta R.T.: 0.023 min
Response: 26428
Conc: 0.07 ng/ml

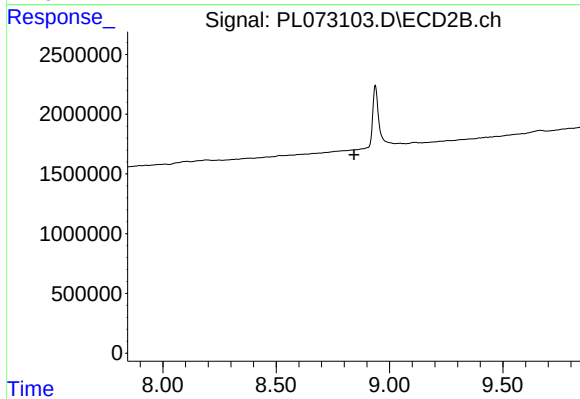

#14 Endrin


R.T.: 0.000 min
Exp R.T. : 8.844 min
Response: 0
Conc: N.D.

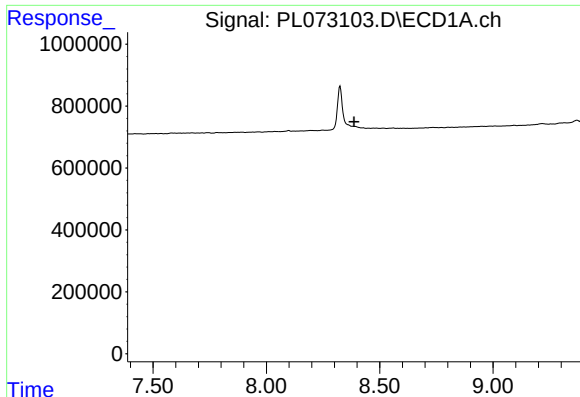

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T.: 8.386 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

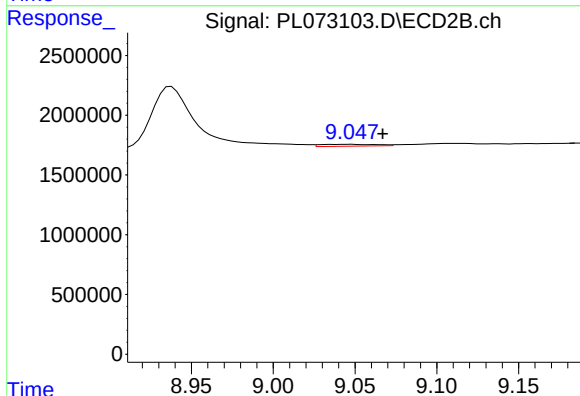


#15 Endosulfan II

R.T.: 9.048 min
Delta R.T.: -0.019 min
Response: 371651
Conc: 0.27 ng/ml

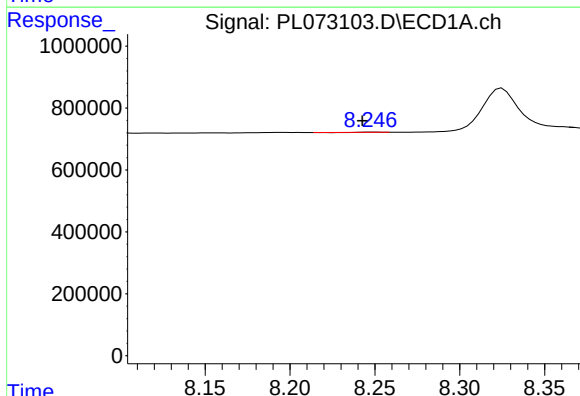


#16 4,4'-DDD

R.T.: 8.248 min
Delta R.T.: 0.005 min
Response: 3555
Conc: 0.01 ng/ml

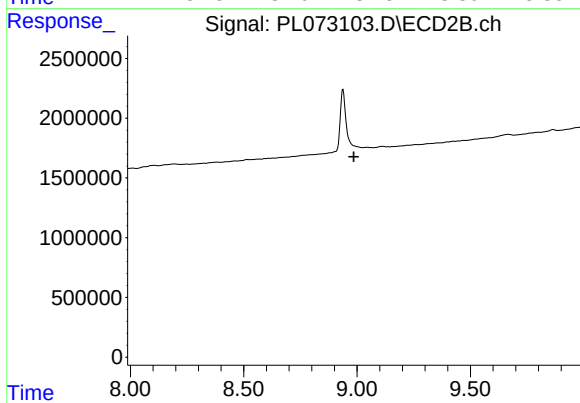

#16 4,4'-DDD


R.T.: 0.000 min
Exp R.T.: 8.985 min
Response: 0
Conc: N.D.

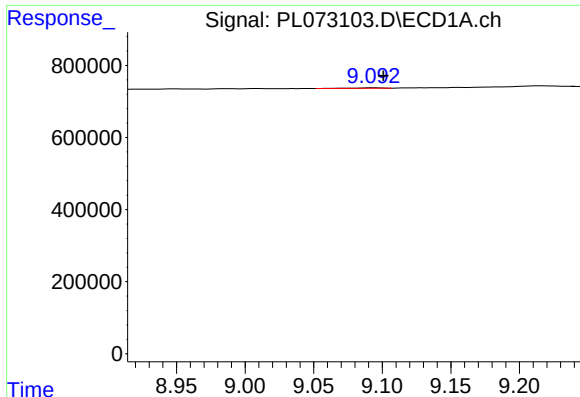

#20 Methoxychlor


R.T.: 9.093 min
Delta R.T.: -0.007 min
Response: 16535
Conc: 0.07 ng/ml

Instrument :
ECD_L
ClientSampleId :

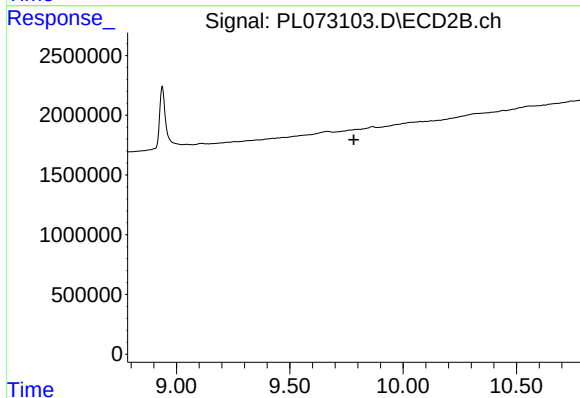


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 9.783 min
Response: 0
Conc: N.D.

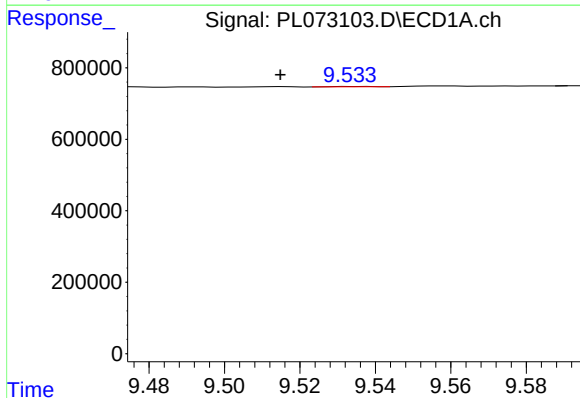


#22 Mirex

R.T.: 9.537 min
Delta R.T.: 0.022 min
Response: 5932
Conc: 0.01 ng/ml

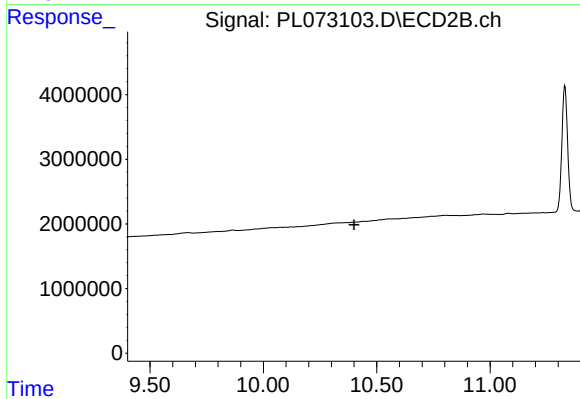

#22 Mirex


R.T.: 0.000 min
Exp R.T. : 10.400 min
Response: 0
Conc: N.D.

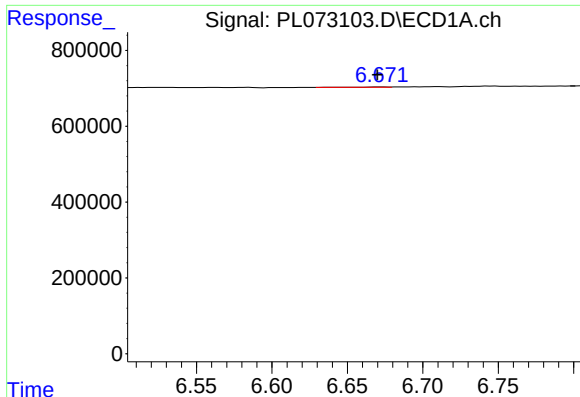

#24 Chlordane-2


R.T.: 6.673 min
Delta R.T.: 0.003 min
Response: 9311
Conc: 0.47 ng/ml

Instrument :
ECD_L
ClientSampleId :

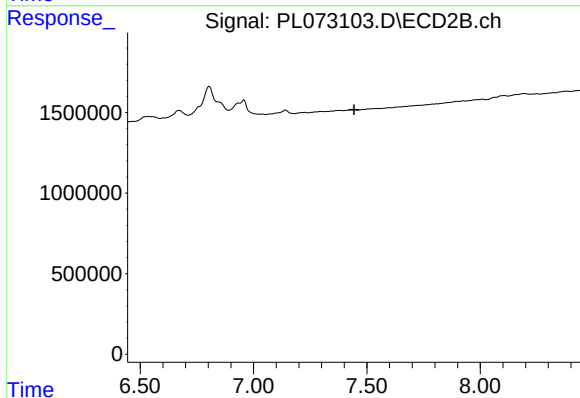


#24 Chlordane-2

R.T.: 0.000 min
Exp R.T. : 7.443 min
Response: 0
Conc: N.D.

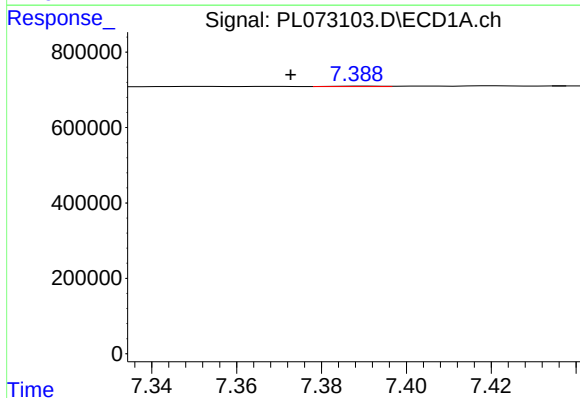


#25 Chlordane-3

R.T.: 7.390 min
Delta R.T.: 0.017 min
Response: 8997
Conc: 0.18 ng/ml

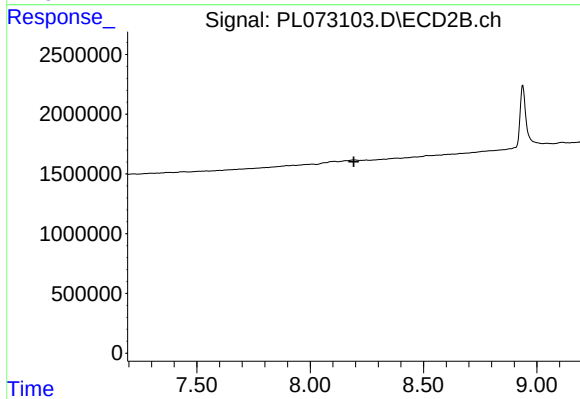

#25 Chlordane-3


R.T.: 0.000 min
Exp R.T. : 8.192 min
Response: 0
Conc: N.D.

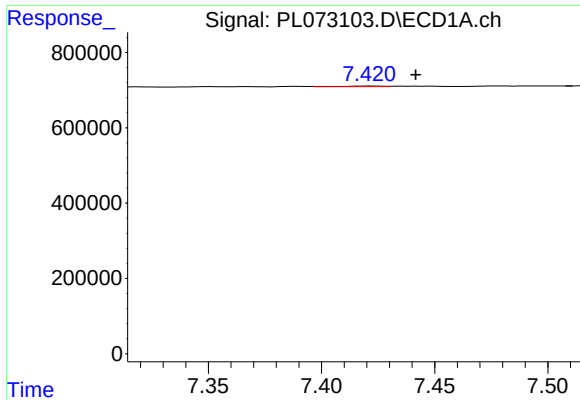

#26 Chlordane-4


R.T.: 7.421 min
Delta R.T.: -0.020 min
Response: 21737
Conc: 0.41 ng/ml

Instrument :
ECD_L
ClientSampleId :

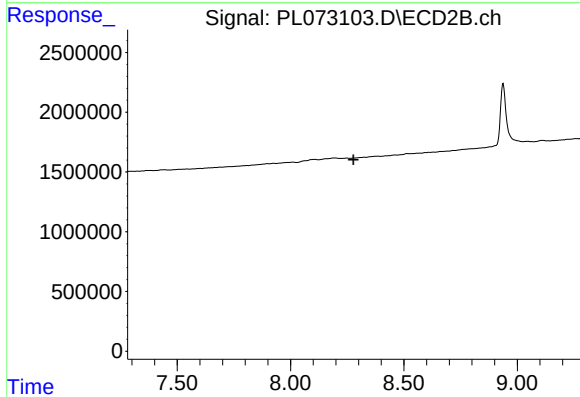


#26 Chlordane-4

R.T.: 0.000 min
Exp R.T. : 8.278 min
Response: 0
Conc: N.D.

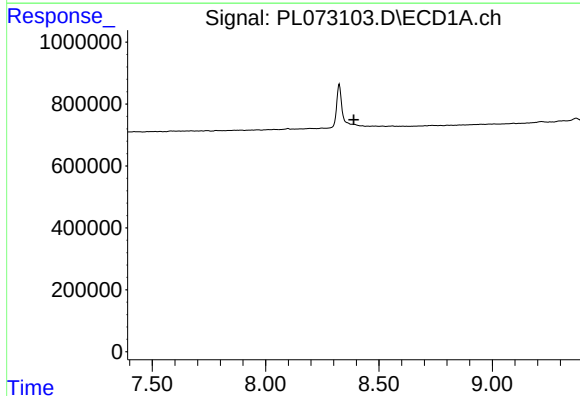


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 8.389 min
Response: 0
Conc: N.D.

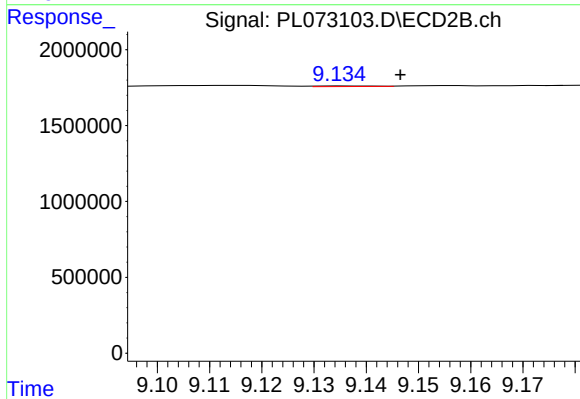

#27 Chlordane-5


R.T.: 9.136 min
Delta R.T.: -0.010 min
Response: 30117
Conc: 0.56 ng/ml

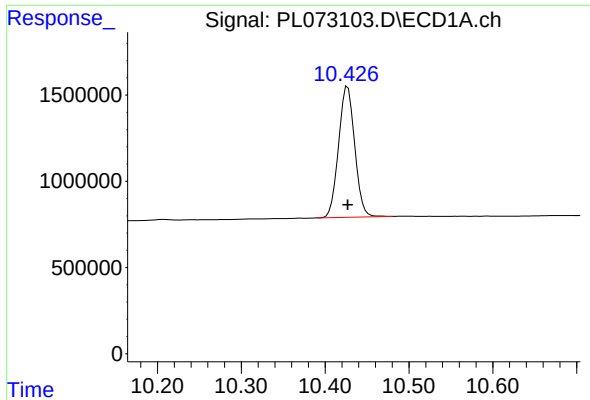

#28 Decachlorobiphenyl

R.T.: 10.427 min
Delta R.T.: 0.000 min
Response: 10177244
Conc: 21.74 ng/ml

Instrument :
ECD_L
ClientSampleId :

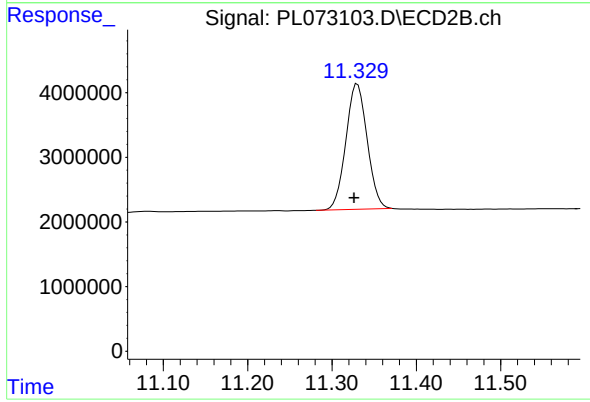

#28 Decachlorobiphenyl

R.T.: 11.330 min
Delta R.T.: 0.004 min
Response: 34081451
Conc: 21.60 ng/ml