

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030321\
 Data File : PL065036.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2021 15:33
 Operator : AR\AJ
 Sample : M1540-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 PR-01-030221

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 01:17:01 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.421	4.097	45789928	38789699	16.275	17.957
28)	SA Decachlor...	8.144	9.256	35066982	33298892	15.594	17.531
Target Compounds							
3)	MA gamma-BHC...	4.139	0.000	1699296	0	0.393	N.D. #
9)	A Endosulfan I	5.472	0.000	3597104	0	1.122	N.D. #
10)	B gamma-Chl...	5.342	0.000	2379345	0	0.679	N.D. #
16)	A 4,4'-DDD	6.096	0.000	1890893	0	0.747	N.D. #
17)	MA 4,4'-DDT	0.000	7.266	0	3683691	N.D.	2.416 #
20)	A Methoxychlor	6.899f	0.000	80957	0	0.063	N.D. #
23)	Chlordane-1	4.311f	0.000	1615862	0	14.215	N.D. #
25)	Chlordane-3	5.342	0.000	2379345	0	7.241	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030321\
Data File : PL065036.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2021 15:33
Operator : AR\AJ
Sample : M1540-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :
PR-01-030221

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 01:17:01 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

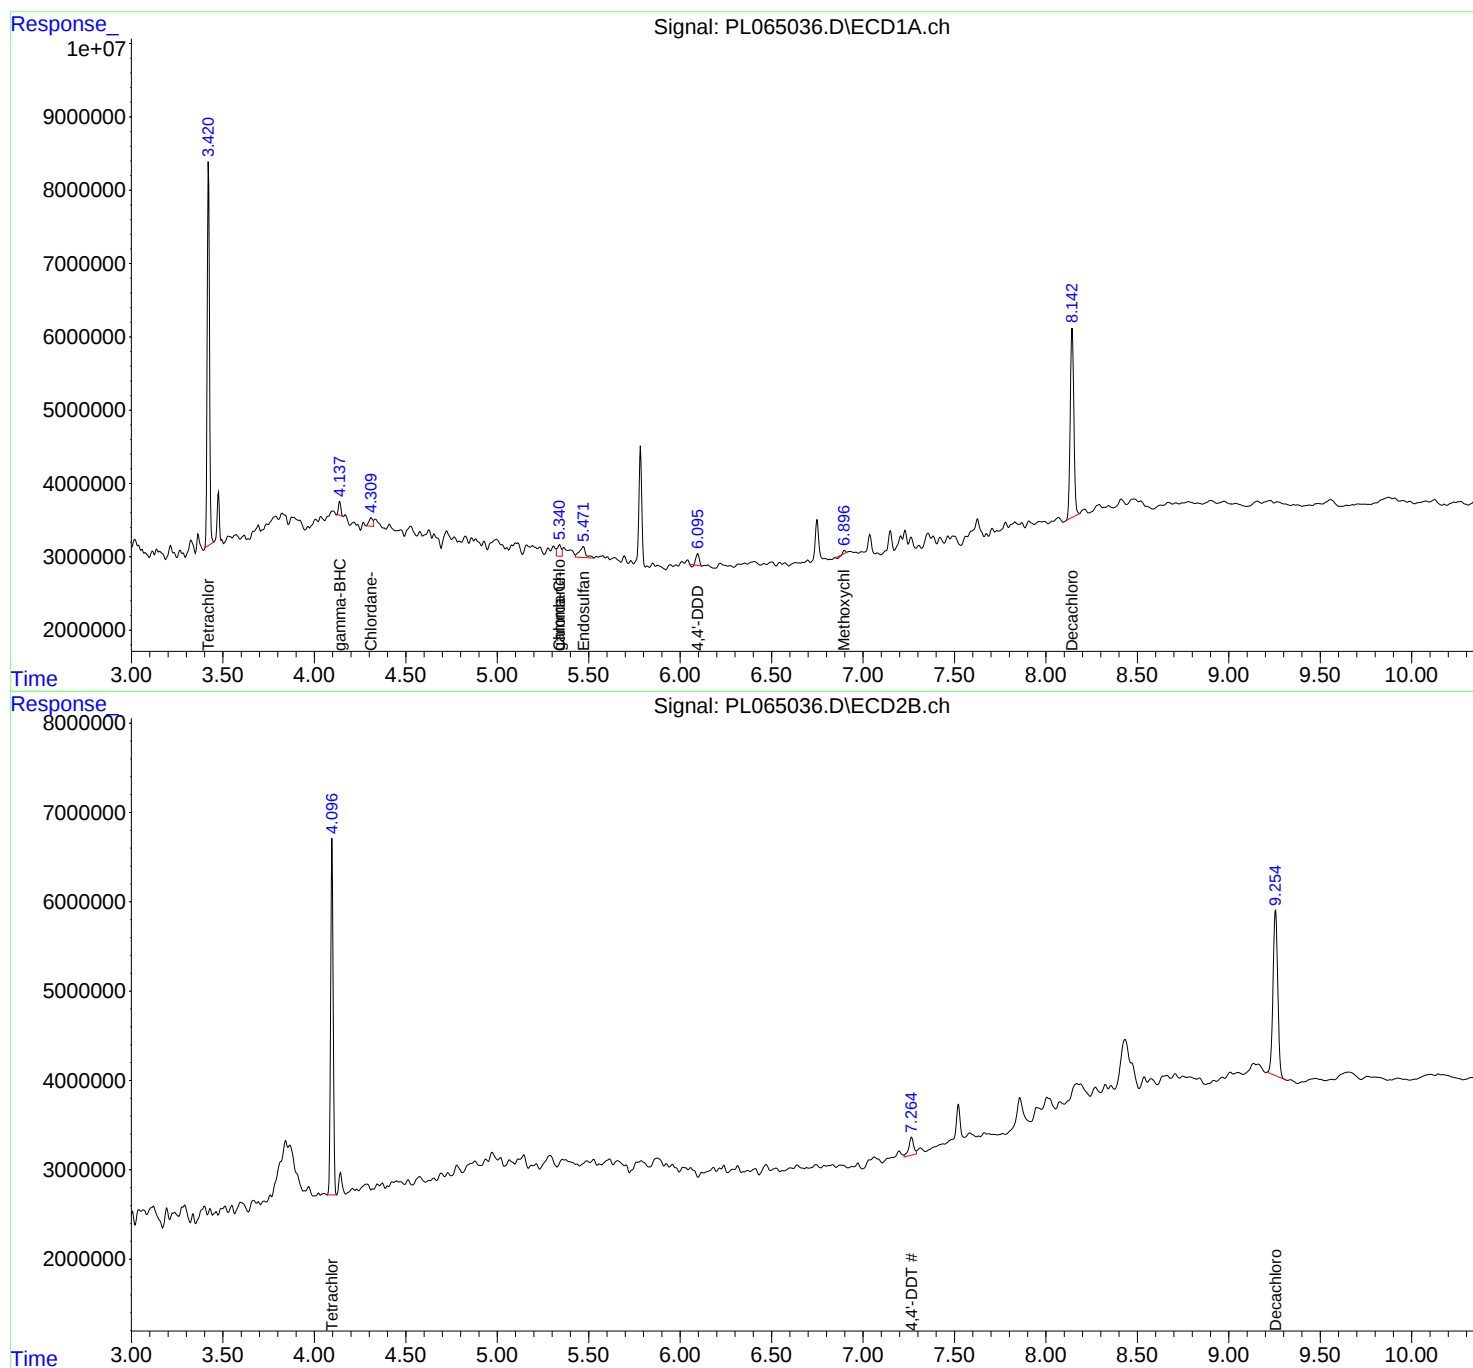


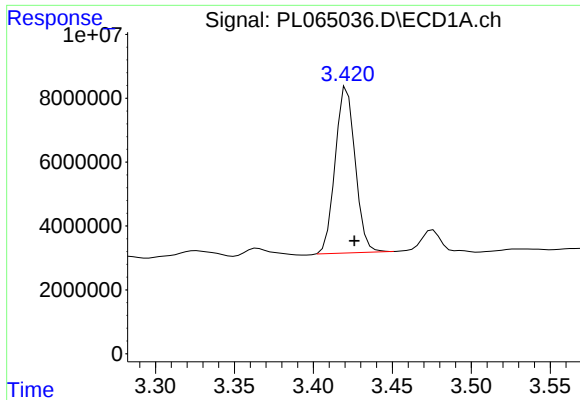

#1 Tetrachloro-m-xylene


R.T.: 3.421 min
Delta R.T.: -0.005 min
Response: 45789928
Conc: 16.28 ng/ml

Instrument :
ECD_L
ClientSampleId :
PR-01-030221

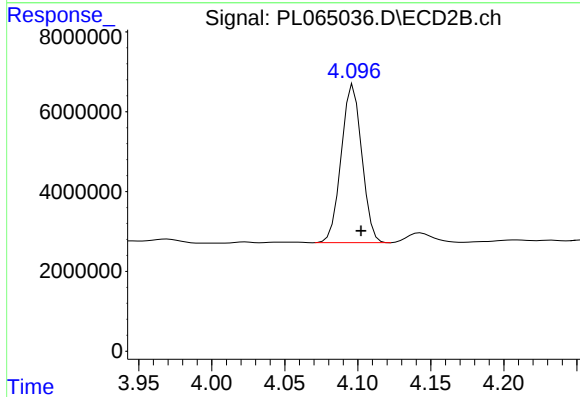


#1 Tetrachloro-m-xylene

R.T.: 4.097 min
Delta R.T.: -0.005 min
Response: 38789699
Conc: 17.96 ng/ml

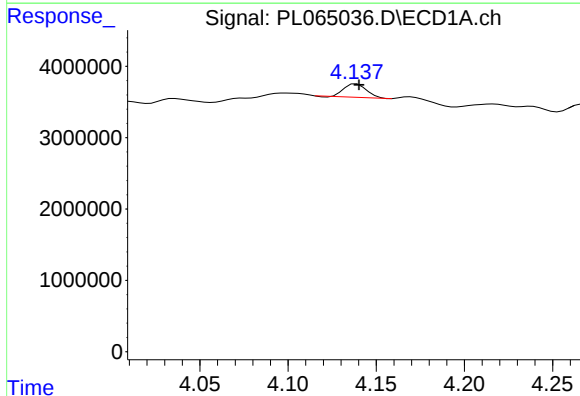


#3 gamma-BHC (Lindane)

R.T.: 4.139 min
Delta R.T.: -0.001 min
Response: 1699296
Conc: 0.39 ng/ml

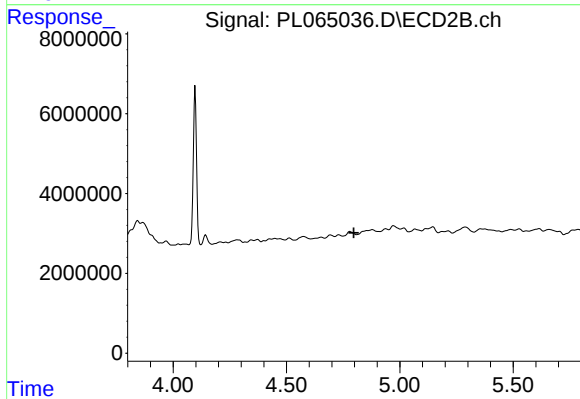

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T.: 4.797 min
Response: 0
Conc: N.D.

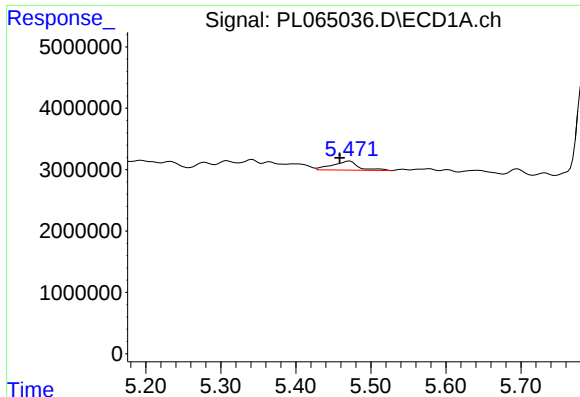

#9 Endosulfan I


R.T.: 5.472 min
Delta R.T.: 0.013 min
Response: 3597104
Conc: 1.12 ng/ml

Instrument :
ECD_L
ClientSampleId :
PR-01-030221

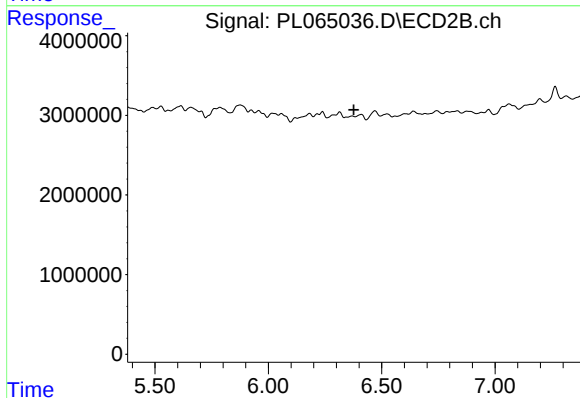


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.376 min
Response: 0
Conc: N.D.

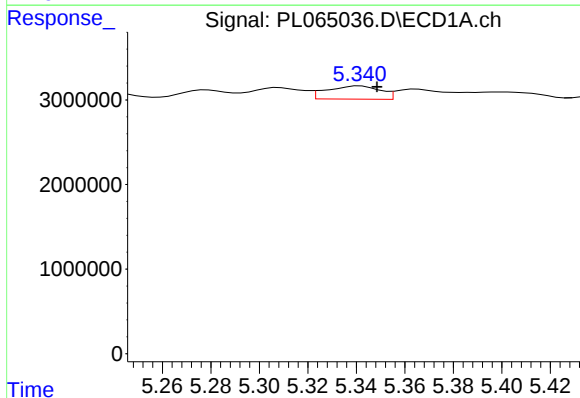


#10 gamma-Chlordane

R.T.: 5.342 min
Delta R.T.: -0.007 min
Response: 2379345
Conc: 0.68 ng/ml

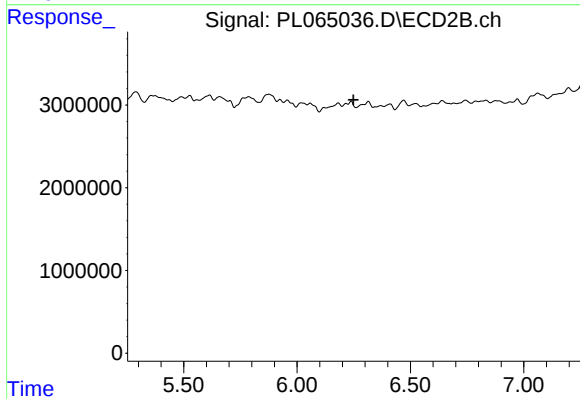

#10 gamma-Chlordane


R.T.: 0.000 min
Exp R.T. : 6.249 min
Response: 0
Conc: N.D.

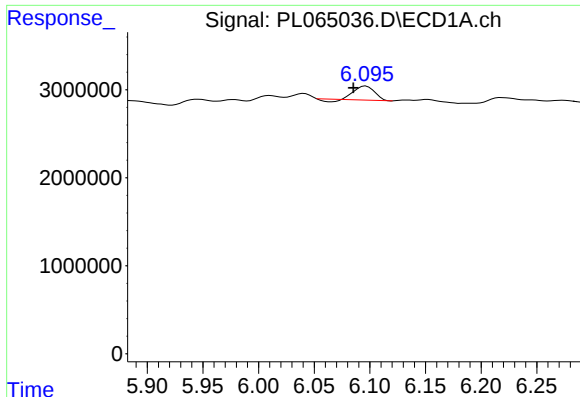

#16 4,4'-DDD


R.T.: 6.096 min
Delta R.T.: 0.011 min
Response: 1890893
Conc: 0.75 ng/ml

Instrument :
ECD_L
ClientSampleId :
PR-01-030221

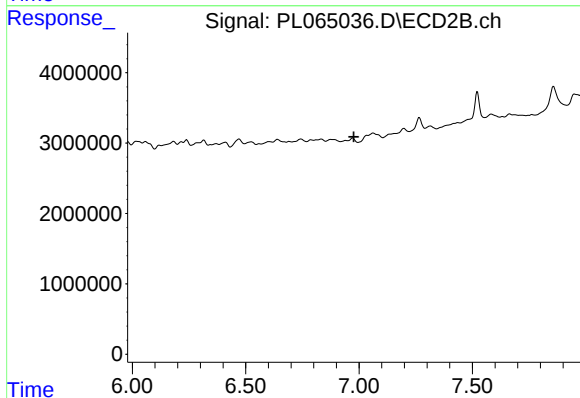


#16 4,4'-DDD

R.T.: 0.000 min
Exp R.T. : 6.977 min
Response: 0
Conc: N.D.

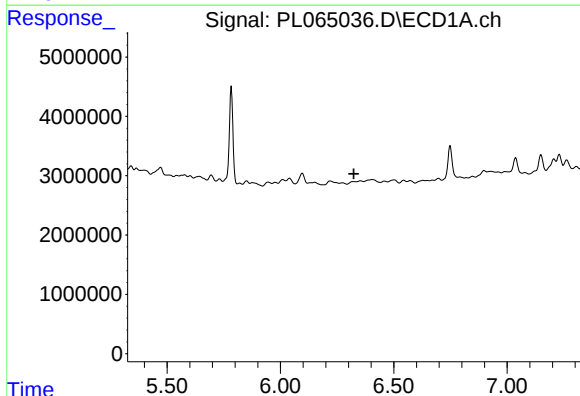


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.324 min
Response: 0
Conc: N.D.

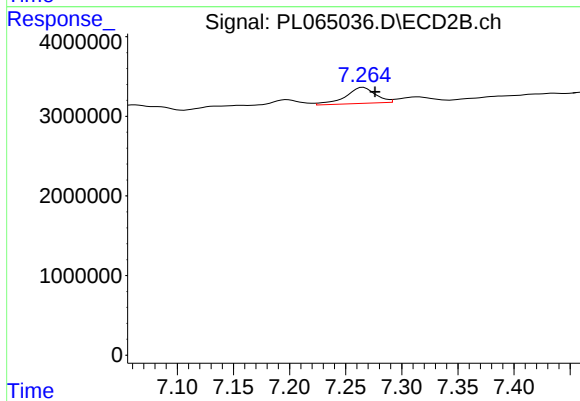

#17 4,4'-DDT


R.T.: 7.266 min
Delta R.T.: -0.011 min
Response: 3683691
Conc: 2.42 ng/ml

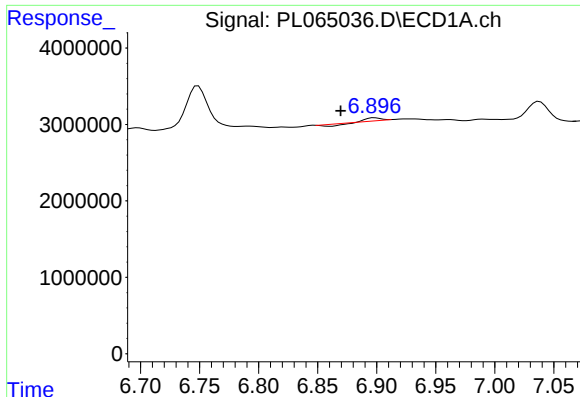

#20 Methoxychlor


R.T.: 6.899 min
Delta R.T.: 0.029 min
Response: 80957
Conc: 0.06 ng/ml

Instrument :
ECD_L
ClientSampleId :
PR-01-030221

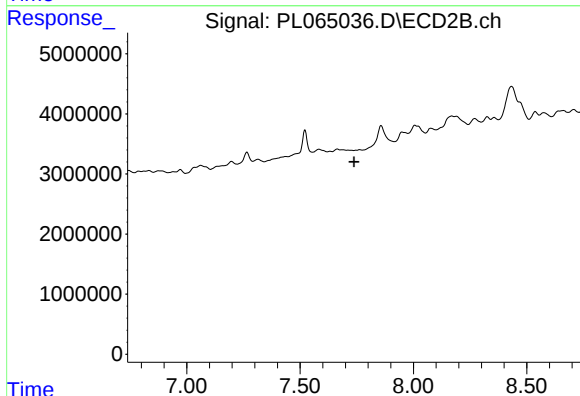


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.739 min
Response: 0
Conc: N.D.

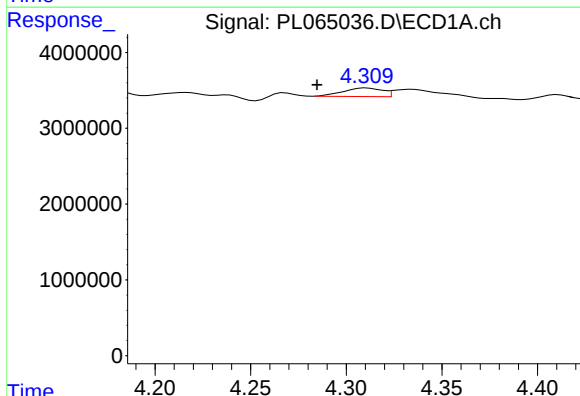


#23 Chlordane-1

R.T.: 4.311 min
Delta R.T.: 0.026 min
Response: 1615862
Conc: 14.21 ng/ml

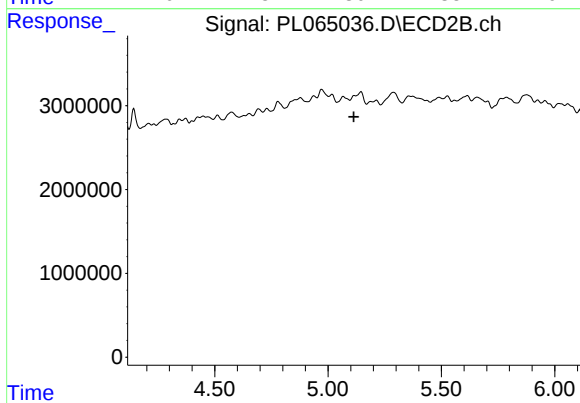

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

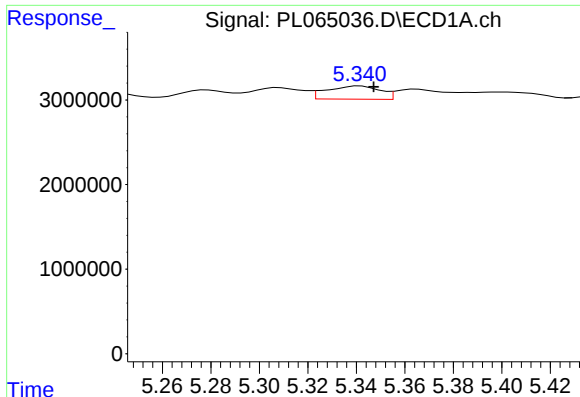

#25 Chlordane-3


R.T.: 5.342 min
Delta R.T.: -0.006 min
Response: 2379345
Conc: 7.24 ng/ml

Instrument :
ECD_L
ClientSampleId :
PR-01-030221

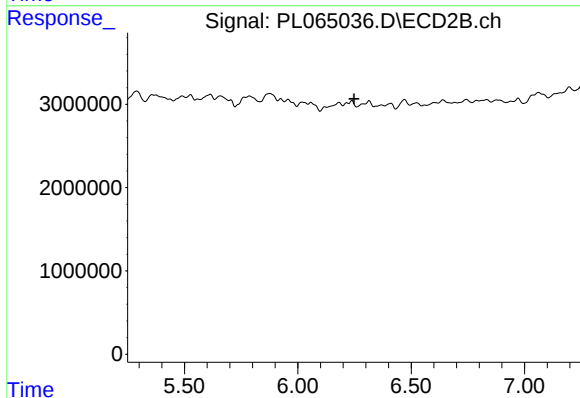


#25 Chlordane-3

R.T.: 0.000 min
Exp R.T. : 6.248 min
Response: 0
Conc: N.D.

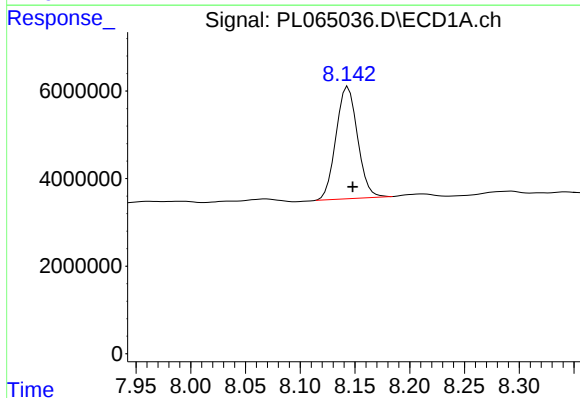

#28 Decachlorobiphenyl

R.T.: 8.144 min
Delta R.T.: -0.004 min
Response: 35066982
Conc: 15.59 ng/ml

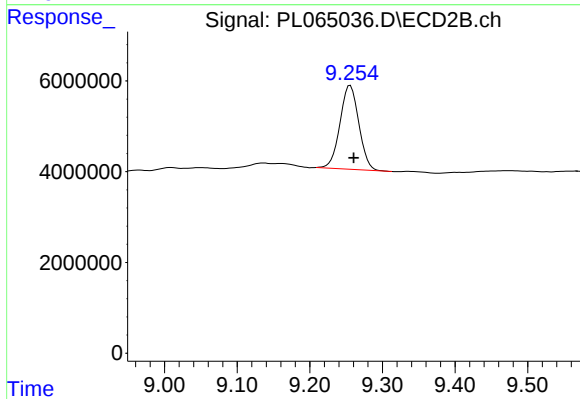

#28 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.005 min
Response: 33298892
Conc: 17.53 ng/ml