

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030321\
 Data File : PL065043.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2021 17:44
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 01:19:13 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.423	4.098	59927718	49443249	21.300	22.888
28)	SA Decachlor...	8.144	9.257	41593416	36673075	18.496	19.308
Target Compounds							
6)	B beta-BHC	0.000	4.973	0	5096719	N.D.	0.165 #
13)	MA Dieldrin	0.000	6.617f	0	1494539	N.D.	0.699 #
14)	MA Endrin	5.957	0.000	2730798	0	0.909	N.D. #
18)	B Endrin al...	6.390	0.000	3876996	0	1.590	N.D. #
23)	Chlordane-1	4.310f	0.000	5785306	0	50.893	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030321\
Data File : PL065043.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2021 17:44
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 01:19:13 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

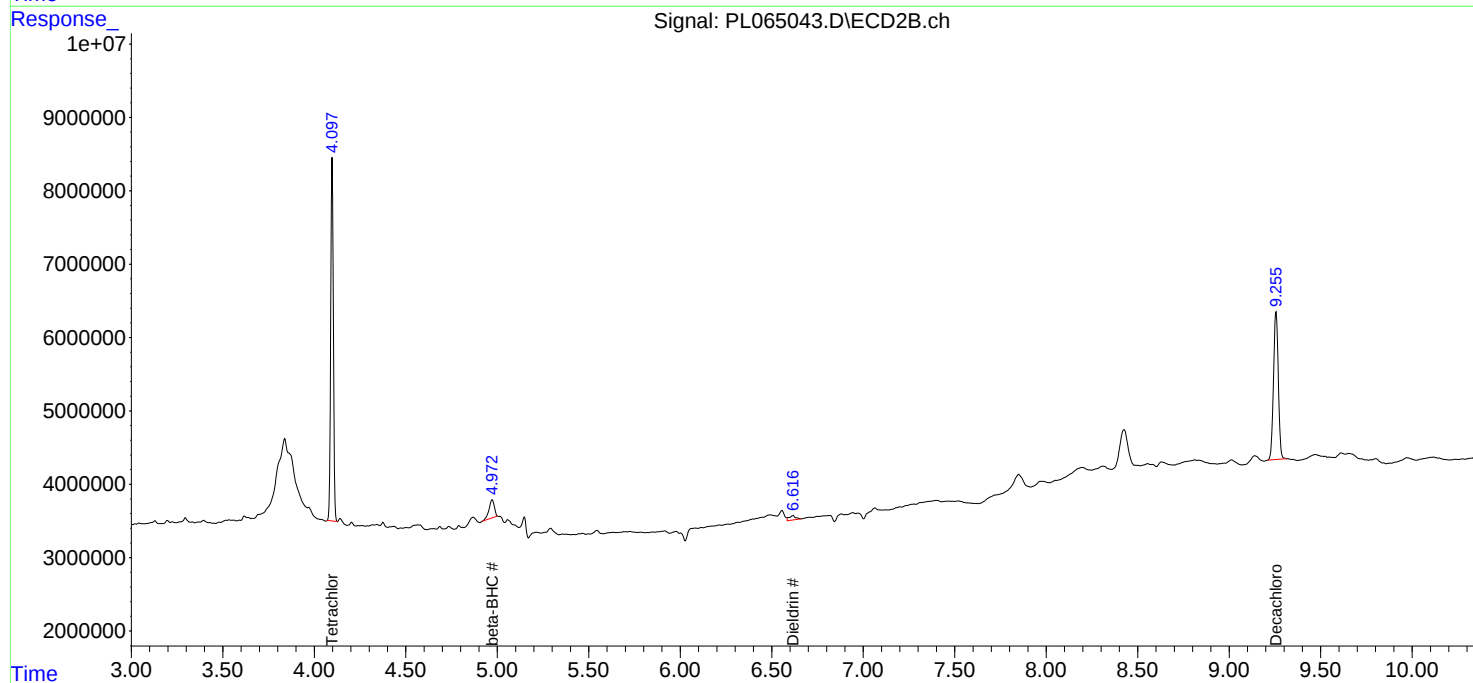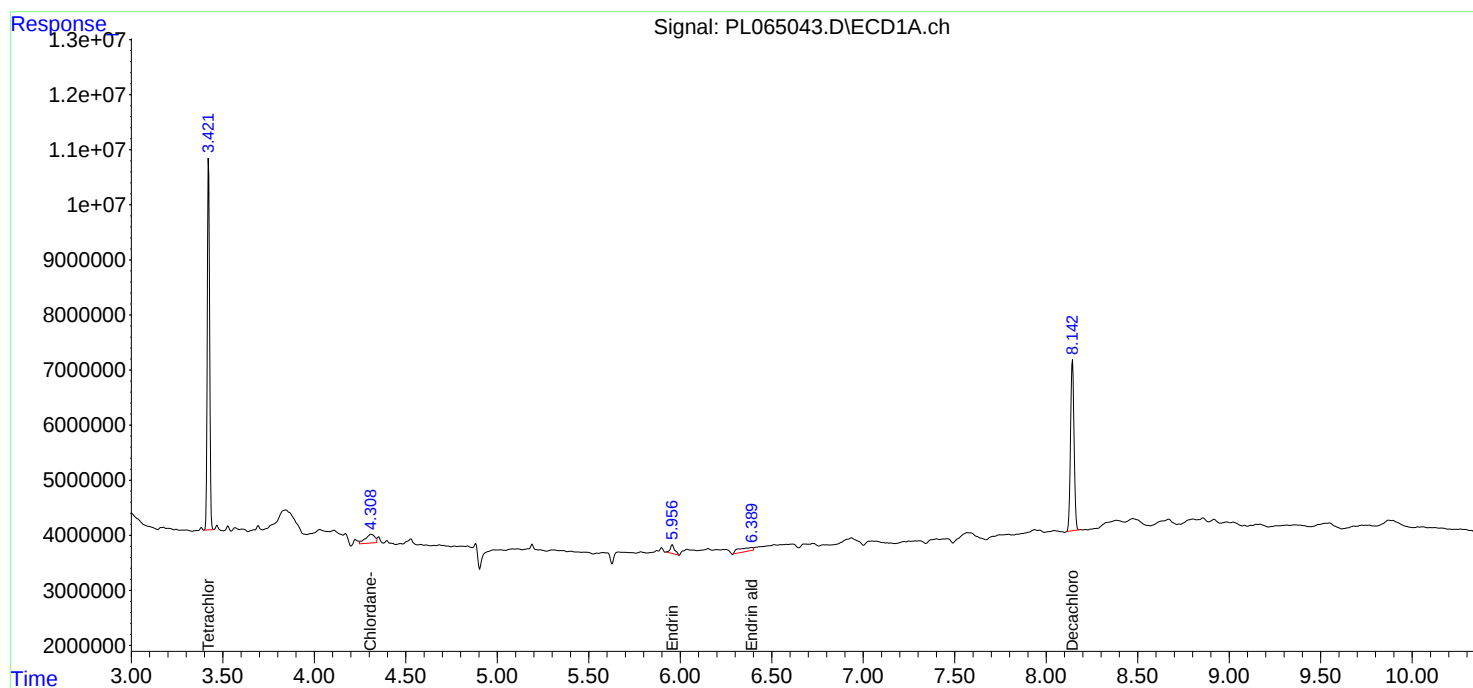


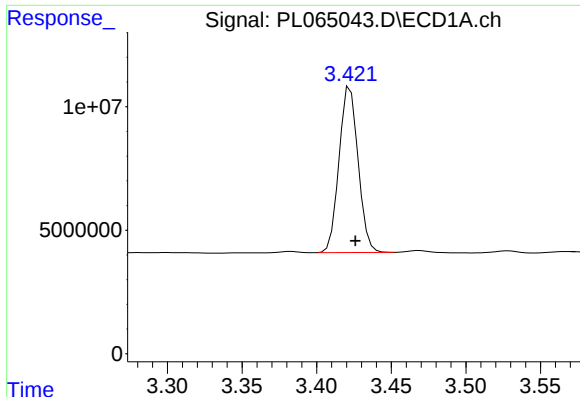

#1 Tetrachloro-m-xylene


R.T.: 3.423 min
Delta R.T.: -0.003 min
Response: 59927718
Conc: 21.30 ng/ml

Instrument :
ECD_L
ClientSampleId :

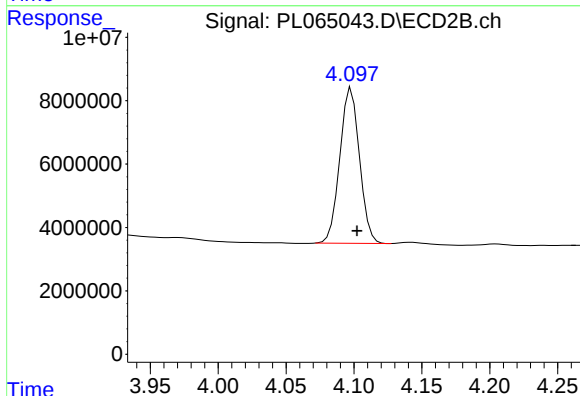


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: -0.004 min
Response: 49443249
Conc: 22.89 ng/ml

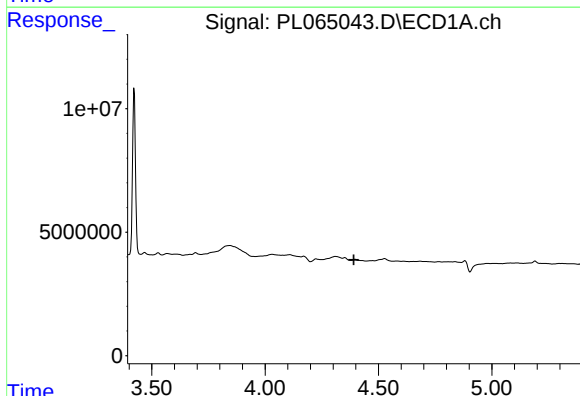


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.391 min
Response: 0
Conc: N.D.

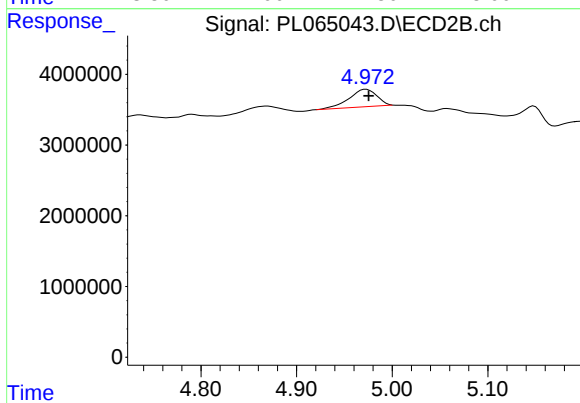

#6 beta-BHC


R.T.: 4.973 min
Delta R.T.: -0.003 min
Response: 5096719
Conc: 0.17 ng/ml

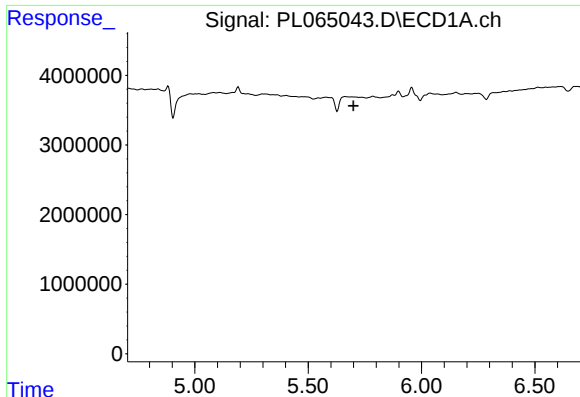

#13 Dieldrin


R.T.: 0.000 min
Exp R.T.: 5.701 min
Response: 0
Conc: N.D.

Instrument :
ECD_L
ClientSampleId :

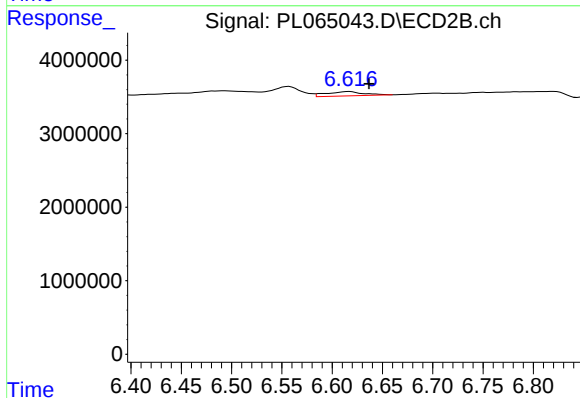


#13 Dieldrin

R.T.: 6.617 min
Delta R.T.: -0.019 min
Response: 1494539
Conc: 0.70 ng/ml

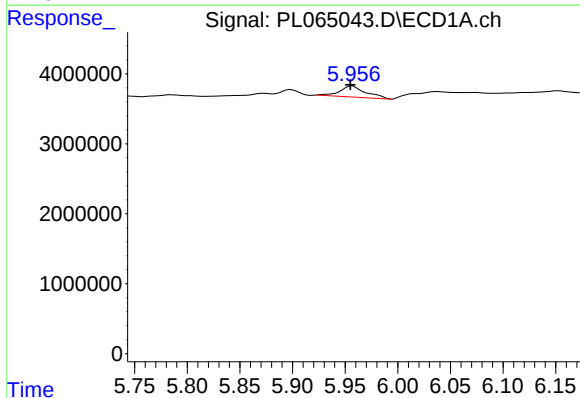


#14 Endrin

R.T.: 5.957 min
Delta R.T.: 0.002 min
Response: 2730798
Conc: 0.91 ng/ml

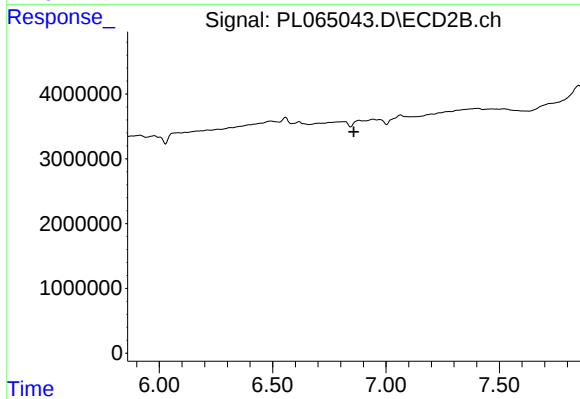

#14 Endrin


R.T.: 0.000 min
Exp R.T.: 6.858 min
Response: 0
Conc: N.D.

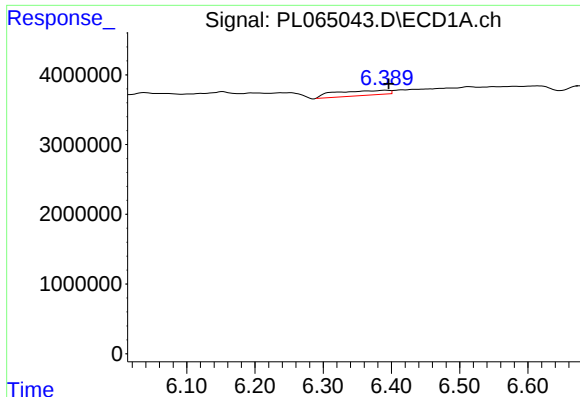

#18 Endrin aldehyde


R.T.: 6.390 min
Delta R.T.: -0.005 min
Response: 3876996
Conc: 1.59 ng/ml

Instrument :
ECD_L
ClientSampleId :

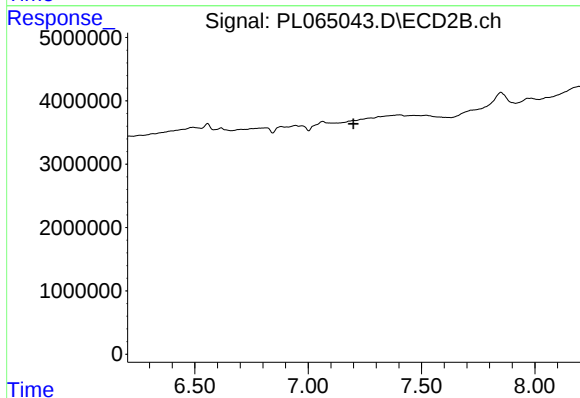


#18 Endrin aldehyde

R.T.: 0.000 min
Exp R.T. : 7.200 min
Response: 0
Conc: N.D.

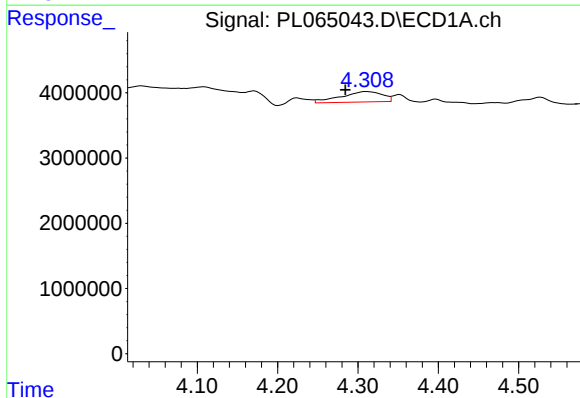


#23 Chlordane-1

R.T.: 4.310 min
Delta R.T.: 0.025 min
Response: 5785306
Conc: 50.89 ng/ml

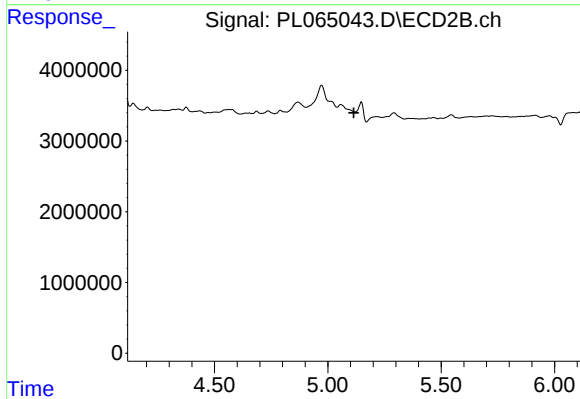

#23 Chlordane-1


R.T.: 0.000 min
Exp R.T. : 5.114 min
Response: 0
Conc: N.D.

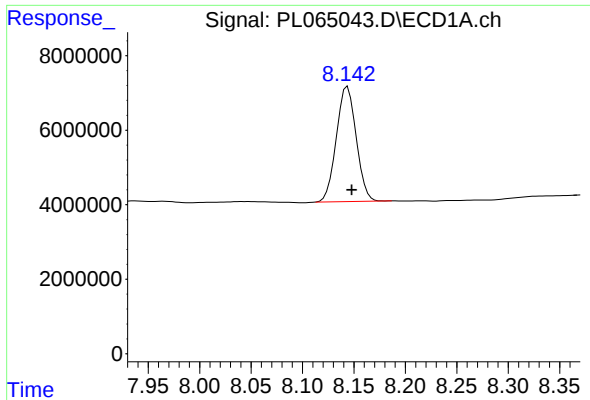

#28 Decachlorobiphenyl

R.T.: 8.144 min
Delta R.T.: -0.004 min
Response: 41593416
Conc: 18.50 ng/ml

Instrument :
ECD_L
ClientSampleId :

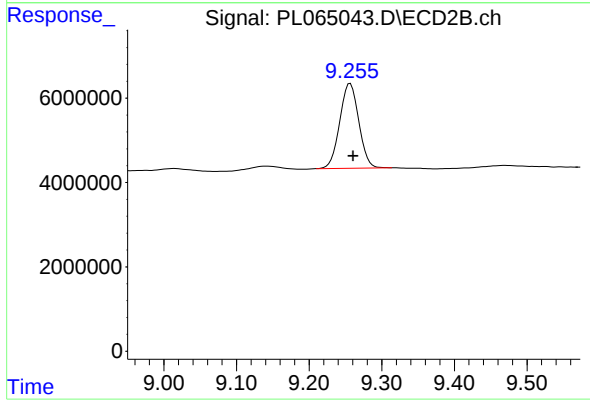

#28 Decachlorobiphenyl

R.T.: 9.257 min
Delta R.T.: -0.004 min
Response: 36673075
Conc: 19.31 ng/ml