

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030321\
 Data File : PL065031.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 03 Mar 2021 14:22
 Operator : AR\AJ
 Sample : M1542-01
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :
 SU-03-030221

Manual Integrations
 APPROVED

Ankita
 3/4/2021 9:08:44 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 04 01:15:21 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
 Quant Title : GC Extractables
 QLast Update : Tue Feb 09 04:41:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.422	4.098	37130479	31653886	13.197	14.653
28)	SA Decachlor...	8.144	9.256	32599006	30286098	14.496	15.945
Target Compounds							
11)	B alpha-Chl...	5.400	6.315	2759668	2759691	0.797m	1.199m#
12)	B 4,4'-DDE	5.565	6.473	7326218	7422437	2.341m	3.660 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030321\
Data File : PL065031.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 03 Mar 2021 14:22
Operator : AR\AJ
Sample : M1542-01
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_L
ClientSampleId :
SU-03-030221


Manual Integrations
APPROVED

Ankita
3/4/2021 9:08:44 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 04 01:15:21 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL020821.M
Quant Title : GC Extractables
QLast Update : Tue Feb 09 04:41:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

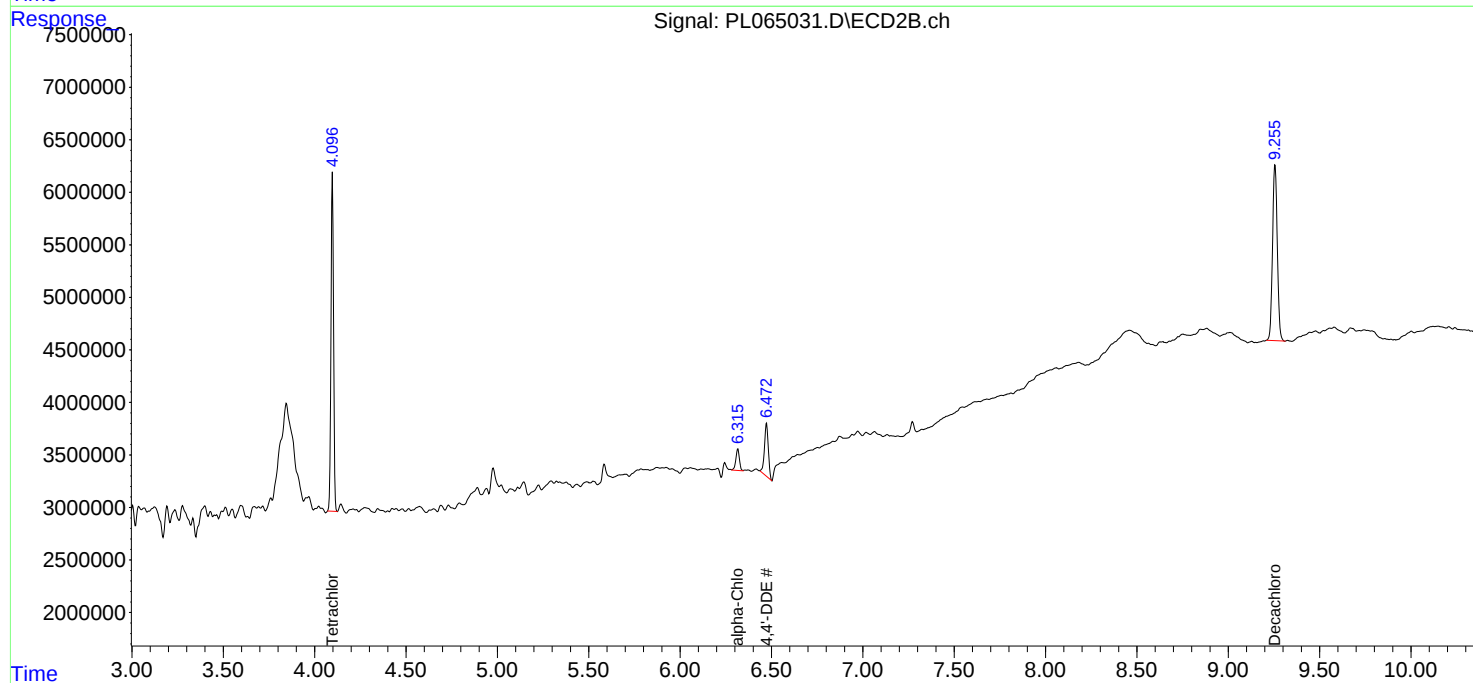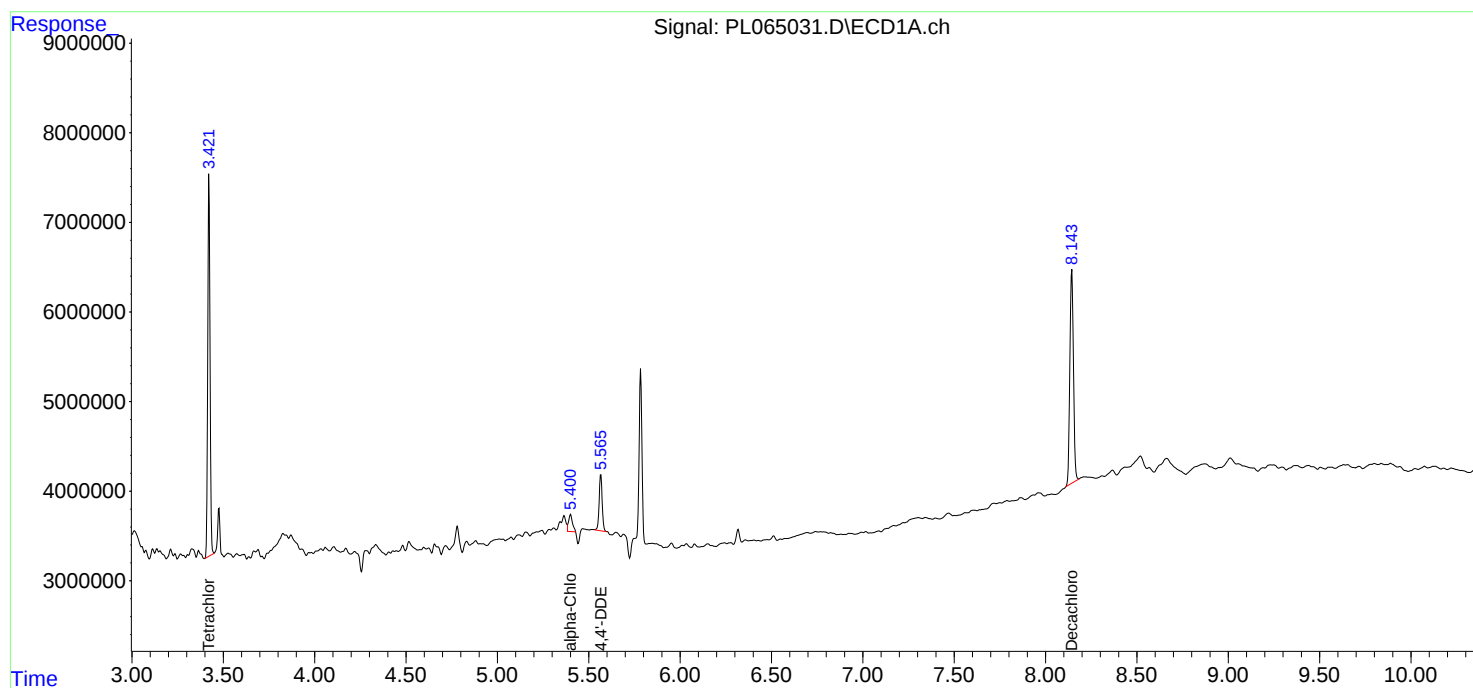

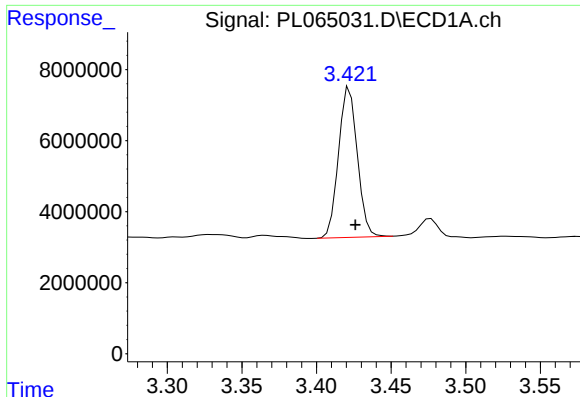


#1 Tetrachloro-m-xylene

R.T.: 3.422 min
Delta R.T.: -0.004 min
Response: 37130479
Conc: 13.20 ng/ml

Instrument :
ECD_L
ClientSampleId :
SU-03-030221


Manual Integrations
APPROVED

Ankita
3/4/2021 9:08:44 AM

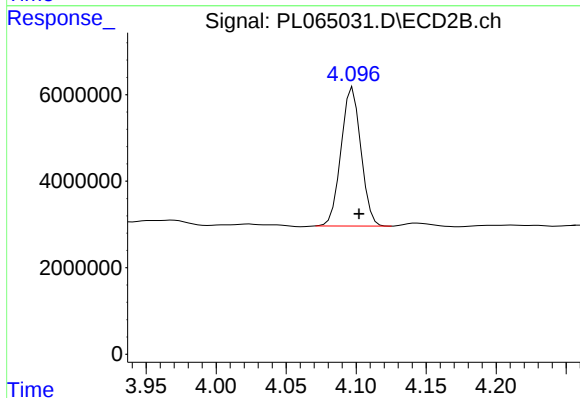


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: -0.004 min
Response: 31653886
Conc: 14.65 ng/ml

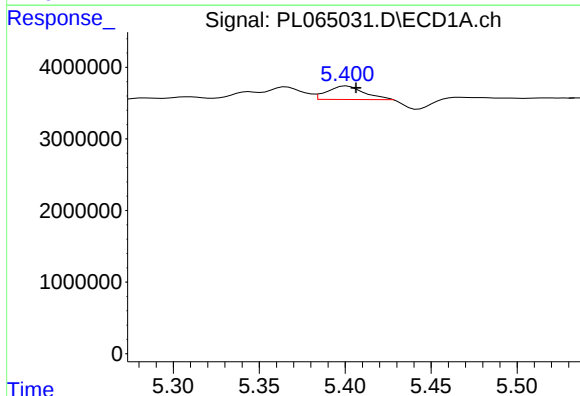


#11 alpha-Chlordane

R.T.: 5.400 min
Delta R.T.: -0.007 min
Response: 2759668
Conc: 0.80 ng/ml m

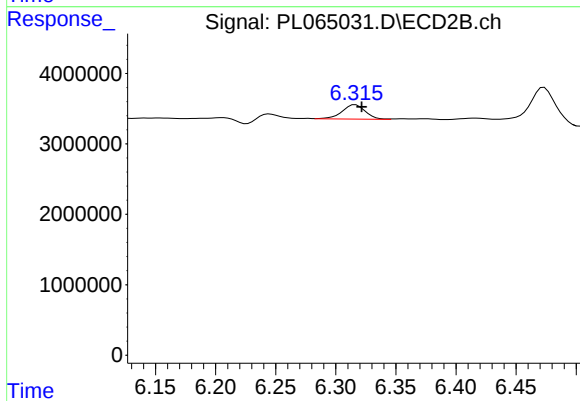

#11 alpha-Chlordane

R.T.: 6.315 min
Delta R.T.: -0.007 min
Response: 2759691
Conc: 1.20 ng/ml m

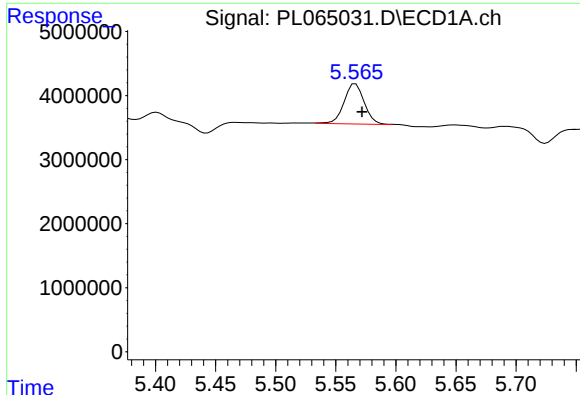


#12 4,4'-DDE

R.T.: 5.565 min
Delta R.T.: -0.007 min
Response: 7326218
Conc: 2.34 ng/ml m

Instrument :
ECD_L
ClientSampleId :
SU-03-030221


Manual Integrations
APPROVED

Ankita
3/4/2021 9:08:44 AM

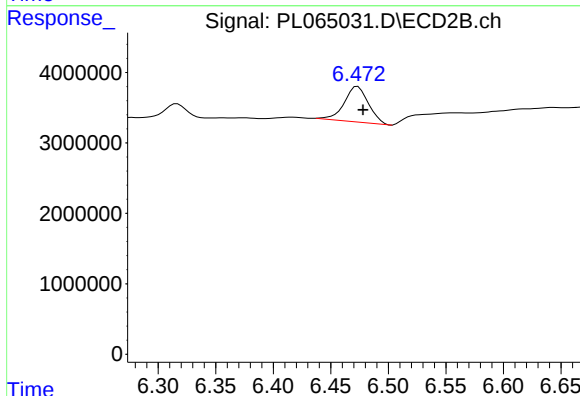


#12 4,4'-DDE

R.T.: 6.473 min
Delta R.T.: -0.005 min
Response: 7422437
Conc: 3.66 ng/ml

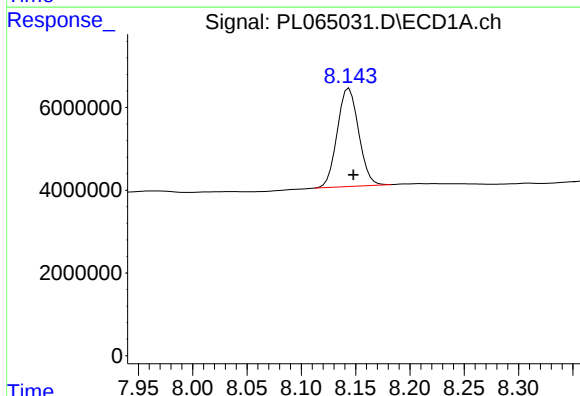

#28 Decachlorobiphenyl

R.T.: 8.144 min
Delta R.T.: -0.004 min
Response: 32599006
Conc: 14.50 ng/ml

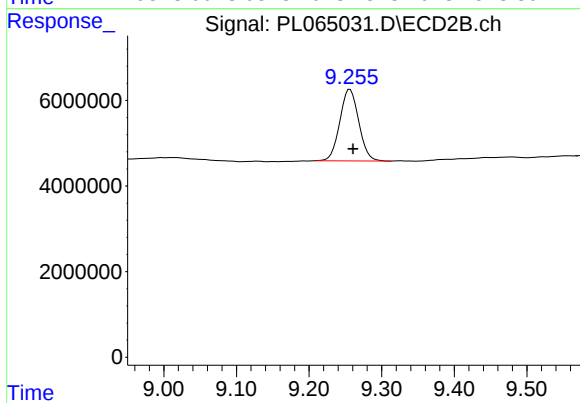

#28 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: -0.004 min
Response: 30286098
Conc: 15.95 ng/ml