

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030921\
 Data File : PL065161.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Mar 2021 10:32
 Operator : AR\AJ
 Sample : PB135034BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_L
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Mar 10 06:17:26 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
 Quant Title : GC Extractables
 QLast Update : Fri Mar 05 02:26:14 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.428	4.098	63306392	52392041	21.530	21.098
28)	SA Decachlor...	8.150	9.256	58885631	45161445	21.219	20.560
Target Compounds							
4)	MA Heptachlor	4.406f	0.000	1668359	0	0.379	N.D. #
6)	B beta-BHC	4.406f	0.000	1668359	0	0.893	N.D. #
8)	B Heptachlo...	0.000	6.003	0	28702845	N.D.	11.853 #
14)	MA Endrin	5.965f	0.000	22352875	0	6.512	N.D. #
15)	B Endosulfa...	6.217	0.000	2297302	0	0.732	N.D. #
27)	Chlordane-5	6.217	0.000	2297302	0	17.692	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_L\Data\PL030921\
Data File : PL065161.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Mar 2021 10:32
Operator : AR\AJ
Sample : PB135034BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_L
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Mar 10 06:17:26 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_L\methods\PL030521.M
Quant Title : GC Extractables
QLast Update : Fri Mar 05 02:26:14 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x0.5µm

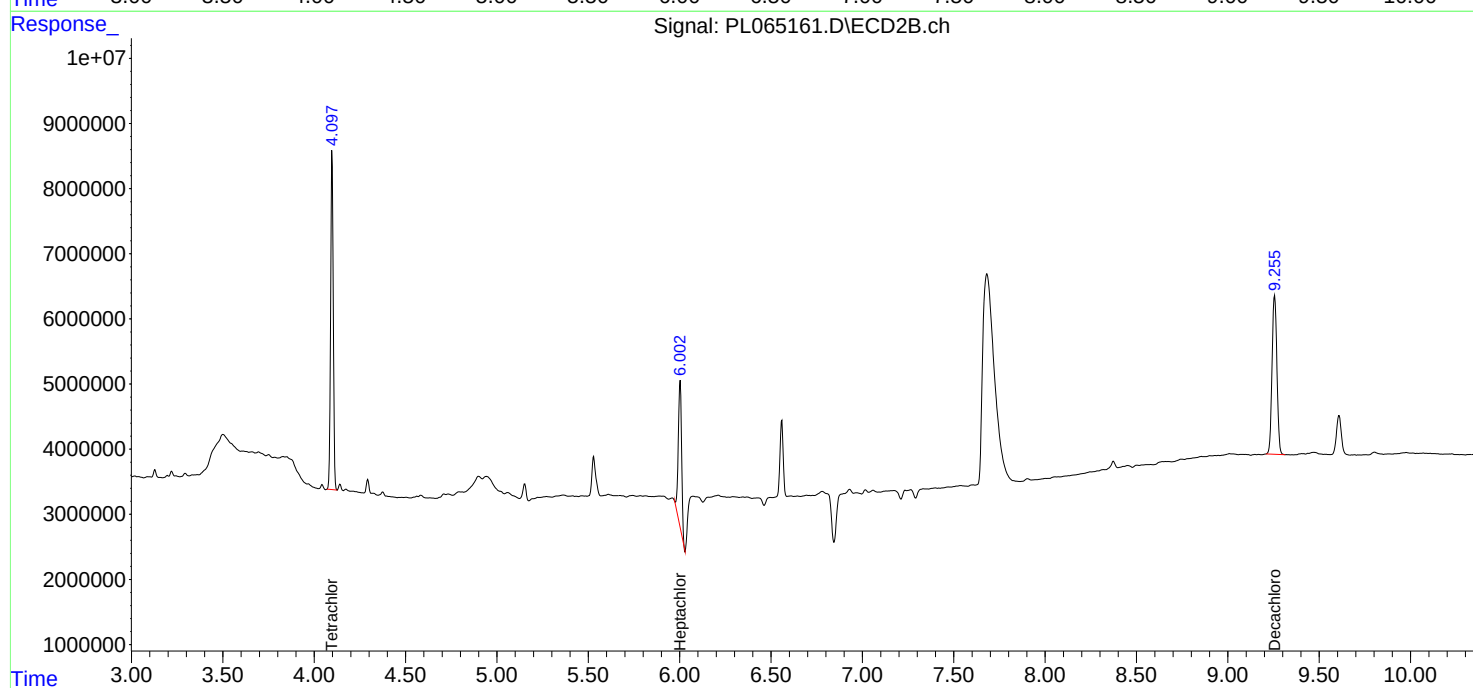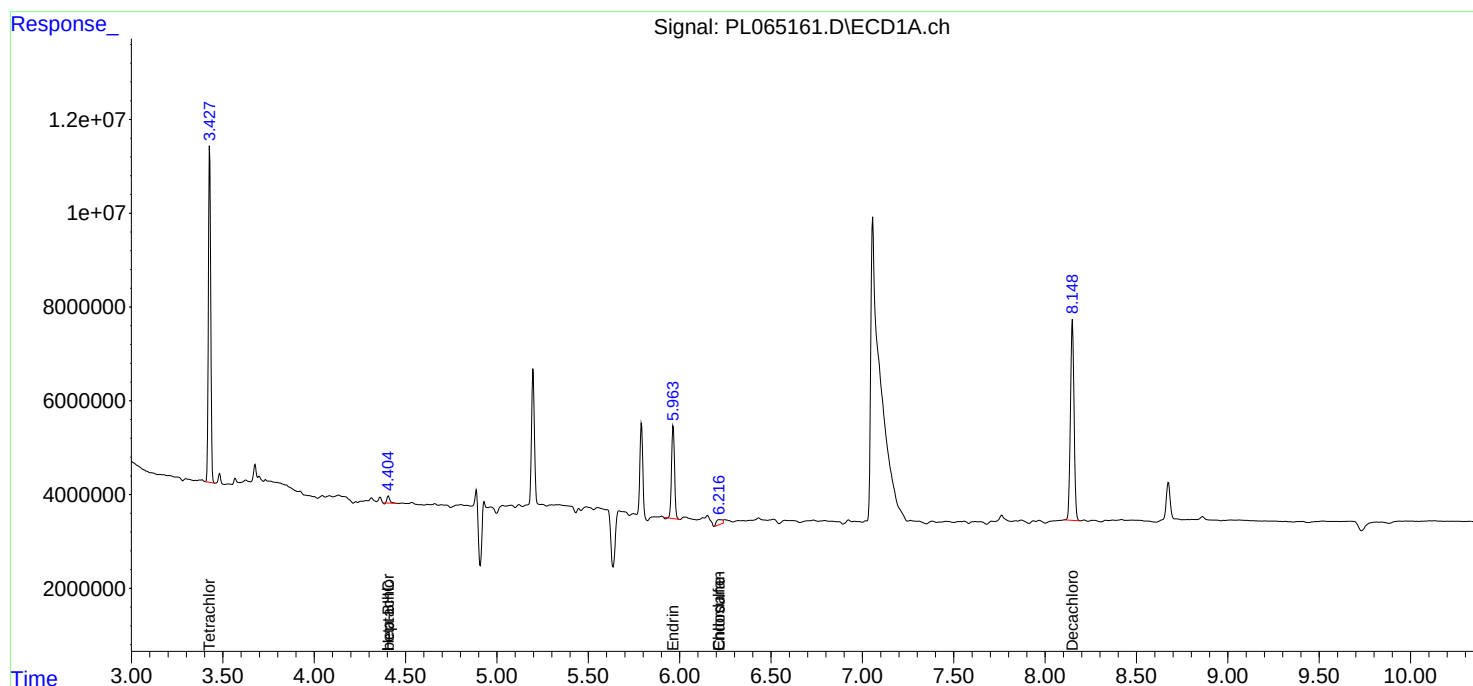


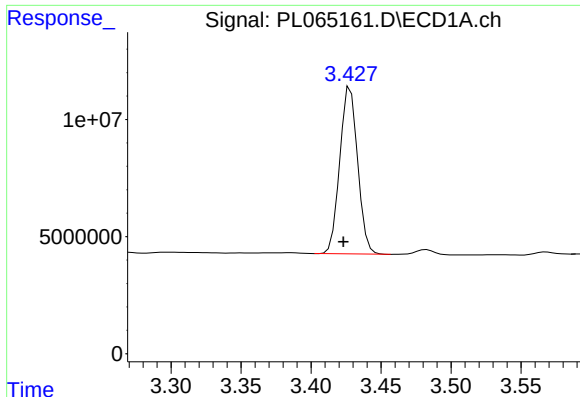

#1 Tetrachloro-m-xylene


R.T.: 3.428 min
Delta R.T.: 0.005 min
Response: 63306392
Conc: 21.53 ng/ml

Instrument :
ECD_L
ClientSampleId :

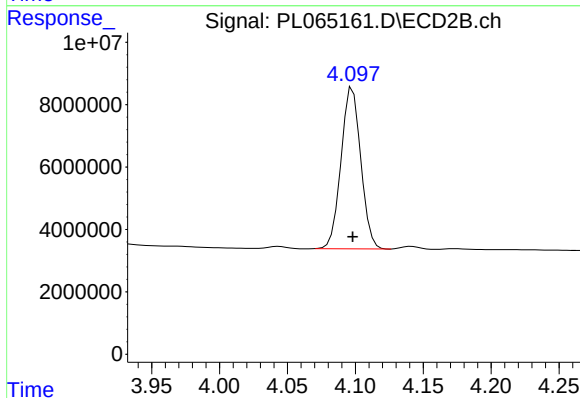


#1 Tetrachloro-m-xylene

R.T.: 4.098 min
Delta R.T.: 0.000 min
Response: 52392041
Conc: 21.10 ng/ml

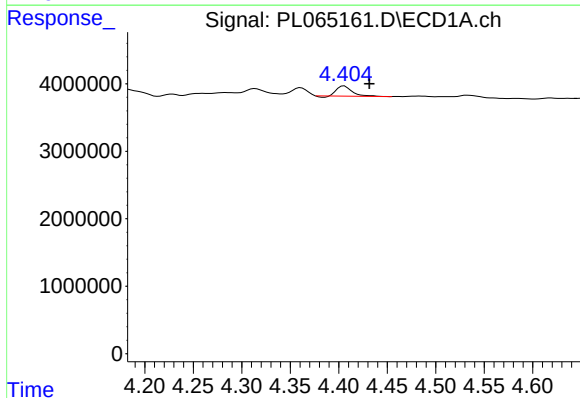


#4 Heptachlor

R.T.: 4.406 min
Delta R.T.: -0.026 min
Response: 1668359
Conc: 0.38 ng/ml

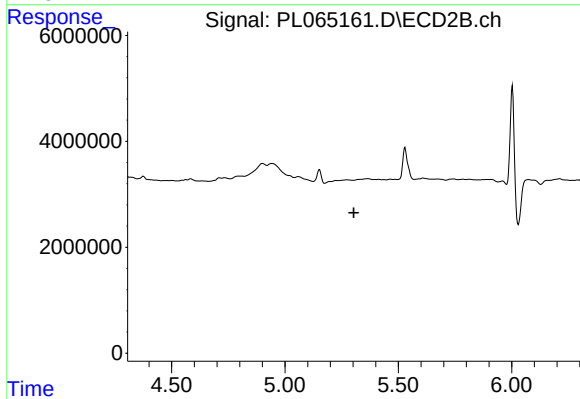

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 5.304 min
Response: 0
Conc: N.D.

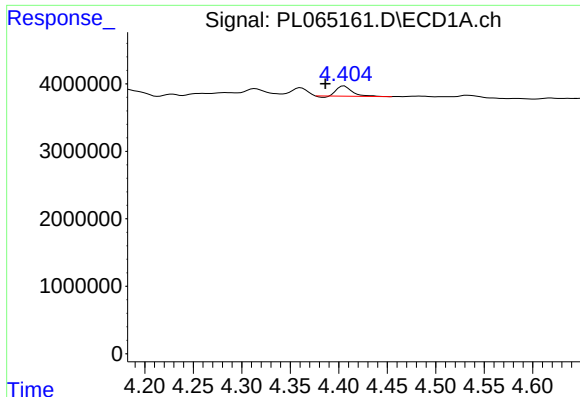

#6 beta-BHC


R.T.: 4.406 min
Delta R.T.: 0.019 min
Response: 1668359
Conc: 0.89 ng/ml

Instrument :
ECD_L
ClientSampleId :

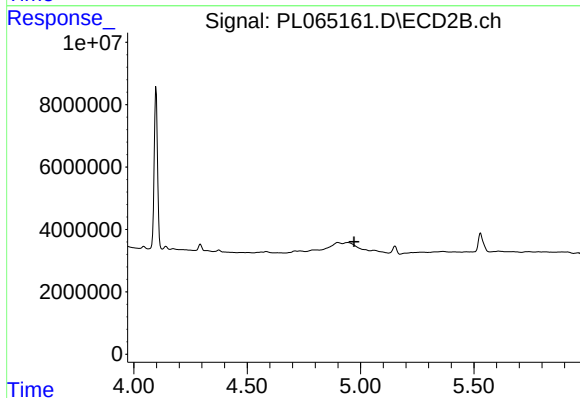


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.972 min
Response: 0
Conc: N.D.

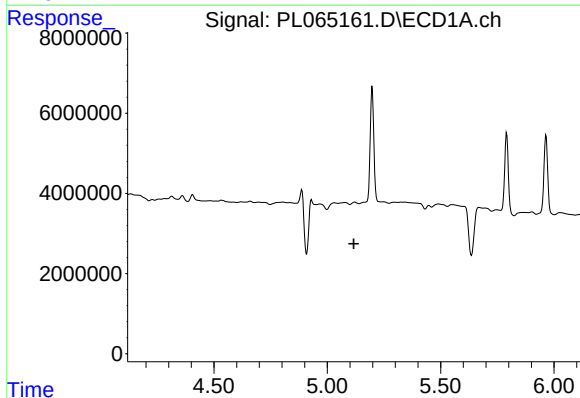


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 5.117 min
Response: 0
Conc: N.D.

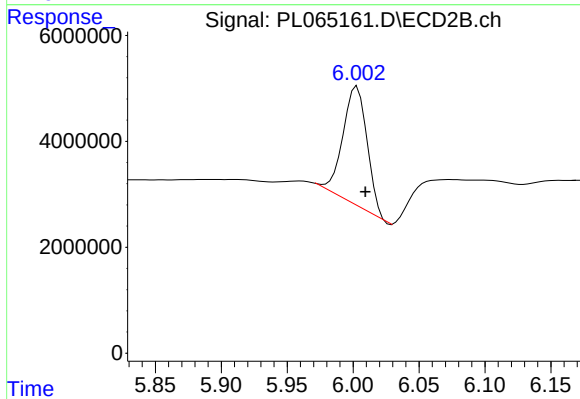

#8 Heptachlor epoxide


R.T.: 6.003 min
Delta R.T.: -0.006 min
Response: 28702845
Conc: 11.85 ng/ml

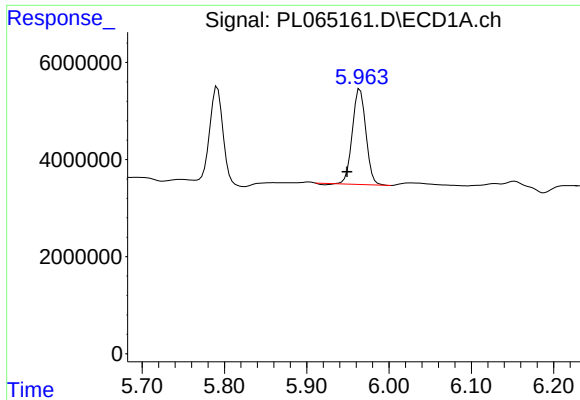

#14 Endrin


R.T.: 5.965 min
Delta R.T.: 0.016 min
Response: 22352875
Conc: 6.51 ng/ml

Instrument :
ECD_L
ClientSampleId :

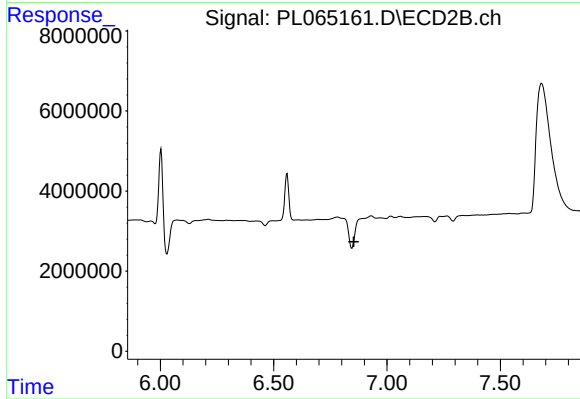


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 6.853 min
Response: 0
Conc: N.D.

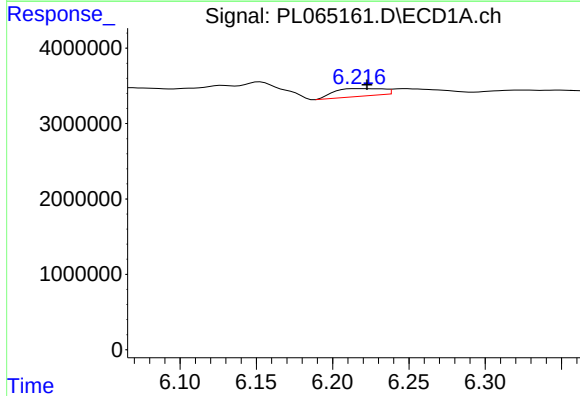


#15 Endosulfan II

R.T.: 6.217 min
Delta R.T.: -0.006 min
Response: 2297302
Conc: 0.73 ng/ml

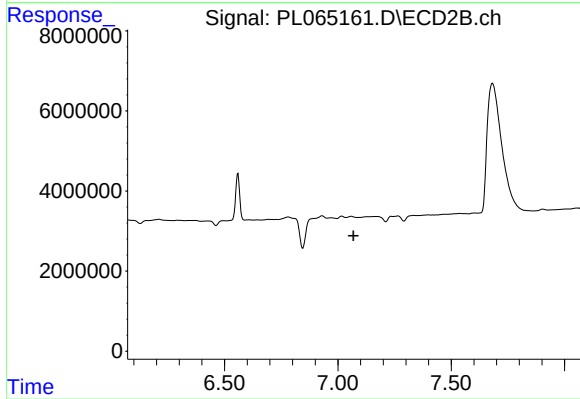

#15 Endosulfan II


R.T.: 0.000 min
Exp R.T. : 7.069 min
Response: 0
Conc: N.D.

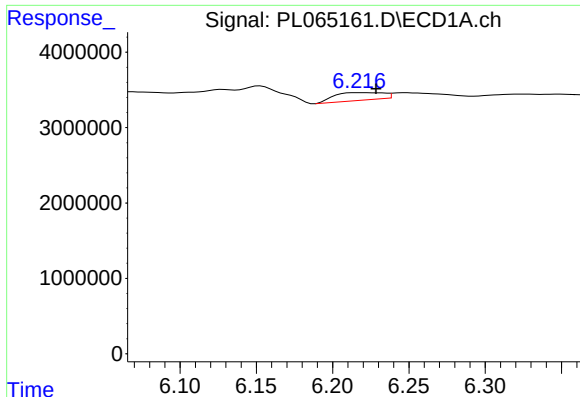

#27 Chlordane-5


R.T.: 6.217 min
Delta R.T.: -0.012 min
Response: 2297302
Conc: 17.69 ng/ml

Instrument :
ECD_L
ClientSampleId :

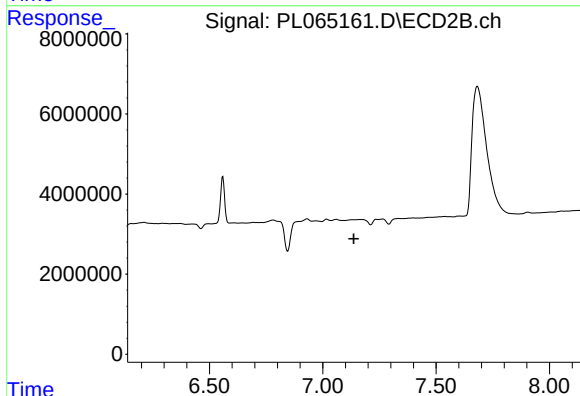


#27 Chlordane-5

R.T.: 0.000 min
Exp R.T. : 7.137 min
Response: 0
Conc: N.D.

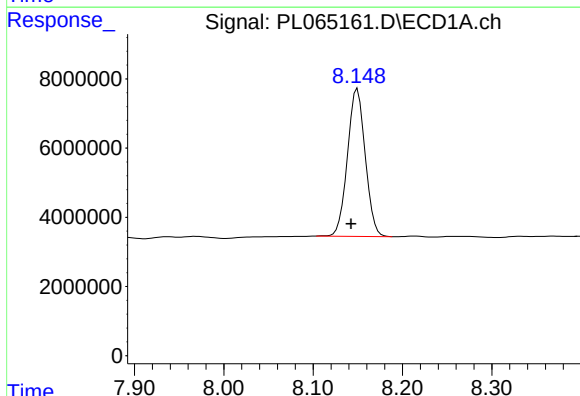

#28 Decachlorobiphenyl

R.T.: 8.150 min
Delta R.T.: 0.007 min
Response: 58885631
Conc: 21.22 ng/ml

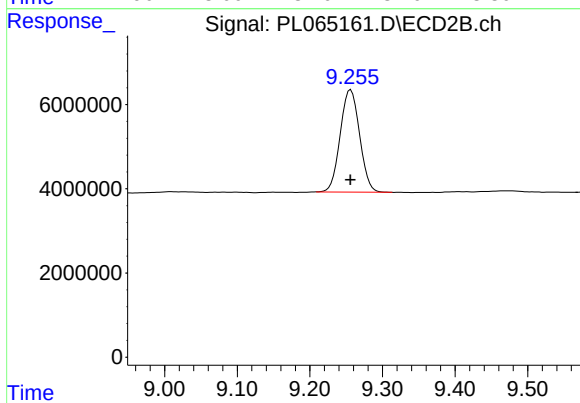

#28 Decachlorobiphenyl

R.T.: 9.256 min
Delta R.T.: 0.000 min
Response: 45161445
Conc: 20.56 ng/ml